
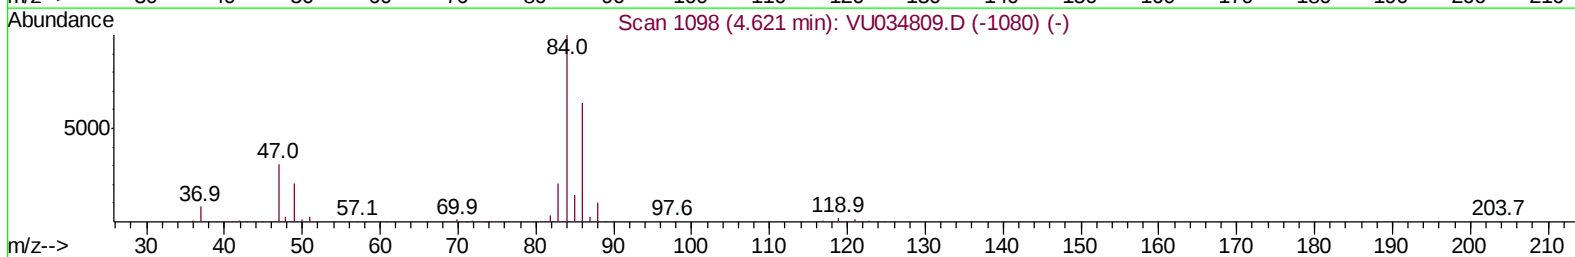
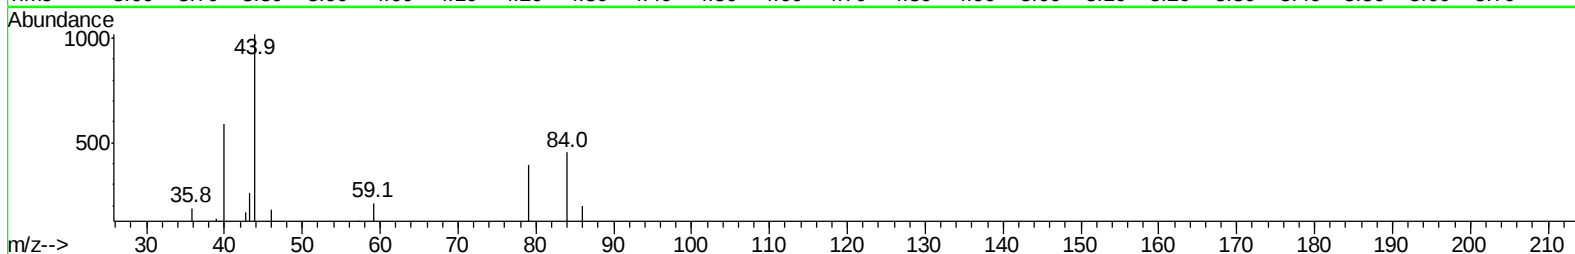


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
 Data File : VU034816.D
 Acq On : 25 Sep 2019 20:44
 Operator : JC/SP
 Sample : K4983-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 26 07:56:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 06:56:48 2019
 Response via : Initial Calibration

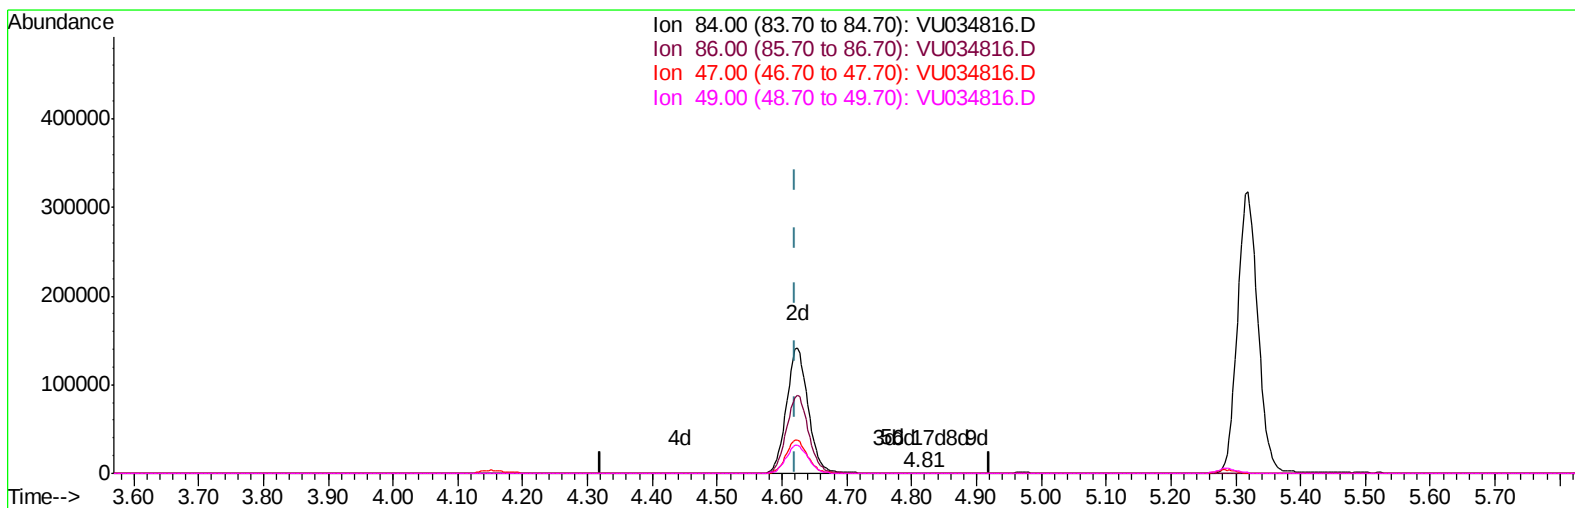

TIC: VU034816.D

(24) Chloroform-d (S)

4.810min (+0.190) 0.04ug/L

response 268

Ion	Exp%	Act%
84.00	100	100
86.00	61.70	60.82
47.00	58.40	41.79
49.00	34.10	43.66