
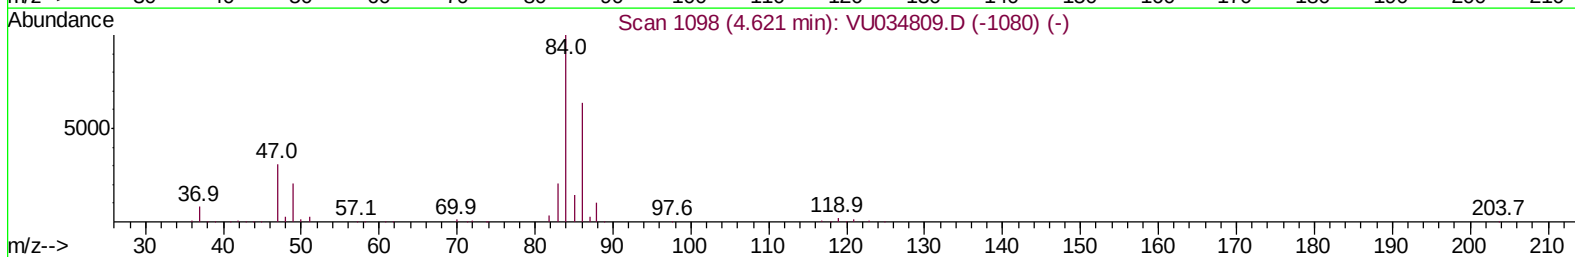
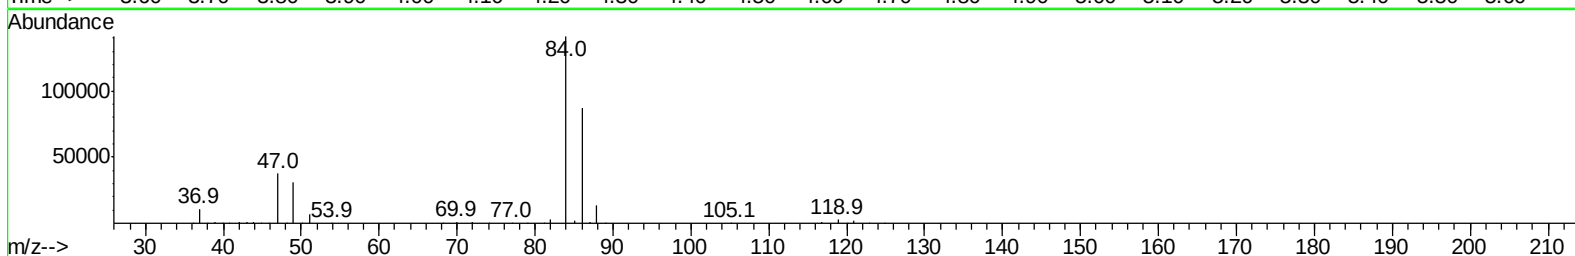


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
Data File : VU034816.D
Acq On : 25 Sep 2019 20:44
Operator : JC/SP
Sample : K4983-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 26 07:56:15 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 06:56:48 2019
Response via : Initial Calibration

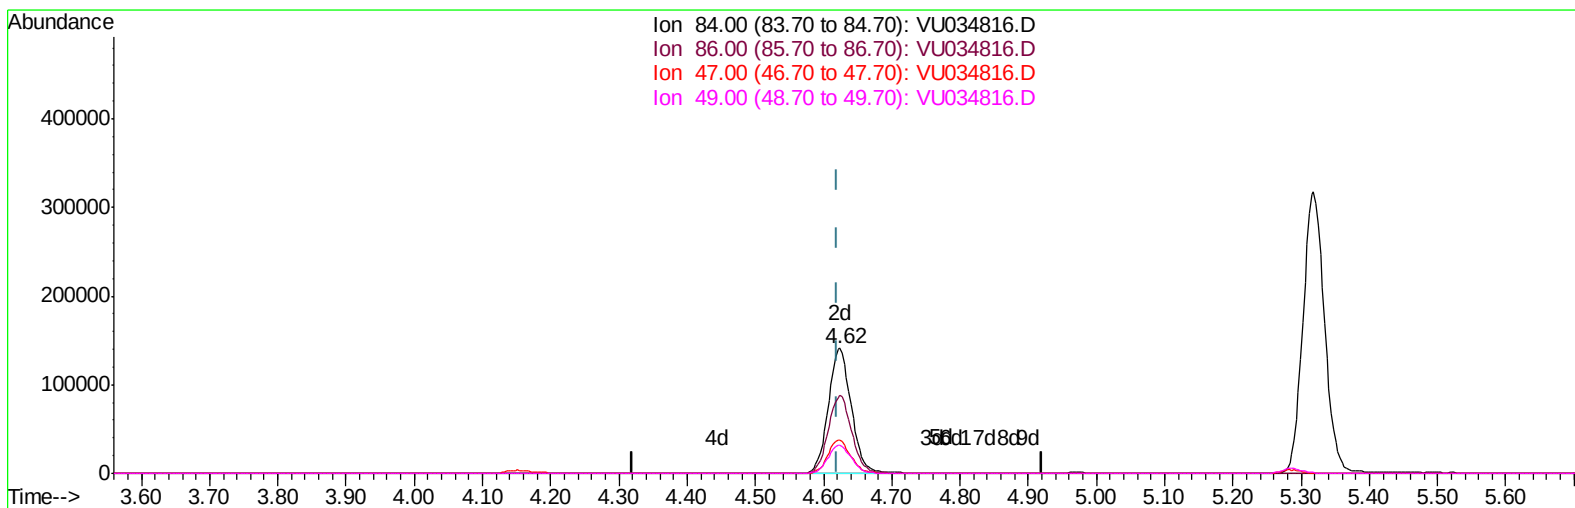

TIC: VU034816.D

(24) Chloroform-d (S)

4.624min (+0.003) 54.21ug/L m

response 328648

Ion	Exp%	Act%
84.00	100	100
86.00	61.70	0.05#
47.00	58.40	0.03#
49.00	34.10	0.04#