
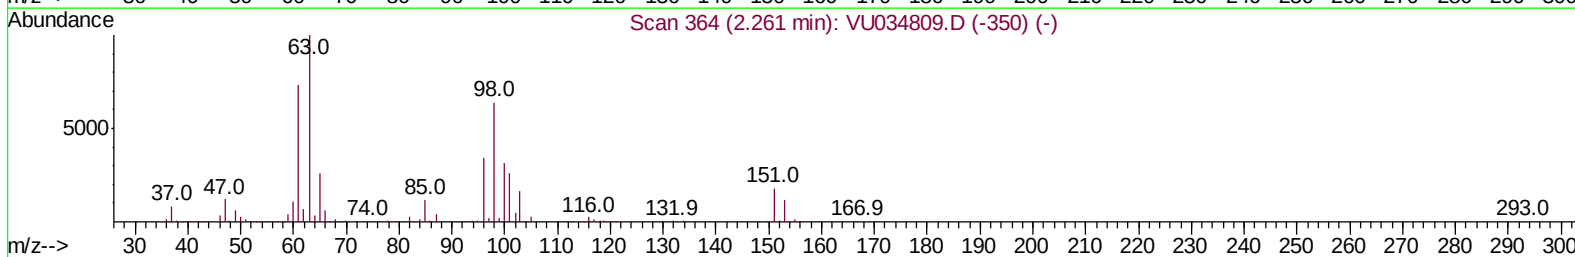
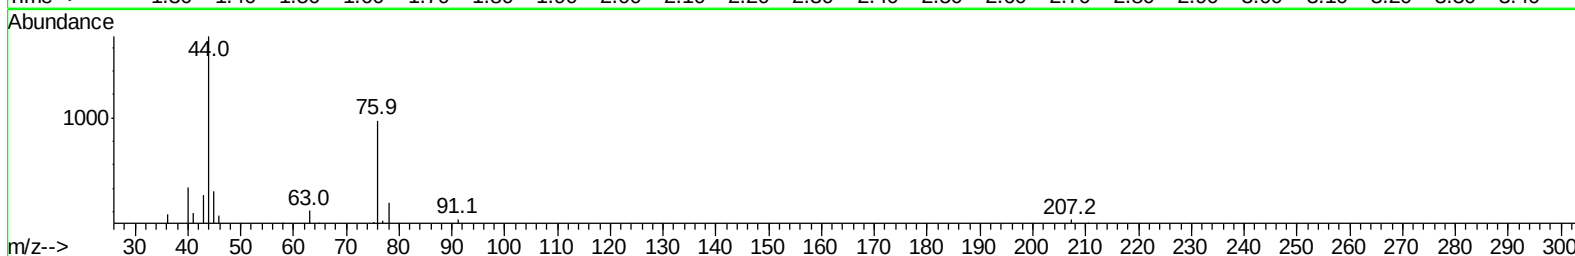


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
Data File : VU034821.D
Acq On : 25 Sep 2019 22:41
Operator : JC/SP
Sample : K4983-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Sep 26 08:02:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 06:56:48 2019
Response via : Initial Calibration

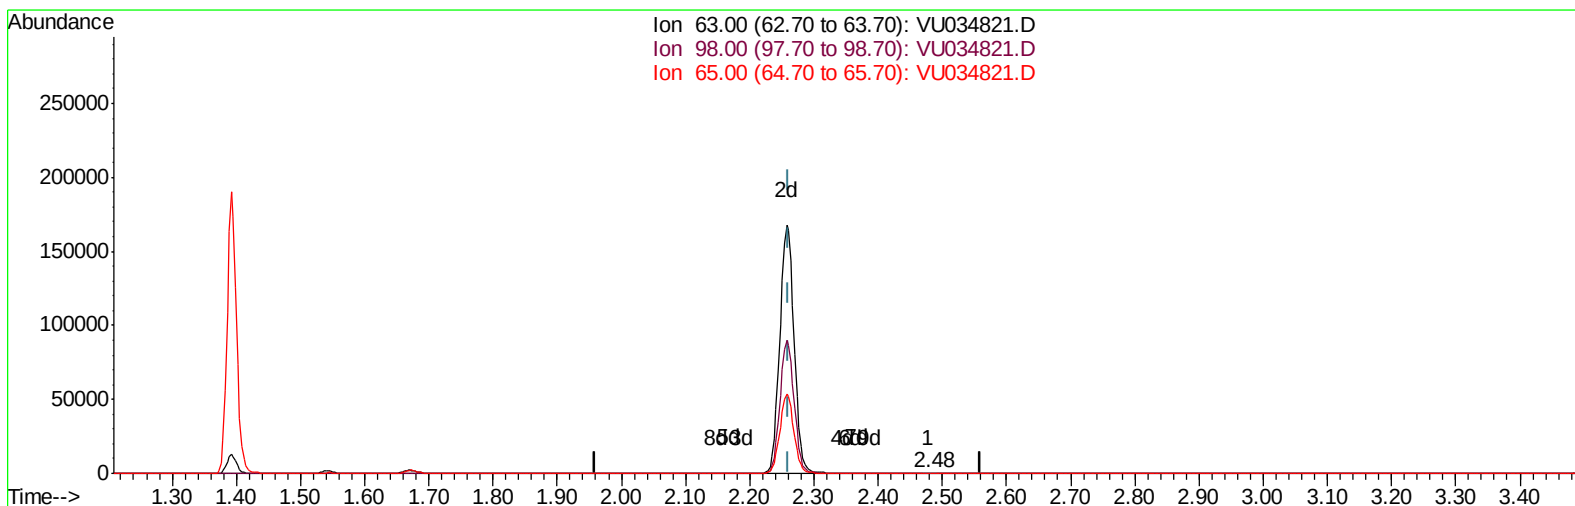

TIC: VU034821.D

(11) 1,1-Dichloroethene-d2 (S)

2.479min (+0.219) 0.02ug/L

response 186

Ion	Exp%	Act%
63.00	100	100
98.00	57.60	40.32
65.00	24.00	21.51
0.00	0.00	0.00