
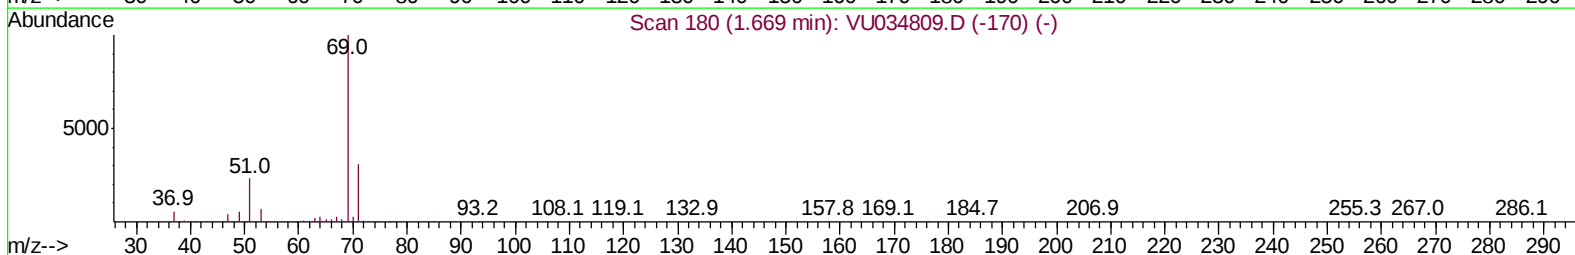
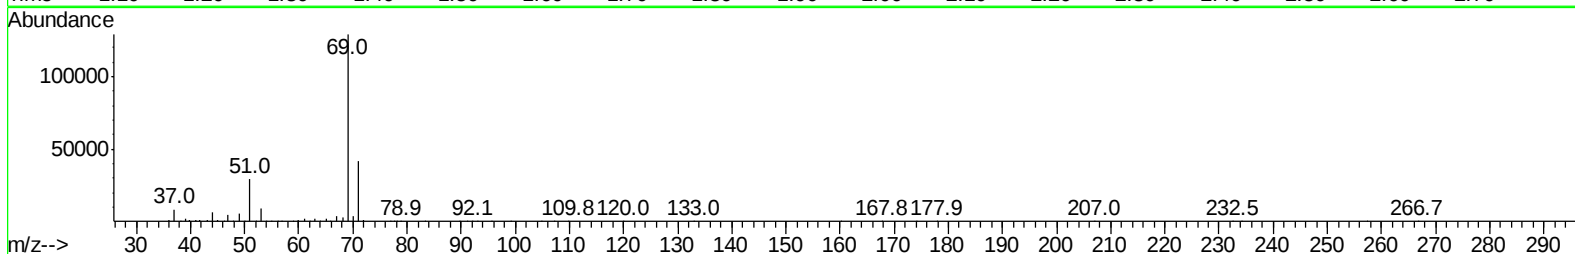


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
 Data File : VU034828.D
 Acd On : 26 Sep 2019 01:25
 Operator : JC/SP
 Sample : K4983-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Quant Time: Sep 26 07:03:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 06:56:48 2019
 Response via : Initial Calibration

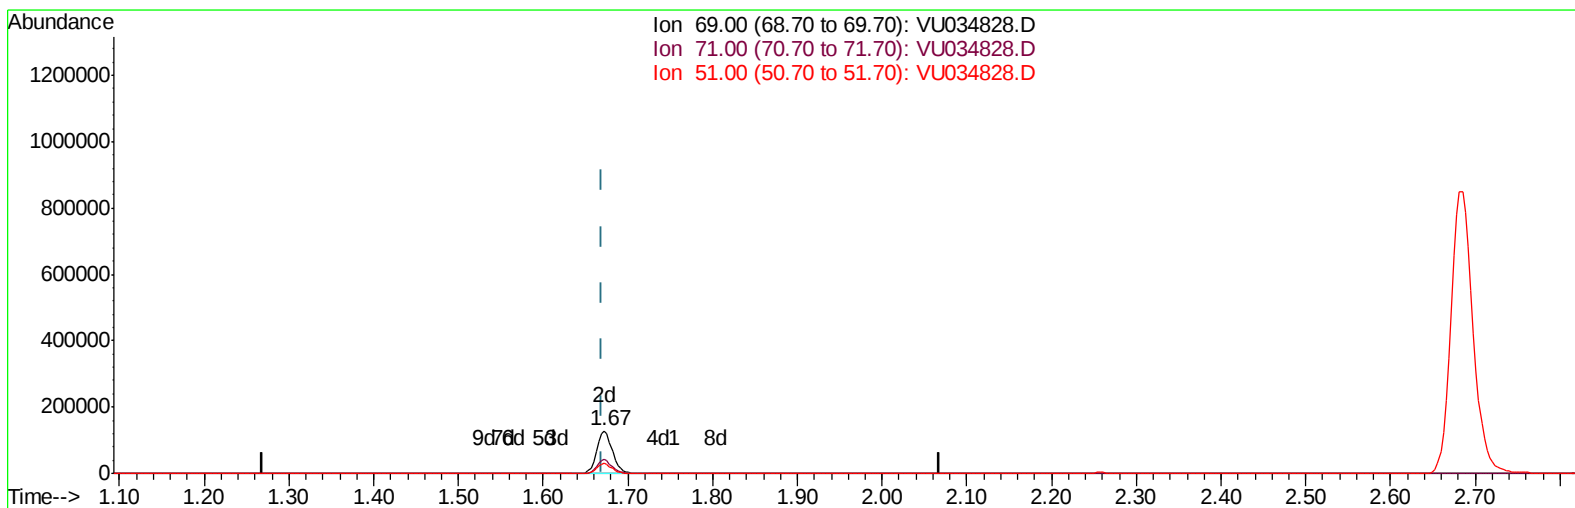

TIC: VU034828.D

(7) Chloroethane-d5 (S)

1.672min (+0.003) 47.85ug/L m

response 164256

Ion	Exp%	Act%
69.00	100	100
71.00	31.80	0.08#
51.00	32.70	0.08#
0.00	0.00	0.00