
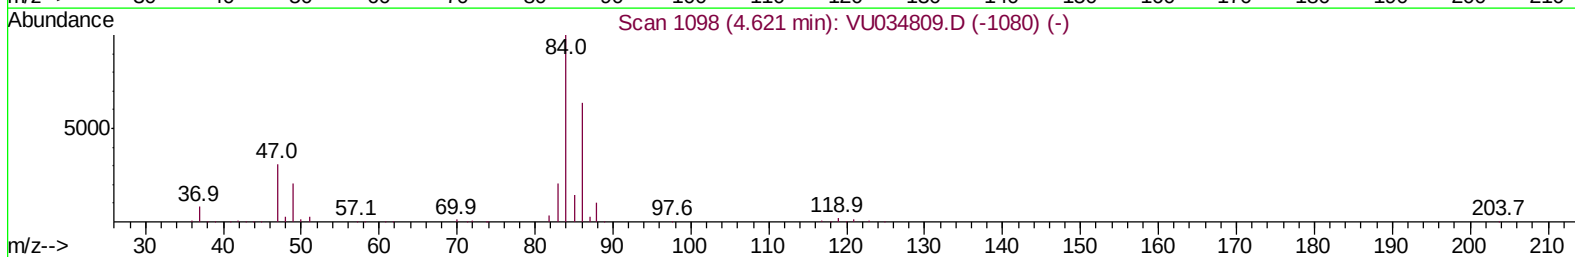
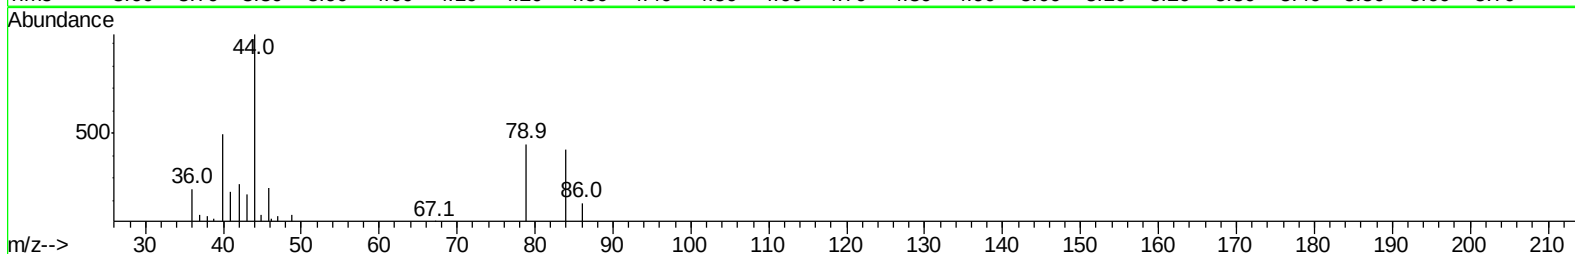


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
Data File : VU034830.D
Acq On : 26 Sep 2019 02:12
Operator : JC/SP
Sample : K4983-20
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Sep 26 07:04:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 06:56:48 2019
Response via : Initial Calibration

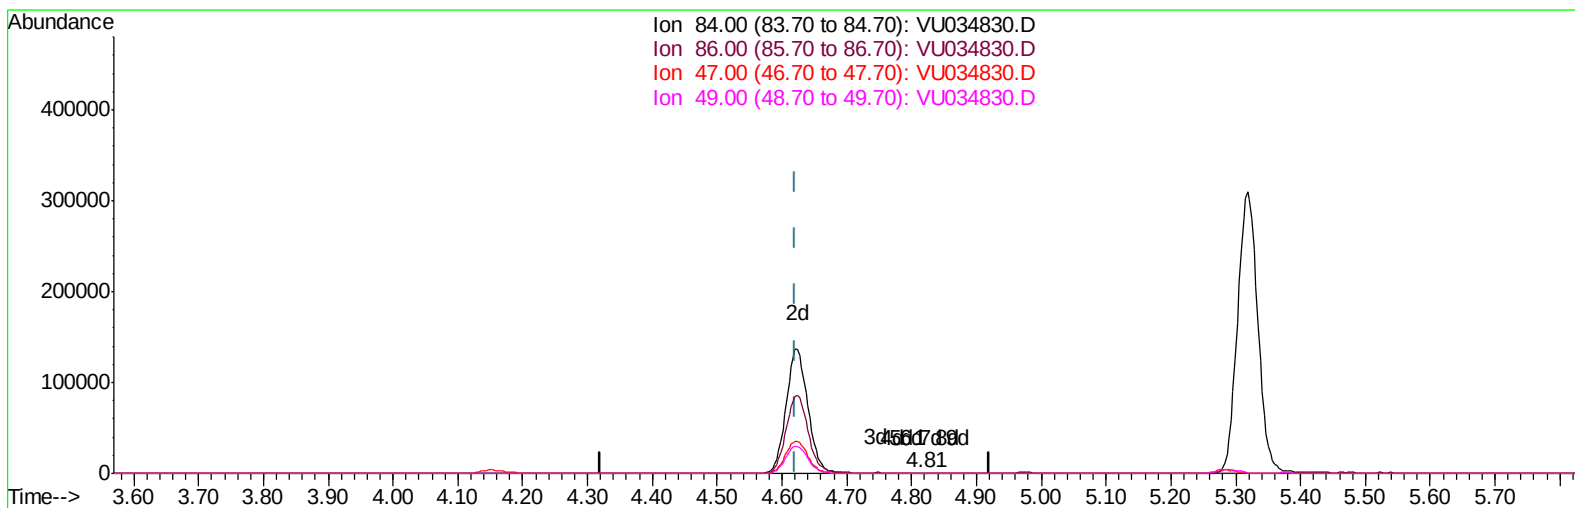

TIC: VU034830.D

(24) Chloroform-d (S)

4.813min (+0.193) 0.03ug/L

response 192

Ion	Exp%	Act%
84.00	100	100
86.00	61.70	72.92
47.00	58.40	60.42
49.00	34.10	42.71