
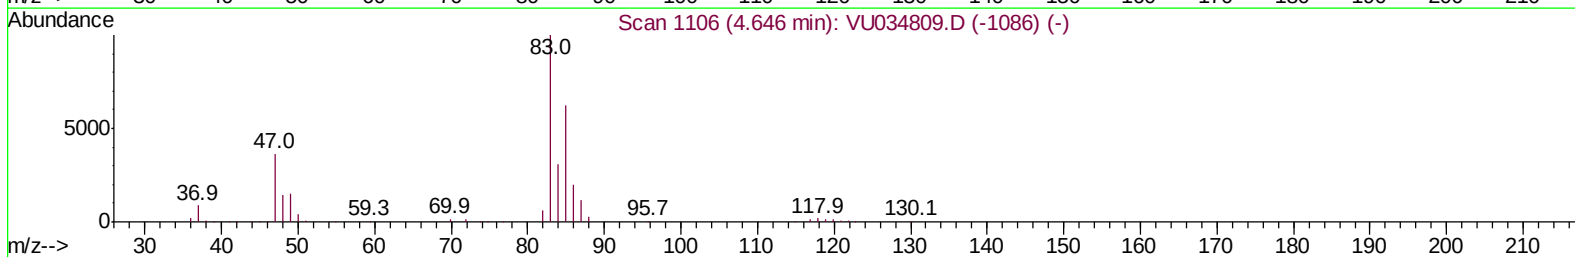
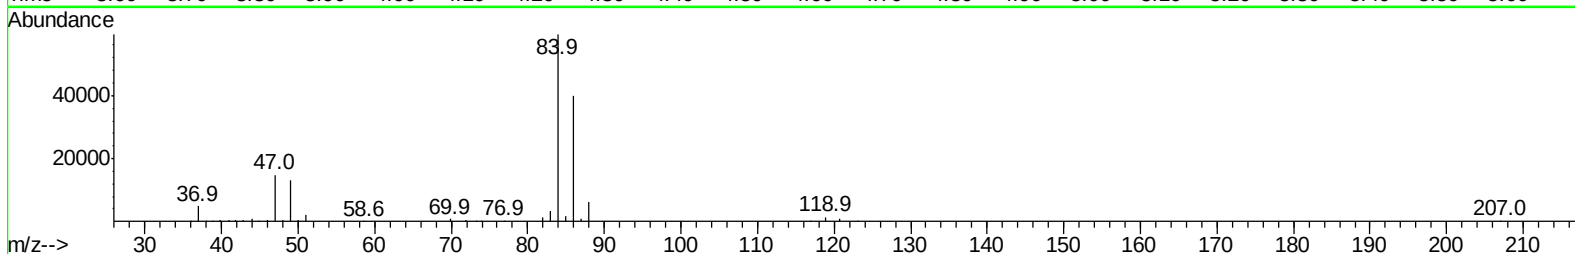


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
 Data File : VU034814.D
 Acd On : 25 Sep 2019 19:57
 Operator : JC/SP
 Sample : K4983-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Quant Time: Sep 26 08:32:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 06:56:48 2019
 Response via : Initial Calibration

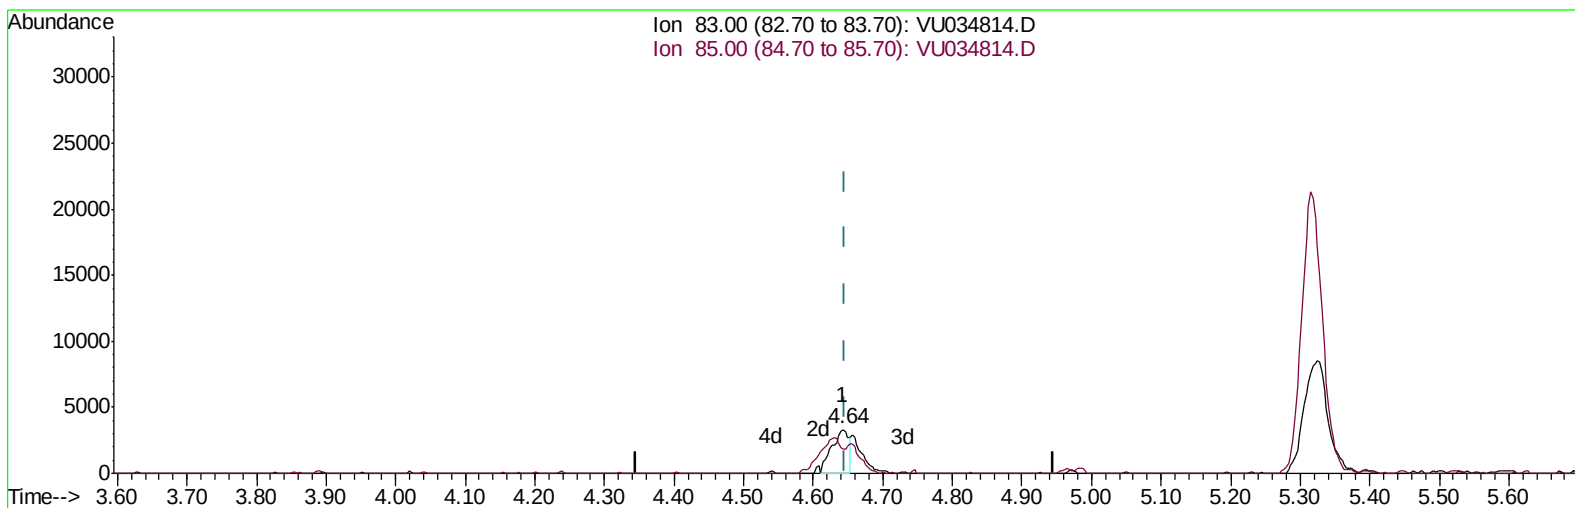

TIC: VU034814.D

(25) Chloroform (T)

4.643min (-0.003) 0.83ug/L

response 5726

Ion	Exp%	Act%
83.00	100	100
85.00	62.80	54.59
0.00	0.00	0.00
0.00	0.00	0.00