


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
Data File : VU034792.D
Acq On : 25 Sep 2019 09:58
Operator : JC/SP
Sample : BFB38
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Title : VOC Analysis
Last Update : Fri Sep 27 10:57:29 2019

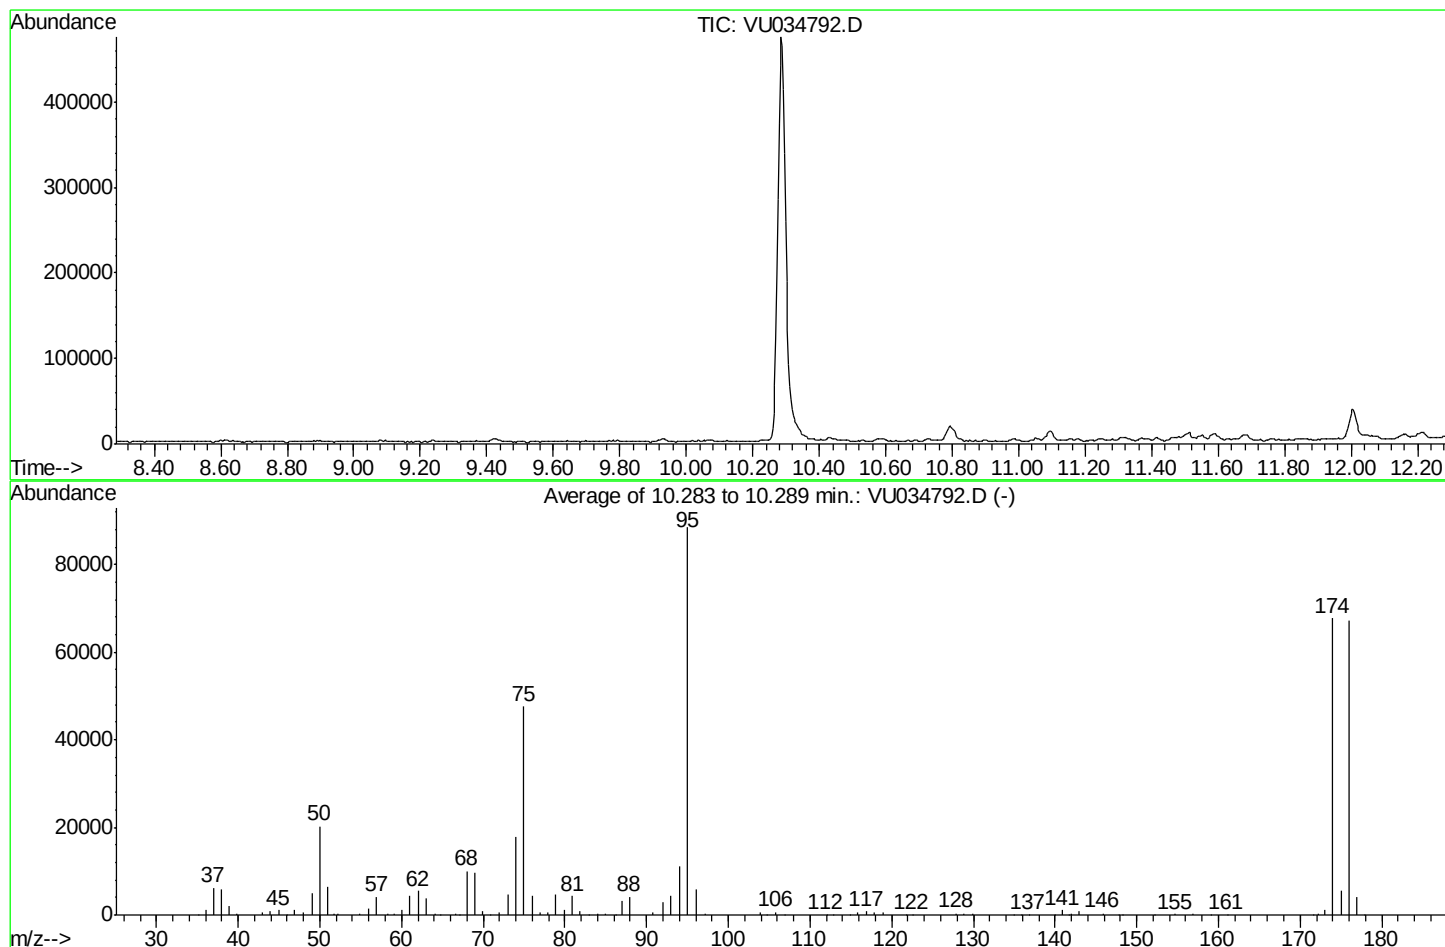

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	20189	PASS
75	95	30	80	53.8	47581	PASS
95	95	100	100	100.0	88488	PASS
96	95	5	9	6.8	5975	PASS
173	174	0.00	2	1.6	1113	PASS
174	95	50	120	76.5	67672	PASS
175	174	5	9	8.2	5532	PASS
176	174	95	101	99.3	67213	PASS
177	176	5	9	6.1	4069	PASS

m/z	Abundance
36.00	1365.0
37.00	6194.0
38.00	6113.0
38.90	2110.0
40.00	608.0
41.00	224.0
41.90	127.0
43.00	780.0
43.90	1708.0
44.90	1345.0
47.00	1302.0
47.90	582.0
49.00	4925.0
50.00	19600.0
51.00	6210.0
51.80	279.0
52.20	227.0
54.90	471.0
56.00	1768.0
57.00	3872.0
58.30	171.0
59.10	152.0
60.00	1350.0
61.00	4446.0
62.00	5262.0
63.00	3577.0
64.10	273.0
66.50	130.0
68.00	9851.0
69.00	9168.0
69.90	1003.0
70.90	228.0
72.00	583.0
73.00	4570.0
74.00	17184.0
75.00	45776.0
76.00	4421.0
77.10	495.0
77.90	472.0
78.90	4754.0
80.00	957.0
80.90	4214.0
81.80	922.0
84.00	181.0
85.00	209.0
86.20	180.0
87.00	3007.0
87.90	4073.0
90.80	400.0
91.90	2829.0
93.00	4525.0
94.00	10921.0
95.00	84016.0
96.00	6027.0
97.10	143.0
103.90	486.0
104.80	144.0
105.90	601.0
106.80	110.0
112.00	106.0
112.90	111.0
114.90	139.0
115.80	419.0
116.90	768.0
117.80	469.0
118.90	504.0
122.50	108.0
127.90	474.0
128.90	180.0
129.90	297.0
136.80	101.0
140.00	112.0
140.90	1043.0
141.70	122.0
142.10	140.0
142.90	726.0
145.90	320.0
148.20	119.0
152.10	106.0
154.70	152.0
156.90	231.0
161.10	140.0
171.60	164.0
172.20	160.0
173.10	1003.0
174.00	64112.0
175.00	5406.0
176.00	64128.0
177.00	3820.0
207.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	1315.0
37.00	6606.0
38.00	6123.0
39.00	2254.0
40.00	546.0
41.00	264.0
42.00	103.0
43.00	868.0
44.00	1955.0
44.90	1378.0
45.90	140.0
47.00	1349.0
47.90	691.0
49.00	5030.0
50.00	20824.0
51.00	6740.0
51.80	288.0
52.20	243.0
54.90	476.0
56.00	1773.0
57.00	4624.0
58.30	205.0
59.10	199.0
60.00	1283.0
61.00	4498.0
62.00	5939.0
63.00	3760.0
64.10	307.0
64.80	107.0
66.50	261.0
68.00	10167.0
69.00	10025.0
70.00	1063.0
70.90	289.0
72.00	624.0
73.00	4767.0
74.00	18664.0
75.00	48928.0
76.00	4541.0
77.00	588.0
77.90	554.0
78.90	5043.0
80.00	1116.0
80.90	4471.0
81.80	916.0
82.90	131.0
83.90	245.0
84.90	181.0
87.00	3184.0
87.90	4212.0
90.80	510.0
91.90	2953.0
93.00	4667.0
94.00	11506.0
95.00	91264.0
96.00	6003.0
97.10	184.0
104.00	459.0
104.70	131.0
105.90	616.0
106.90	117.0
112.90	103.0
115.80	496.0
116.90	835.0
117.90	551.0
118.90	545.0
127.90	440.0
128.90	179.0
129.80	210.0
136.80	155.0
139.90	149.0
140.90	1141.0
142.00	171.0
142.90	743.0
145.90	317.0
147.80	120.0
154.70	252.0
156.80	241.0
161.10	151.0
171.60	106.0
172.20	182.0
173.00	1155.0
174.00	69976.0
175.00	5768.0
176.00	69488.0
177.00	4109.0
207.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.10	103.0
36.00	1138.0
37.00	6436.0
38.00	5524.0
39.00	2129.0
39.90	563.0
41.00	353.0
42.10	136.0
43.00	920.0
44.00	1869.0
45.00	1295.0
45.90	176.0
46.90	1255.0
47.90	808.0
49.00	4737.0
50.00	20144.0
51.00	6312.0
52.10	335.0
54.90	377.0
56.00	1789.0
57.00	4433.0
58.30	234.0
59.10	146.0
60.00	1106.0
61.00	4281.0
62.00	5396.0
63.00	3778.0
64.00	309.0
64.80	183.0
66.60	300.0
67.10	190.0
68.00	9840.0
69.00	10047.0
70.00	1011.0
70.90	255.0
72.00	690.0
73.00	4519.0
74.00	17736.0
75.00	48040.0
76.00	4414.0
76.90	673.0
77.90	459.0
78.90	4603.0
80.00	1093.0
80.90	4222.0
81.90	864.0
82.80	133.0
83.90	262.0
84.90	189.0
87.00	3498.0
87.90	4070.0
90.80	543.0
92.00	3051.0
93.00	4368.0
94.00	11179.0
95.00	90184.0
96.00	5896.0
97.10	188.0
104.00	435.0
105.80	574.0
112.80	133.0
115.90	462.0
117.00	741.0
117.90	507.0
119.00	538.0
121.80	106.0
127.90	414.0
128.90	157.0
129.80	211.0
135.00	113.0
135.90	114.0
136.80	201.0
139.90	128.0
140.90	1182.0
141.90	209.0
142.90	800.0
145.90	305.0
147.80	119.0
154.70	313.0
156.80	191.0
159.00	105.0
161.00	165.0
172.10	141.0
173.00	1181.0
174.00	68928.0
175.00	5422.0
176.00	68024.0
176.90	4278.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

Scan 2847 (10.244 min): VU034792.D
BFB38

m/z	Abundance
37.20	127.0
39.00	192.0
39.90	377.0
40.90	348.0
42.20	467.0
42.90	405.0
43.90	1034.0
45.00	190.0
55.10	133.0
56.00	243.0
56.80	163.0
60.20	123.0
63.70	113.0
71.00	228.0
207.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38