

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092520\
 Data File : VU040280.D
 Acq On : 24 Sep 2020 19:20
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Quant Time: Sep 25 03:13:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR092420WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 25 02:46:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	208445	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	208180	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.81	152	95643	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	64570	4.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.00%
7) Chloroethane-d5	1.92	69	56139	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.00%
11) 1,1-Dichloroethene-d2	2.58	65	33883	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.00%
20) 2-Butanone-d5	4.66	46	250282	49.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.68%
24) Chloroform-d	5.08	84	125999	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.72	65	81276	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.74	84	250717	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.70	67	84170	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.91	98	214217	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	8.19	79	32994	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
46) 2-Hexanone-d5	8.64	63	179896	48.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.90%
56) 1,1,2,2-Tetrachloroethane-	10.75	84	67600	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
66) 1,2-Dichlorobenzene-d4	12.19	152	82605	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	3489	0.171 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092520\
Data File : VU040280.D
Acq On : 24 Sep 2020 19:20
Operator : SY/MD
Sample : VU0924WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Time: Sep 25 03:13:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR092420WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 25 02:46:27 2020
Response via : Initial Calibration

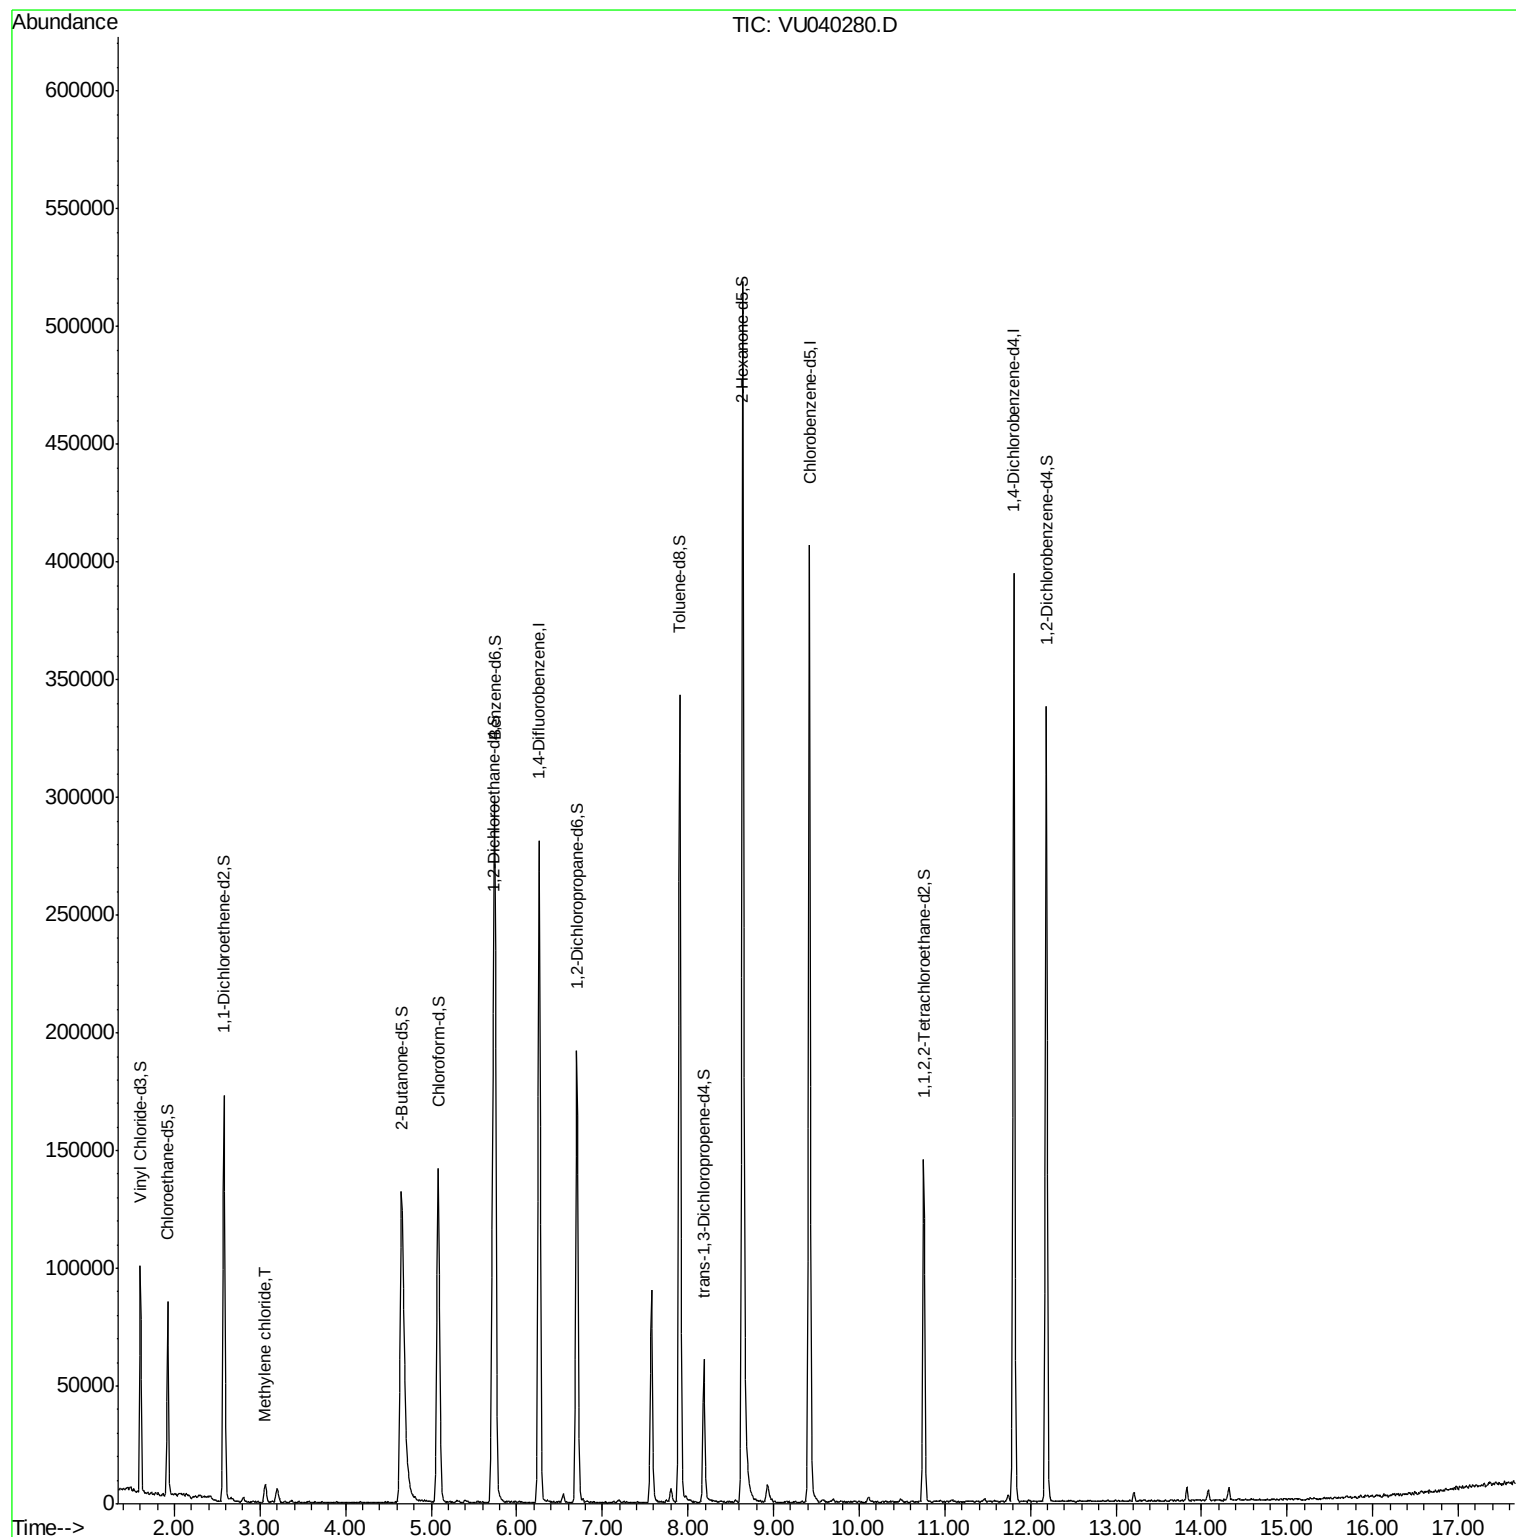

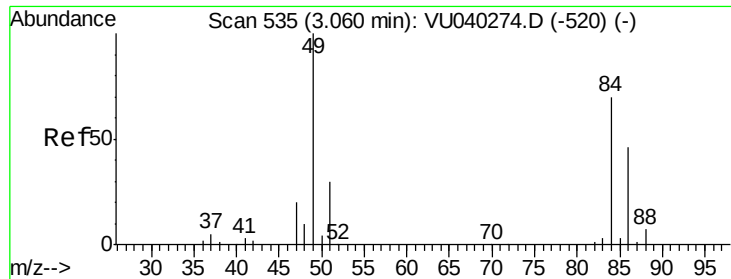

#16
 Methylene chloride
 Concen: 0.171 ug/L
 RT: 3.06 min Scan# 534
 Delta R.T. -0.00 min
 Lab File: VU040280.D
 Acq: 24 Sep 2020 19:20

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Tot Ion: 84 Resp: 3489
 Ion Ratio Lower Upper
 84 100
 86 57.9 45.8 85.0
 49 106.4 100.4 186.4

