


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092520\
 Data File : VU040271.D
 Acq On : 24 Sep 2020 14:54
 Operator : SY/MD
 Sample : BFB01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB2101

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR092420WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Sep 25 02:46:27 2020

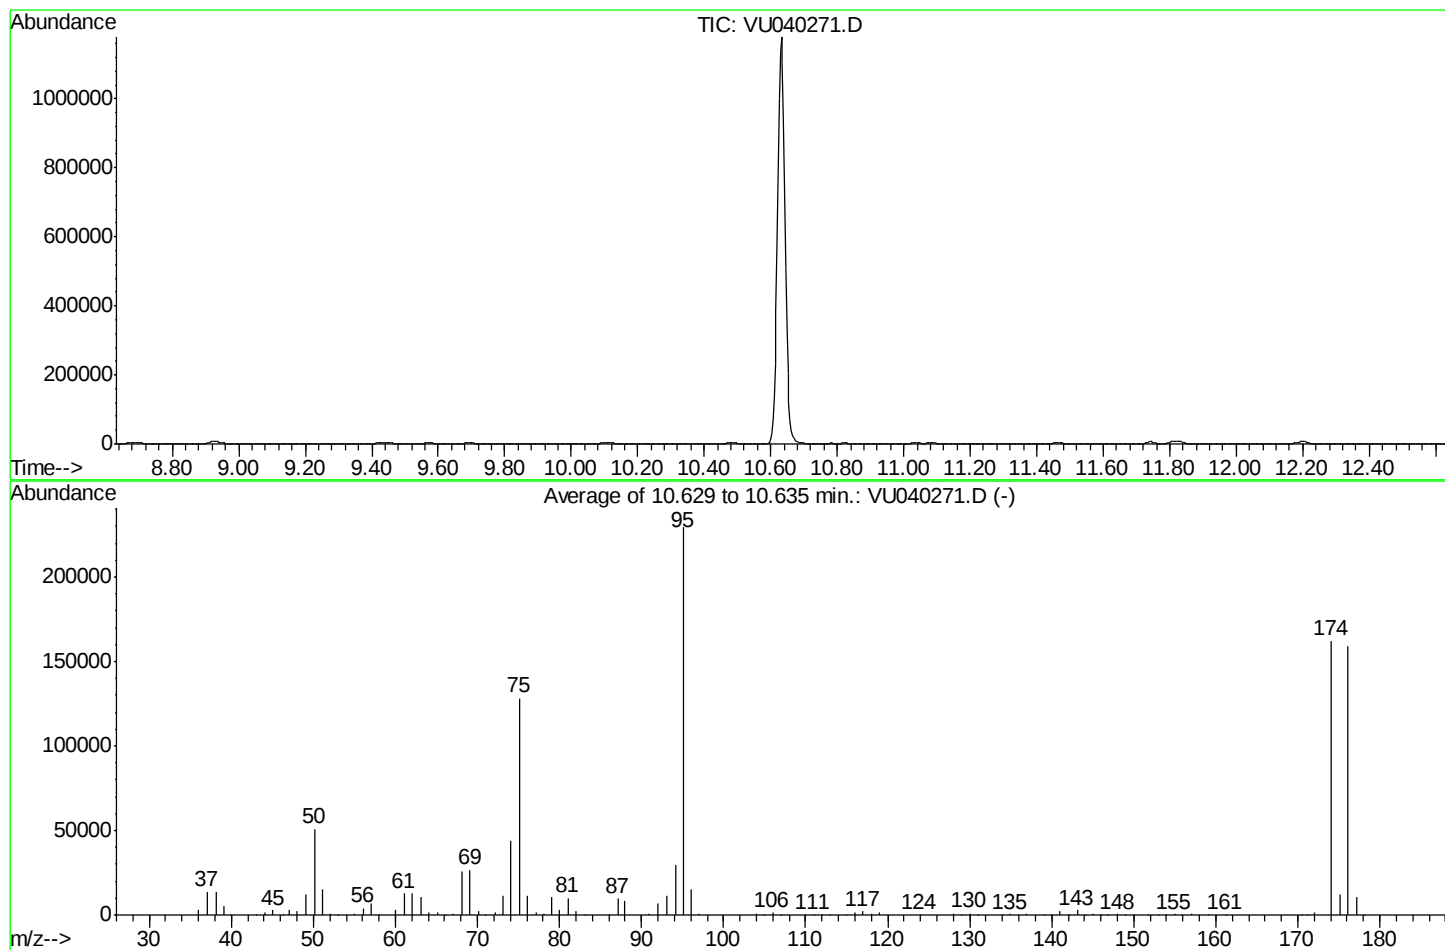

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	50936	PASS
75	95	30	80	56.0	128402	PASS
95	95	100	100	100.0	229482	PASS
96	95	5	9	6.8	15551	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.8	162496	PASS
175	174	5	9	7.4	11963	PASS
176	174	95	101	97.8	158976	PASS
177	176	5	9	6.5	10362	PASS

m/z	Abundance
36.00	2690.0
37.10	14134.0
38.10	13783.0
39.10	5147.0
40.00	390.0
43.00	163.0
44.10	2123.0
45.00	2772.0
46.20	267.0
47.10	2846.0
48.00	2047.0
49.00	12095.0
50.10	52216.0
51.10	15470.0
52.00	788.0
53.00	222.0
55.00	888.0
56.10	4412.0
57.10	7099.0
58.00	345.0
60.00	2557.0
61.10	13135.0
62.10	13044.0
63.10	11202.0
64.10	1397.0
65.10	1360.0
66.10	218.0
67.10	748.0
68.10	26248.0
69.10	27928.0
70.10	2110.0
70.90	199.0
72.10	1794.0
73.10	11544.0
74.10	45656.0
75.10	128416.0
76.10	11218.0
77.10	1360.0
78.10	894.0
79.00	10555.0
80.00	3153.0
81.00	10225.0
81.90	2281.0
83.10	240.0
87.10	9180.0
88.00	7983.0
91.00	1083.0
92.00	6607.0
93.10	11381.0
94.10	29568.0
95.10	230016.0
96.10	15584.0
97.00	525.0
104.00	1137.0
104.90	407.0
106.00	1329.0
107.00	335.0
109.90	150.0
111.00	371.0
111.90	222.0
112.90	379.0
114.90	330.0
116.00	1547.0
117.00	1985.0
118.00	925.0
119.00	1839.0
123.90	119.0
128.00	802.0
128.90	323.0
130.00	956.0
131.00	384.0
135.00	462.0
136.90	445.0
139.10	129.0
140.00	122.0
141.00	2577.0
142.00	353.0
143.10	2944.0
144.00	160.0
145.00	433.0
145.90	360.0
146.80	128.0
148.00	523.0
149.00	100.0
149.90	153.0
153.00	166.0
153.90	170.0
155.00	468.0
157.00	462.0
159.00	226.0
161.20	216.0
170.40	232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

172.10	1485.0
174.10	158528.0
175.10	11708.0
176.10	155264.0
177.10	10133.0
178.10	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

m/z	Abundance
36.00	2976.0
37.10	14157.0
38.10	14114.0
39.10	5189.0
40.00	331.0
43.00	241.0
44.10	2074.0
45.10	2863.0
46.20	316.0
47.10	3124.0
48.00	2019.0
49.00	12207.0
50.10	52344.0
51.10	15955.0
52.00	776.0
53.00	197.0
55.00	849.0
56.10	4288.0
57.10	7338.0
58.00	374.0
60.00	2848.0
61.10	13167.0
62.10	12873.0
63.10	10791.0
64.10	1296.0
65.10	1241.0
66.10	233.0
67.10	737.0
68.10	26888.0
69.10	27560.0
70.10	2094.0
70.90	194.0
72.10	1770.0
73.10	11958.0
74.10	45376.0
75.10	132864.0
76.10	11657.0
77.10	1473.0
78.00	826.0
79.00	10934.0
80.00	3104.0
81.00	10530.0
82.00	2267.0
83.00	271.0
86.10	339.0
87.10	9822.0
88.00	8254.0
90.90	950.0
92.00	6891.0
93.10	11552.0
94.10	30608.0
95.10	236928.0
96.10	16190.0
97.00	474.0
104.00	1165.0
104.90	354.0
106.00	1288.0
107.00	271.0
109.90	161.0
111.00	405.0
112.00	294.0
112.90	337.0
115.00	335.0
116.00	1499.0
117.00	2178.0
118.00	965.0
119.00	1950.0
123.90	153.0
128.00	785.0
128.90	294.0
130.00	906.0
131.00	412.0
134.00	108.0
135.00	459.0
137.00	443.0
139.00	167.0
140.00	179.0
141.00	2585.0
142.00	436.0
143.10	3079.0
144.10	125.0
145.00	412.0
146.00	413.0
146.80	128.0
148.00	485.0
150.00	174.0
153.00	161.0
153.90	189.0
155.00	493.0
157.00	477.0
159.00	216.0
161.20	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

170.40	223.0
171.10	312.0
172.10	1538.0
174.10	167616.0
175.10	12302.0
176.10	164480.0
177.10	10781.0
178.10	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

m/z	Abundance
36.00	2656.0
37.00	13242.0
38.10	12714.0
39.10	4947.0
40.00	361.0
43.00	216.0
44.10	1749.0
45.10	2564.0
46.20	358.0
47.00	2980.0
48.00	1891.0
49.10	11094.0
50.10	48248.0
51.10	14874.0
52.00	708.0
53.00	192.0
55.00	727.0
56.10	3799.0
57.00	6956.0
58.00	352.0
60.00	2811.0
61.10	12279.0
62.10	11847.0
63.10	9580.0
64.10	1109.0
65.10	1197.0
66.00	252.0
67.00	673.0
68.10	24320.0
69.10	24784.0
70.10	1883.0
71.00	133.0
72.10	1654.0
73.10	10921.0
74.10	41584.0
75.10	123928.0
76.10	11159.0
77.10	1454.0
78.00	801.0
79.00	10227.0
80.00	2801.0
81.00	9807.0
82.00	2182.0
83.00	247.0
86.00	301.0
87.10	9595.0
88.00	7793.0
90.90	856.0
92.00	6808.0
93.10	10383.0
94.10	28352.0
95.10	221504.0
96.10	14879.0
97.00	325.0
104.00	1130.0
104.90	290.0
106.00	1104.0
107.00	200.0
110.00	155.0
111.00	426.0
112.00	275.0
112.90	235.0
115.00	329.0
116.00	1237.0
117.00	2085.0
118.00	953.0
119.00	1704.0
123.90	197.0
128.00	756.0
129.00	288.0
130.00	738.0
131.00	401.0
134.90	510.0
137.00	386.0
139.00	158.0
139.90	171.0
141.00	2520.0
142.00	391.0
143.10	2831.0
145.00	509.0
146.00	369.0
146.80	105.0
148.10	498.0
148.90	104.0
150.00	240.0
151.80	114.0
153.00	144.0
153.90	183.0
155.00	453.0
155.80	103.0
157.10	423.0
159.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

161.20	255.0
170.40	133.0
171.10	256.0
172.10	1479.0
174.10	161344.0
175.10	11879.0
176.10	157184.0
177.10	10172.0
178.10	317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101

Scan 2874 (10.581 min): VU040271.D
BFB01

m/z	Abundance
39.90	139.0
44.00	627.0

Instrument :
MSVOA_U
ClientSampleId :
BFB2101