

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
 Data File : VU044882.D
 Acq On : 26 Sep 2021 09:46
 Operator : SY/MD
 Sample : M3893-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP-1

Quant Time: Sep 27 03:21:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 25 09:30:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.379	168	205067	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	362104	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	331654	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	154196	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	163626	45.719	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.440%	
35) Dibromofluoromethane	5.295	113	114516	46.100	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.200%	
50) Toluene-d8	7.903	98	452807	48.264	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.520%	
62) 4-Bromofluorobenzene	10.636	95	161193	46.258	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.520%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	1056	0.283	ug/l	92
4) Vinyl Chloride	1.607	62	14352	4.126	ug/l	98
5) Bromomethane	1.858	94	227	Below Cal		94
6) Chloroethane	1.932	64	3083	0.957	ug/l	91
11) Tert butyl alcohol	3.189	59	1425	1.364	ug/l #	72
12) 1,1-Dichloroethene	2.584	96	38148	15.450	ug/l	95
16) Acetone	2.636	43	4501	2.230	ug/l	98
17) Carbon Disulfide	2.800	76	2254	0.325	ug/l	98
24) 1,1-Dichloroethane	3.874	63	61998	11.280	ug/l	99
27) cis-1,2-Dichloroethene	4.674	96	7604	2.365	ug/l	92
31) Cyclohexane	5.379	56	5827	1.134	ug/l #	6
32) 1,1,1-Trichloroethane	5.324	97	4563	1.022	ug/l #	52
36) 1,1-Dichloropropene	5.379	75	19274	5.017	ug/l #	50
38) Carbon Tetrachloride	5.379	117	21552	6.275	ug/l #	15
39) Methylcyclohexane	6.768	83	1580	0.364	ug/l #	83
40) Benzene	5.777	78	2372	0.202	ug/l	92
42) 1,2-Dichloroethane	5.800	62	6193	1.344	ug/l	88
43) Isopropyl Acetate	5.838	43	14521	1.841	ug/l #	61
44) Trichloroethene	6.546	130	1089	0.387	ug/l	86
49) 1,4-Dioxane	6.977	88	25805	271.234	ug/l	93
51) 4-Methyl-2-Pentanone	7.899	43	2158	0.384	ug/l #	1
52) Toluene	7.973	92	4778	0.682	ug/l	99
56) Ethyl methacrylate	8.243	69	20	1.889	ug/l #	1
58) 2-Chloroethyl Vinyl ether	7.253	63	551	23.675	ug/l #	49
68) m/p-Xylenes	9.697	106	2711	0.577	ug/l	93
69) o-Xylene	10.102	106	944	0.208	ug/l	93
76) 1,2,3-Trichloropropane	10.636	75	86841	18.598	ug/l #	41
81) trans-1,4-Dichloro-2-b...	10.636	75	86841	60.248	ug/l #	11
86) p-Isopropyltoluene	12.012	119	2469	0.262	ug/l	98
89) n-Butylbenzene	12.185	91	717	1.348	ug/l #	1
95) Naphthalene	14.092	128	4019	1.276	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
Data File : VU044882.D
Acq On : 26 Sep 2021 09:46
Operator : SY/MD
Sample : M3893-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP-1

Quant Time: Sep 27 03:21:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 25 09:30:46 2021
Response via : Initial Calibration




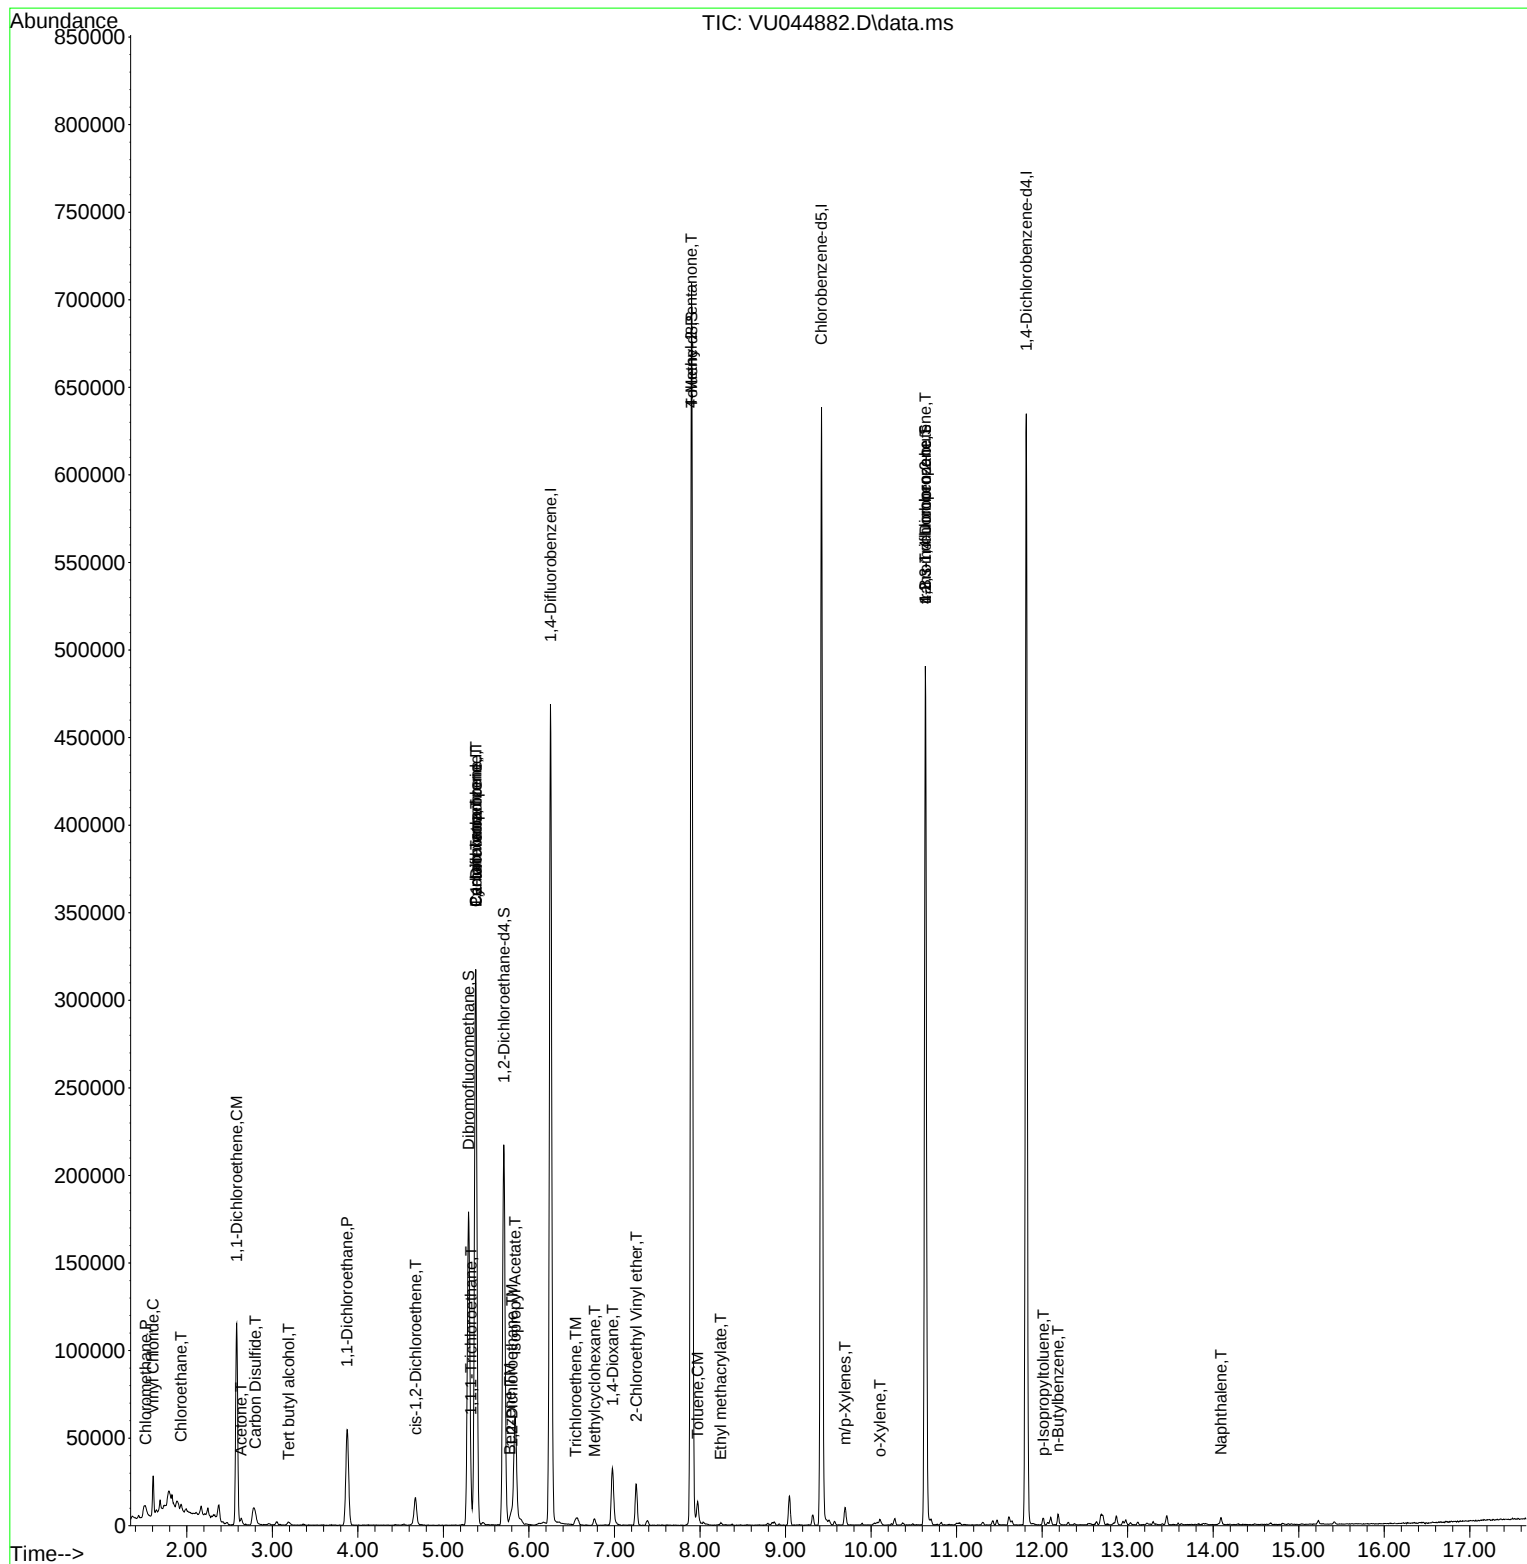




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 1256
Delta R.T. 0.001 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion:168 Resp: 205067
Ion Ratio Lower Upper
168 100
99 64.2 51.4 77.0

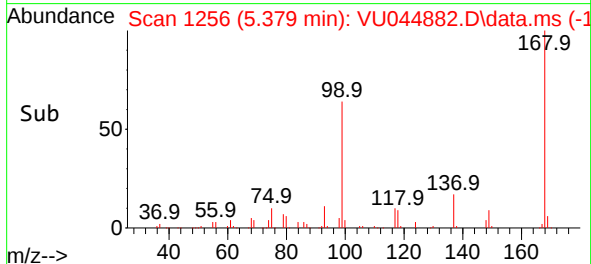

#3
Chloromethane
Concen: 0.283 ug/l
RT: 1.520 min Scan# 56
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 50 Resp: 1056
Ion Ratio Lower Upper
50 100
52 37.4 26.3 39.5


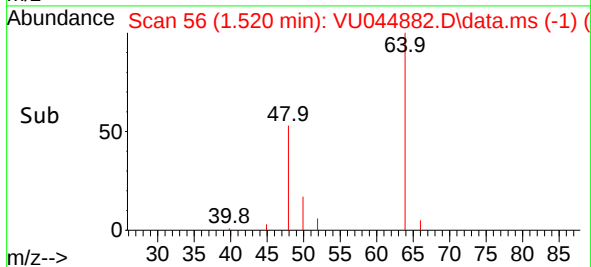

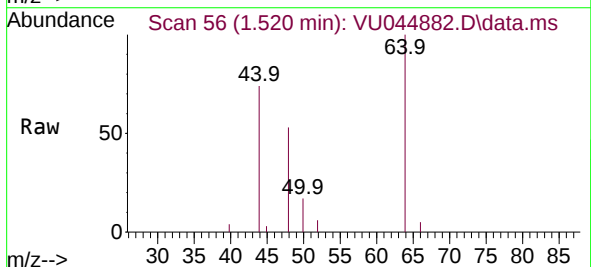


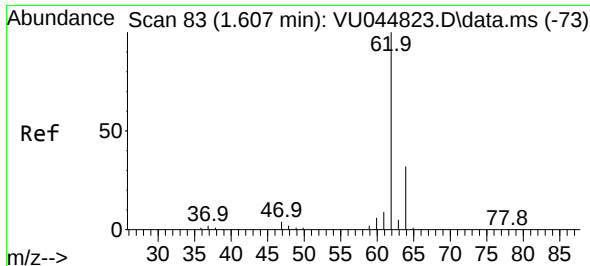

#4
 Vinyl Chloride
 Concen: 4.126 ug/l
 RT: 1.607 min Scan# 83
 Delta R.T. -0.000 min
 Lab File: VU044882.D
 Acq: 26 Sep 2021 09:46




Instrument :
 MSVOA_U
 ClientSampled :
 DUP-1


Tgt Ion: 62 Resp: 14352
 Ion Ratio Lower Upper
 62 100
 64 31.1 25.6 38.4

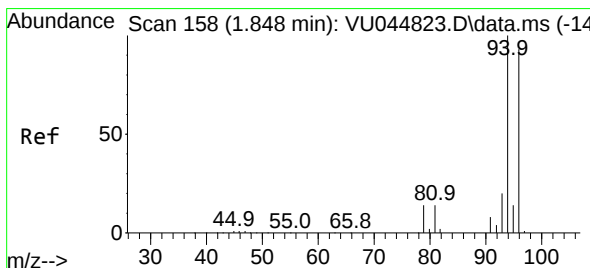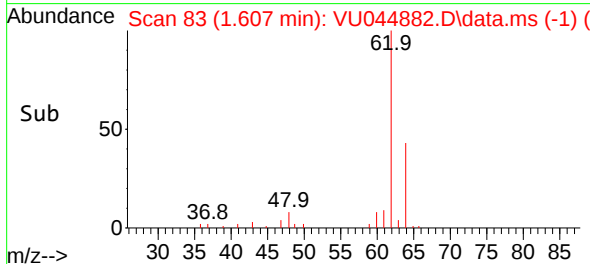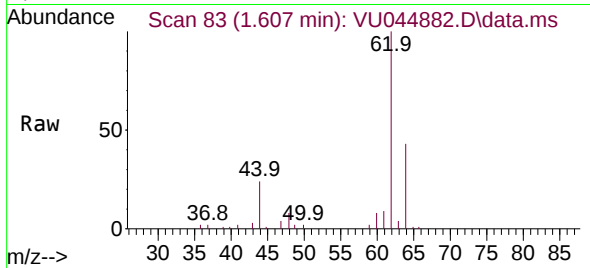

#5
 Bromomethane
 Concen: Below Cal
 RT: 1.858 min Scan# 161
 Delta R.T. 0.010 min
 Lab File: VU044882.D
 Acq: 26 Sep 2021 09:46

Tgt Ion: 94 Resp: 227
 Ion Ratio Lower Upper
 94 100
 96 98.5 74.5 111.7


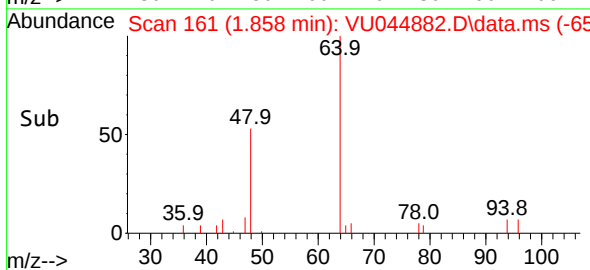

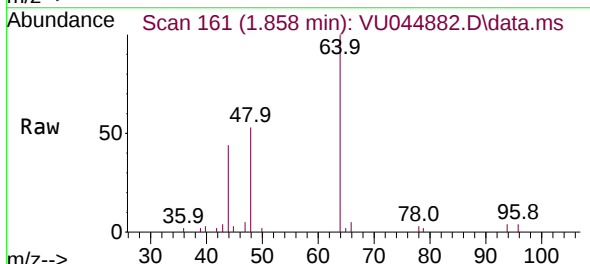




#6
Chloroethane
Concen: 0.957 ug/l
RT: 1.932 min Scan# 184
Delta R.T. 0.004 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 64 Resp: 3083
Ion Ratio Lower Upper
64 100
66 27.0 25.8 38.8

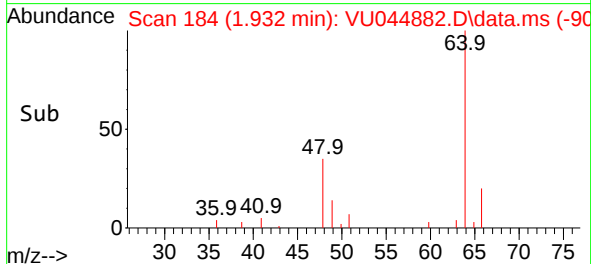

#11
Tert butyl alcohol
Concen: 1.364 ug/l
RT: 3.189 min Scan# 575
Delta R.T. -0.016 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 59 Resp: 1425
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


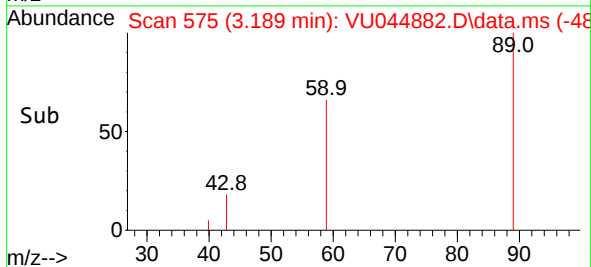

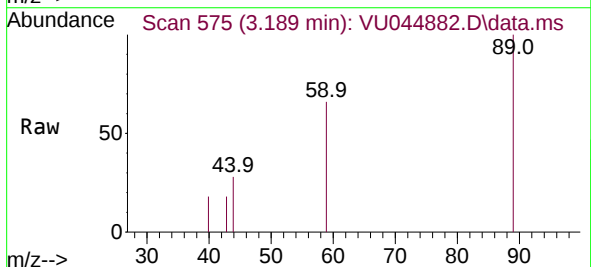




#12
1,1-Dichloroethene
Concen: 15.450 ug/l
RT: 2.584 min Scan# 387
Delta R.T. 0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampleId :
DUP-1


Tgt Ion: 96 Resp: 38148
Ion Ratio Lower Upper
96 100
61 172.5 145.4 218.0
98 63.2 50.9 76.3

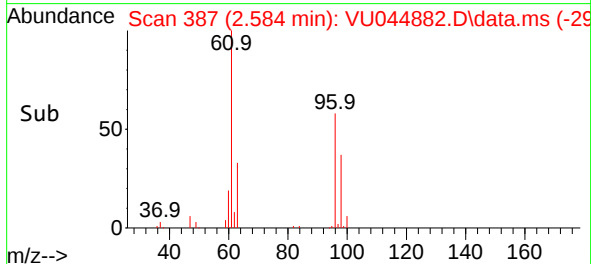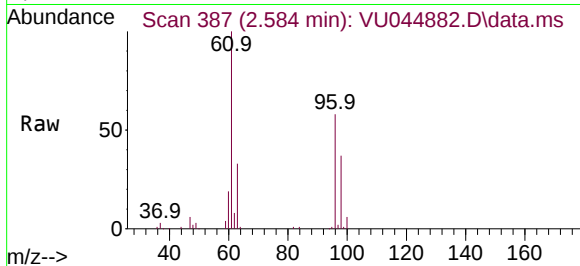

#16
Acetone
Concen: 2.230 ug/l
RT: 2.636 min Scan# 403
Delta R.T. 0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 43 Resp: 4501
Ion Ratio Lower Upper
43 100
58 32.8 25.2 37.8


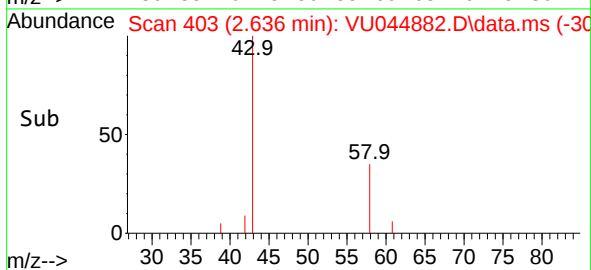

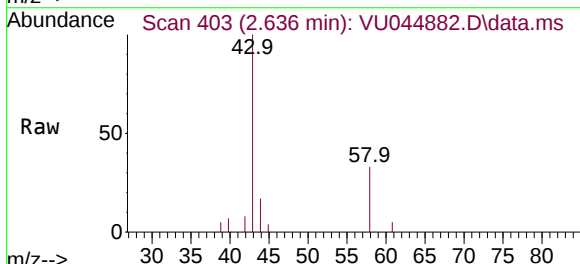




#17
Carbon Disulfide
Concen: 0.325 ug/l
RT: 2.800 min Scan# 454
Delta R.T. 0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 76 Resp: 2254
Ion Ratio Lower Upper
76 100
78 9.8 7.4 11.0

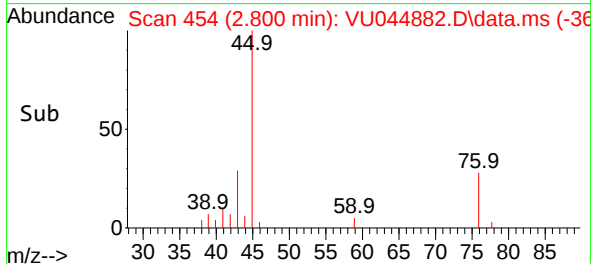

#24
1,1-Dichloroethane
Concen: 11.280 ug/l
RT: 3.874 min Scan# 788
Delta R.T. -0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 63 Resp: 61998
Ion Ratio Lower Upper
63 100
98 6.5 3.5 10.4
100 4.9 2.1 6.3

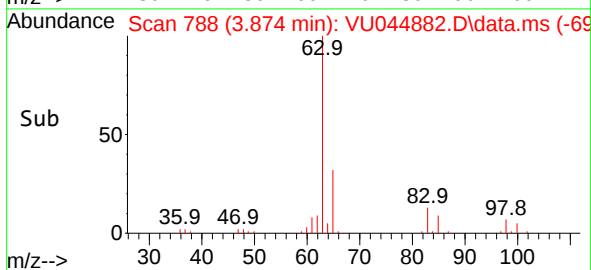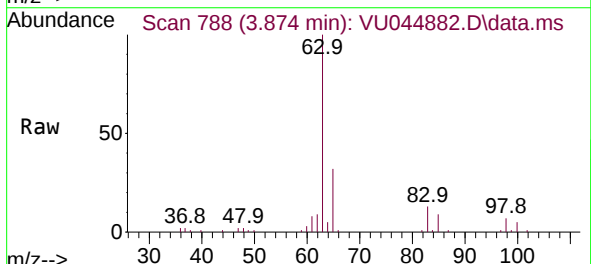







#27

cis-1,2-Dichloroethene
Concen: 2.365 ug/l
RT: 4.674 min Scan# 1037
Delta R.T. 0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Instrument :
MSVOA_U
ClientSampled :
DUP-1




Tgt Ion:	96	Resp:	7604
Ion	Ratio	Lower	Upper
96	100		
61	144.8	0.0	313.4
98	66.4	0.0	127.0

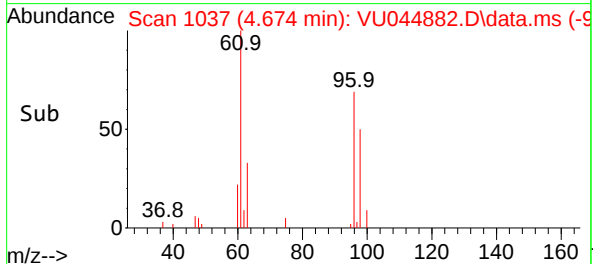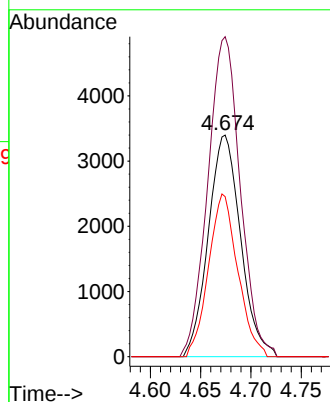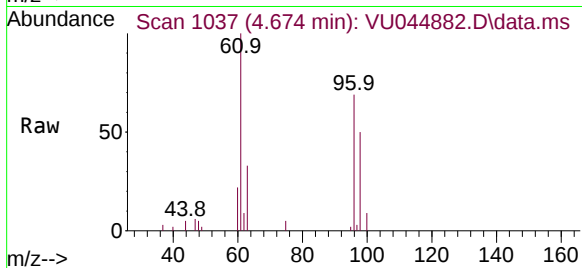


#31

Cyclohexane
Concen: 1.134 ug/l
RT: 5.379 min Scan# 1256
Delta R.T. -0.016 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion:	56	Resp:	5827
Ion	Ratio	Lower	Upper
56	100		
69	158.4	25.2	37.8#
84	121.4	66.4	99.6#

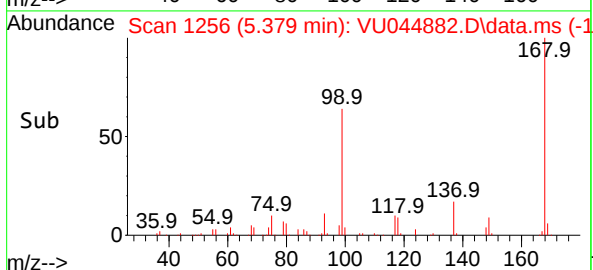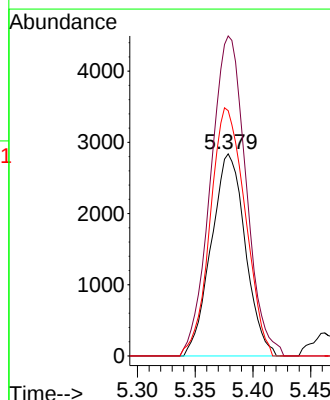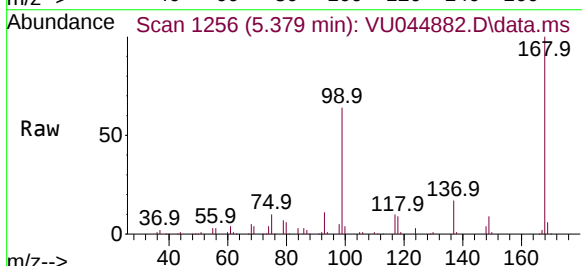



#32

1,1,1-Trichloroethane

Concen: 1.022 ug/l

RT: 5.324 min Scan# 1239

Delta R.T. 0.003 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46

Tgt Ion: 97 Resp: 4563

Ion Ratio Lower Upper

97 100

99 0.0 50.9 76.3#





61 55.2 40.7 61.1

Instrument :

MSVOA_U

ClientSampleId :

DUP-1



#33

1,2-Dichloroethane-d4

Concen: 45.719 ug/l

RT: 5.706 min Scan# 1358

Delta R.T. 0.000 min

Lab File: VU044882.D




Acq: 26 Sep 2021 09:46


Tgt Ion: 65 Resp: 163626

Ion Ratio Lower Upper

65 100

67 52.0 0.0 104.8

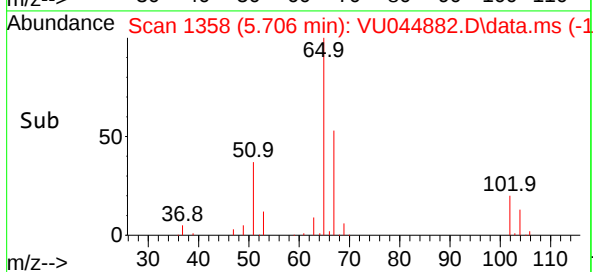



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1528

Delta R.T. 0.000 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46





Tgt Ion:114 Resp: 362104

Ion Ratio Lower Upper

114 100

63 23.1 0.0 47.8

88 17.4 0.0 32.8

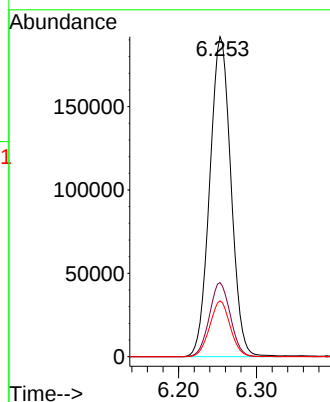

#35

Dibromofluoromethane

Concen: 46.100 ug/l

RT: 5.295 min Scan# 1230

Delta R.T. 0.000 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46




Tgt Ion:113 Resp: 114516


Ion Ratio Lower Upper

113 100

111 101.4 84.1 126.1

192 17.9 14.8 22.2

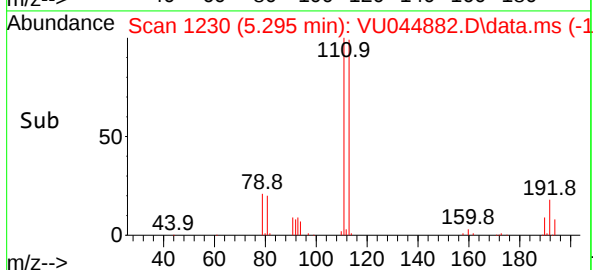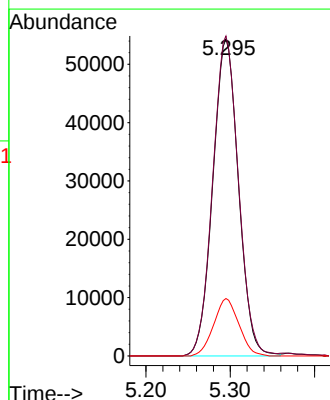







#36

1,1-Dichloropropene
Concen: 5.017 ug/l
RT: 5.379 min Scan# 1256
Delta R.T. -0.151 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Instrument :
MSVOA_U
ClientSampled :
DUP-1




Tgt Ion: 75 Resp: 19274
Ion Ratio Lower Upper
75 100
110 7.5 16.3 48.9#
77 0.0 25.0 37.4#

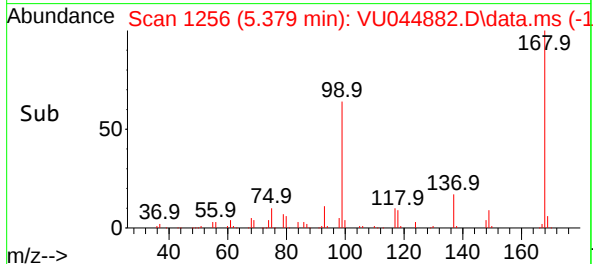


#38

Carbon Tetrachloride
Concen: 6.275 ug/l
RT: 5.379 min Scan# 1256
Delta R.T. -0.151 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 117 Resp: 21552
Ion Ratio Lower Upper
117 100
119 4.9 77.4 116.2#
121 0.0 24.5 36.7#

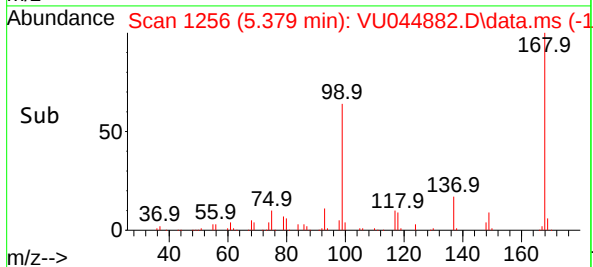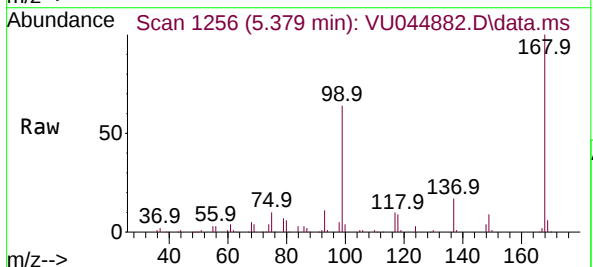



#39

Methylcyclohexane

Concen: 0.364 ug/l

RT: 6.768 min Scan# 1688

Delta R.T. 0.000 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46





Instrument :

MSVOA_U

ClientSampled :

DUP-1

Tgt Ion:	83	Resp:	1580
Ion	Ratio	Lower	Upper
83	100		
55	60.2	66.2	99.4#
98	48.7	37.5	56.3

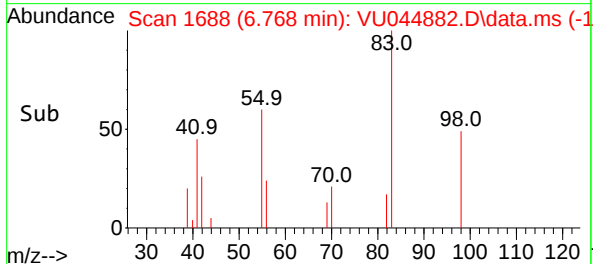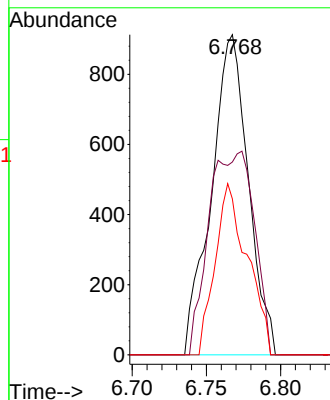

#40

Benzene

Concen: 0.202 ug/l




RT: 5.777 min Scan# 1380


Delta R.T. 0.000 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46

Tgt Ion:	78	Resp:	2372
Ion	Ratio	Lower	Upper
78	100		
77	27.9	19.1	28.7

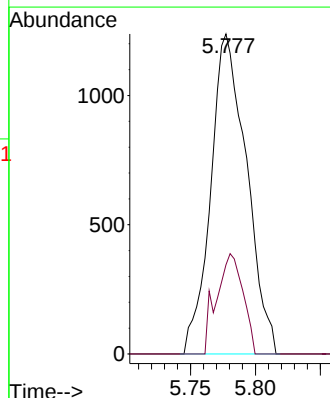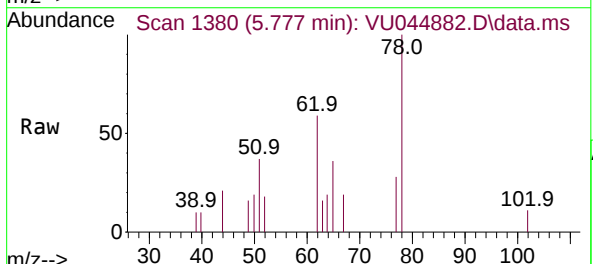



#42

1,2-Dichloroethane

Concen: 1.344 ug/l

RT: 5.800 min Scan# 1387

Delta R.T. 0.000 min

Lab File: VU044882.D





Acq: 26 Sep 2021 09:46

Tgt Ion: 62 Resp: 6193

Ion Ratio Lower Upper

62 100

98 4.7 0.0 17.8

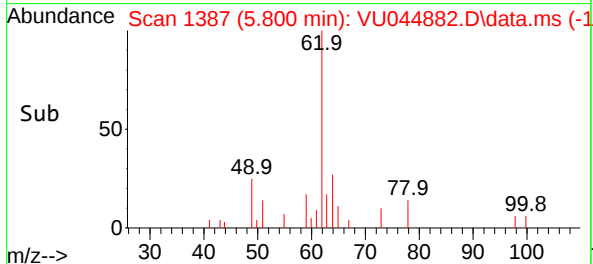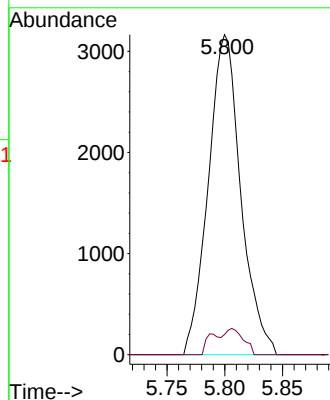

#43

Isopropyl Acetate

Concen: 1.841 ug/l

RT: 5.838 min Scan# 1399

Delta R.T. -0.077 min

Lab File: VU044882.D

Acq: 26 Sep 2021 09:46




Tgt Ion: 43 Resp: 14521


Ion Ratio Lower Upper

43 100

61 0.0 16.1 24.1#

87 0.0 10.3 15.5#


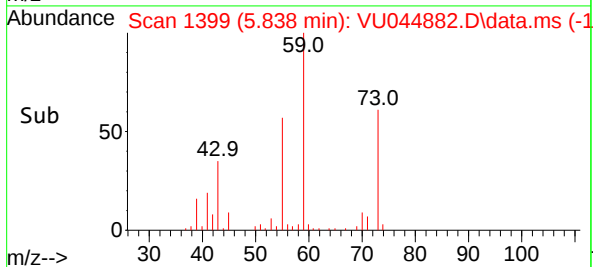
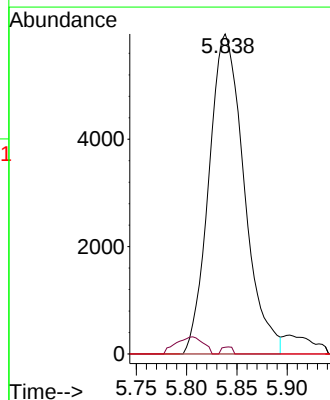
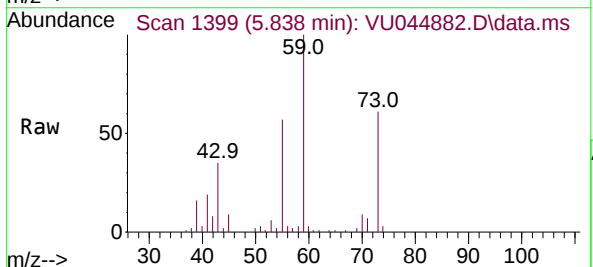




#44
Trichloroethene
Concen: 0.387 ug/l
RT: 6.546 min Scan# 1619
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion:130 Resp: 1089
Ion Ratio Lower Upper
130 100
95 119.3 0.0 209.0

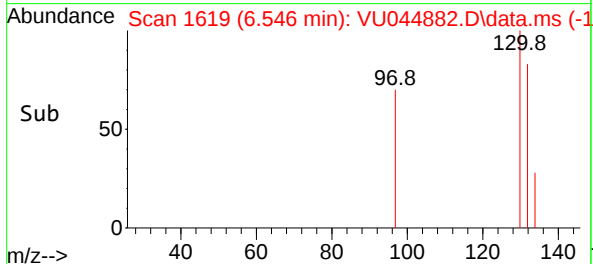

#49
1,4-Dioxane
Concen: 271.234 ug/l
RT: 6.977 min Scan# 1753
Delta R.T. -0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 88 Resp: 25805
Ion Ratio Lower Upper
88 100
43 29.9 25.8 38.6
58 69.8 61.3 91.9


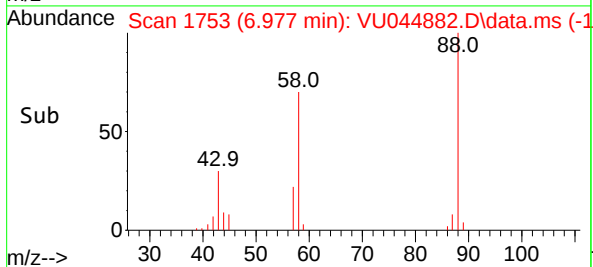

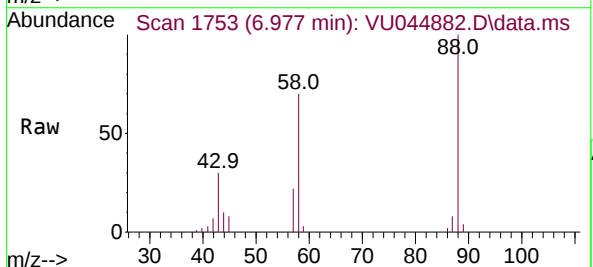




#50
Toluene-d8
Concen: 48.264 ug/l
RT: 7.903 min Scan# 2041
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 98 Resp: 452807
Ion Ratio Lower Upper
98 100
100 65.7 52.5 78.7

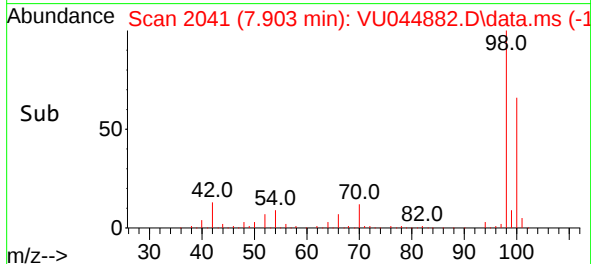

#51
4-Methyl-2-Pentanone
Concen: 0.384 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. 0.103 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 43 Resp: 2158
Ion Ratio Lower Upper
43 100
58 189.6 32.4 48.6#


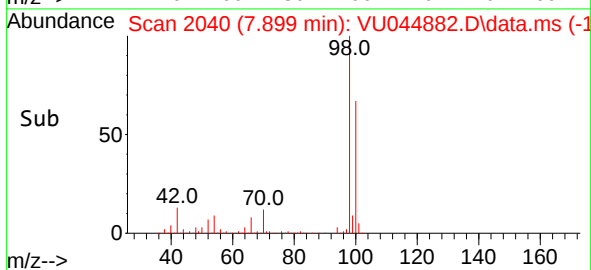

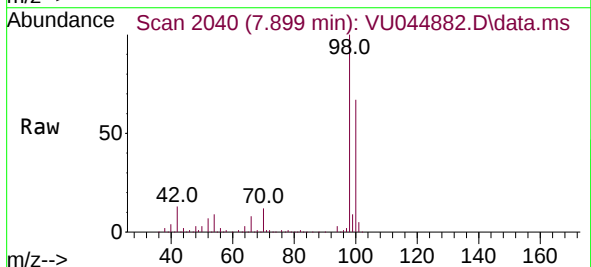




#52
Toluene
Concen: 0.682 ug/l
RT: 7.973 min Scan# 2063
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 92 Resp: 4778
Ion Ratio Lower Upper
92 100
91 170.0 136.9 205.3

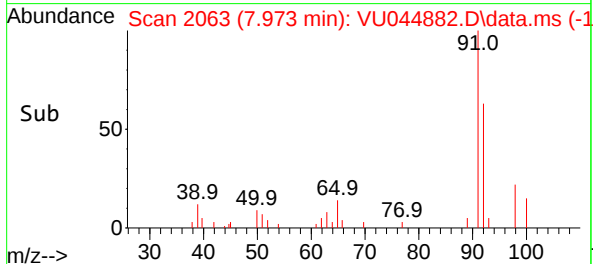

#56
Ethyl methacrylate
Concen: 1.889 ug/l
RT: 8.243 min Scan# 2147
Delta R.T. -0.094 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 69 Resp: 20
Ion Ratio Lower Upper
69 100
41 375.0 53.5 80.3#
39 430.0 31.1 46.7#


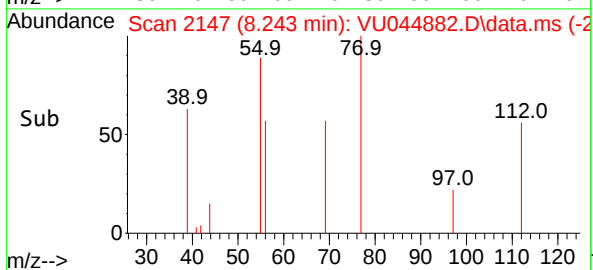

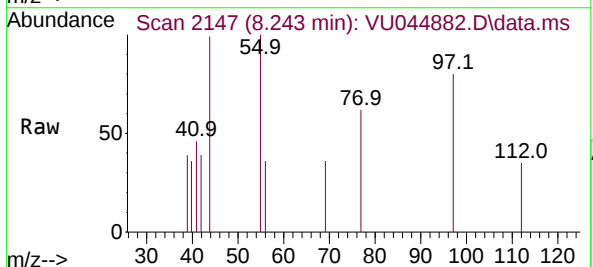




#58
2-Chloroethyl Vinyl ether
Concen: 23.675 ug/l
RT: 7.253 min Scan# 1839
Delta R.T. -0.215 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 63 Resp: 551
Ion Ratio Lower Upper
63 100
106 0.0 20.5 30.7#

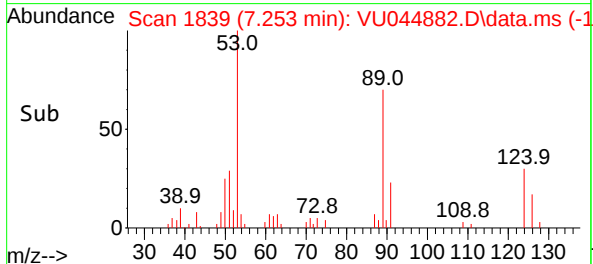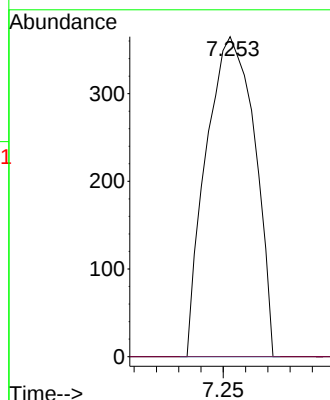

#62
4-Bromofluorobenzene
Concen: 46.258 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 95 Resp: 161193
Ion Ratio Lower Upper
95 100
174 70.8 0.0 146.6
176 68.3 0.0 141.2


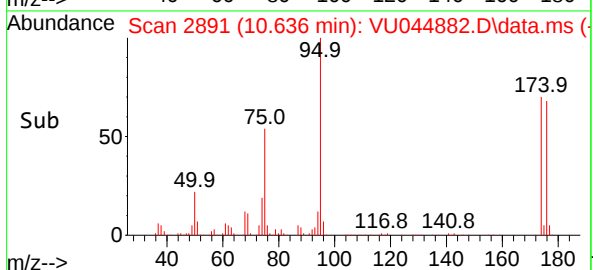
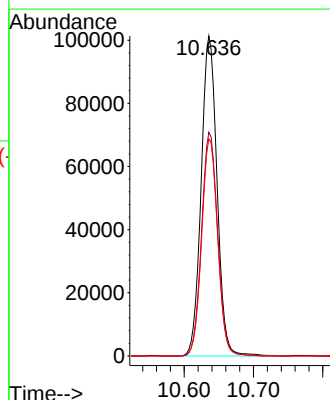
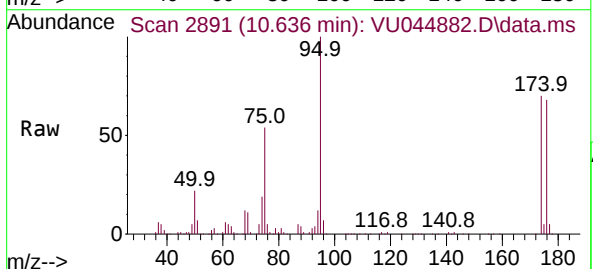




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion:117 Resp: 331654
Ion Ratio Lower Upper
117 100
82 60.1 47.8 71.8
119 31.6 25.8 38.6

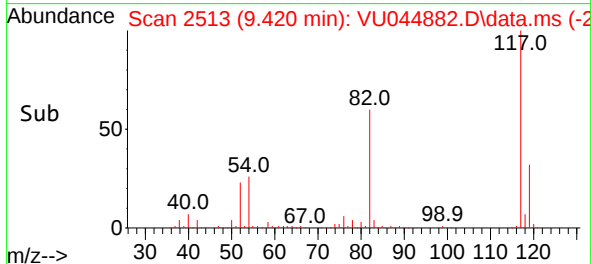

#68
m/p-Xylenes
Concen: 0.577 ug/l
RT: 9.697 min Scan# 2599
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion:106 Resp: 2711
Ion Ratio Lower Upper
106 100
91 195.1 164.2 246.2


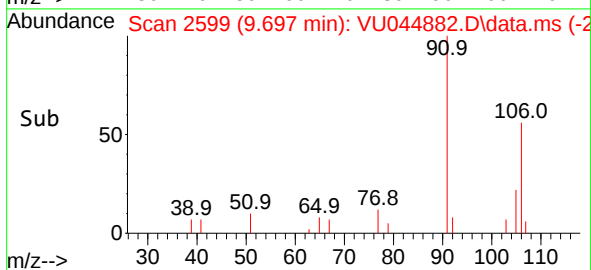

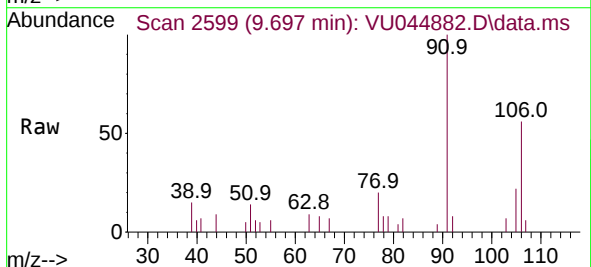




#69
o-Xylene
Concen: 0.208 ug/l
RT: 10.102 min Scan# 2725
Delta R.T. -0.003 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion:106 Resp: 944
Ion Ratio Lower Upper
106 100
91 228.8 108.9 326.7

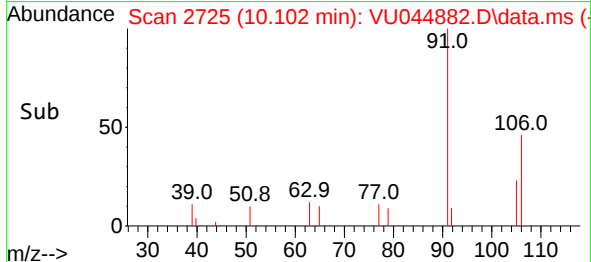

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.816 min Scan# 3258
Delta R.T. 0.000 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion:152 Resp: 154196
Ion Ratio Lower Upper
152 100
115 60.7 43.5 130.7
150 156.7 0.0 350.0


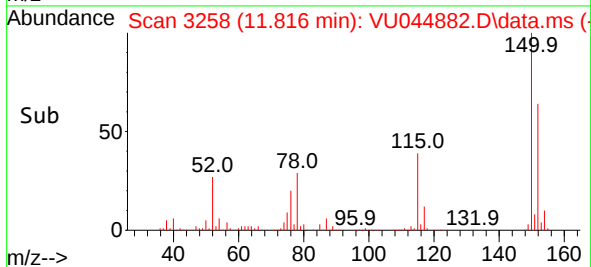

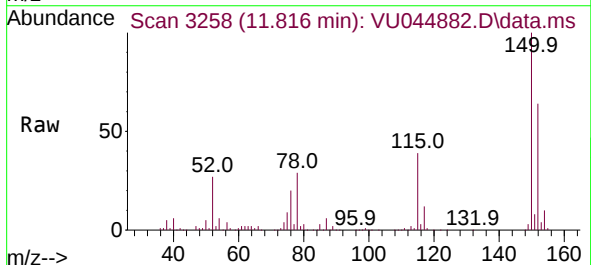




#76
1,2,3-Trichloropropane
Concen: 18.598 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. -0.193 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion: 75 Resp: 86841
Ion Ratio Lower Upper
75 100
77 1.5 17.9 53.7#

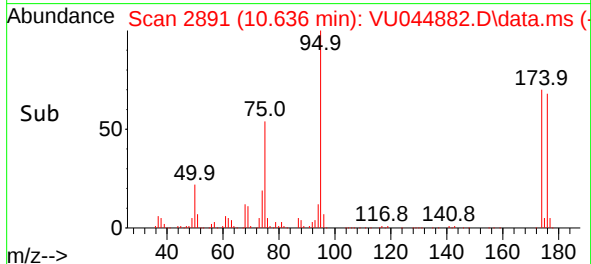

#81
trans-1,4-Dichloro-2-butene
Concen: 60.248 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.084 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46

Tgt Ion: 75 Resp: 86841
Ion Ratio Lower Upper
75 100
53 0.8 82.0 123.0#
89 3.9 34.2 51.4#


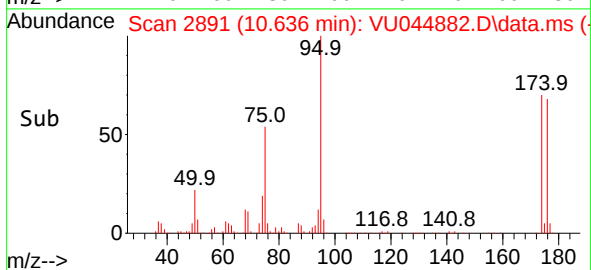

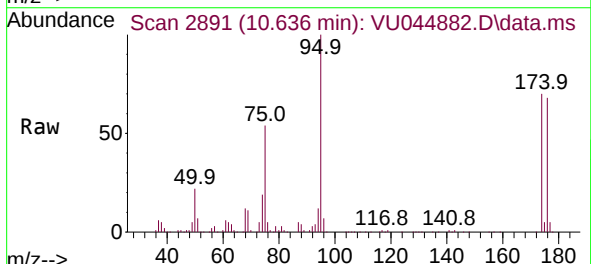


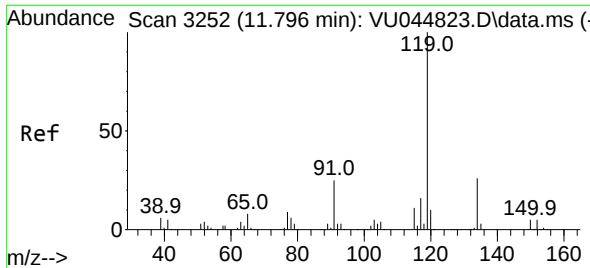

#86
p-Isopropyltoluene
Concen: 0.262 ug/l
RT: 12.012 min Scan# 3319
Delta R.T. 0.215 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46




Instrument :
MSVOA_U
ClientSampled :
DUP-1


Tgt Ion:	119	Resp:	2469
Ion	Ratio	Lower	Upper
119	100		
134	26.1	12.8	38.3
91	25.7	12.2	36.6

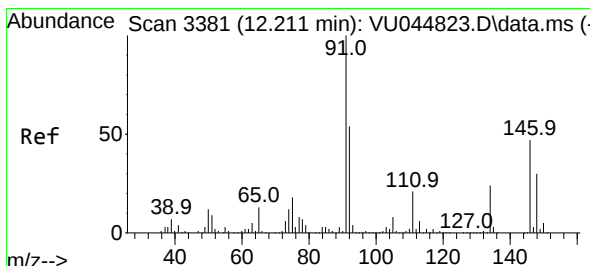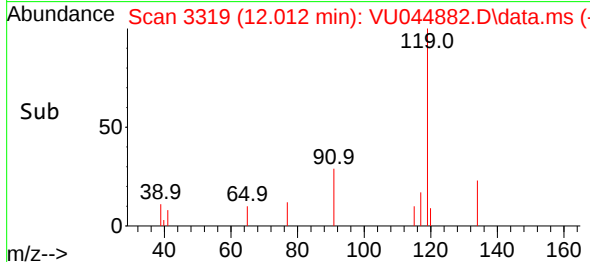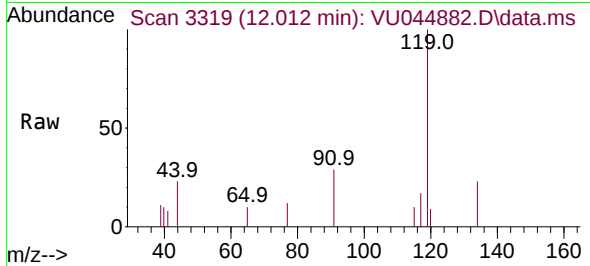

#89
n-Butylbenzene
Concen: 1.348 ug/l
RT: 12.185 min Scan# 3373
Delta R.T. -0.026 min
Lab File: VU044882.D
Acq: 26 Sep 2021 09:46


Tgt Ion:	91	Resp:	717
Ion	Ratio	Lower	Upper
91	100		
92	0.0	26.8	80.4#
134	110.9	11.8	35.4#

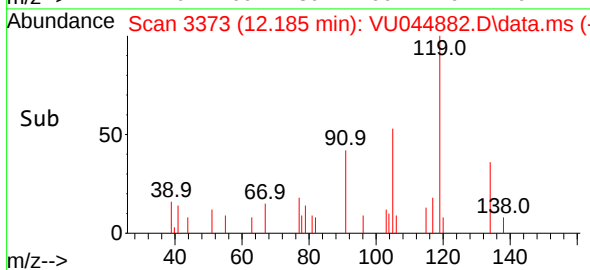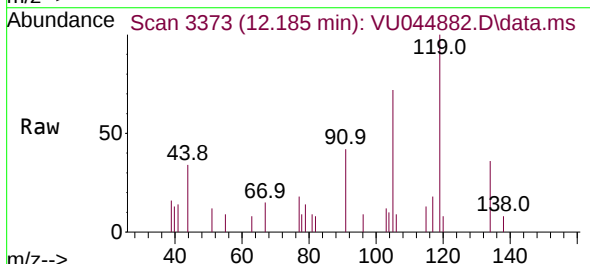

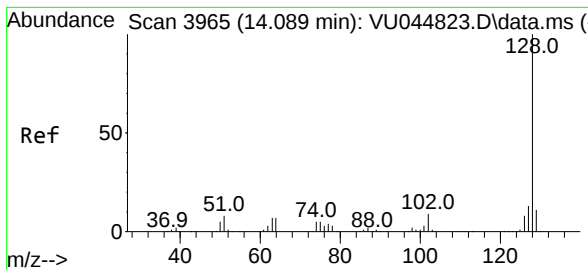

#95
 Naphthalene
 Concen: 1.276 ug/l
 RT: 14.092 min Scan# 3966
 Delta R.T. 0.003 min
 Lab File: VU044882.D
 Acq: 26 Sep 2021 09:46

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP-1

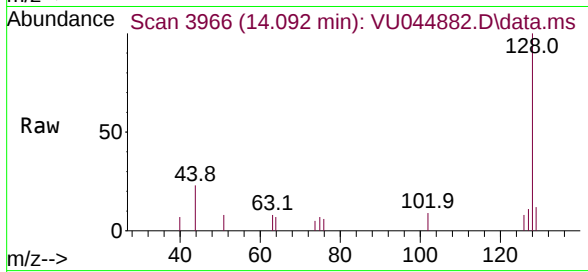

Tgt Ion	Ratio	Lower	Upper
128	100		
127	9.5	10.4	15.6#
129	9.1	8.6	13.0

