


Bromomethane

Response Ratio

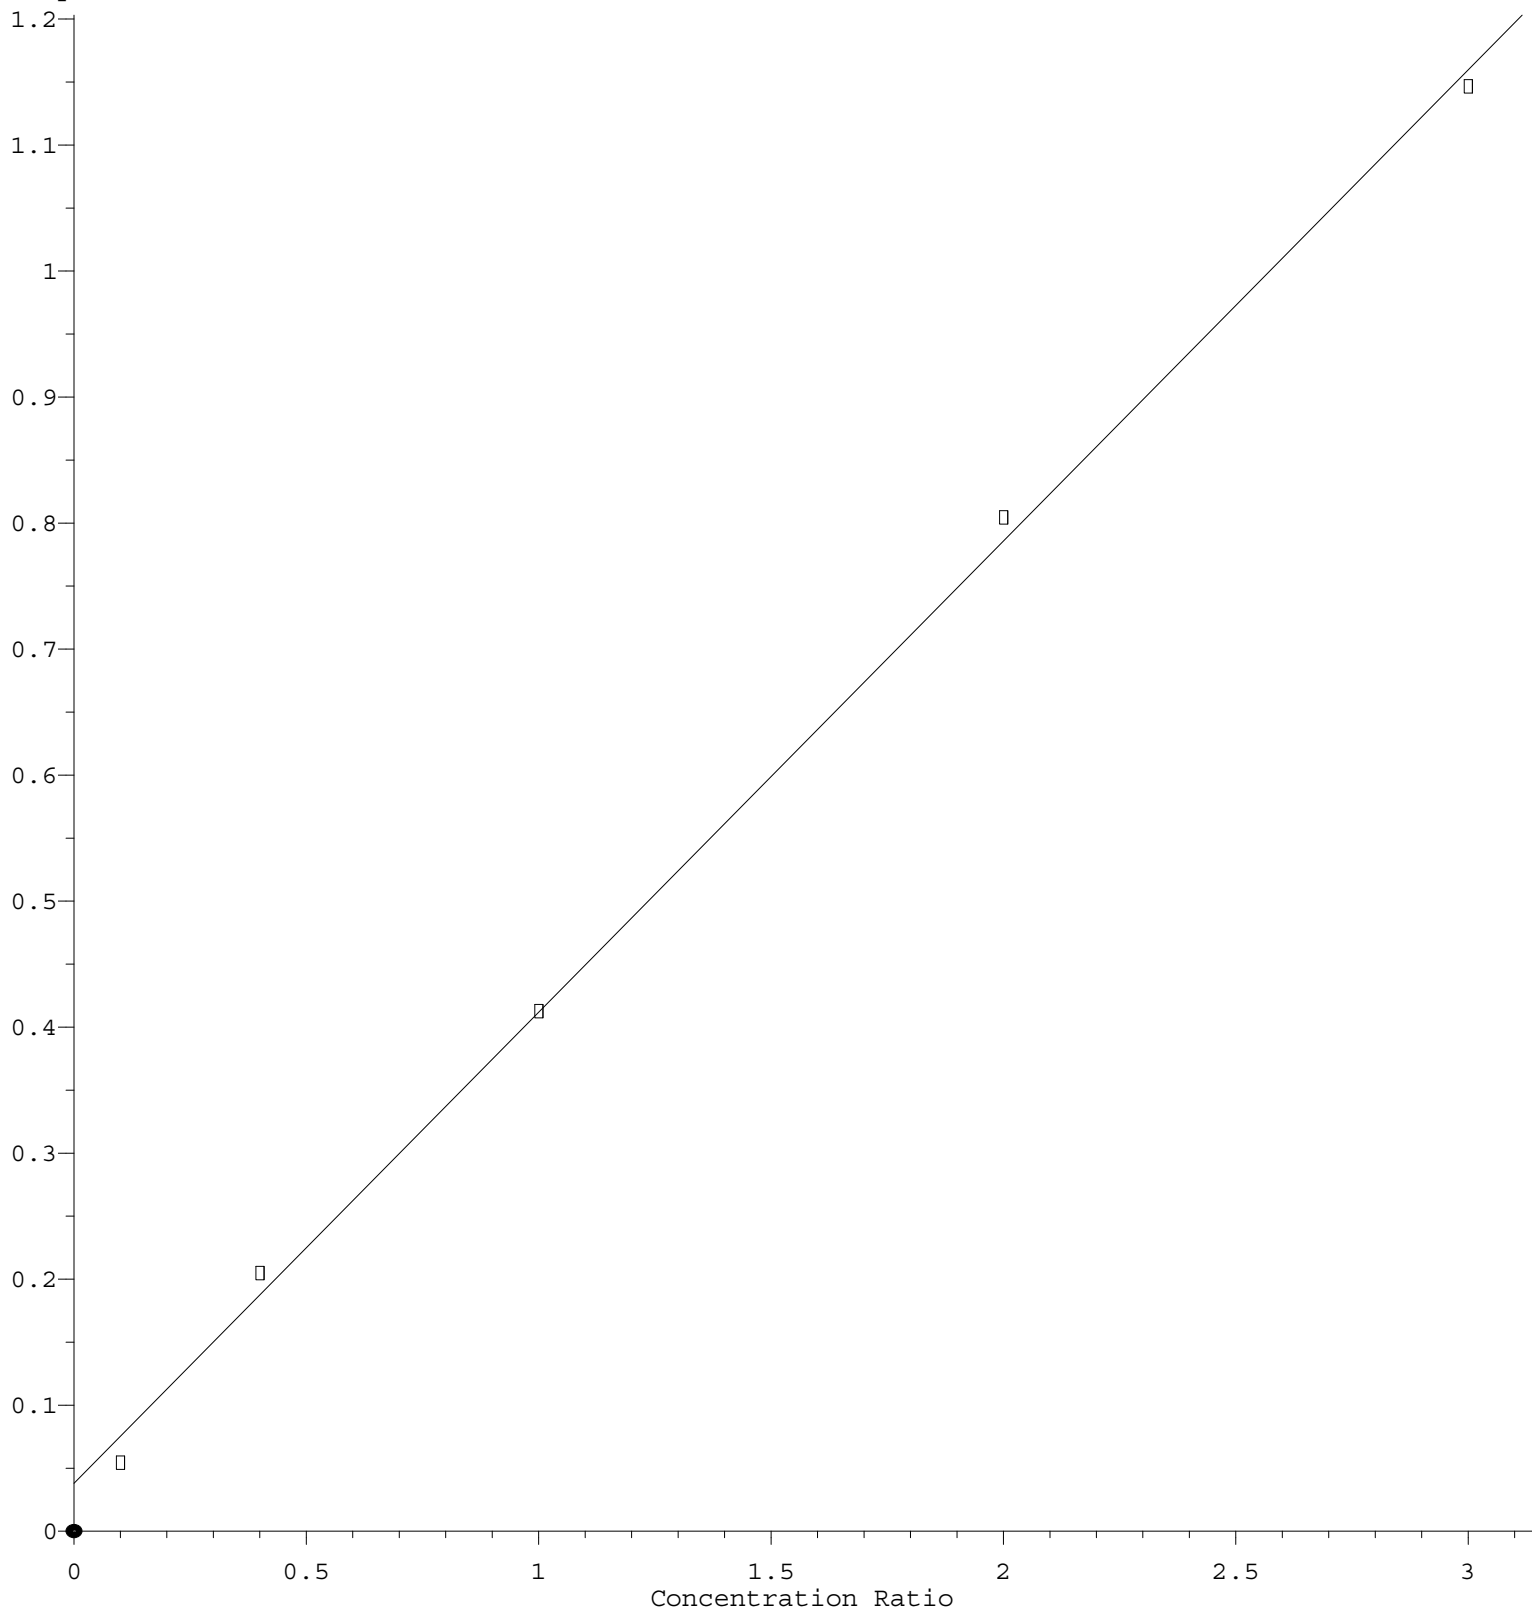

$$\text{Response} = 3.739\text{e-}001 * \text{Amt} + 3.842\text{e-}002$$


Coef of Det (r^2) = 0.998423 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

Chloroethane


Response Ratio

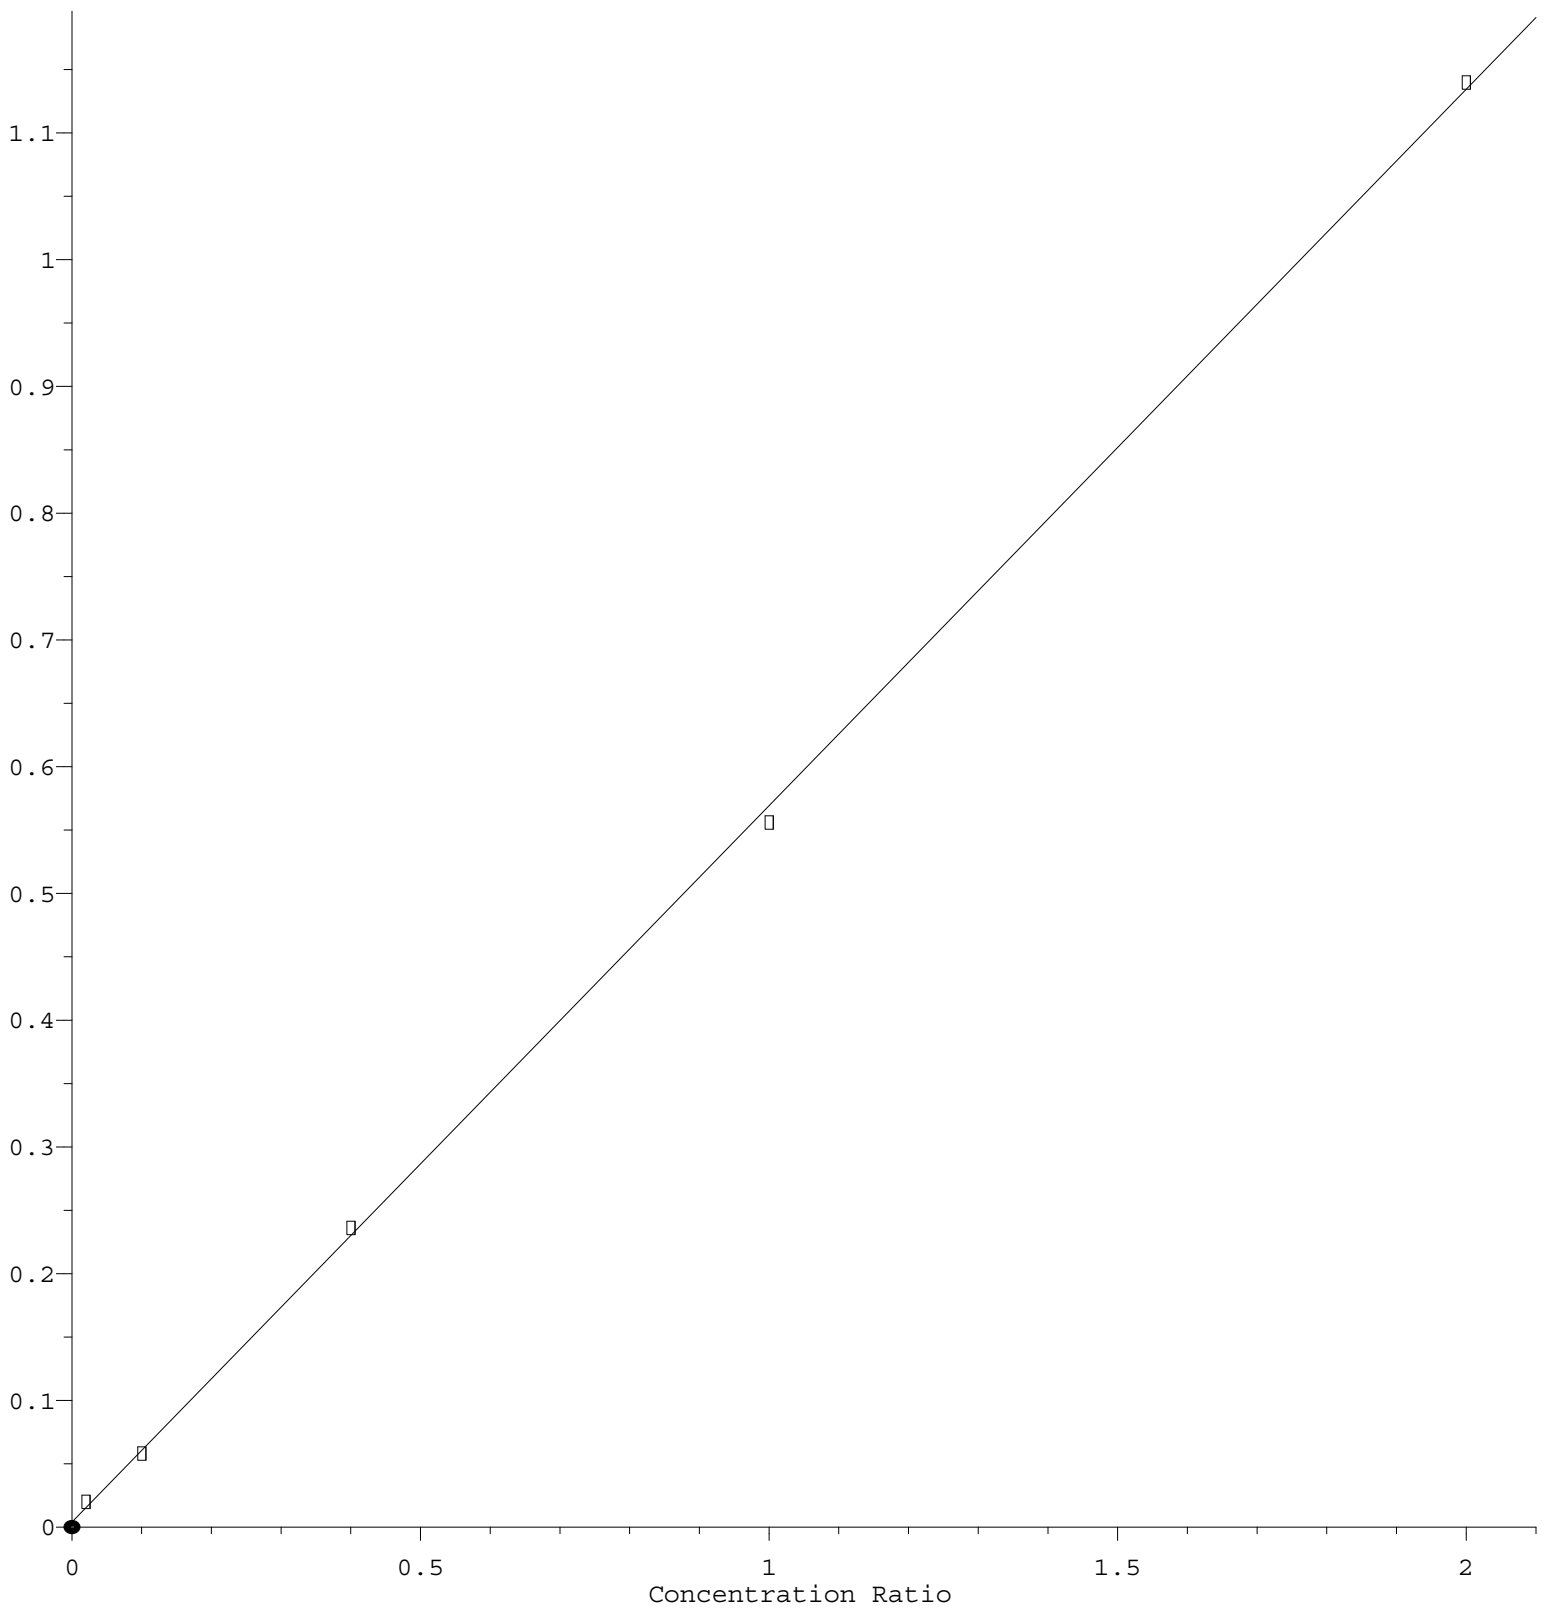

Response = 5.649e-001 * Amt + 4.219e-003
 Coef of Det (r^2) = 0.999688 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M
 Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

Acrolein

Response Ratio

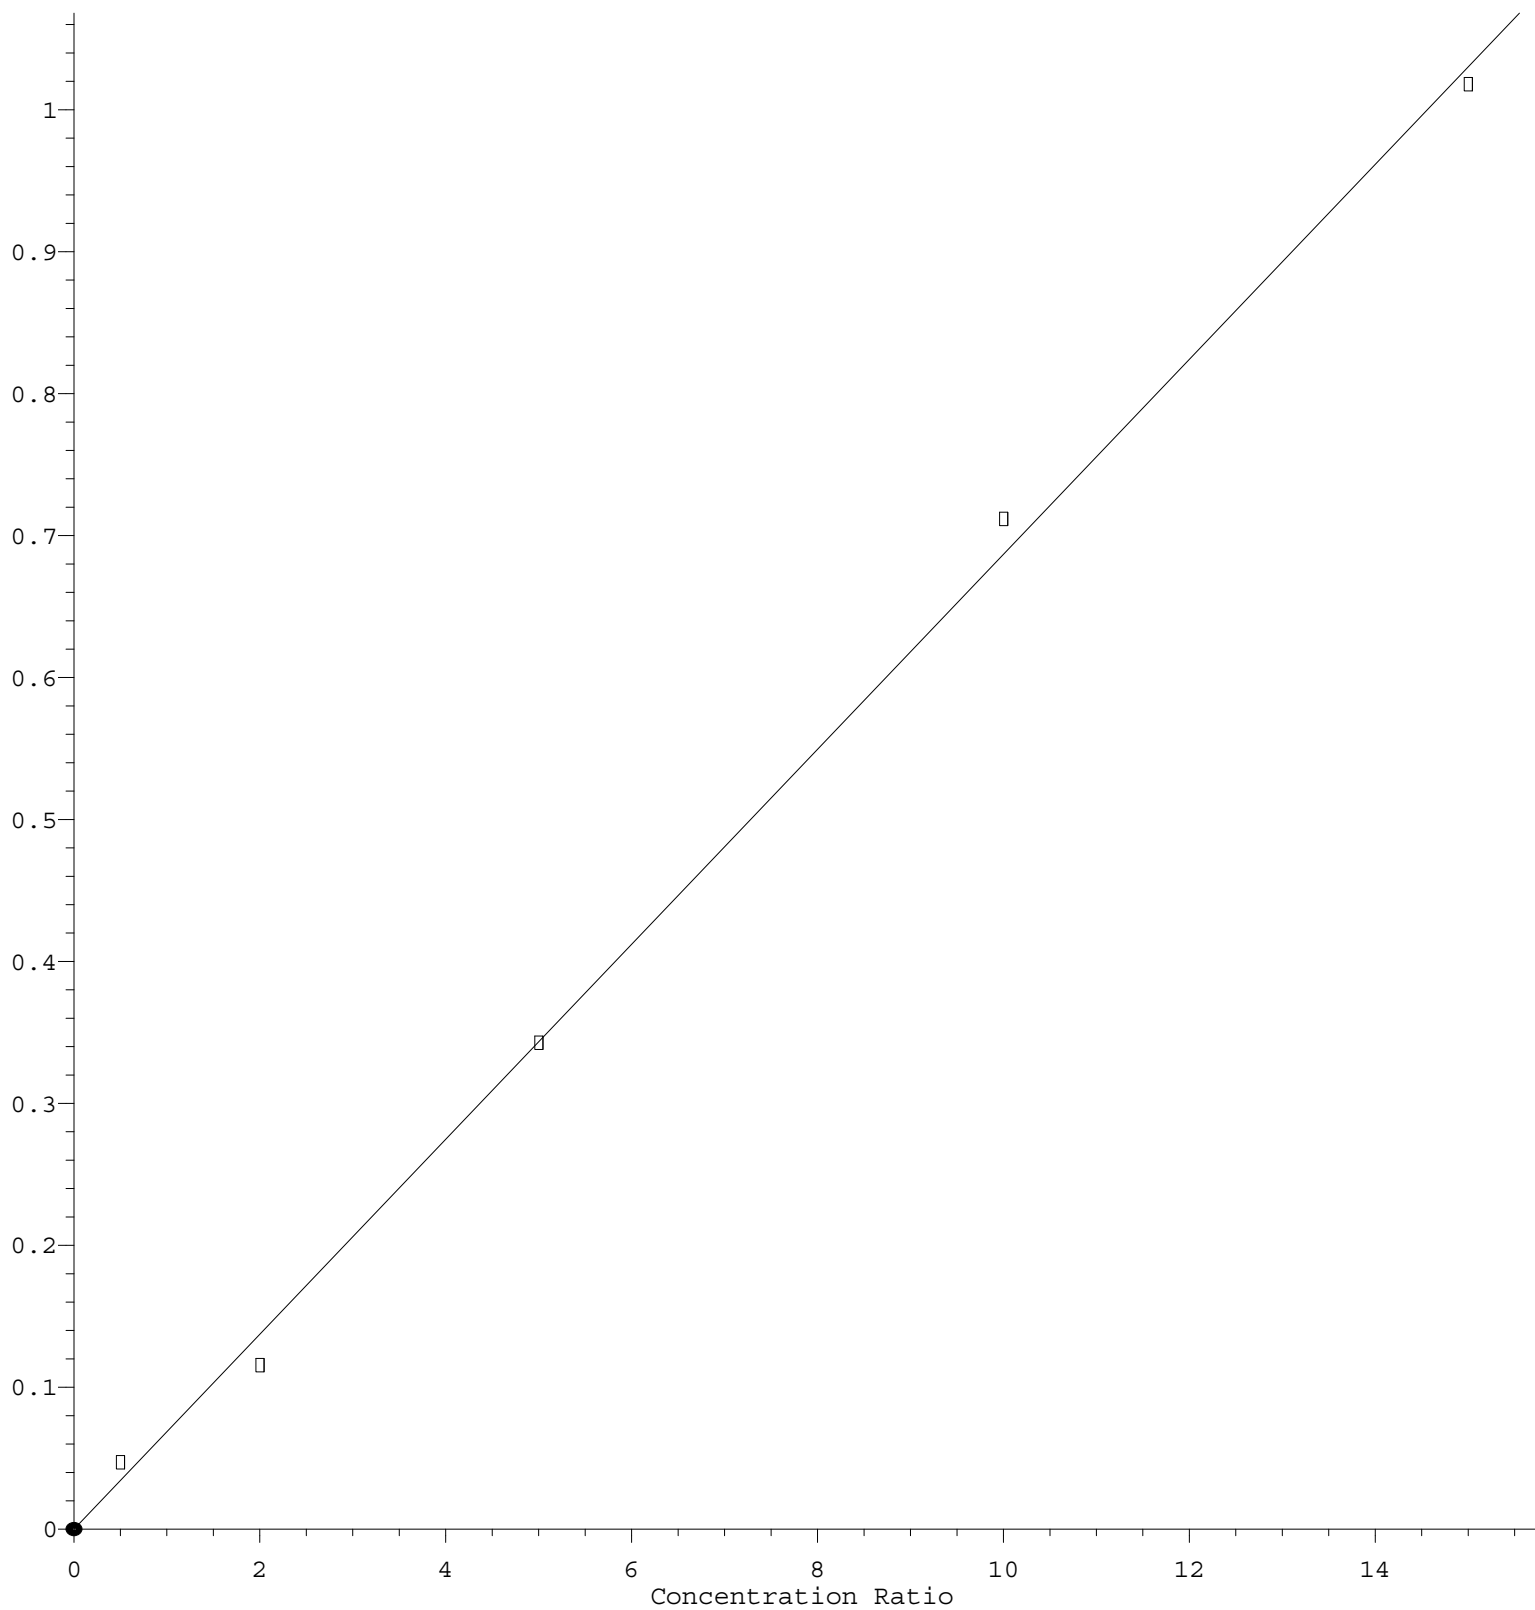

$$\text{Response} = 6.872\text{e-}002 * \text{Amt} + 3.419\text{e-}004$$


Coef of Det (r^2) = 0.997913 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

Ethyl methacrylate

Response Ratio

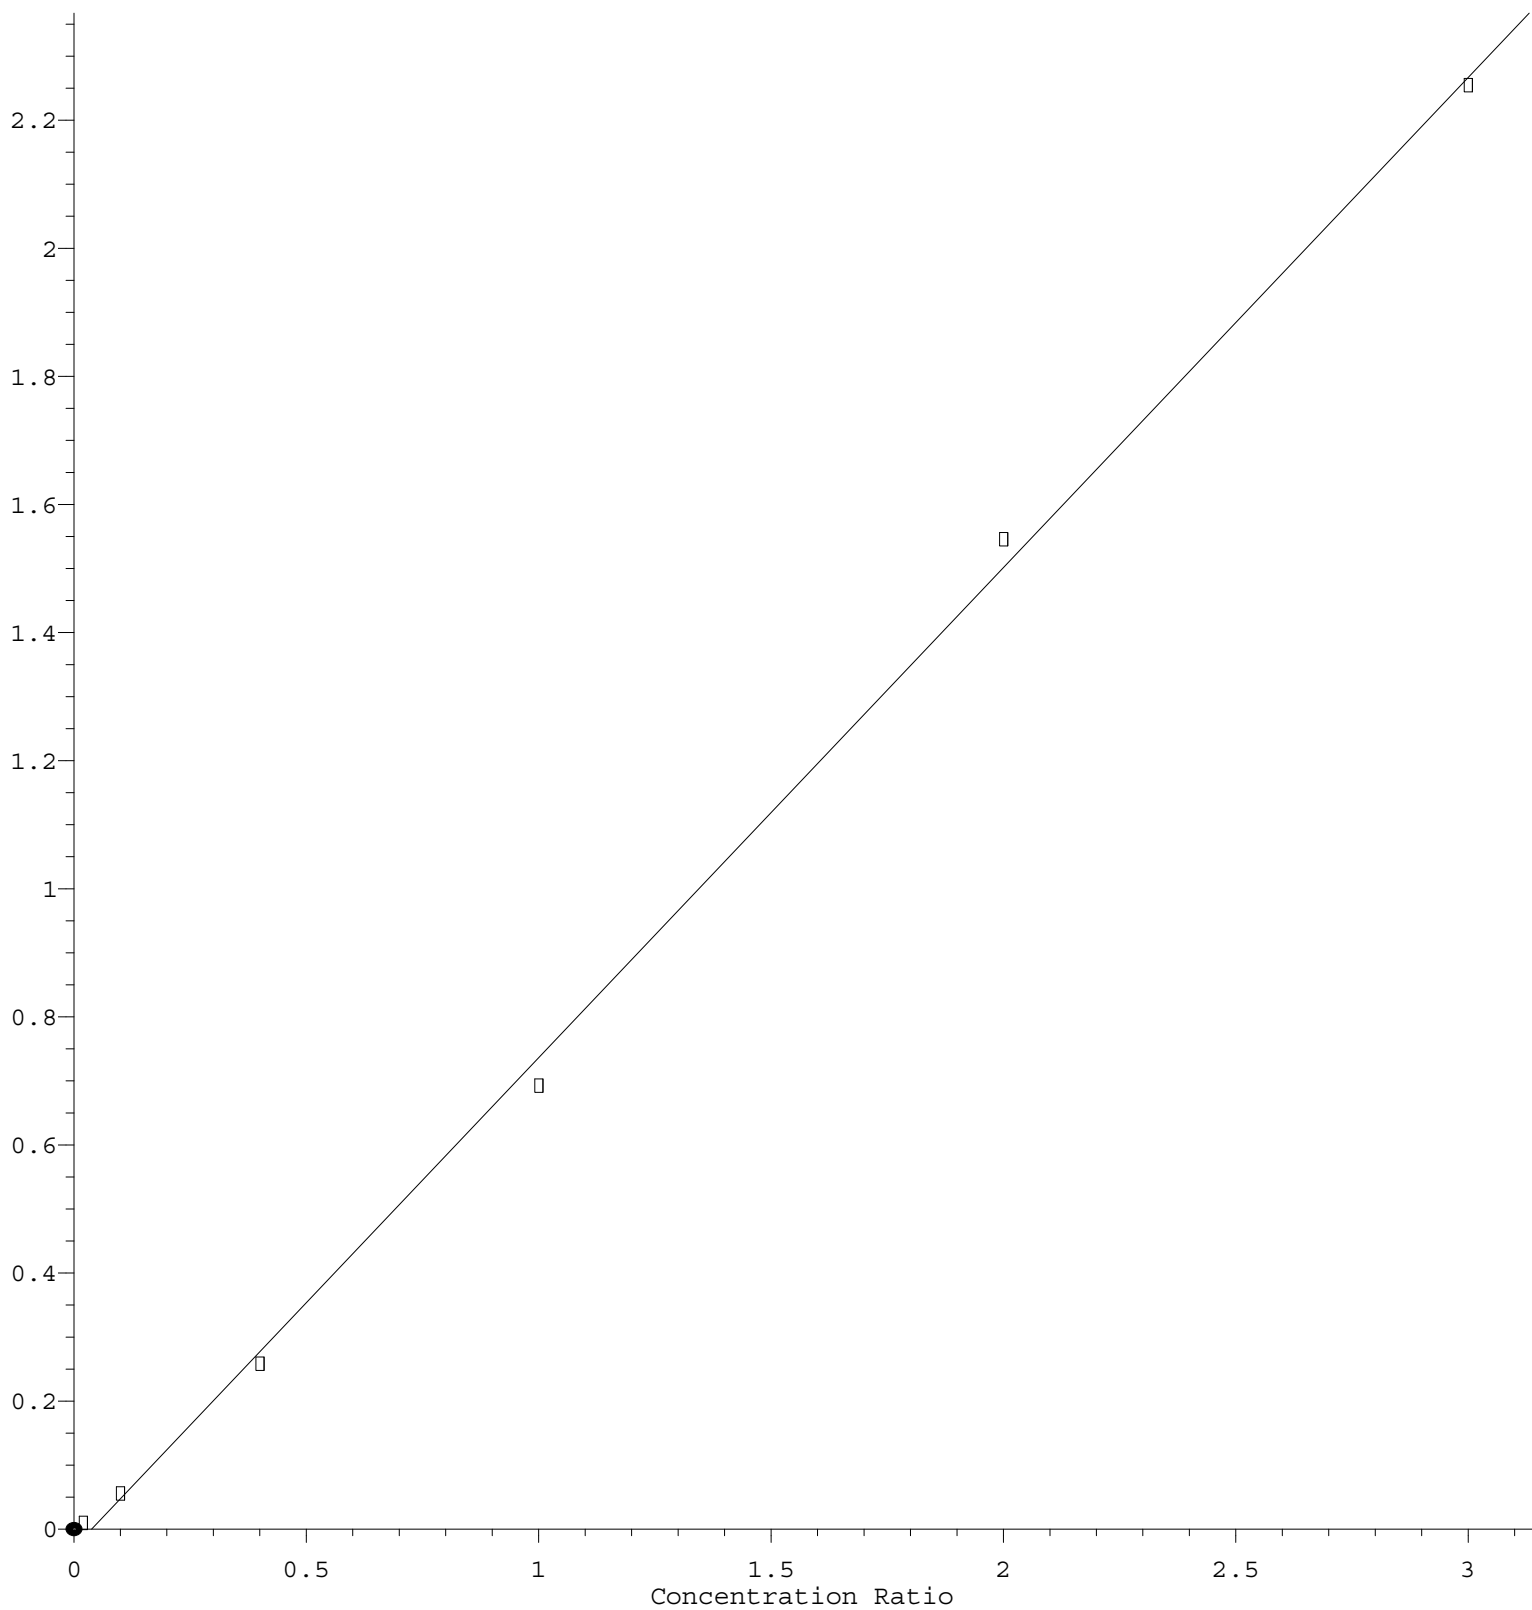

$$\text{Response} = 7.653\text{e-}001 * \text{Amt} - 2.886\text{e-}002$$


Coef of Det (r^2) = 0.998806 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

2-Chloroethyl Vinyl ether

Response Ratio

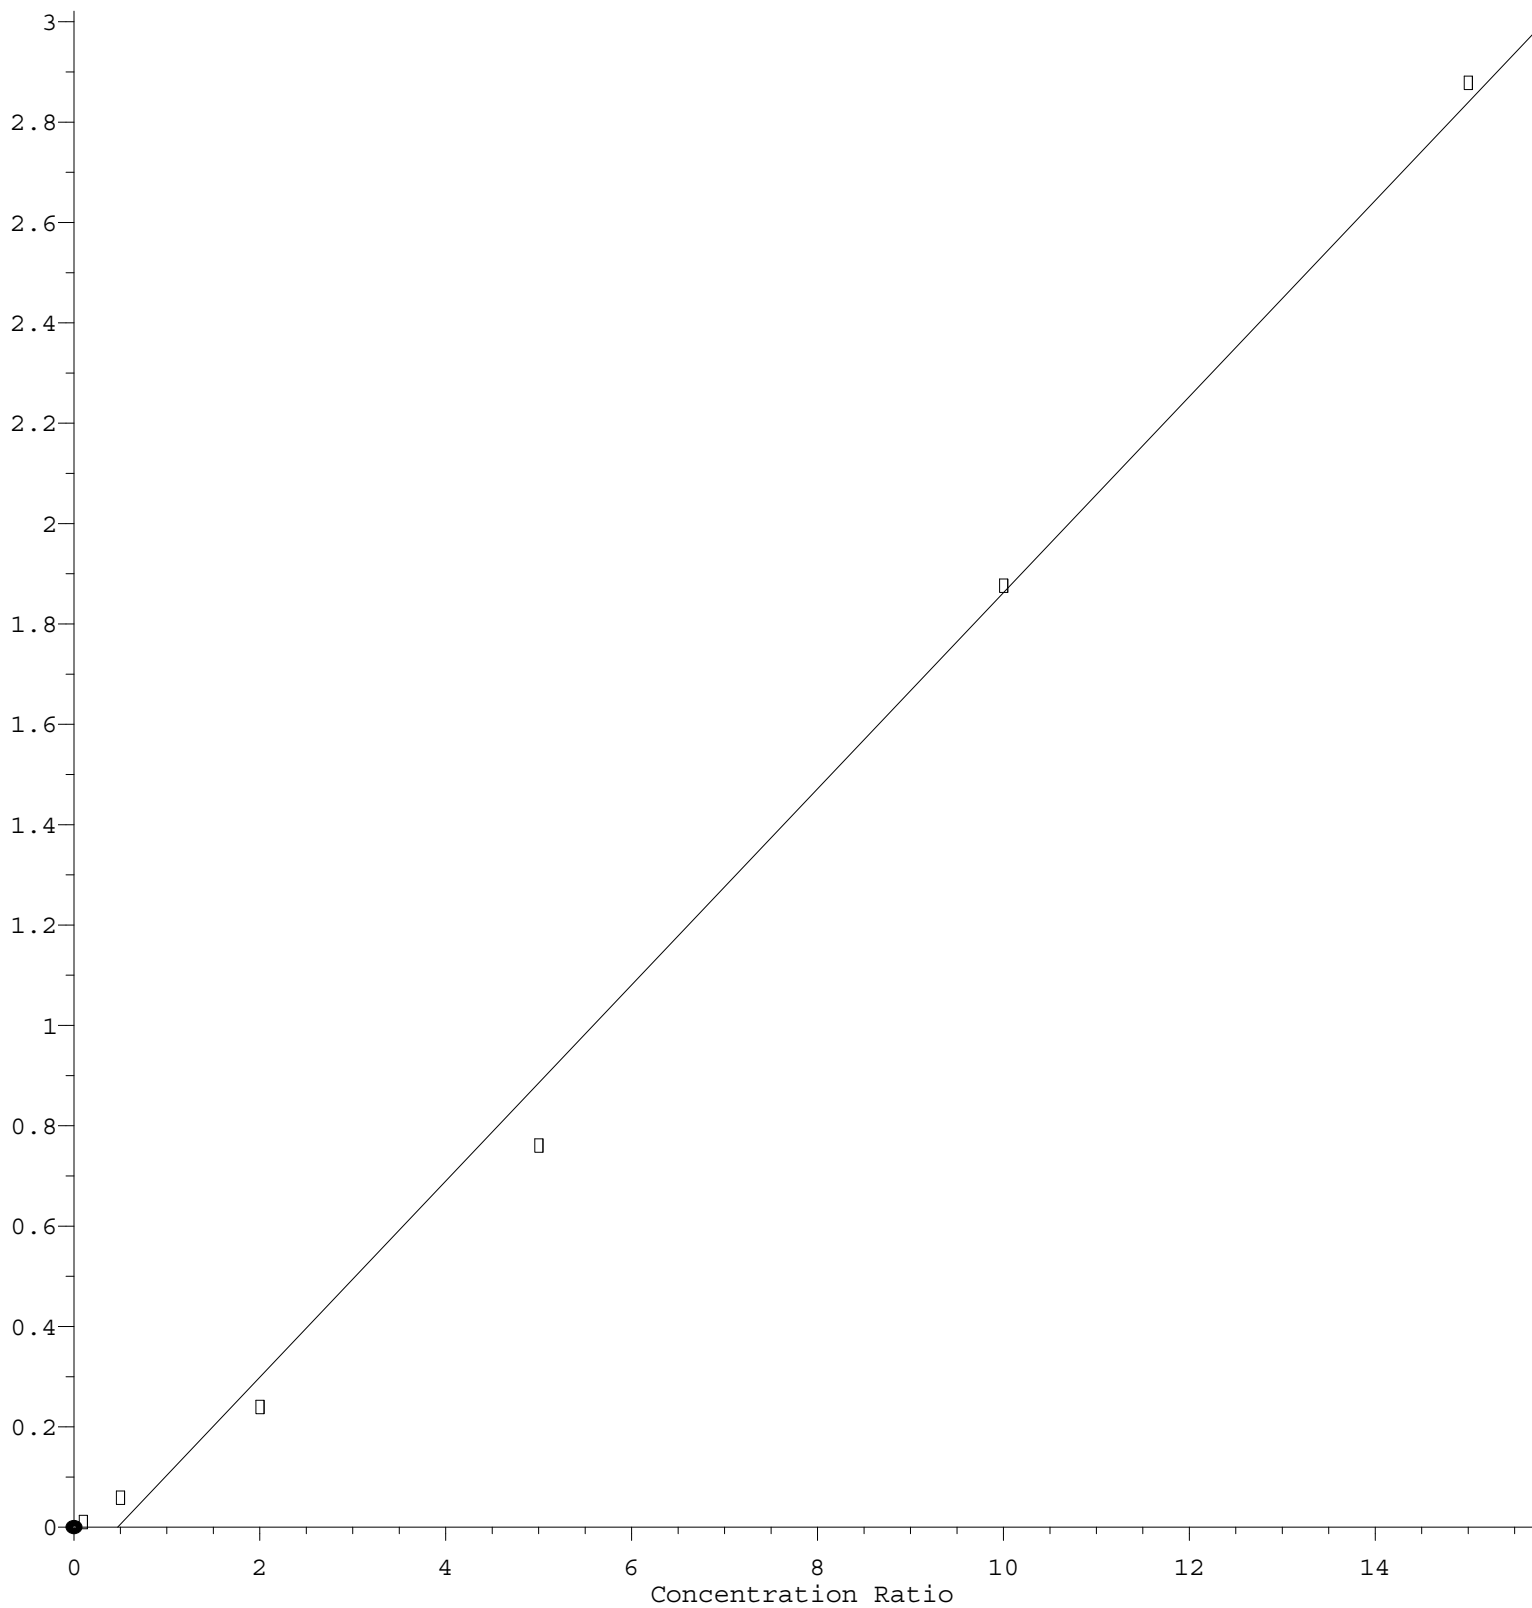

$$\text{Response} = 1.954\text{e-}001 * \text{Amt} - 9.098\text{e-}002$$


Coef of Det (r^2) = 0.995516 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

Styrene


Response Ratio

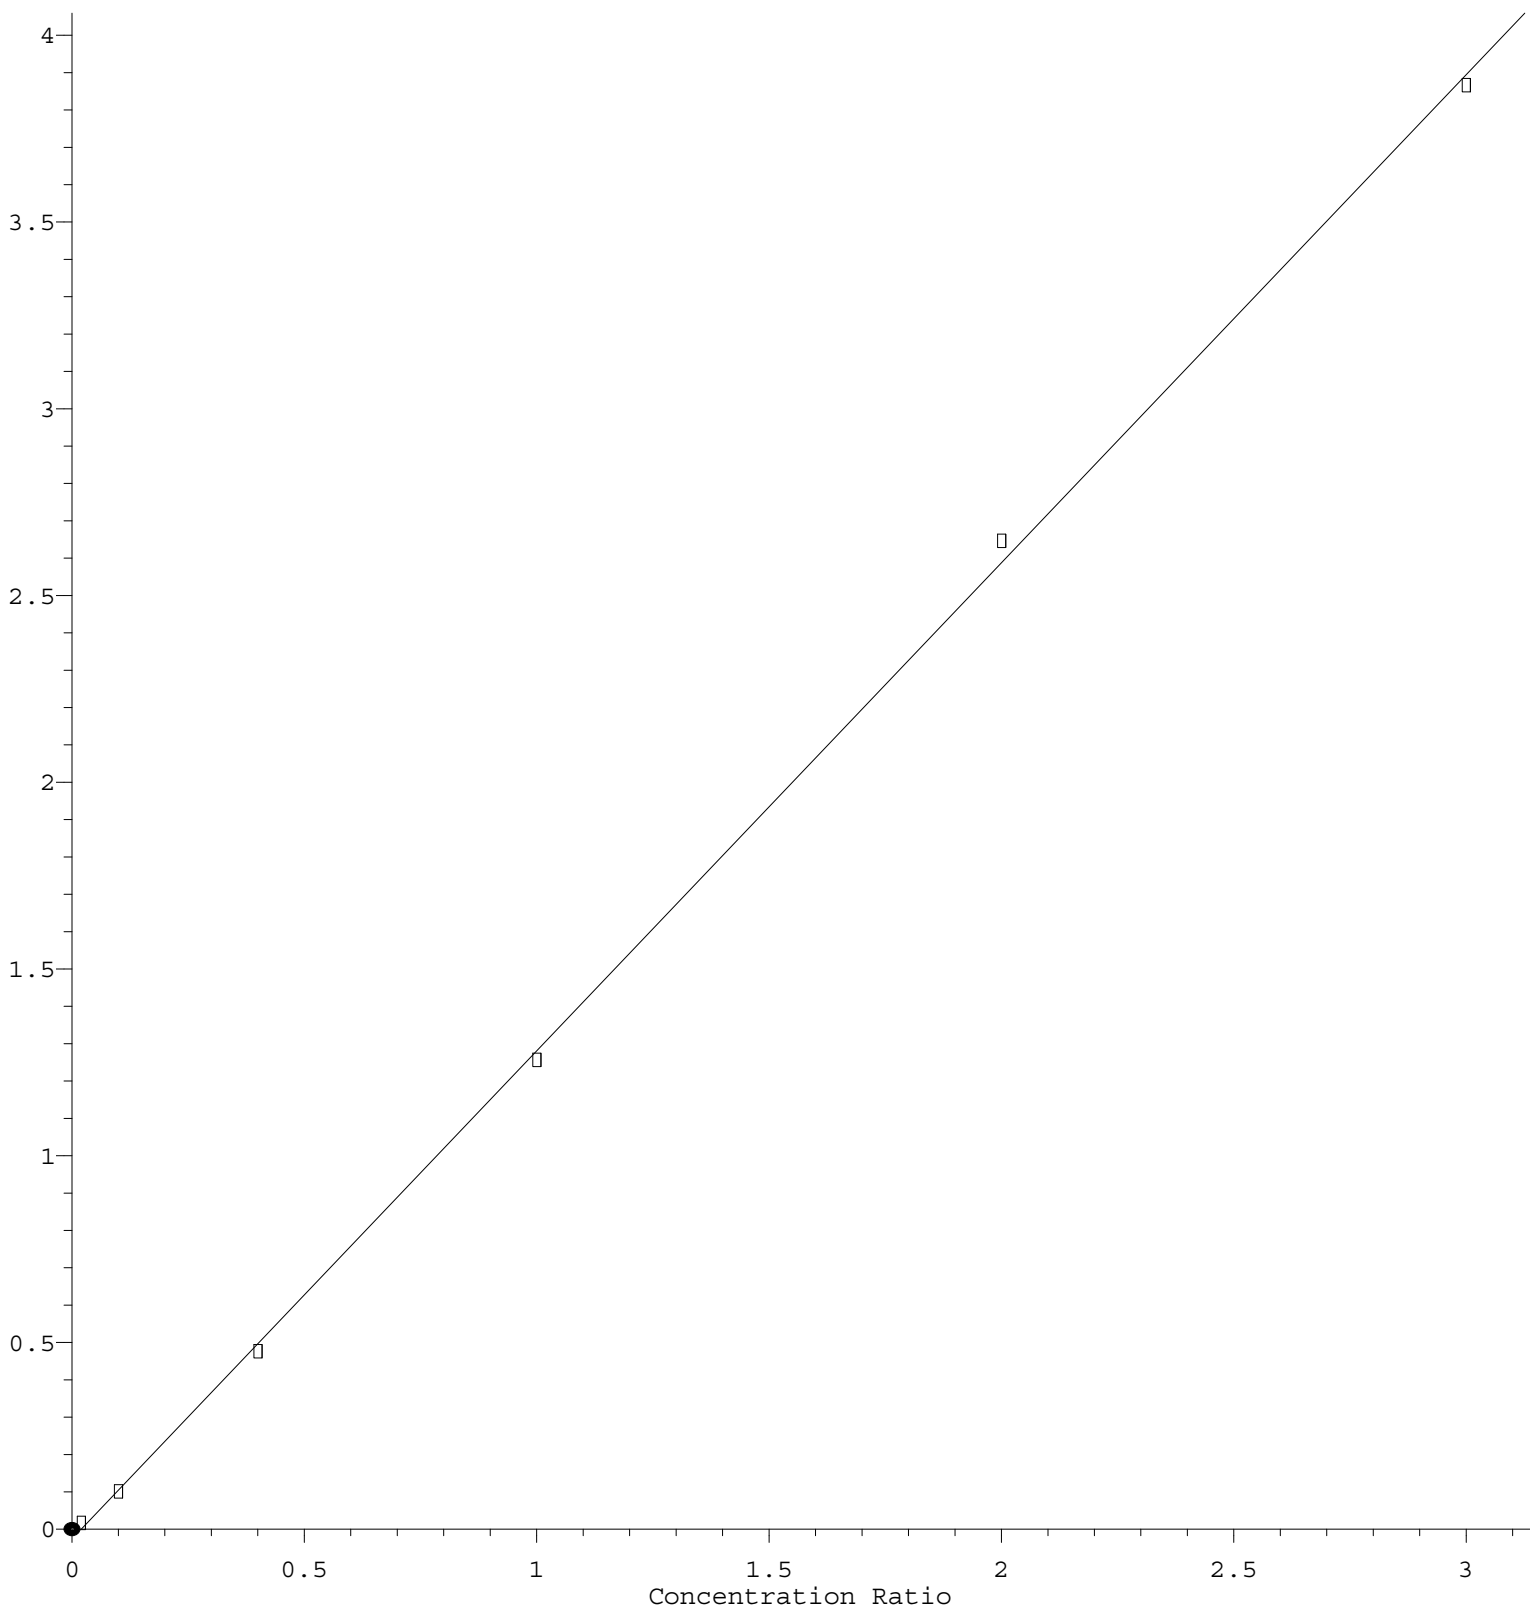

$\text{Response} = 1.307\text{e}+000 * \text{Amt} - 2.643\text{e}-002$
 Coef of Det (r^2) = 0.999546 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M
 Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

n-Butylbenzene

Response Ratio

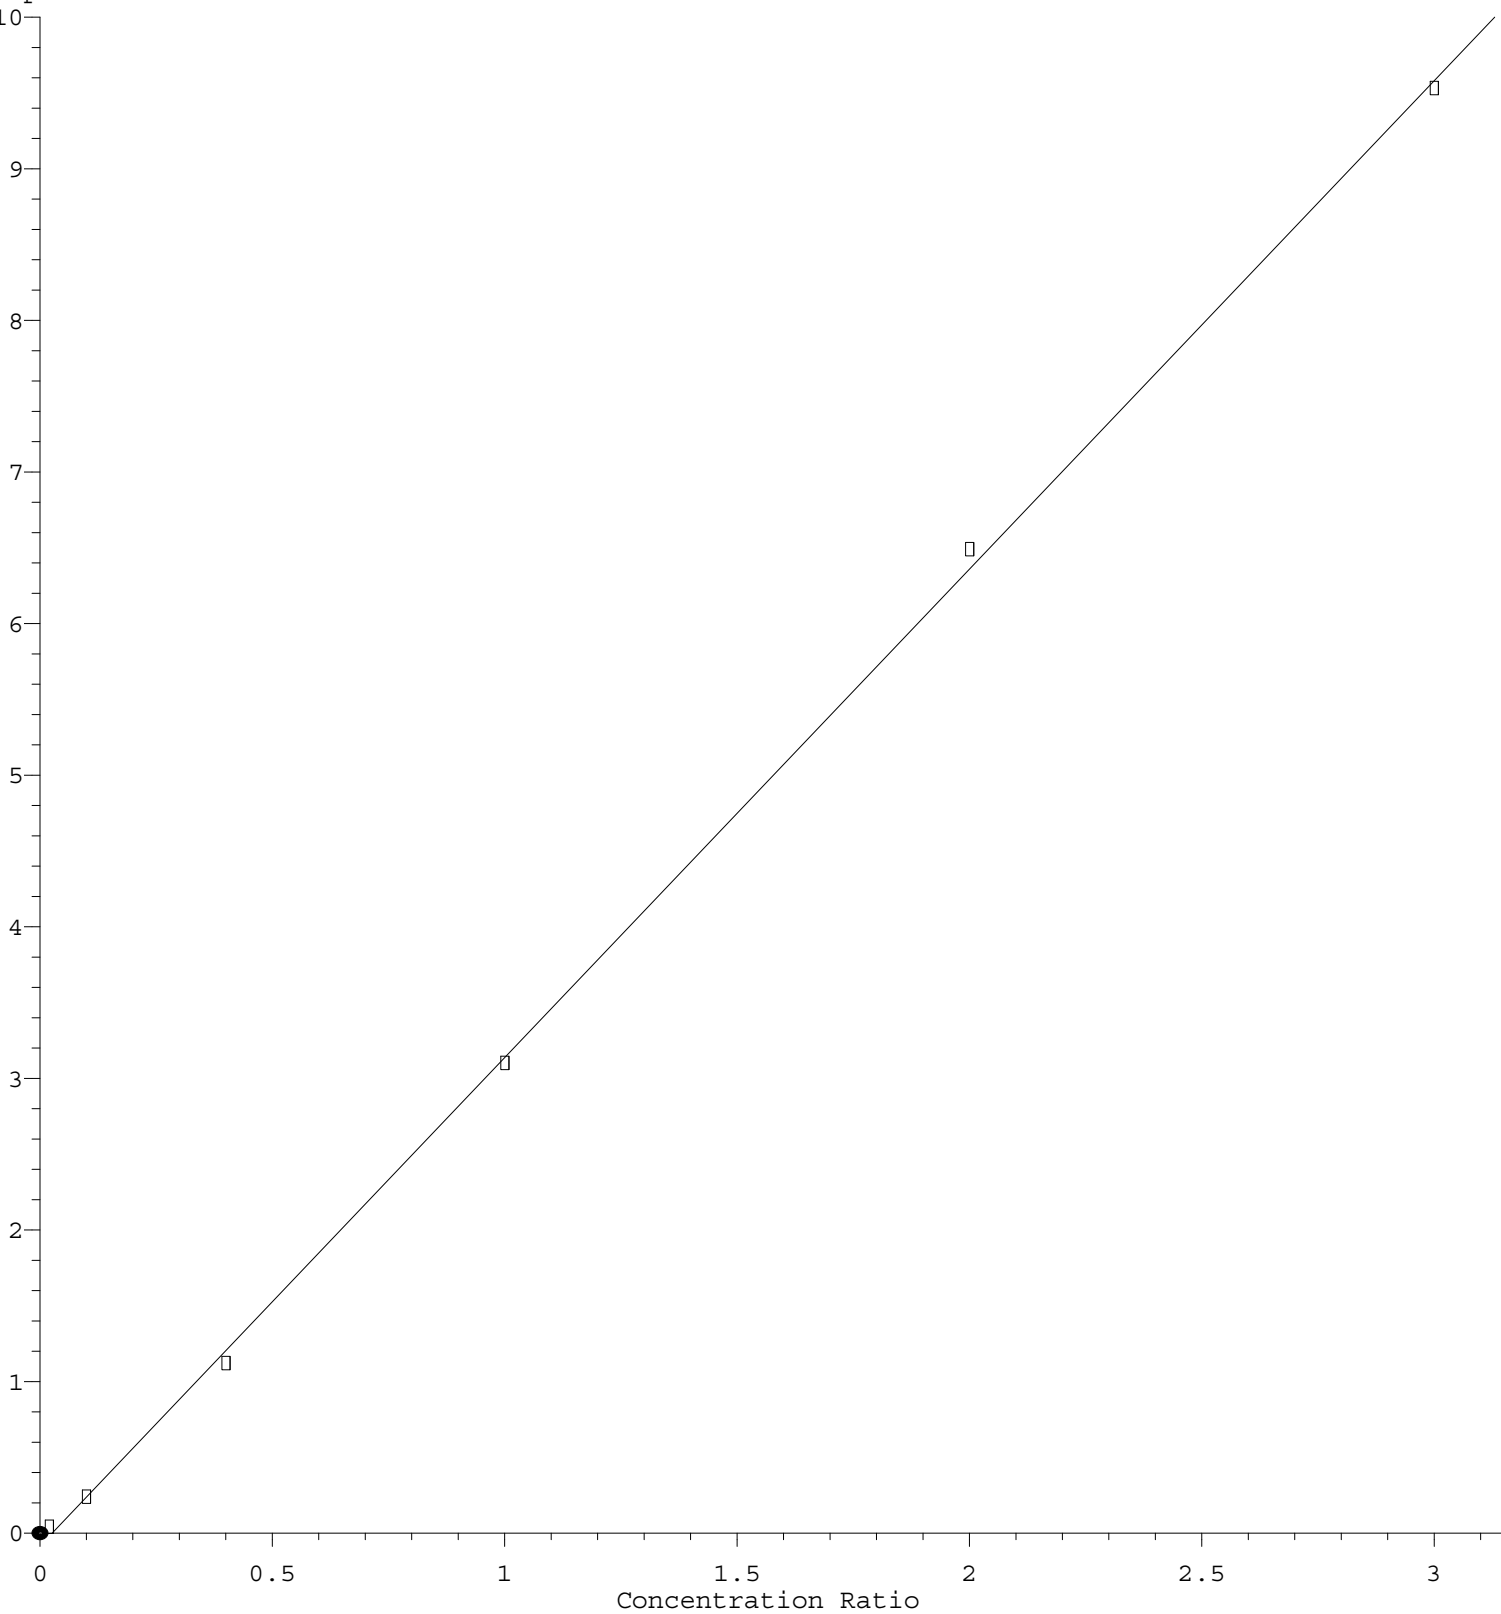

$$\text{Response} = 3.224\text{e}+000 * \text{Amt} - 8.226\text{e}-002$$


Coef of Det (r^2) = 0.999573 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021

Naphthalene

Response Ratio

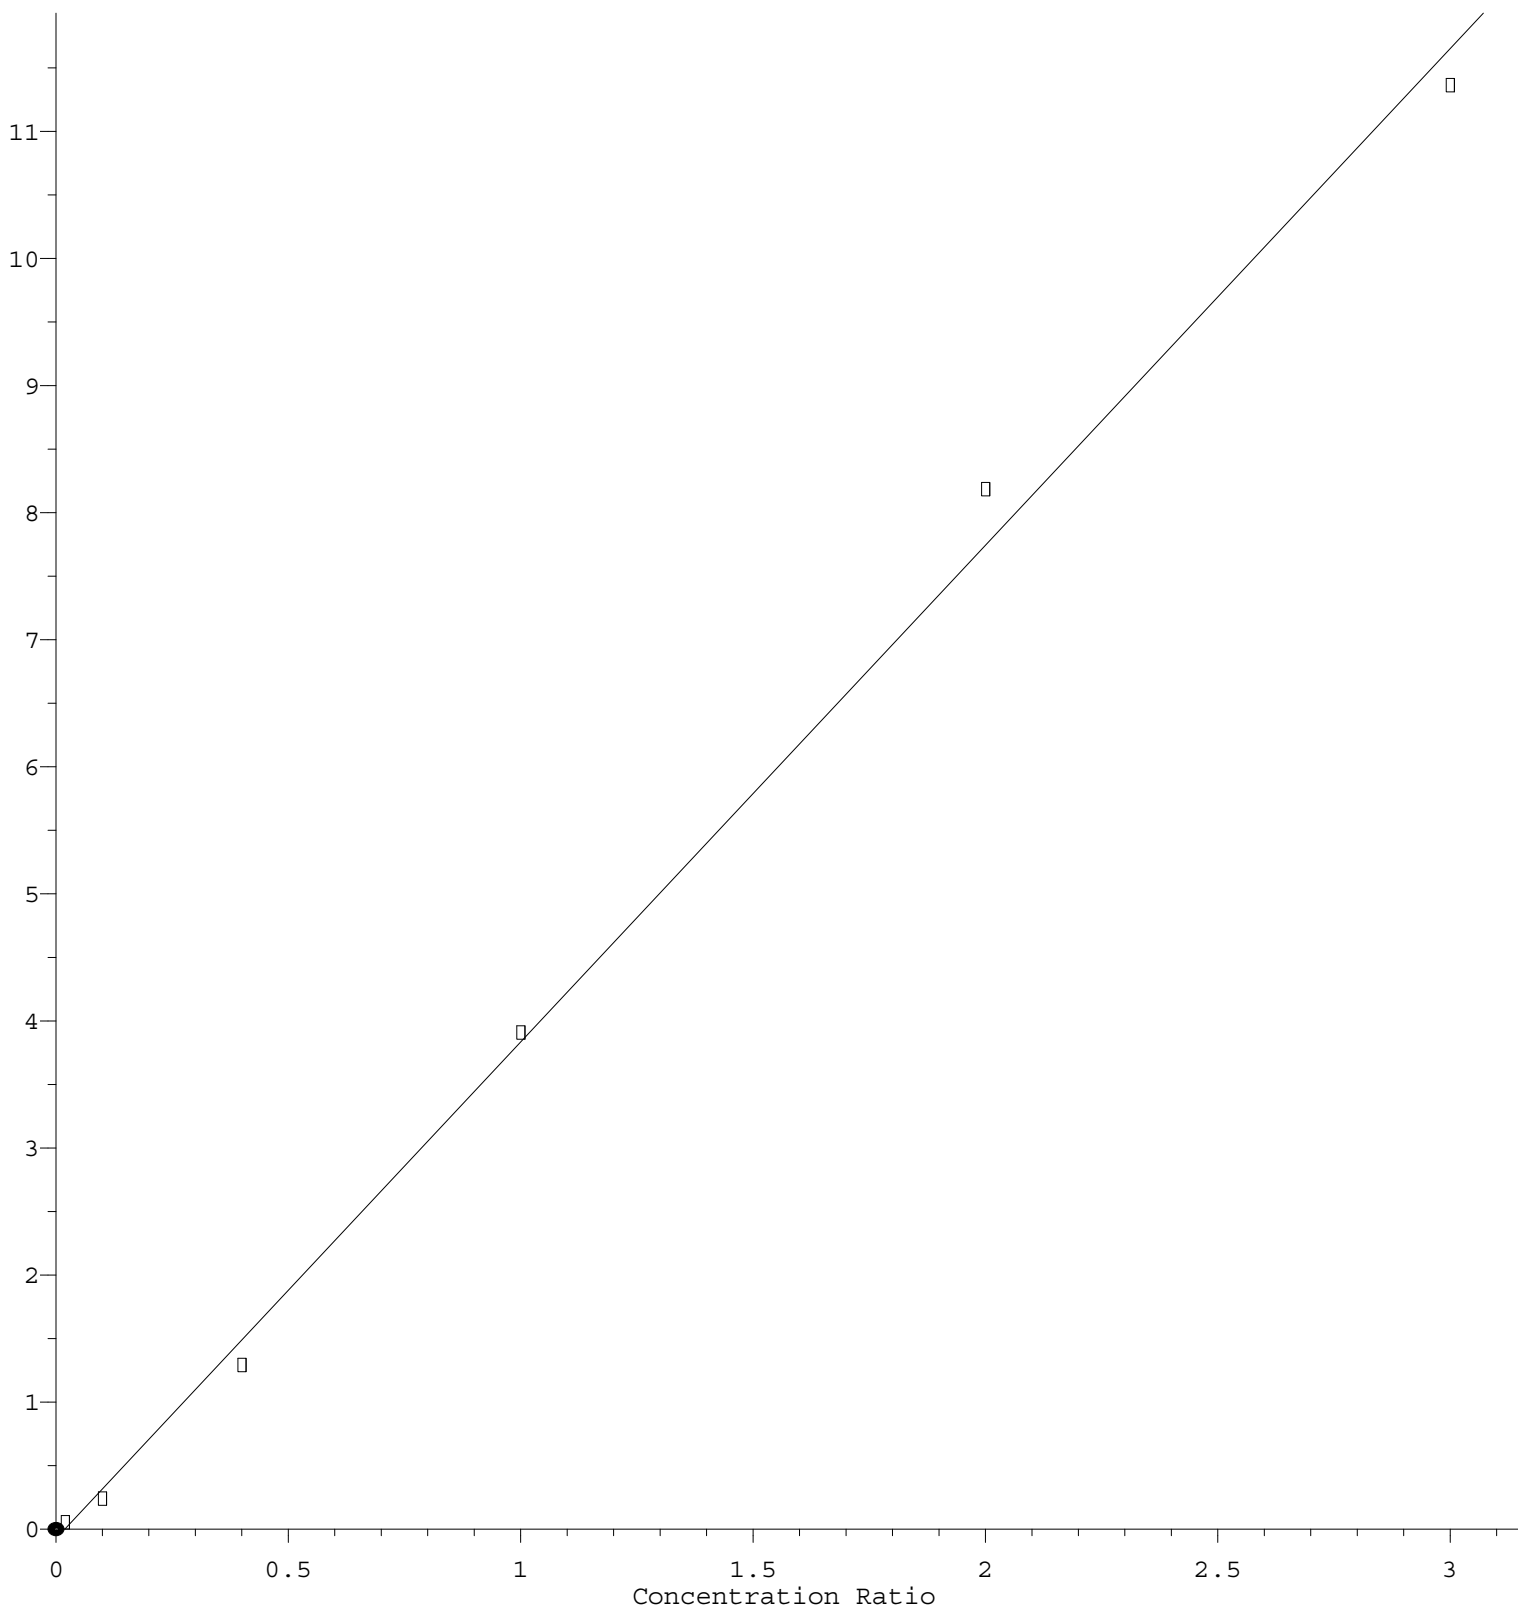

$$\text{Response} = 3.909\text{e}+000 * \text{Amt} - 7.372\text{e}-002$$

Coef of Det (r^2) = 0.996961 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092421W.M

Calibration Table Last Updated: Tue Sep 28 11:39:06 2021