

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
 Data File : VU044882.D
 Acq On : 26 Sep 2021 09:46
 Operator : SY/MD
 Sample : M3893-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Title : SW846 8260

Signal : TIC: VU044882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	76	83	90	rBV	22565	25340	2.08%	0.352%
2	2.375	314	322	334	rVB5	9800	17535	1.44%	0.244%
3	2.584	375	387	398	rBV	114649	187888	15.44%	2.613%
4	2.784	435	449	474	rBV2	9841	29848	2.45%	0.415%
5	3.874	771	788	806	rBV	54664	127273	10.46%	1.770%
6	4.674	1014	1037	1051	rBV2	15675	35649	2.93%	0.496%
7	5.295	1214	1230	1243	rBV	178969	387133	31.81%	5.384%
8	5.379	1243	1256	1275	rVB	316971	645737	53.07%	8.981%
9	5.706	1343	1358	1375	rBV	217251	444436	36.52%	6.181%
10	5.838	1375	1399	1434	rVB3	61240	170952	14.05%	2.378%
11	6.253	1513	1528	1552	rBV	467728	880070	72.32%	12.240%
12	6.565	1607	1625	1636	rVB8	4162	12272	1.01%	0.171%
13	6.977	1740	1753	1773	rBV2	32636	68472	5.63%	0.952%
14	7.253	1829	1839	1853	rBV2	23655	41443	3.41%	0.576%
15	7.903	2015	2041	2055	rBV	709166	1216855	100.00%	16.925%
16	7.973	2056	2063	2074	rVB2	12326	21041	1.73%	0.293%
17	9.047	2387	2397	2407	rVB3	16716	26308	2.16%	0.366%
18	9.420	2499	2513	2536	rBV	638442	1053639	86.59%	14.655%
19	9.697	2589	2599	2610	rBV2	10017	16299	1.34%	0.227%
20	10.636	2879	2891	2908	rBV	490393	779750	64.08%	10.845%
21	11.816	3245	3258	3278	rBV	634405	1001882	82.33%	13.935%




Sum of corrected areas: 7189822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
Data File : VU044882.D
Acq On : 26 Sep 2021 09:46
Operator : SY/MD
Sample : M3893-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

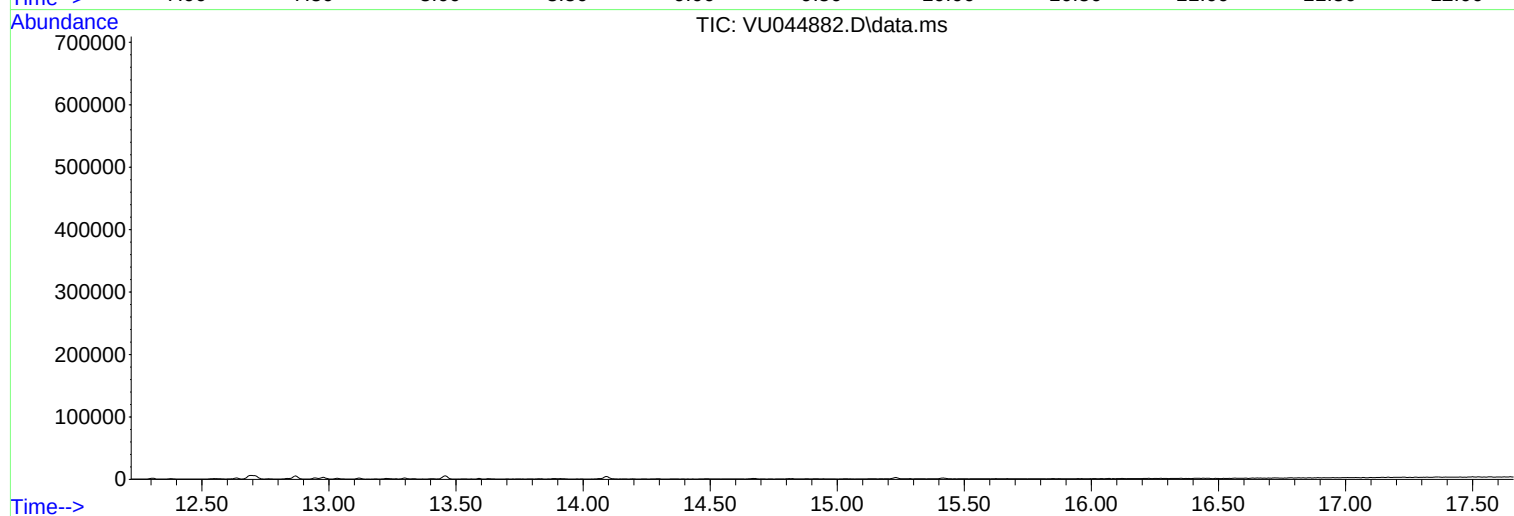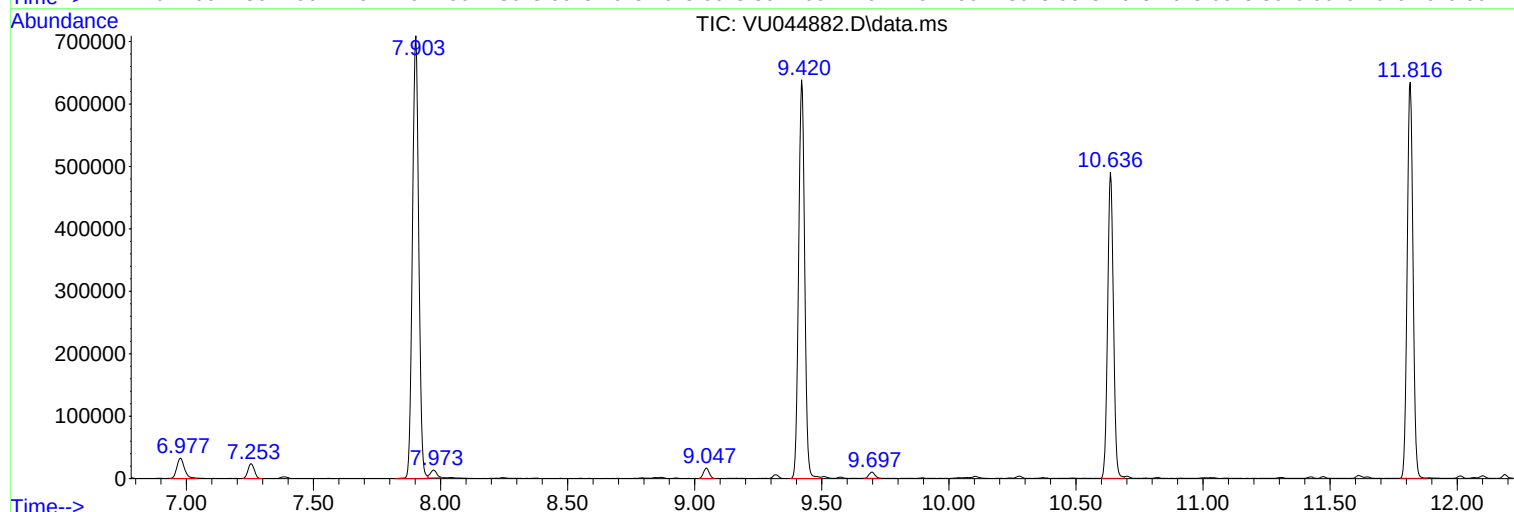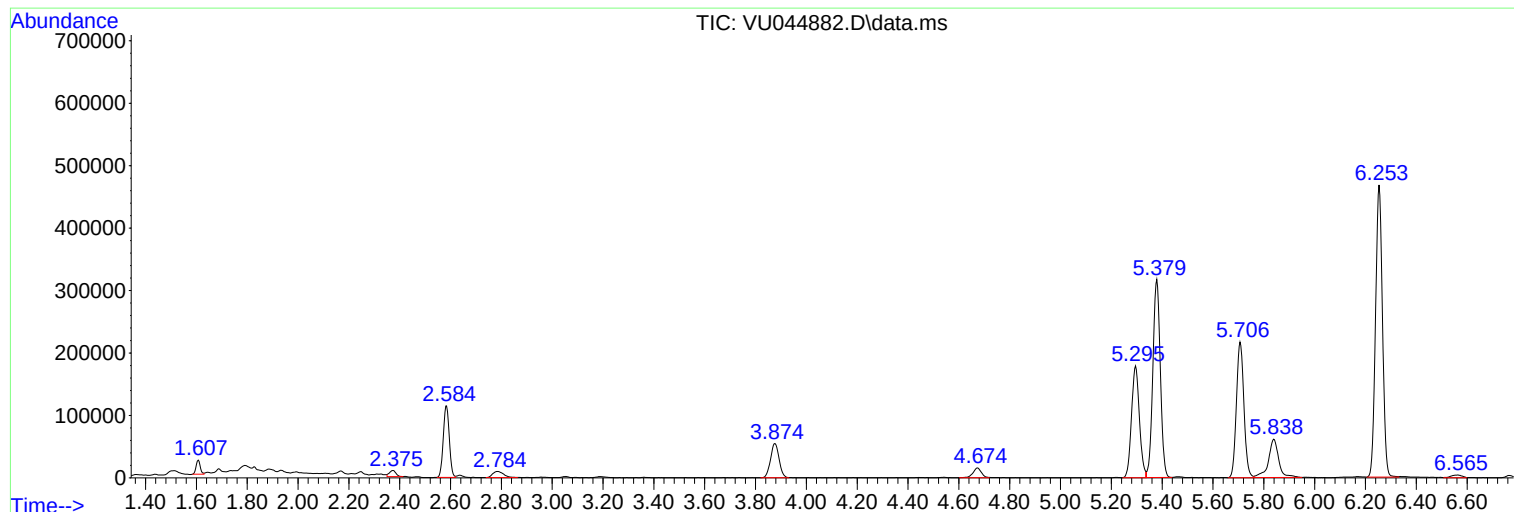

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
Data File : VU044882.D
Acq On : 26 Sep 2021 09:46
Operator : SY/MD
Sample : M3893-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092521\
Data File : VU044882.D
Acq On : 26 Sep 2021 09:46
Operator : SY/MD
Sample : M3893-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------