


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055499.D
Acq On : 25 Sep 2023 16:47
Operator : MD/SY
Sample : 04579-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 25 01:08:17 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
Supervised By :Semsettin Yesilyurt 09/28/2023

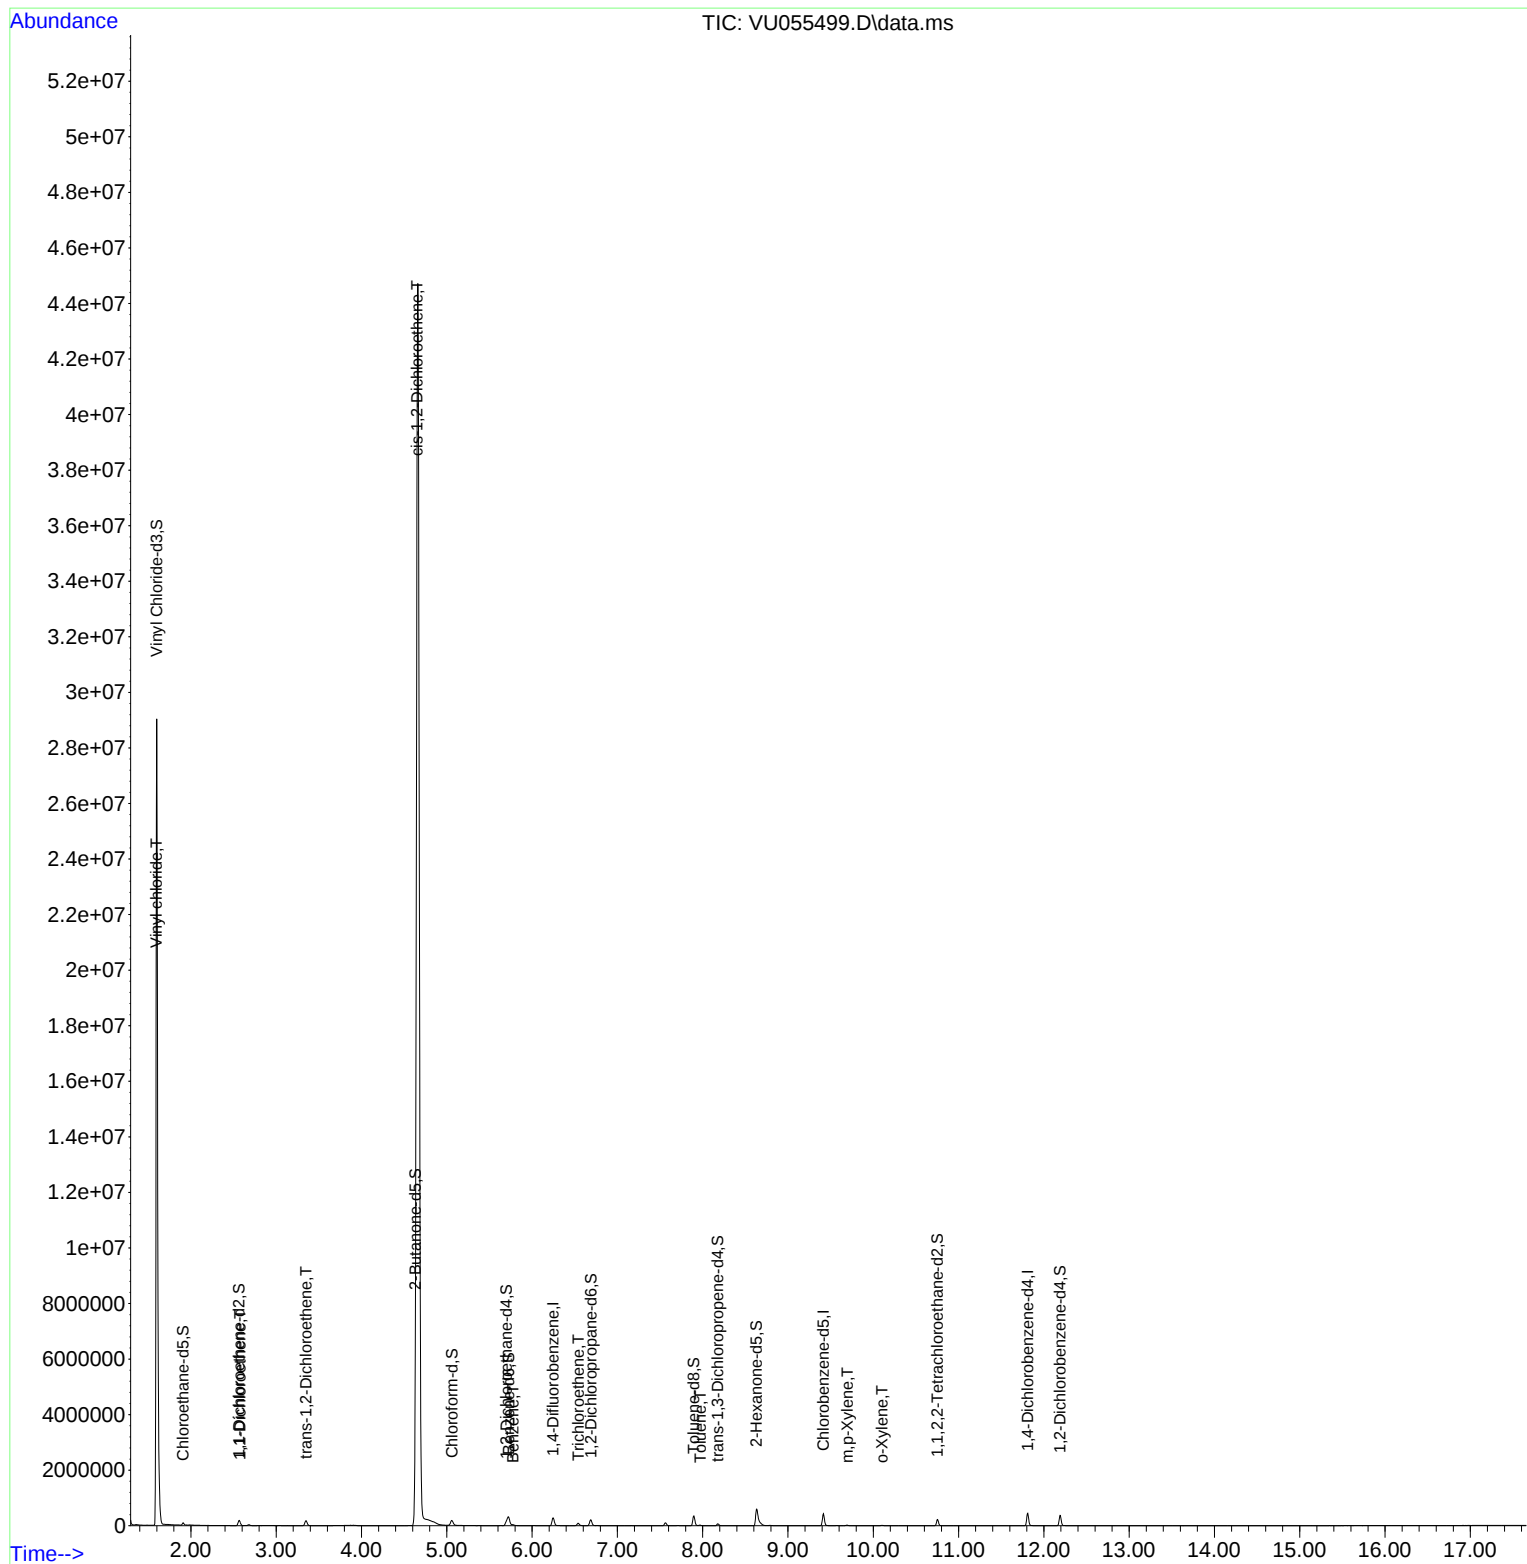




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055499.D
Acq On : 25 Sep 2023 16:47
Operator : MD/SY
Sample : 04579-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 25 01:08:17 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
Supervised By :Semsettin Yesilyurt 09/28/2023

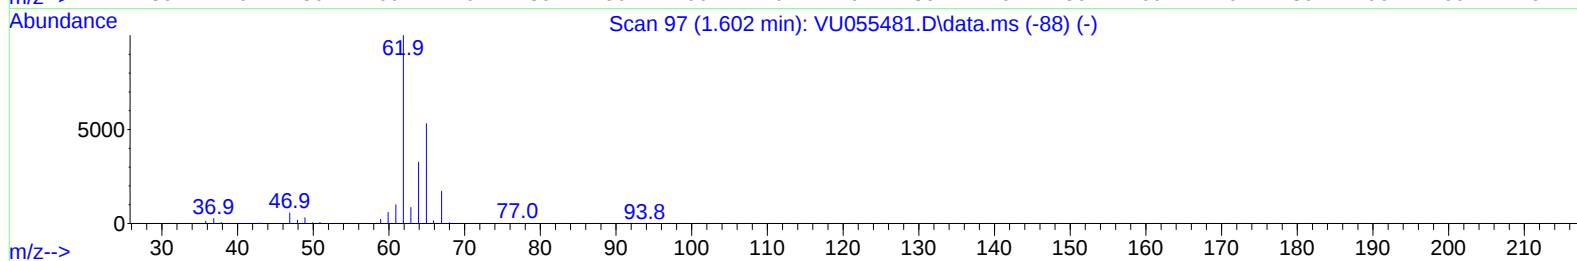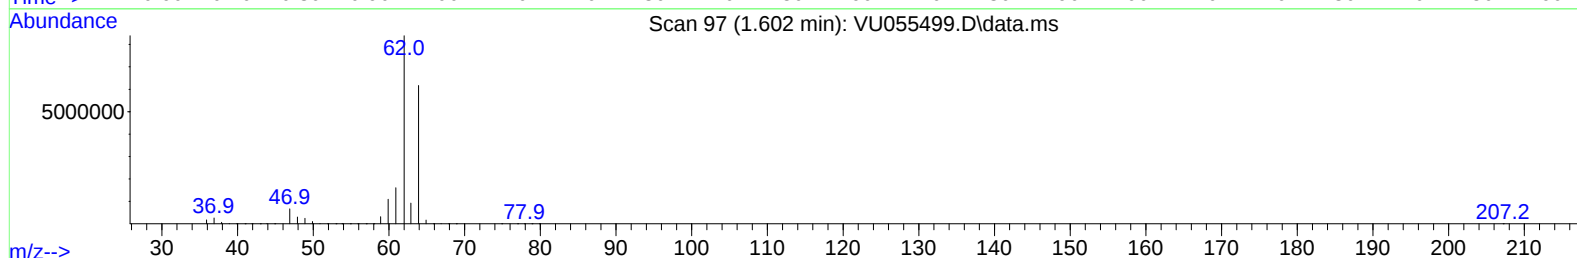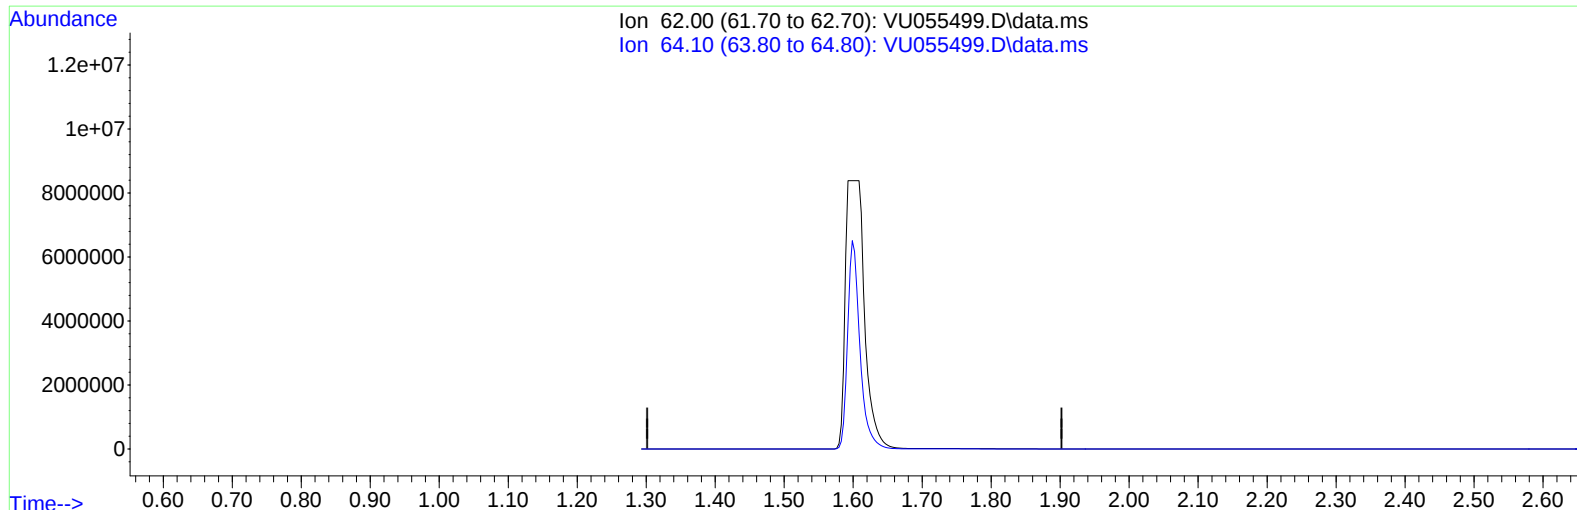

TIC: VU055499.D\data.ms

(5) Vinyl chloride (T)

1.602min (-1.602) 0.00 ug/L

response 0

Ion	Exp%	Act%
62.00	100.00	0.00
64.10	31.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055499.D
Acq On : 25 Sep 2023 16:47
Operator : MD/SY
Sample : 04579-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 25 01:08:17 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
Supervised By :Semsettin Yesilyurt 09/28/2023

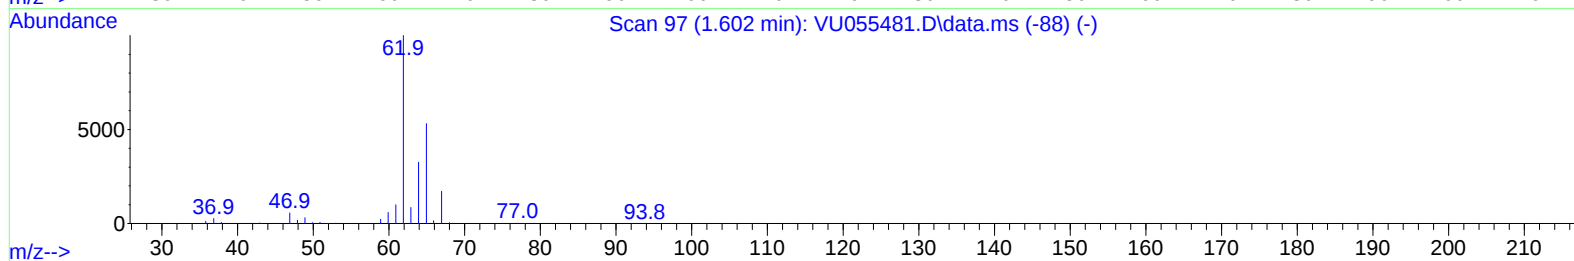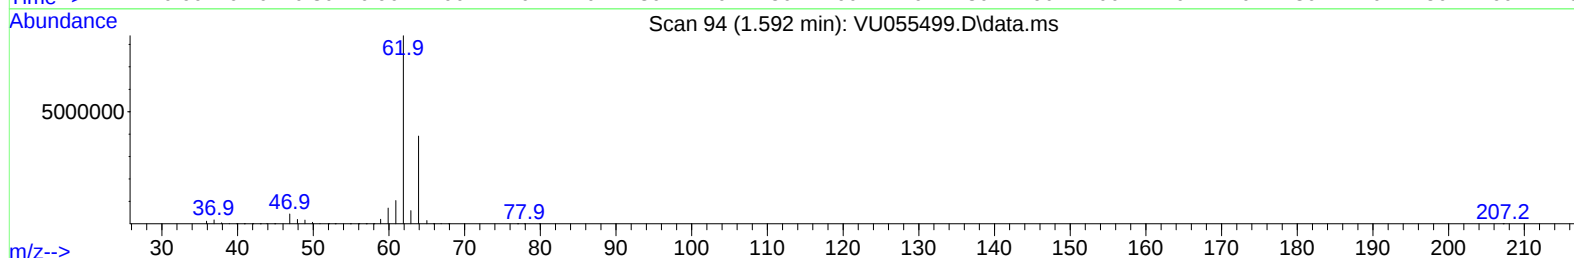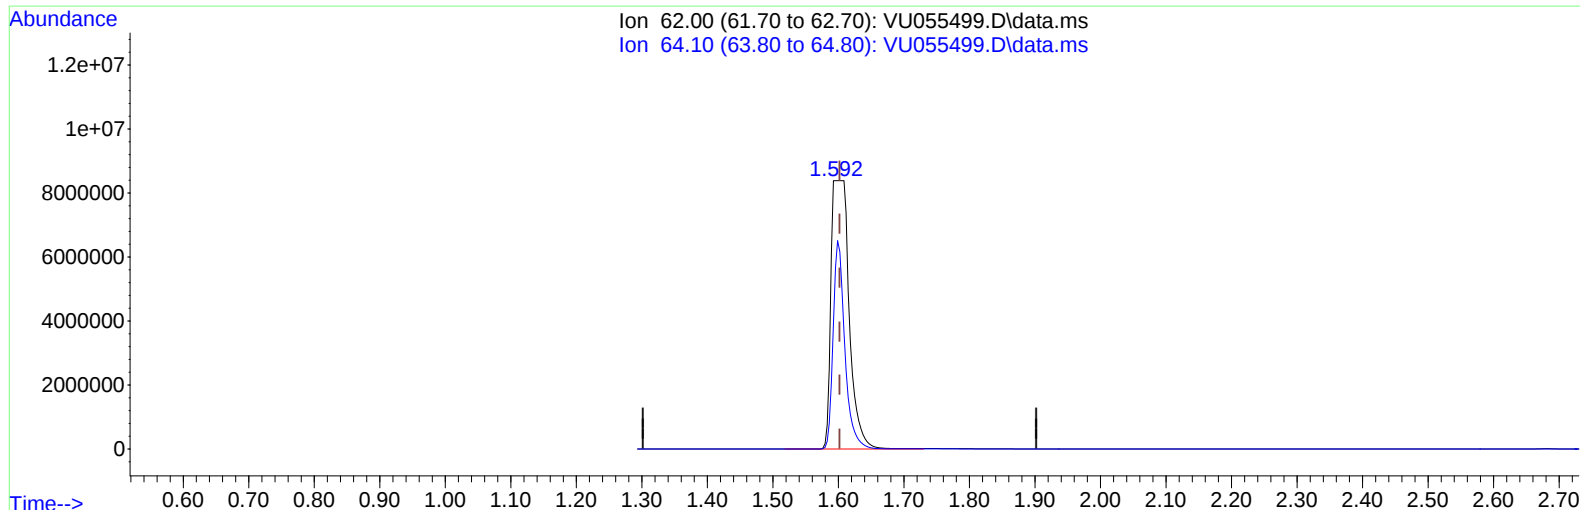

TIC: VU055499.D\data.ms

(5) Vinyl chloride (T)

1.592min (-0.009) 728.88 ug/L m

response 16236279

Ion	Exp%	Act%
62.00	100.00	100.00
64.10	31.90	46.68#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
 Data File : VU055499.D
 Acq On : 25 Sep 2023 16:47
 Operator : MD/SY
 Sample : 04579-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 25 01:08:17 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
 Supervised By :Semsettin Yesilyurt 09/28/2023

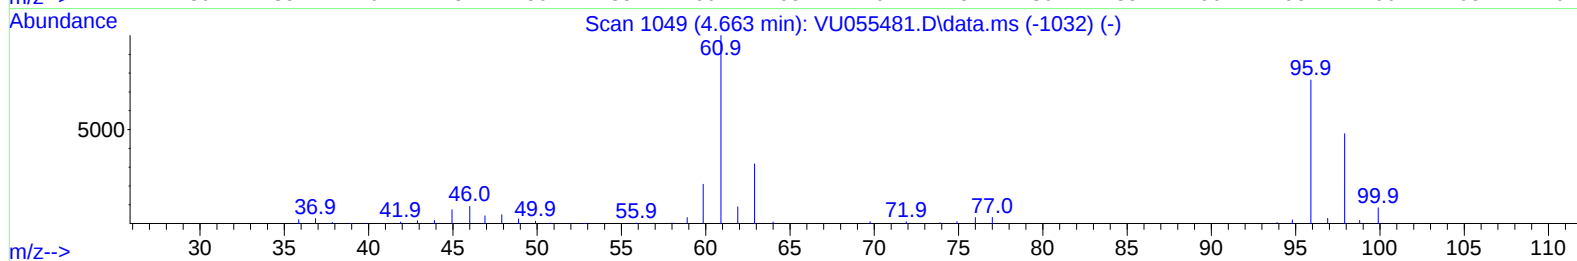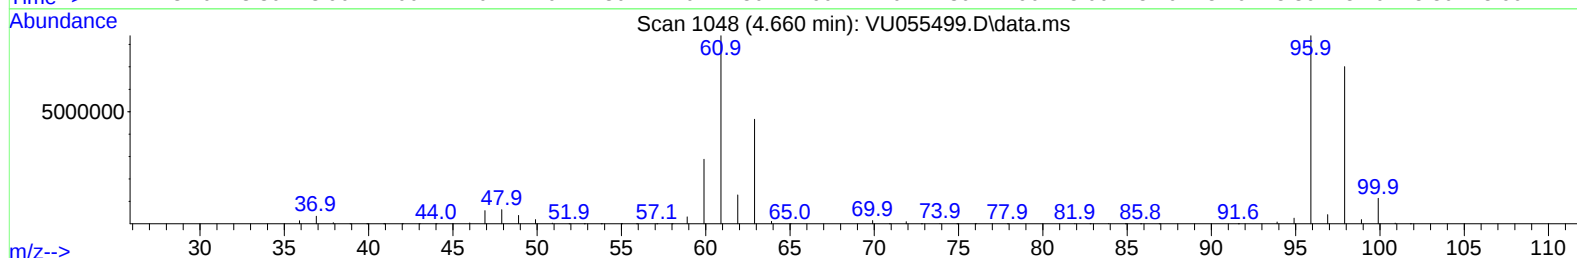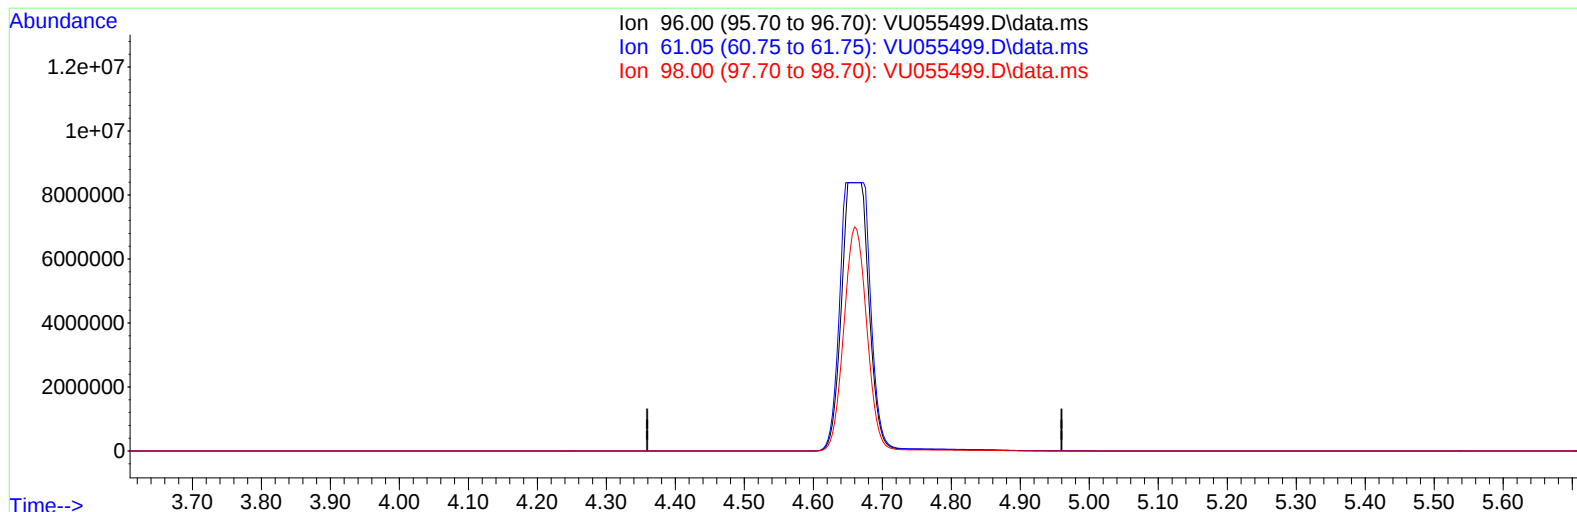

TIC: VU055499.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.660min (-4.660) 0.00 ug/L

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
61.05	125.50	0.00#
98.00	63.40	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
 Data File : VU055499.D
 Acq On : 25 Sep 2023 16:47
 Operator : MD/SY
 Sample : 04579-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 25 01:08:17 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
 Supervised By :Semsettin Yesilyurt 09/28/2023

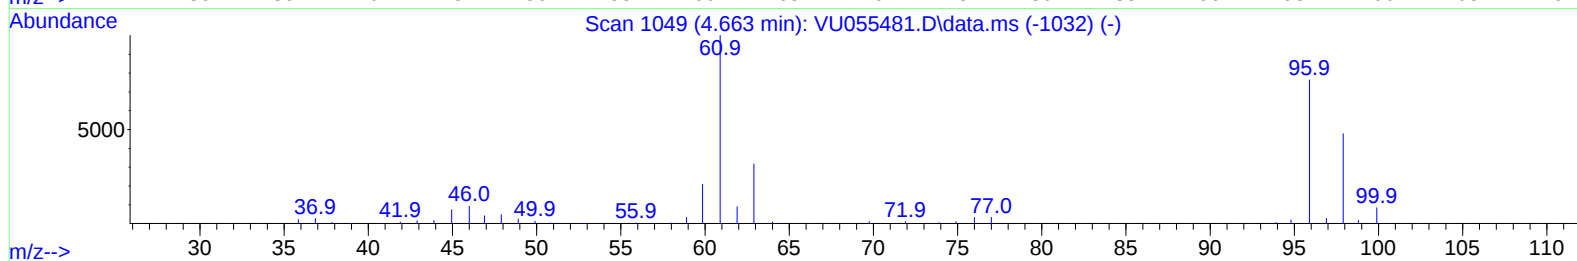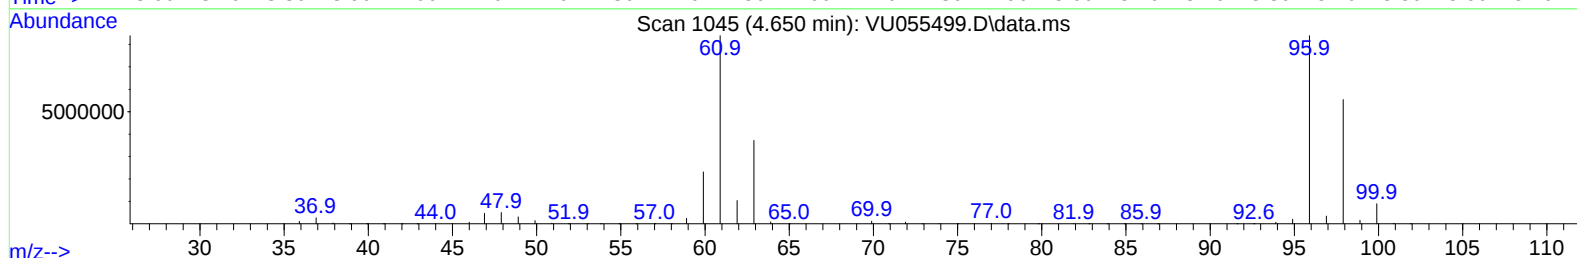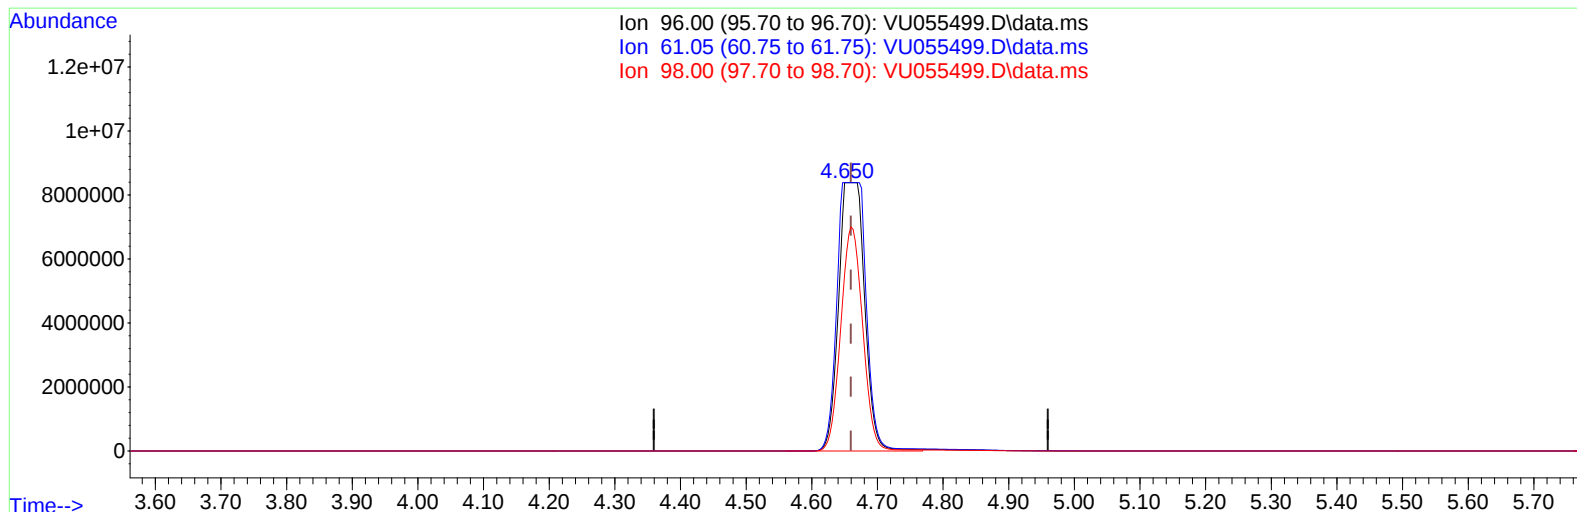

TIC: VU055499.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.650min (-0.009) 1168.57 ug/L m

response 23016999

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	125.50	100.00
98.00	63.40	66.07
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
 Data File : VU055499.D
 Acq On : 25 Sep 2023 16:47
 Operator : MD/SY
 Sample : 04579-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHY8

Manual IntegrationsAPPROVED

Quant Time: Sep 26 01:23:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 25 01:08:17 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/28/2023
 Supervised By :Semsettin Yesilyurt 09/28/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	241075	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	247859	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	124829	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	243325	9.986	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	199.800%#	
7) Chloroethane-d5	1.907	69	58820	2.739	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	54.800%#	
11) 1,1-Dichloroethene-d2	2.563	65	28495	2.841	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.800%#	
20) 2-Butanone-d5	4.631	46	343569	78.067	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	156.140%#	
24) Chloroform-d	5.058	84	169045	3.836	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	76.800%	
26) 1,2-Dichloroethane-d4	5.698	65	97146	4.583	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.600%	
32) Benzene-d6	5.724	84	306758	3.538	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	70.800%	
36) 1,2-Dichloropropane-d6	6.689	67	107015	4.131	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	82.600%	
41) Toluene-d8	7.894	98	250241	3.167	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	63.400%#	
43) trans-1,3-Dichloroprop...	8.177	79	41088	4.520	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.631	63	197124	71.292	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	142.580%#	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	115878	5.969	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	119.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	103805	4.120	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	82.400%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.592	62	16236279m	728.884	ug/L	
12) 1,1-Dichloroethene	2.576	96	24486	1.453	ug/L	# 63
18) trans-1,2-Dichloroethene	3.348	96	79279	4.667	ug/L	98
22) cis-1,2-Dichloroethene	4.650	96	23016999m	1168.573	ug/L	
33) Benzene	5.775	78	33633	0.471	ug/L	100
34) Trichloroethene	6.541	95	30400	1.507	ug/L	98
42) Toluene	7.972	91	14114	0.185	ug/L	96
53) m,p-Xylene	9.695	106	5091	0.167	ug/L	82
54) o-Xylene	10.103	106	4296	0.145	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed