

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
 Data File : VU055484.D
 Acq On : 25 Sep 2023 10:42
 Operator : MD/SY
 Sample : 04579-10DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHZ2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	85	96	113	rBV2	429117	524621	38.72%	4.447%
2	1.911	185	193	205	rBV	147880	191593	14.14%	1.624%
3	2.563	383	396	412	rBV	258546	421486	31.11%	3.573%
4	3.042	530	545	560	rVB3	12518	24312	1.79%	0.206%
5	3.181	573	588	602	rBV2	10419	25681	1.90%	0.218%
6	4.660	1025	1048	1074	rBV2	423865	1354992	100.00%	11.485%
7	5.058	1156	1172	1193	rBV	269164	592893	43.76%	5.025%
8	5.721	1355	1378	1405	rBV2	505017	1332196	98.32%	11.292%
9	6.245	1527	1541	1559	rBV	377411	723763	53.41%	6.135%
10	6.531	1619	1630	1642	rVB10	9064	19339	1.43%	0.164%
11	6.689	1664	1679	1697	rBV	311473	630531	46.53%	5.344%
12	7.563	1938	1951	1978	rBV2	148345	275120	20.30%	2.332%
13	7.894	2042	2054	2089	rBV	580082	1039007	76.68%	8.807%
14	8.177	2130	2142	2162	rBV	87675	160832	11.87%	1.363%
15	8.634	2272	2284	2327	rBV3	534578	1305327	96.33%	11.064%
16	9.415	2512	2527	2554	rBV	545121	939444	69.33%	7.963%
17	10.753	2931	2943	2963	rBV	241793	398889	29.44%	3.381%
18	11.811	3259	3272	3291	rBV	562743	926420	68.37%	7.852%
19	12.190	3371	3390	3413	rBV	533831	911539	67.27%	7.726%




Sum of corrected areas: 11797985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055484.D
Acq On : 25 Sep 2023 10:42
Operator : MD/SY
Sample : 04579-10DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

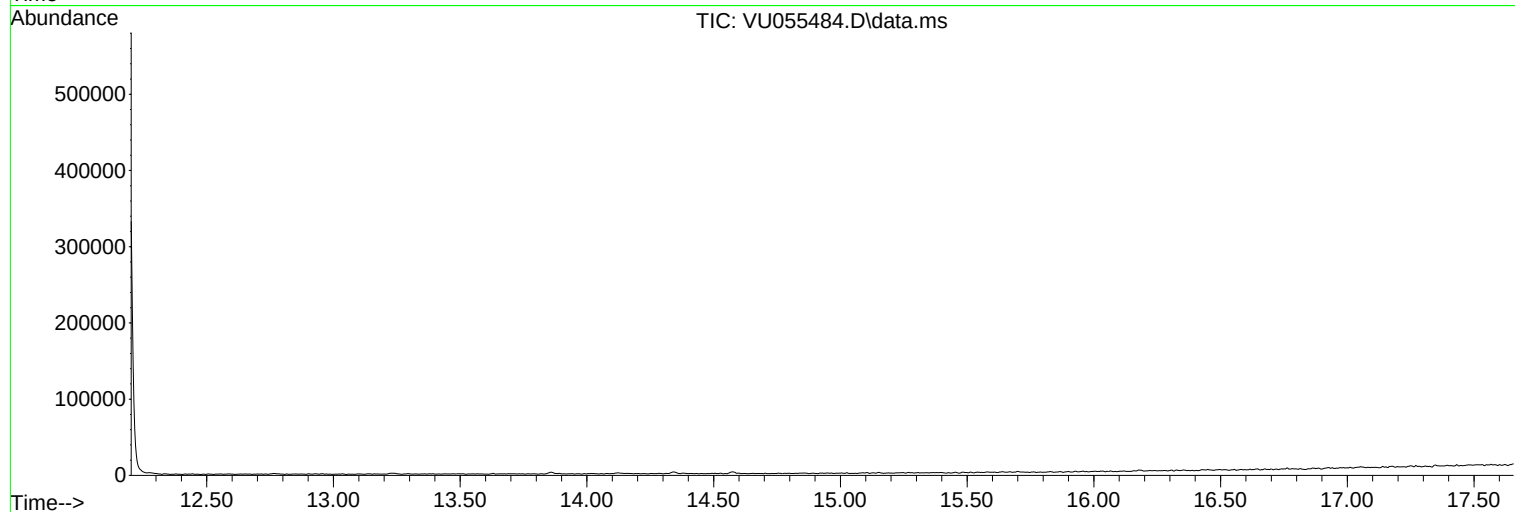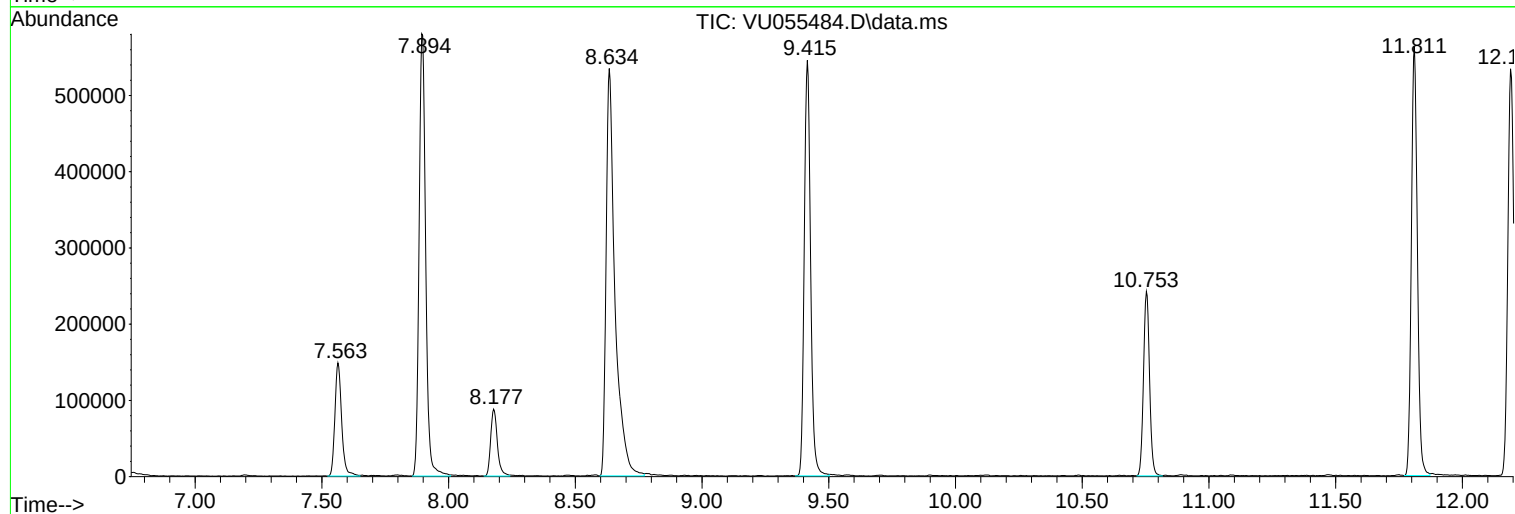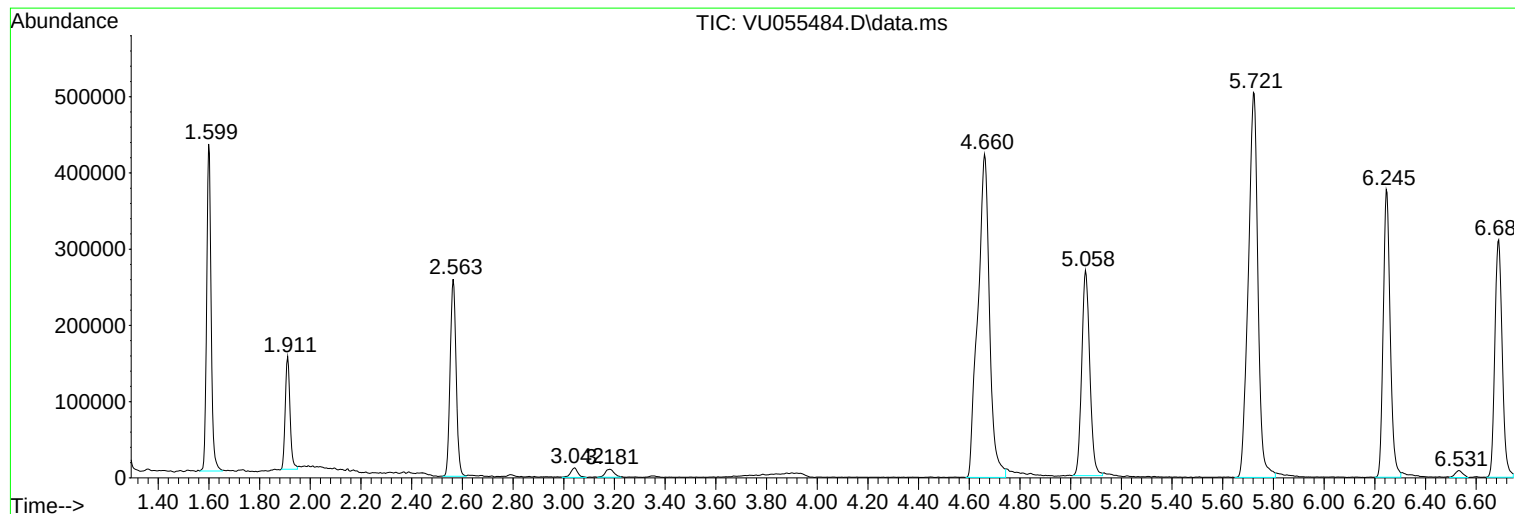

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055484.D
Acq On : 25 Sep 2023 10:42
Operator : MD/SY
Sample : 04579-10DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055484.D
Acq On : 25 Sep 2023 10:42
Operator : MD/SY
Sample : 04579-10DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc