


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092523\
Data File : VU055480.D
Acq On : 25 Sep 2023 08:25
Operator : MD/SY
Sample : BFB051
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB051

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 27 23:33:30 2023

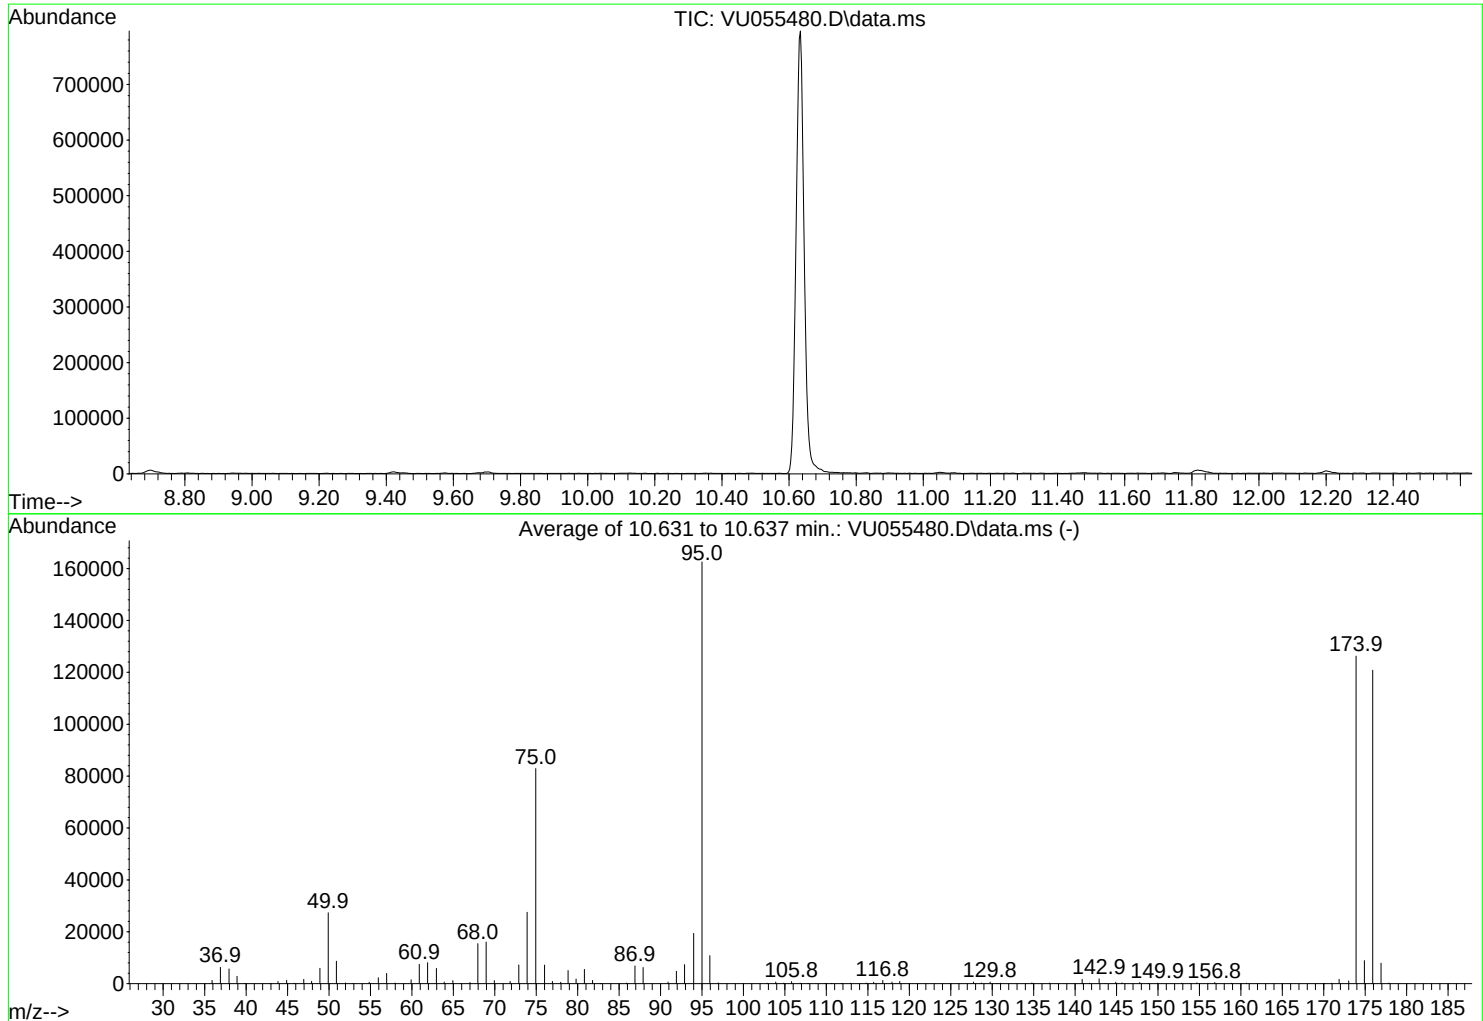

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	27315	PASS
75	95	30	80	51.0	82915	PASS
95	95	100	100	100.0	162603	PASS
96	95	5	9	6.6	10792	PASS
173	174	0.00	2	0.9	1075	PASS
174	95	50	120	77.6	126235	PASS
175	174	5	9	7.0	8881	PASS
176	174	95	101	95.7	120851	PASS
177	176	5	9	6.5	7890	PASS

m/z	Abundance
39.90	249.0
43.80	462.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

m/z	Abundance
35.90	1173.0
36.90	6059.0
38.00	5744.0
38.90	2978.0
39.80	318.0
43.90	1238.0
44.90	1252.0
45.80	253.0
46.90	1759.0
47.90	1017.0
48.90	5991.0
49.90	28136.0
50.90	9156.0
52.00	357.0
52.90	135.0
54.80	477.0
55.90	2230.0
56.90	4019.0
57.90	237.0
59.90	1441.0
60.90	7835.0
61.90	8285.0
63.00	6001.0
63.90	670.0
64.90	1181.0
66.90	542.0
68.00	15830.0
69.00	16341.0
70.00	1210.0
71.80	860.0
72.90	7179.0
73.90	28000.0
74.90	84320.0
76.00	7439.0
76.90	805.0
78.00	575.0
78.80	5111.0
79.80	1672.0
80.80	5689.0
81.80	1284.0
85.90	308.0
86.90	7028.0
87.90	6299.0
90.90	694.0
91.90	4816.0
92.90	7617.0
94.00	19984.0
95.00	166528.0
95.90	10710.0
96.90	329.0
102.80	158.0
103.90	628.0
104.80	237.0
105.80	863.0
106.80	251.0
107.80	154.0
109.90	150.0
110.60	152.0
111.80	111.0
112.90	152.0
114.80	279.0
115.70	585.0
116.80	1207.0
117.90	642.0
118.90	991.0
127.70	706.0
128.70	207.0
129.70	651.0
131.00	208.0
134.80	377.0
136.90	353.0
140.80	1579.0
141.80	201.0
142.90	1841.0
143.60	123.0
144.90	516.0
145.60	314.0
147.80	304.0
148.80	148.0
150.00	128.0
152.80	157.0
153.90	132.0
154.70	357.0
156.80	412.0
158.80	232.0
160.60	197.0
170.90	161.0
171.80	1581.0
173.00	1104.0
173.90	126152.0
174.90	9081.0
175.90	120568.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

176.907946.0

177.80230.0

Instrument :

MSVOA_U

ClientSampleId :

BFB051

m/z	Abundance
35.90	1254.0
36.90	6502.0
37.90	5829.0
38.90	2904.0
39.80	299.0
43.90	1272.0
44.90	1373.0
45.80	212.0
47.00	1722.0
47.90	909.0
48.90	6091.0
49.90	28088.0
50.90	8911.0
52.00	292.0
52.90	108.0
54.90	538.0
55.90	2395.0
57.00	4043.0
57.90	265.0
59.90	1475.0
60.90	7705.0
61.90	8400.0
63.00	6009.0
63.90	626.0
64.90	1262.0
65.90	115.0
67.00	460.0
68.00	15849.0
69.00	16608.0
69.90	1230.0
71.80	896.0
72.90	7495.0
73.90	28512.0
75.00	85576.0
76.00	7437.0
77.00	863.0
78.00	604.0
78.90	5203.0
79.80	1888.0
80.80	5689.0
81.80	1310.0
85.90	270.0
86.90	7051.0
87.90	6493.0
90.90	681.0
91.90	4964.0
92.90	7524.0
94.00	20016.0
95.00	167552.0
96.00	11201.0
96.90	324.0
102.80	190.0
103.90	603.0
104.90	206.0
105.80	829.0
106.80	188.0
107.80	108.0
109.80	155.0
110.60	150.0
112.90	169.0
114.80	260.0
115.70	579.0
116.80	1254.0
117.90	638.0
118.90	872.0
125.90	106.0
127.80	644.0
128.70	244.0
129.70	688.0
131.00	171.0
134.80	327.0
136.90	260.0
140.80	1730.0
141.70	221.0
142.90	1915.0
143.70	124.0
144.90	564.0
145.70	331.0
147.80	424.0
148.80	153.0
150.00	190.0
152.90	205.0
153.90	123.0
154.70	322.0
156.80	456.0
158.80	232.0
160.60	170.0
170.00	101.0
171.00	184.0
171.90	1736.0
173.00	1104.0
173.90	130232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

174.90	9143.0
175.90	124992.0
176.90	8137.0
177.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

m/z	Abundance
35.90	1199.0
36.90	6337.0
37.90	5549.0
38.90	2603.0
39.80	306.0
42.90	100.0
43.90	1263.0
44.90	1229.0
45.80	126.0
47.00	1585.0
47.90	729.0
48.90	5668.0
49.90	25720.0
50.90	7845.0
52.00	277.0
52.90	122.0
54.90	578.0
56.00	2240.0
56.90	3740.0
58.00	227.0
59.90	1455.0
60.90	6926.0
61.90	7589.0
62.90	5574.0
63.90	576.0
65.00	1138.0
65.90	111.0
67.10	381.0
67.90	14516.0
68.90	15199.0
69.90	1170.0
71.90	782.0
72.90	6960.0
73.90	25968.0
75.00	78848.0
76.00	6609.0
77.00	892.0
77.90	537.0
78.90	4848.0
79.80	1737.0
80.80	5032.0
81.80	1150.0
82.70	117.0
85.90	178.0
86.90	6466.0
87.90	5994.0
90.90	580.0
91.90	4504.0
92.90	6885.0
94.00	18056.0
95.00	153728.0
96.00	10465.0
97.00	328.0
102.90	158.0
103.90	642.0
104.90	208.0
105.80	672.0
106.90	158.0
107.80	106.0
109.80	145.0
110.70	128.0
112.90	190.0
114.80	212.0
115.70	560.0
116.80	1227.0
117.90	678.0
118.80	812.0
125.90	143.0
127.80	580.0
128.70	240.0
129.80	592.0
130.60	119.0
131.00	140.0
134.80	289.0
136.80	175.0
140.90	1716.0
141.80	224.0
142.90	1814.0
144.90	601.0
145.70	311.0
147.80	542.0
148.80	121.0
149.90	200.0
152.90	194.0
154.70	345.0
156.90	367.0
158.90	173.0
160.70	150.0
171.00	150.0
171.90	1684.0
173.00	1017.0
173.90	122320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

174.90	8420.0
175.90	116992.0
176.90	7588.0
177.80	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051