


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092524\
Data File : VU060995.D
Acq On : 25 Sep 2024 10:23
Operator : MD/SY
Sample : BFB005
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB005

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 26 05:34:11 2024

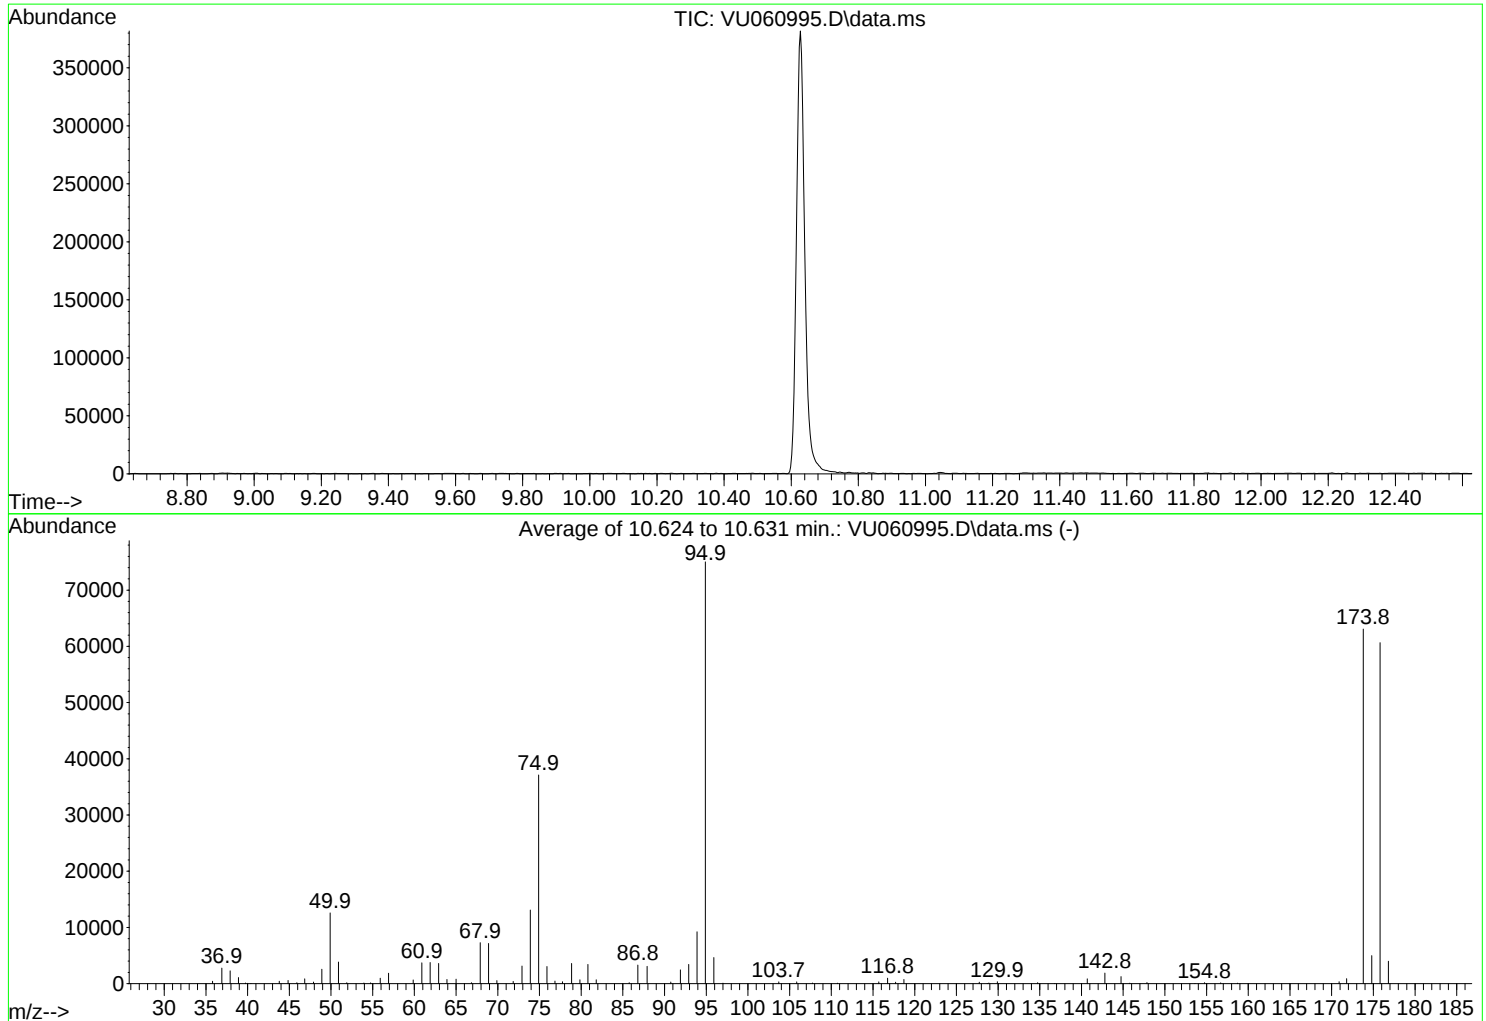

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	12575	PASS
75	95	30	80	49.5	37117	PASS
95	95	100	100	100.0	75029	PASS
96	95	5	9	6.2	4650	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	63072	PASS
175	174	5	9	7.9	4971	PASS
176	174	95	101	96.2	60645	PASS
177	176	5	9	6.6	3981	PASS

m/z	Abundance
43.90	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.70	455.0
36.90	2706.0
37.90	2242.0
38.90	1064.0
39.70	159.0
40.40	114.0
43.80	623.0
44.90	562.0
45.90	164.0
46.90	914.0
47.90	275.0
48.90	2453.0
49.90	12492.0
50.90	4025.0
52.00	190.0
53.90	145.0
54.70	120.0
55.90	928.0
56.90	1866.0
59.80	687.0
60.90	3567.0
61.90	3921.0
62.90	3359.0
63.90	698.0
65.00	794.0
66.90	188.0
67.90	7114.0
68.90	7332.0
69.90	508.0
71.80	347.0
72.90	3060.0
73.90	13272.0
74.90	37480.0
75.90	3324.0
76.80	552.0
77.70	377.0
78.80	3500.0
79.90	692.0
80.80	3268.0
81.80	684.0
85.80	160.0
86.80	3230.0
87.90	2995.0
90.80	352.0
91.90	2440.0
92.90	3542.0
93.90	9104.0
94.90	75176.0
95.90	4738.0
97.00	117.0
103.70	343.0
105.80	294.0
107.90	110.0
115.70	282.0
116.70	840.0
117.70	290.0
118.70	783.0
127.80	297.0
128.70	127.0
129.90	431.0
134.80	159.0
140.70	836.0
142.80	1821.0
144.70	1217.0
145.80	137.0
147.90	239.0
154.70	200.0
156.70	143.0
158.70	135.0
170.90	329.0
171.90	906.0
173.80	61840.0
174.80	4944.0
175.80	58888.0
176.80	4070.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.80	442.0
36.90	2884.0
37.90	2304.0
38.90	1154.0
39.80	161.0
43.80	692.0
44.80	582.0
45.90	185.0
46.90	866.0
47.90	295.0
48.90	2631.0
49.90	13060.0
50.90	3918.0
51.90	164.0
53.90	123.0
54.80	173.0
55.90	999.0
56.90	1911.0
59.90	665.0
60.90	3822.0
61.90	3880.0
62.90	3631.0
63.90	746.0
65.00	801.0
66.90	199.0
67.90	7550.0
68.90	7327.0
69.90	526.0
71.90	433.0
72.90	3233.0
73.90	13586.0
74.90	37872.0
75.90	3077.0
76.90	473.0
77.70	330.0
78.80	3759.0
79.80	697.0
80.80	3504.0
81.80	717.0
85.70	190.0
86.80	3460.0
87.90	3251.0
90.80	274.0
91.90	2561.0
92.90	3532.0
93.90	9600.0
94.90	77672.0
95.90	4806.0
97.00	130.0
103.70	331.0
105.90	315.0
107.70	104.0
110.70	122.0
115.70	329.0
116.80	998.0
117.70	289.0
118.70	779.0
127.70	274.0
128.90	152.0
129.90	327.0
134.70	167.0
140.70	904.0
142.80	1925.0
144.70	1297.0
145.80	103.0
147.90	169.0
154.80	163.0
156.70	163.0
158.70	107.0
170.90	370.0
171.80	911.0
173.80	64872.0
174.80	5101.0
175.80	62424.0
176.80	4156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	391.0
36.90	2689.0
37.90	2292.0
38.90	1059.0
40.00	169.0
43.80	668.0
44.80	525.0
45.90	150.0
46.80	775.0
47.90	297.0
48.90	2611.0
49.90	12174.0
50.90	3577.0
51.80	204.0
54.00	105.0
54.80	180.0
55.90	1021.0
56.90	1818.0
59.90	604.0
60.90	3680.0
61.90	3485.0
62.90	3739.0
63.90	748.0
65.00	825.0
66.00	127.0
66.80	159.0
67.90	7197.0
68.90	6738.0
69.90	556.0
71.90	439.0
72.90	3087.0
73.90	12420.0
74.90	36000.0
75.90	2725.0
76.90	374.0
77.80	292.0
78.90	3542.0
79.80	671.0
80.80	3445.0
81.80	647.0
85.70	175.0
86.80	3223.0
87.90	2984.0
90.70	259.0
91.90	2338.0
92.90	3199.0
93.90	8997.0
94.90	72240.0
95.90	4405.0
103.70	294.0
105.90	292.0
107.70	109.0
110.80	127.0
115.70	362.0
116.80	1071.0
117.70	224.0
118.70	639.0
127.70	229.0
128.90	166.0
129.90	240.0
134.70	176.0
136.80	114.0
140.70	833.0
142.80	1886.0
144.80	1251.0
147.80	159.0
153.60	106.0
154.80	144.0
156.70	163.0
170.90	368.0
171.70	880.0
173.80	62504.0
174.80	4867.0
175.80	60624.0
176.80	3717.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005