

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092525\
 Data File : VU063642.D
 Acq On : 25 Sep 2025 10:32
 Operator : MD/SY
 Sample : VU0925WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK026

Quant Time: Sep 26 05:11:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 25 04:13:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	6424	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	8821	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152	2800	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	2290	0.531	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.000%
4) 1,2-Dichloroethane-d4	5.709	65	1231	0.481	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
7) 1,2-Dichloropropane-d6	6.687	67	1339	0.579	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.887	98	3754	0.507	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1094	0.531	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
6) Trichloroethene	6.544	95	129	0.025	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092525\
Data File : VU063642.D
Acq On : 25 Sep 2025 10:32
Operator : MD/SY
Sample : VU0925WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK026


Quant Time: Sep 26 05:11:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:13:39 2025
Response via : Initial Calibration

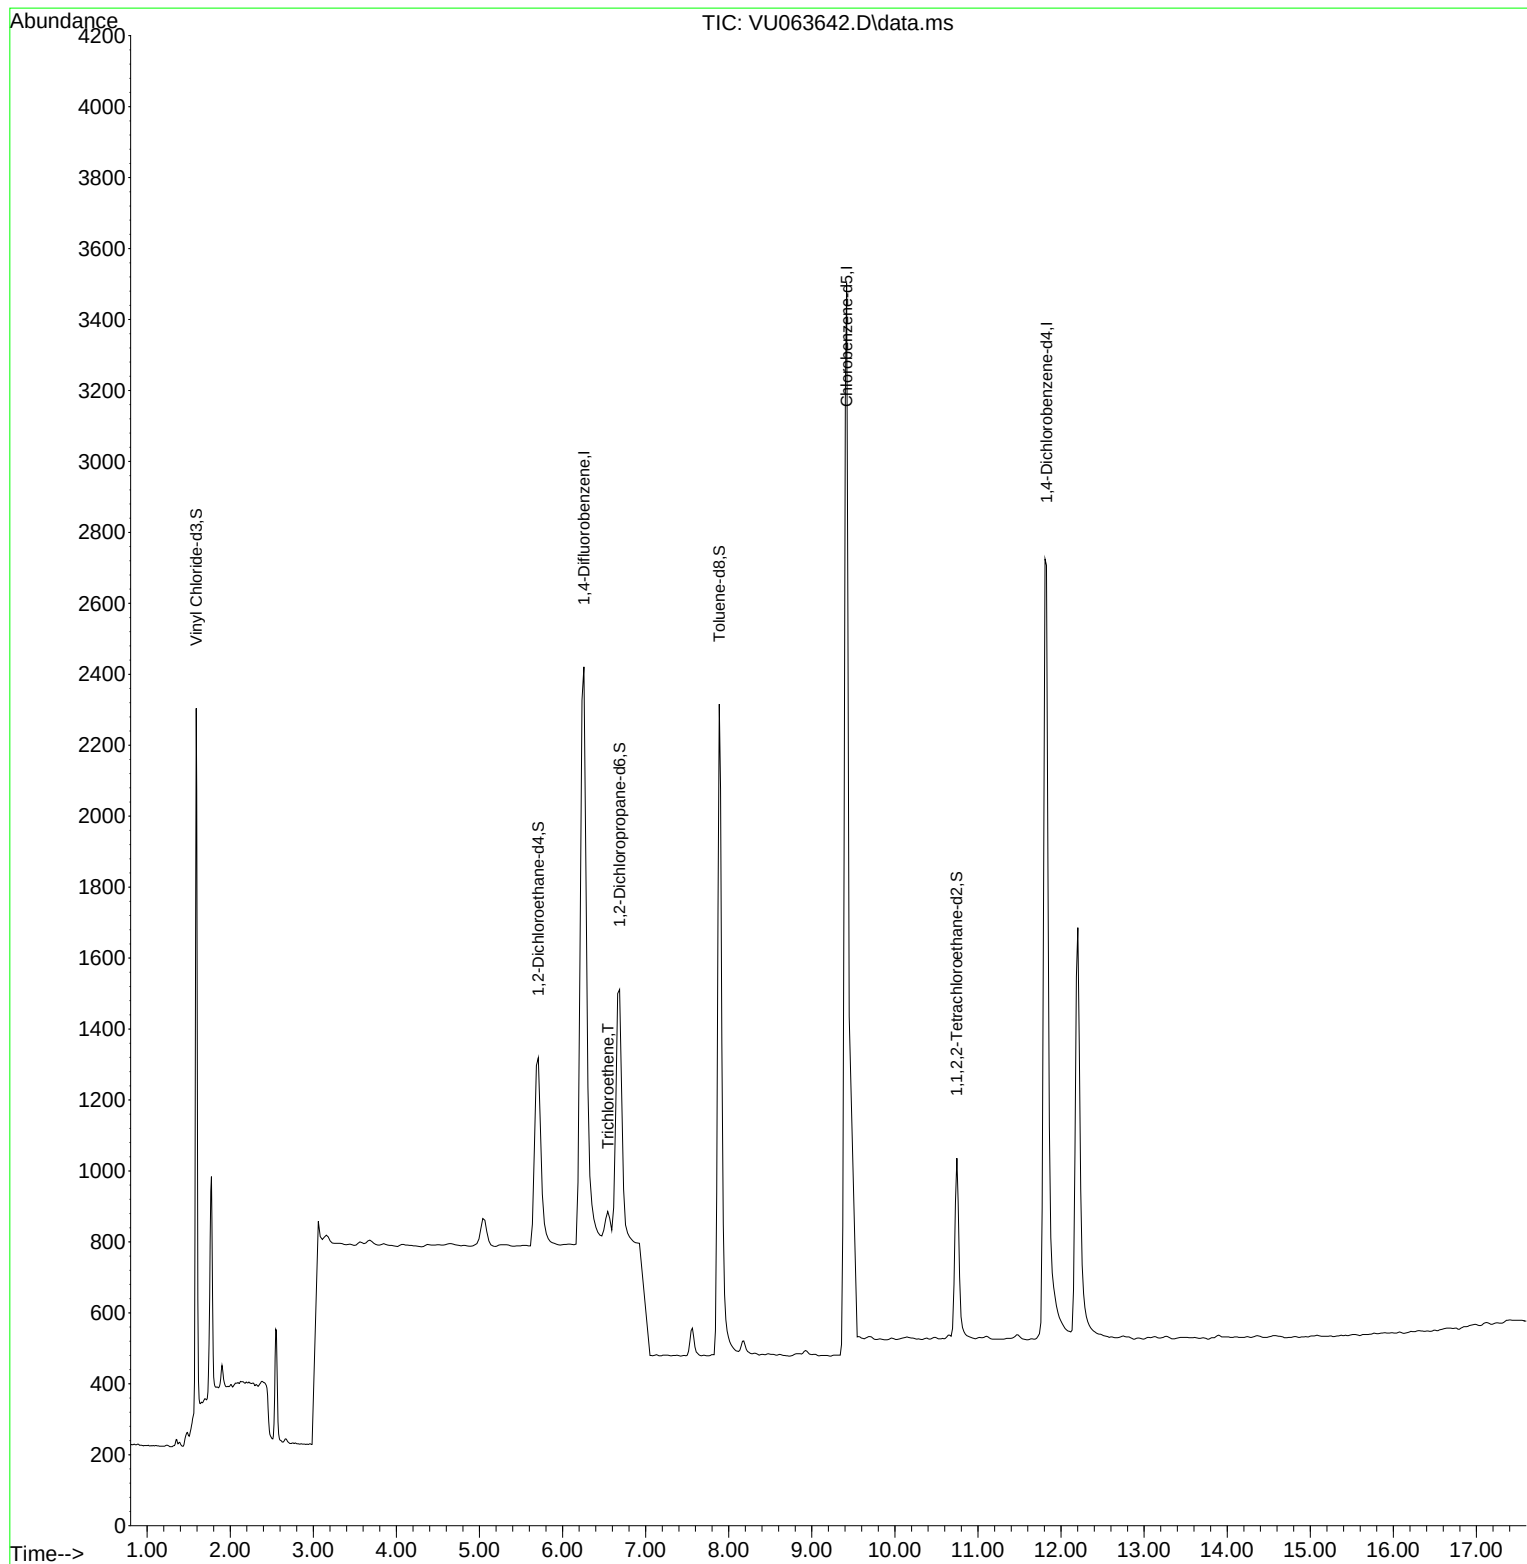

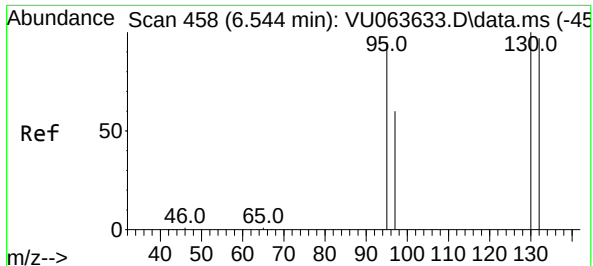

#6
 Trichloroethene
 Concen: 0.025 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. -0.000 min
 Lab File: VU063642.D
 Acq: 25 Sep 2025 10:32

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK026

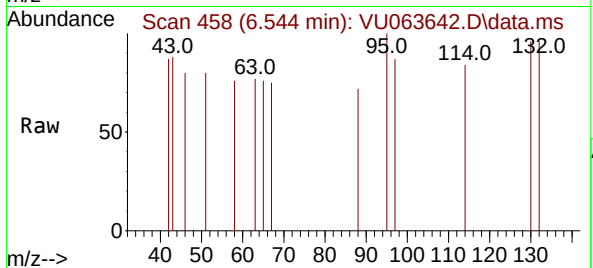

Tgt Ion: 95	Resp: 129
Ion Ratio	Lower Upper
95 100	
97 86.7	46.8 87.0
132 96.0	71.0 131.8
130 96.0	73.4 136.2

