


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092525\
Data File : VU063640.D
Acq On : 25 Sep 2025 08:47
Operator : MD/SY
Sample : BFB027
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB027

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 25 04:13:39 2025

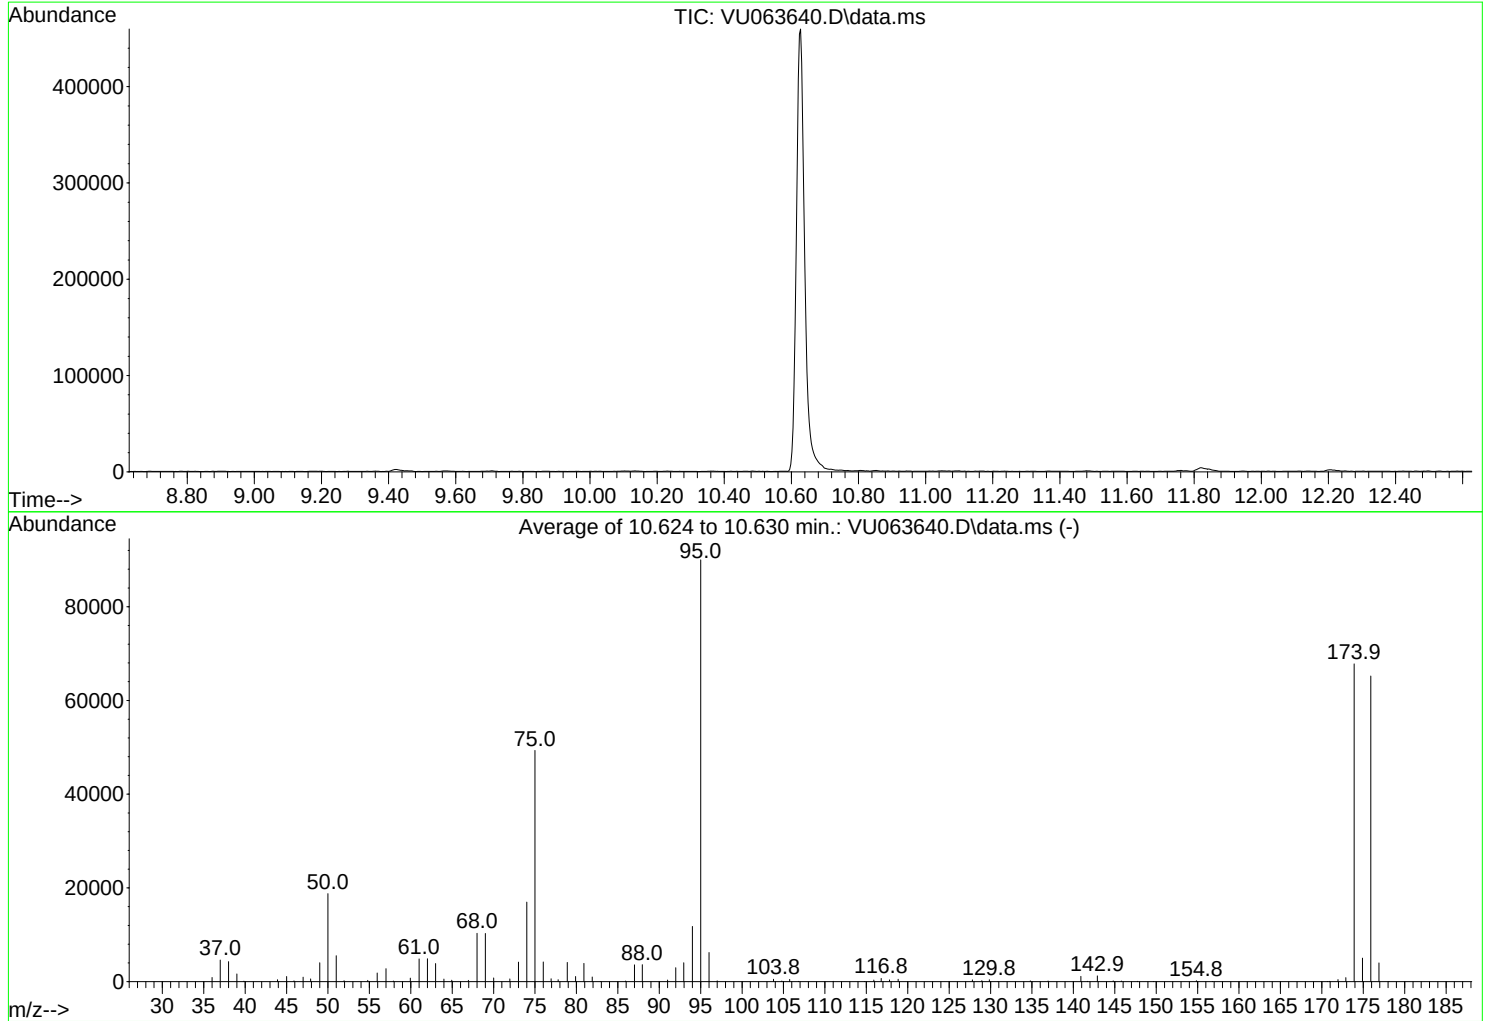

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	18768	PASS
75	95	30	80	54.8	49333	PASS
95	95	100	100	100.0	90000	PASS
96	95	5	9	6.9	6226	PASS
173	174	0.00	2	1.3	863	PASS
174	95	50	120	75.3	67797	PASS
175	174	5	9	7.4	5012	PASS
176	174	95	101	96.2	65203	PASS
177	176	5	9	6.1	4007	PASS