


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092618\
Data File : VU027138.D
Acq On : 25 Sep 2018 18:50
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

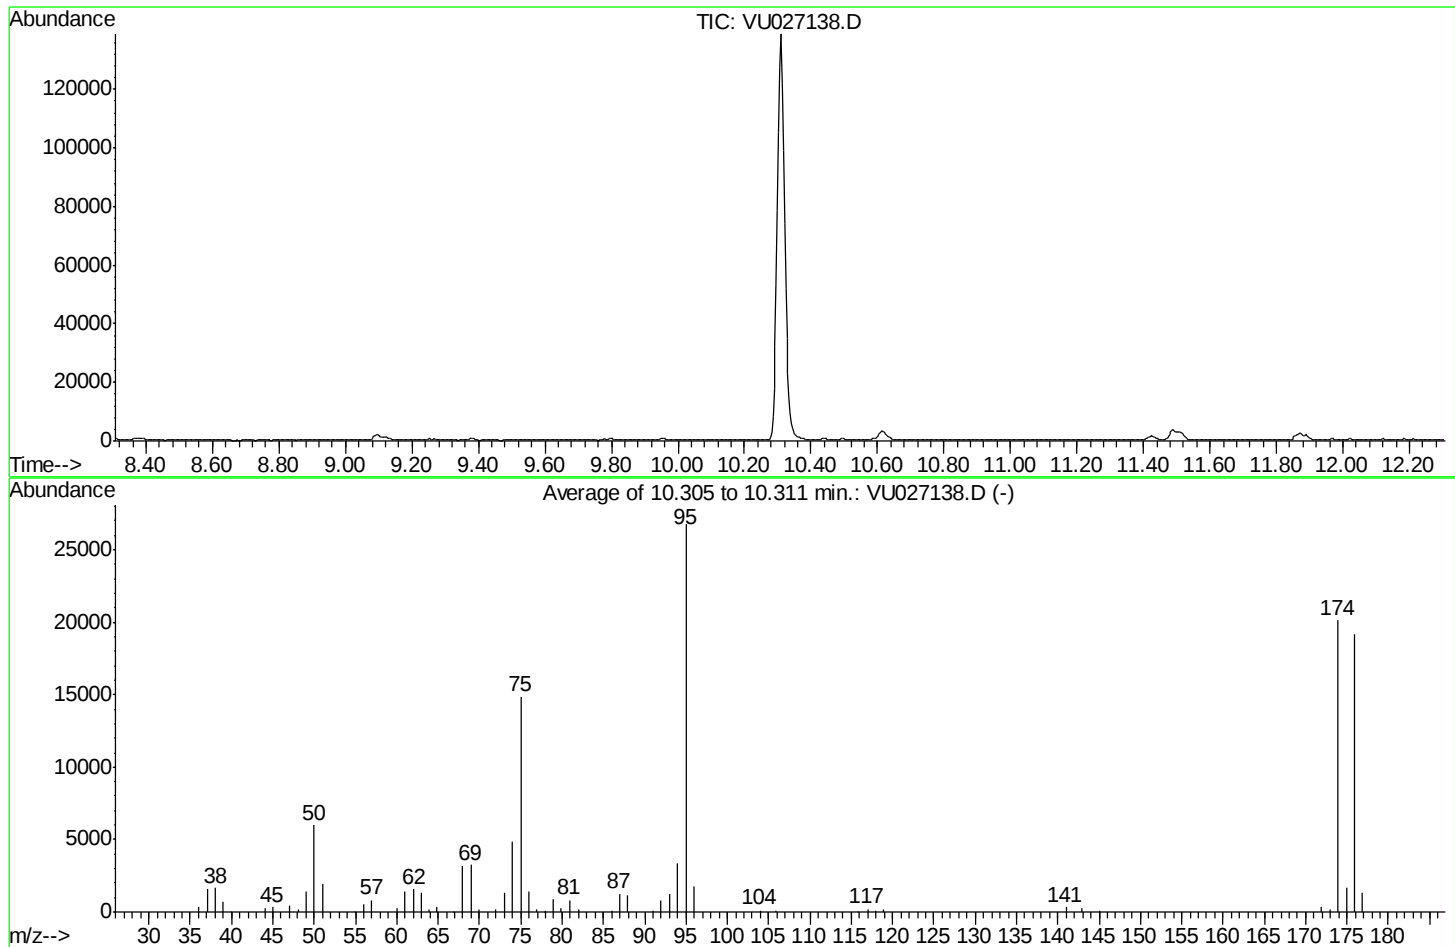

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5977	PASS
75	95	30	60	55.5	14844	PASS
95	95	100	100	100.0	26754	PASS
96	95	5	9	6.7	1781	PASS
173	174	0.00	2	1.0	209	PASS
174	95	50	100	75.3	20136	PASS
175	174	5	9	8.2	1658	PASS
176	174	95	101	95.0	19133	PASS
177	176	5	9	6.9	1314	PASS