


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092618\
Data File : VU027188.D
Acq On : 26 Sep 2018 19:44
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

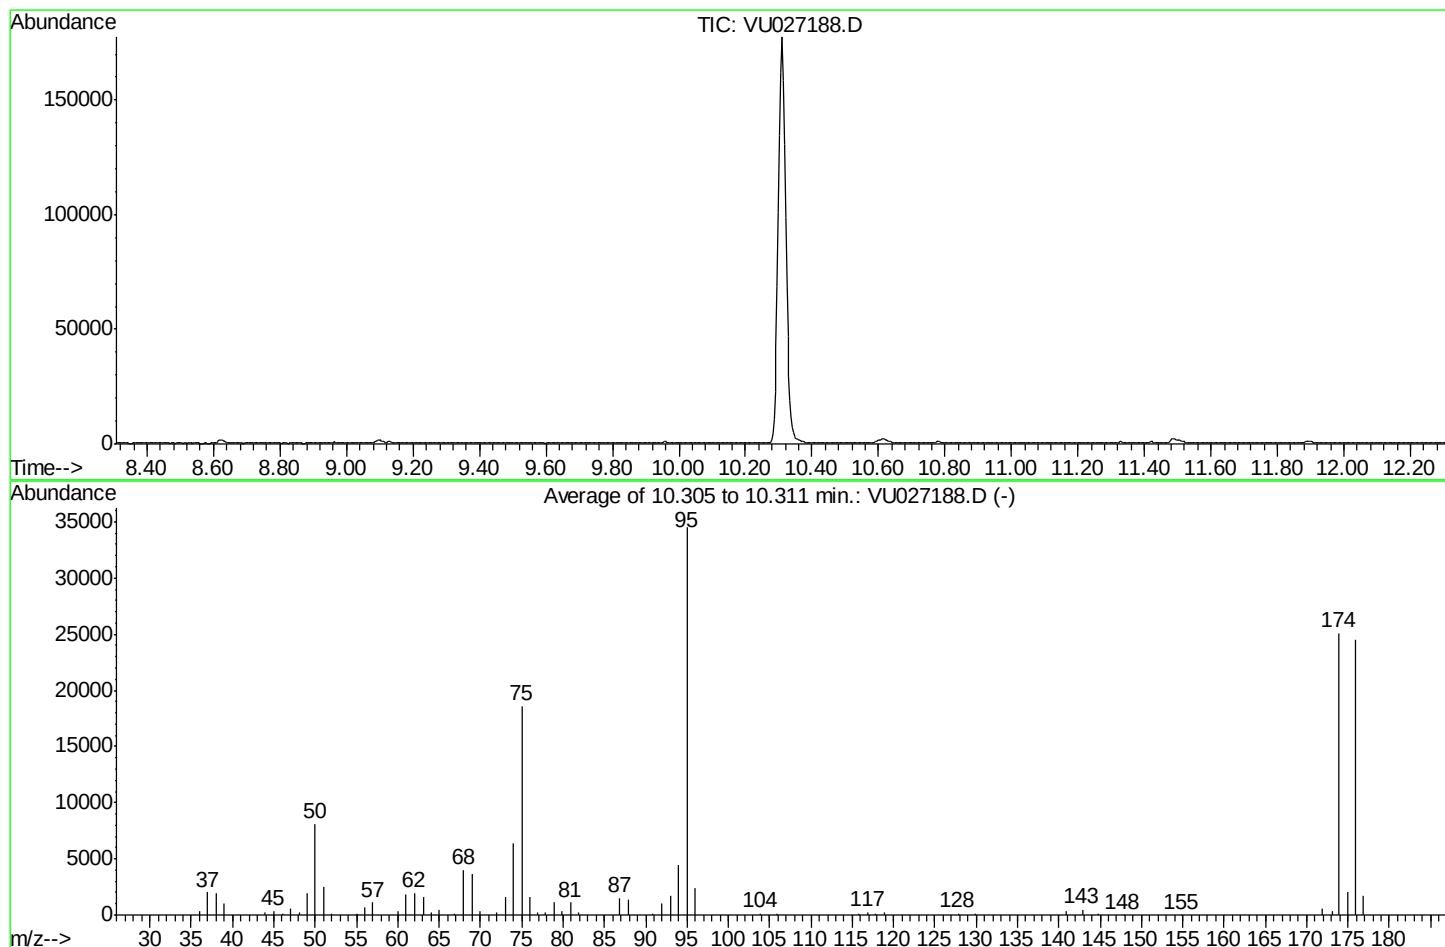

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	8099	PASS
75	95	30	60	53.9	18600	PASS
95	95	100	100	100.0	34514	PASS
96	95	5	9	7.1	2436	PASS
173	174	0.00	2	1.3	327	PASS
174	95	50	100	72.7	25104	PASS
175	174	5	9	8.1	2029	PASS
176	174	95	101	97.4	24453	PASS
177	176	5	9	6.9	1689	PASS