


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092619\
Data File : VU034833.D
Acq On : 26 Sep 2019 08:48
Operator : JC/SP
Sample : BFB39
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Title : VOC Analysis
Last Update : Thu Sep 26 17:15:20 2019

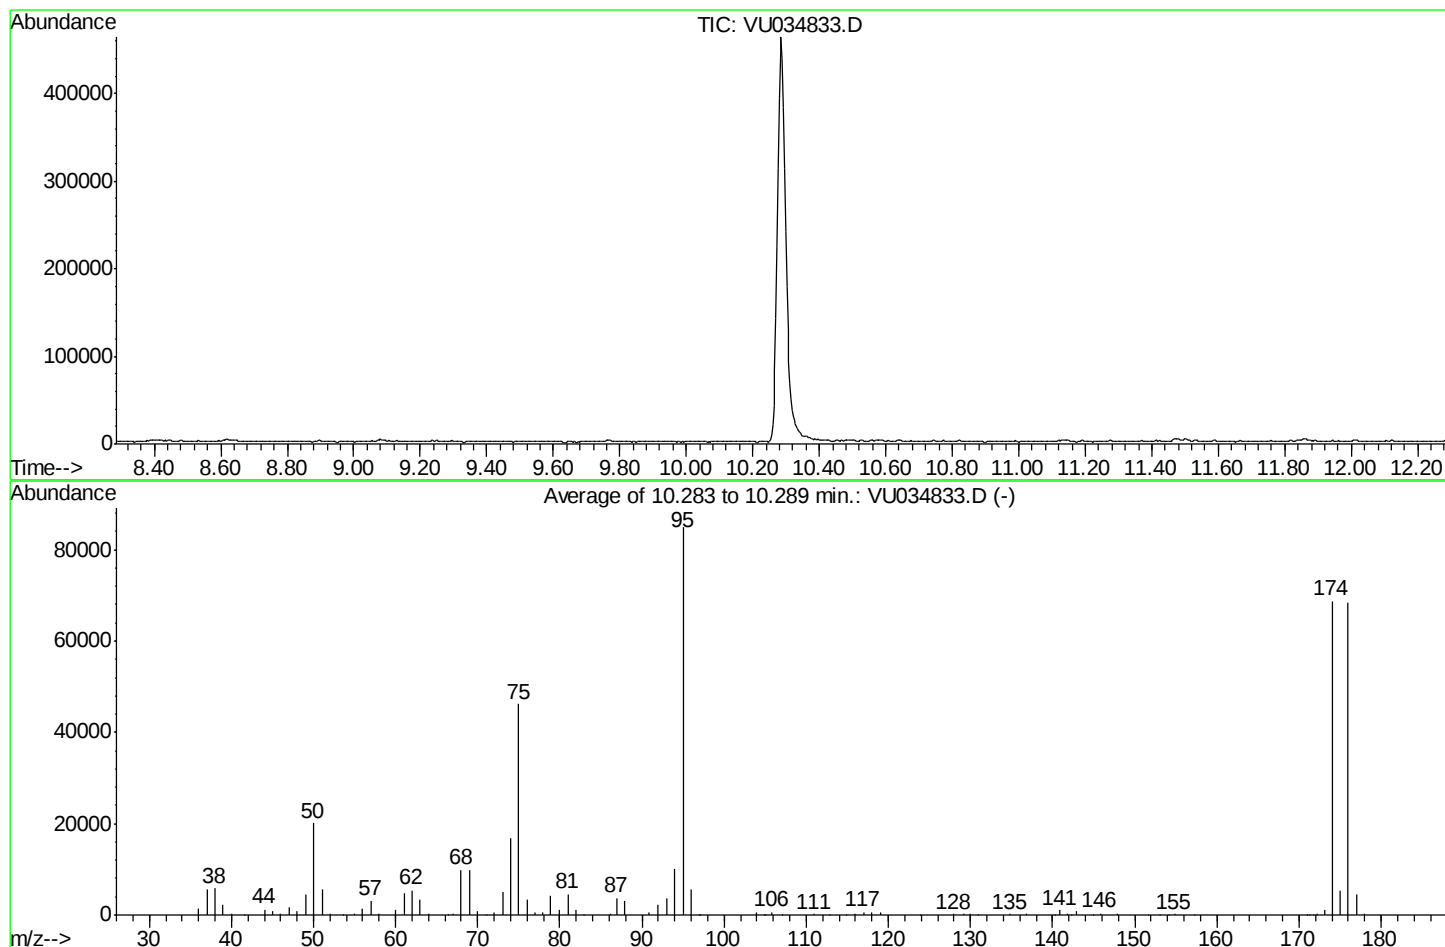

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	20106	PASS
75	95	30	80	54.4	46216	PASS
95	95	100	100	100.0	84893	PASS
96	95	5	9	6.6	5566	PASS
173	174	0.00	2	1.5	1009	PASS
174	95	50	120	80.9	68714	PASS
175	174	5	9	7.7	5265	PASS
176	174	95	101	99.5	68352	PASS
177	176	5	9	6.5	4438	PASS

m/z	Abundance
36.00	1429.0
37.00	5859.0
38.00	5739.0
39.00	2340.0
40.10	418.0
41.60	159.0
43.10	342.0
44.00	1737.0
45.00	1206.0
45.90	145.0
47.00	1689.0
48.10	590.0
49.00	4584.0
50.00	20976.0
51.00	5727.0
52.00	382.0
54.90	232.0
56.00	1633.0
57.00	3020.0
58.00	105.0
59.90	1382.0
61.00	4887.0
62.00	5310.0
63.00	3266.0
63.90	406.0
66.40	114.0
67.00	341.0
68.00	10306.0
69.00	10161.0
70.00	1071.0
72.00	459.0
73.00	5111.0
74.00	16648.0
75.00	46368.0
76.00	3203.0
76.90	506.0
77.90	489.0
78.90	4236.0
79.90	1300.0
80.90	4319.0
81.90	1201.0
83.00	136.0
86.90	3835.0
87.90	3203.0
90.80	500.0
92.00	2391.0
93.00	3450.0
94.00	10254.0
95.00	84664.0
96.10	5670.0
96.90	166.0
103.90	474.0
104.80	155.0
105.80	666.0
111.00	246.0
112.80	138.0
116.00	433.0
116.90	590.0
117.90	498.0
119.00	731.0
128.00	252.0
129.10	176.0
129.90	246.0
134.90	291.0
136.80	166.0
140.90	928.0
141.70	199.0
142.20	124.0
143.00	884.0
145.80	287.0
147.90	355.0
151.70	130.0
153.10	109.0
154.10	131.0
154.80	161.0
157.20	112.0
171.30	149.0
171.80	258.0
172.20	256.0
173.20	1370.0
174.00	67520.0
175.00	5129.0
176.00	66400.0
177.00	4391.0
177.90	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1504.0
37.00	5969.0
38.00	6059.0
39.00	2488.0
40.00	524.0
41.60	137.0
42.00	103.0
42.90	339.0
44.00	1928.0
45.00	1236.0
45.90	226.0
47.00	1756.0
48.10	771.0
49.00	4666.0
50.00	20720.0
51.10	5645.0
52.10	395.0
53.70	127.0
55.00	208.0
55.90	1456.0
57.00	3154.0
58.00	165.0
59.90	1420.0
61.00	5082.0
62.00	5690.0
63.00	3553.0
63.90	373.0
67.00	325.0
68.00	10264.0
69.00	10232.0
70.00	895.0
71.10	139.0
72.00	544.0
73.00	5326.0
74.00	17144.0
75.00	47624.0
76.00	3427.0
76.90	584.0
77.90	492.0
78.90	4392.0
79.90	1121.0
81.00	4718.0
81.90	1154.0
82.90	115.0
86.20	231.0
86.90	3716.0
88.00	3239.0
90.90	451.0
92.00	2261.0
93.00	3783.0
94.00	10425.0
95.00	87416.0
96.00	5688.0
97.10	115.0
103.90	562.0
105.00	163.0
105.80	693.0
107.10	135.0
111.00	267.0
112.80	148.0
114.80	148.0
116.00	419.0
117.00	727.0
117.90	545.0
119.00	642.0
123.90	104.0
128.00	248.0
129.20	177.0
129.90	229.0
134.90	278.0
136.80	217.0
141.00	1105.0
141.80	197.0
142.90	852.0
144.90	112.0
145.90	352.0
147.80	373.0
151.70	153.0
153.10	116.0
154.10	110.0
154.90	167.0
158.80	108.0
170.90	130.0
171.20	105.0
172.10	326.0
173.20	1657.0
174.00	70688.0
175.00	5385.0
176.00	70472.0
177.00	4663.0
178.00	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1381.0
37.00	5369.0
38.00	5848.0
39.00	2237.0
40.00	602.0
42.00	119.0
43.00	315.0
44.00	1871.0
45.10	1123.0
46.00	197.0
47.00	1462.0
48.00	808.0
49.00	4353.0
50.00	18624.0
51.10	5782.0
52.10	331.0
53.60	143.0
55.10	250.0
56.00	1367.0
57.00	3188.0
58.00	218.0
59.90	1219.0
61.00	4646.0
62.00	5382.0
63.00	3612.0
64.00	375.0
67.00	295.0
68.00	9271.0
69.00	9359.0
70.00	688.0
71.10	167.0
72.00	750.0
73.00	4923.0
74.00	16520.0
75.00	44656.0
76.00	3453.0
76.90	596.0
77.90	418.0
78.90	4265.0
79.90	876.0
81.00	4626.0
81.90	959.0
82.90	100.0
86.20	273.0
86.90	3609.0
88.00	3041.0
90.90	365.0
91.90	2360.0
93.00	3604.0
94.00	10026.0
95.00	82600.0
96.00	5341.0
97.10	134.0
103.90	507.0
105.00	189.0
105.90	592.0
107.10	129.0
111.00	195.0
112.80	124.0
114.90	188.0
116.00	389.0
117.00	710.0
117.90	476.0
119.00	591.0
123.90	198.0
128.00	307.0
129.20	143.0
129.90	203.0
130.90	131.0
134.80	225.0
136.80	201.0
140.20	156.0
140.90	1228.0
141.80	143.0
142.90	920.0
144.80	156.0
145.90	380.0
147.80	255.0
151.70	102.0
154.20	107.0
154.90	173.0
158.90	157.0
170.90	141.0
172.10	409.0
174.00	67936.0
175.00	5283.0
176.00	68184.0
177.00	4260.0
177.90	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

Scan 2847 (10.244 min): VU034833.D
BFB39

m/z	Abundance
36.40	108.0
39.00	119.0
40.00	322.0
42.00	110.0
43.00	358.0
44.00	698.0
45.00	305.0
59.90	141.0
122.70	136.0
158.70	104.0
207.20	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39