

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092620\
 Data File : VU040305.D
 Acq On : 25 Sep 2020 17:27
 Operator : SY/MD
 Sample : L4147-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFST2

Manual Integrations
 APPROVED

MMDadoda
 9/28/2020 10:47:28 AM

Quant Time: Sep 26 07:00:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 26 06:44:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	124163	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	125638	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	58009	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	33883	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.92	69	32530	5.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.20%
11) 1,1-Dichloroethene-d2	2.58	63	55741	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	4.66	46	163156	60.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.34%
24) Chloroform-d	5.08	84	75939	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.72	65	47242	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.74	84	141176	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.70	67	49778	5.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.00%
41) Toluene-d8	7.90	98	114232	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	8.19	79	18984	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.64	63	112833	53.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.26%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	42810	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	47392	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%

Target Compounds					Ovalue
3) Chloromethane	1.52	50	12165	1.031 ug/L	99
13) Acetone	2.66	43	19528m	7.780 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092620\
Data File : VU040305.D
Acq On : 25 Sep 2020 17:27
Operator : SY/MD
Sample : L4147-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BFST2

Manual Integrations
APPROVED

MMDadoda
9/28/2020 10:47:28 AM

Quant Time: Sep 26 07:00:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 26 06:44:13 2020
Response via : Initial Calibration

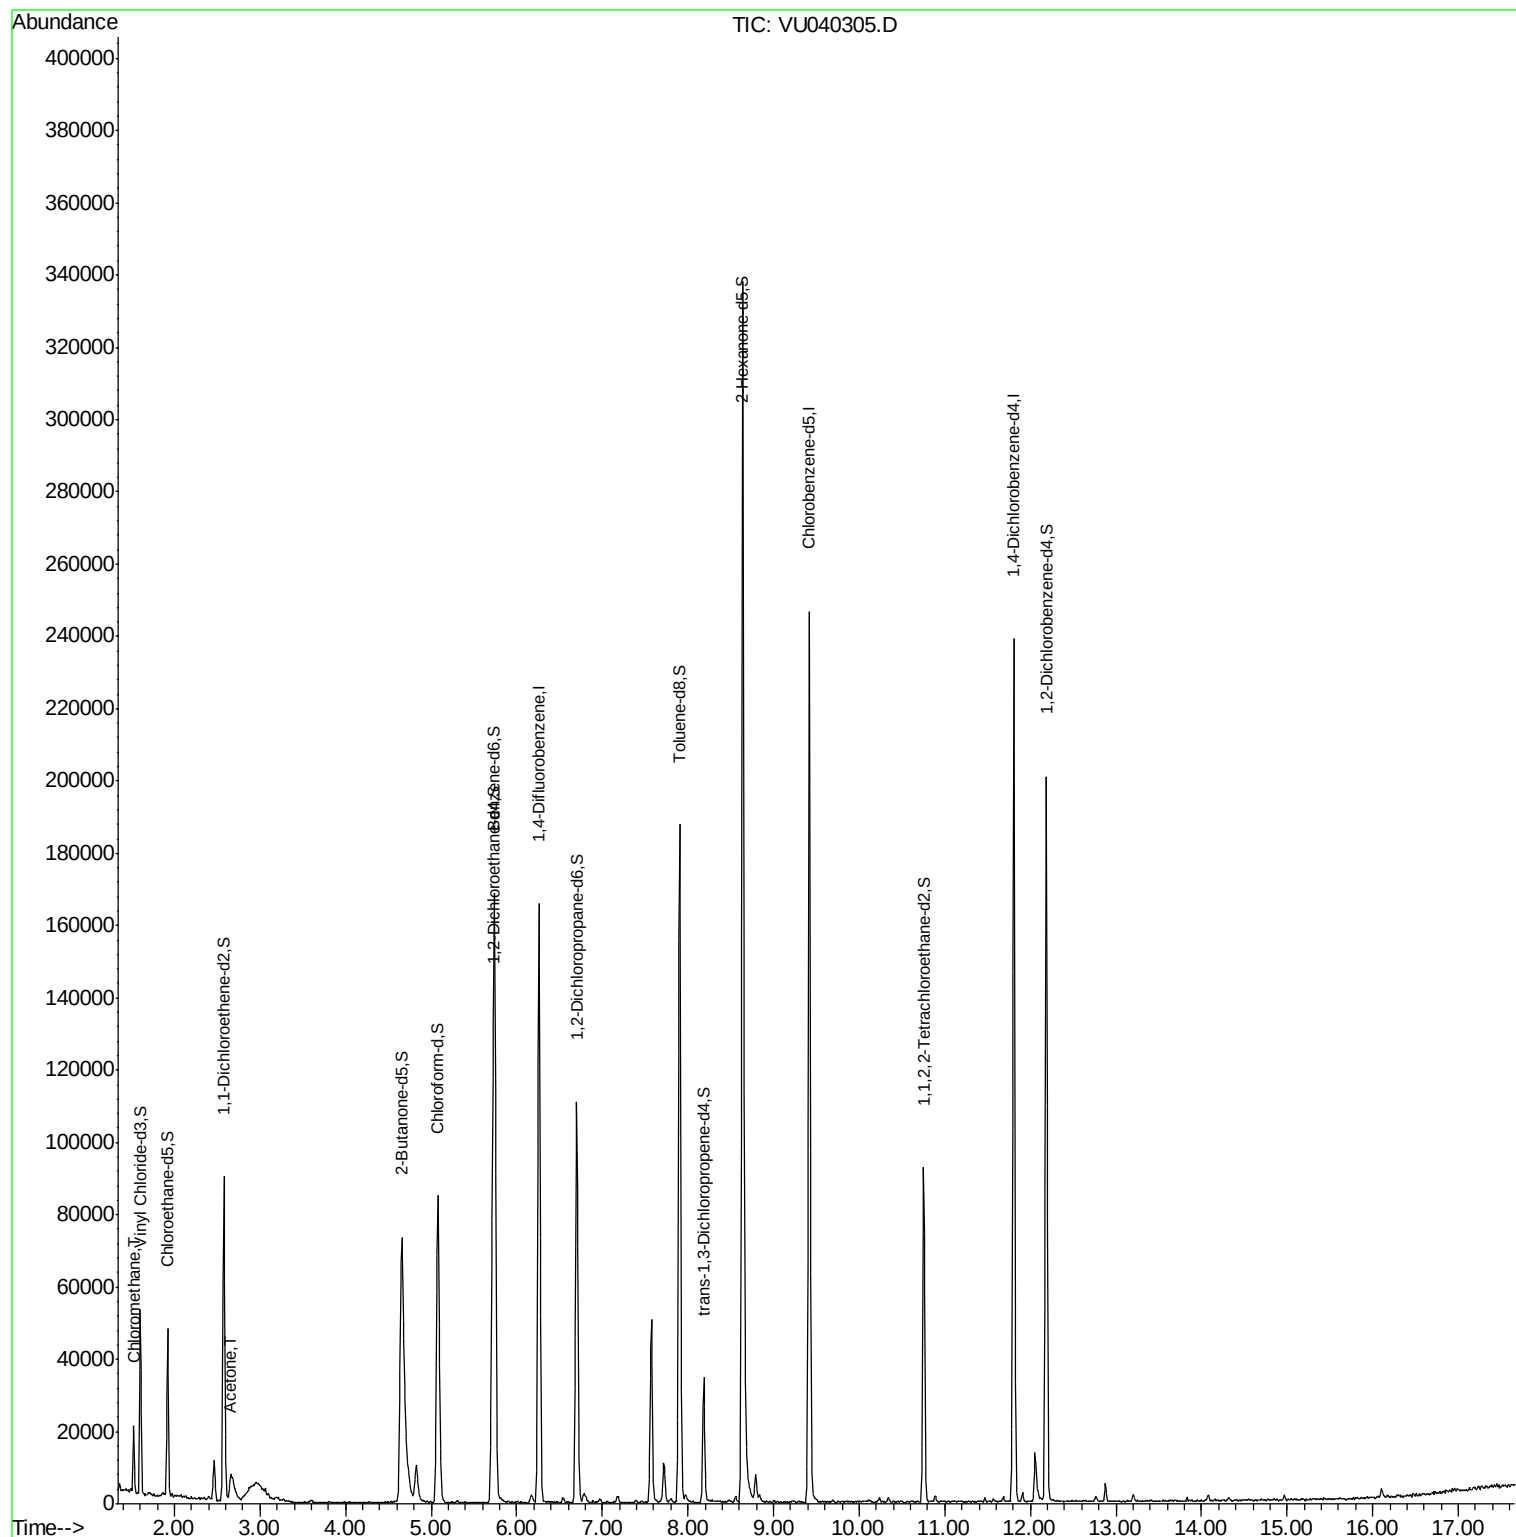

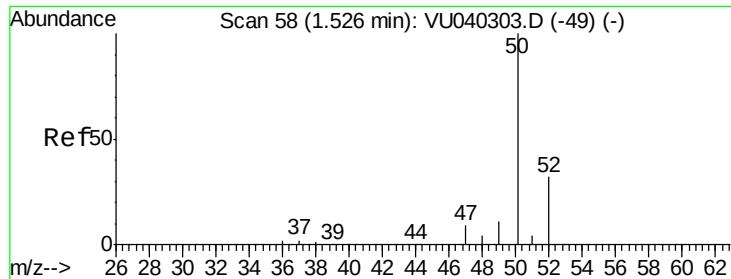

#3

Chloromethane

Concen: 1.031 ug/L

RT: 1.52 min Scan# 57

Delta R.T. -0.00 min

Lab File: VU040305.D

Acq: 25 Sep 2020 17:27

Instrument :

MSVOA_U

ClientSampleId :

BFST2

Tot Ion: 50 Resp: 12165

Ion Ratio Lower Upper

50 100


52 33.4 22.8 42.4

Manual Integrations

APPROVED




MMDadoda

9/28/2020 10:47:28 AM

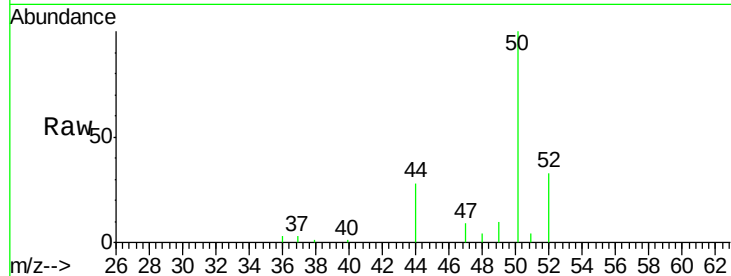

Abundance Ion 50.05 (49.75 to 50.75): VU0

Ion 52.05 (51.75 to 52.75): VU0

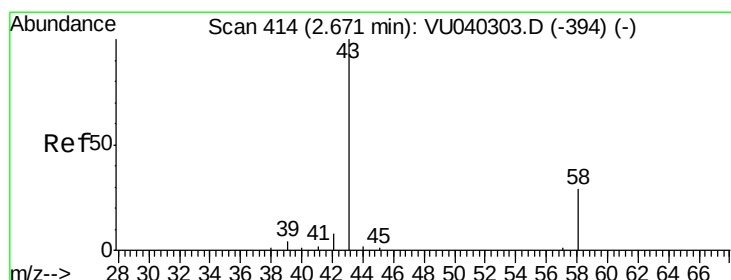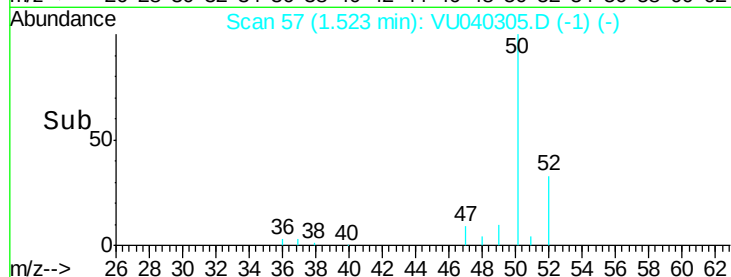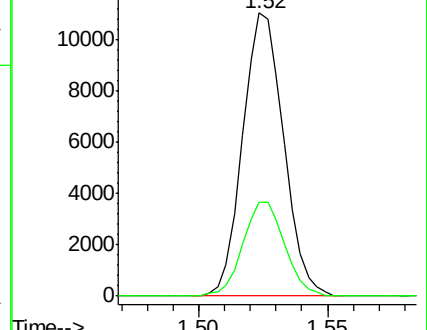

#13

Acetone

Concen: 7.780 ug/L m

RT: 2.66 min Scan# 412

Delta R.T. -0.01 min

Lab File: VU040305.D


Acq: 25 Sep 2020 17:27

Tgt Ion: 43 Resp: 19528

Ion Ratio Lower Upper

43 100

58 12.2 0.0 55.4

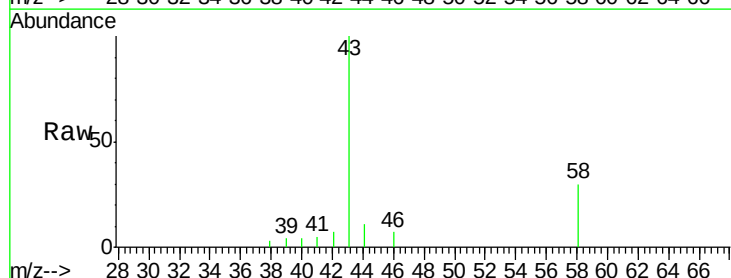

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

