


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092620\
 Data File : VU040287.D
 Acq On : 25 Sep 2020 08:36
 Operator : SY/MD
 Sample : BFB07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Sep 28 13:01:31 2020

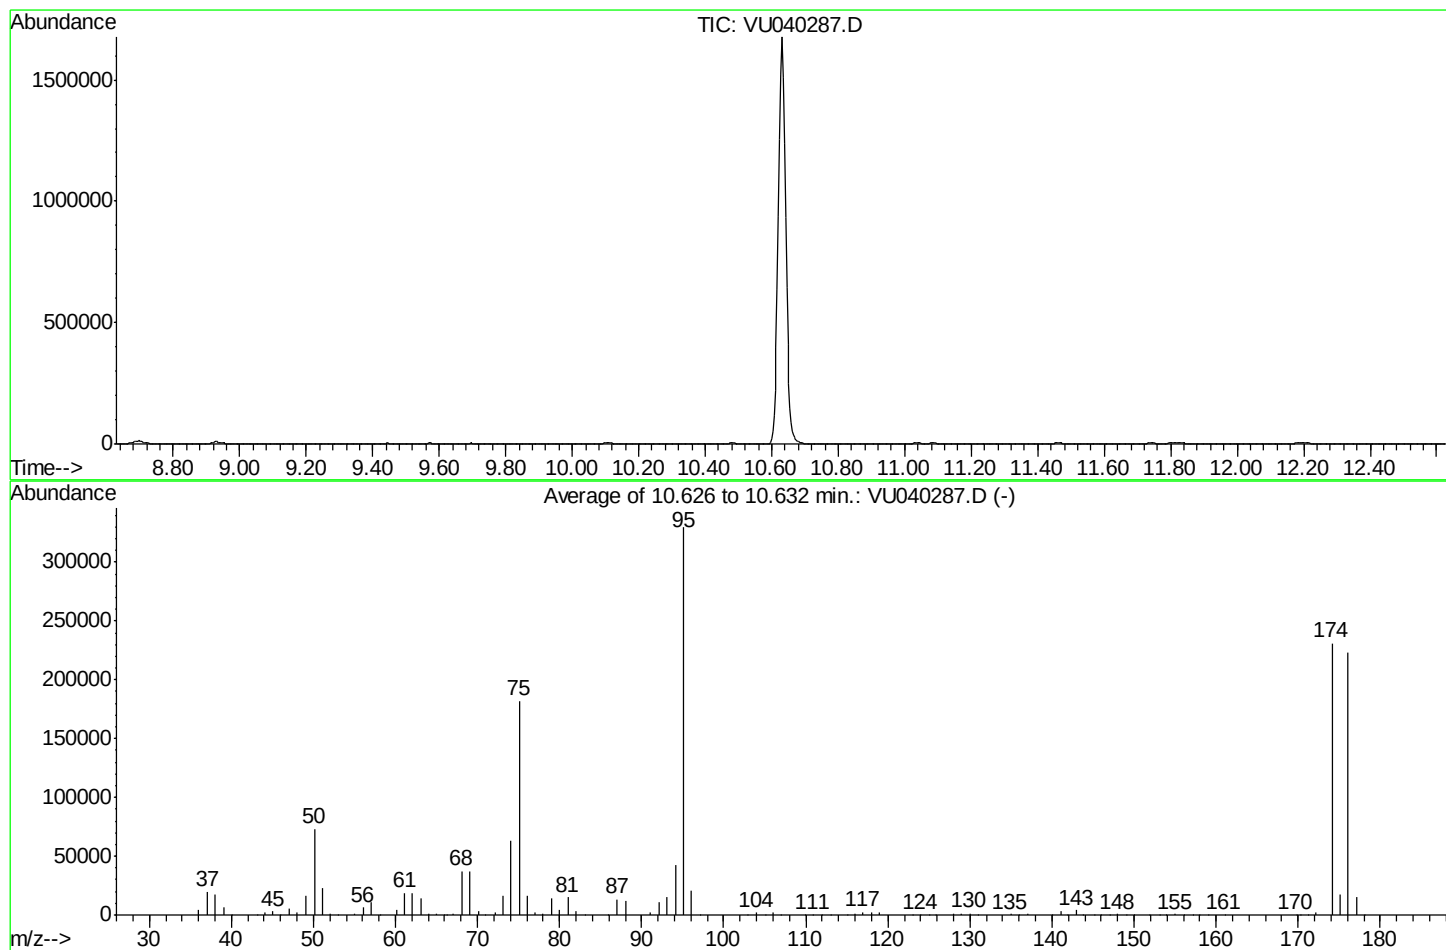

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	73245	PASS
75	95	30	80	55.2	181909	PASS
95	95	100	100	100.0	329685	PASS
96	95	5	9	6.4	21202	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.0	230912	PASS
175	174	5	9	7.6	17472	PASS
176	174	95	101	96.5	222933	PASS
177	176	5	9	6.6	14743	PASS

m/z	Abundance
36.00	4110.0
37.10	18712.0
38.00	17152.0
39.10	6597.0
40.00	534.0
43.10	162.0
44.00	2920.0
45.00	3052.0
46.00	350.0
47.00	4891.0
48.00	2382.0
49.10	16209.0
50.10	69744.0
51.10	21544.0
52.10	890.0
53.00	287.0
55.00	1202.0
56.00	6228.0
57.10	10386.0
58.10	409.0
60.10	3571.0
61.10	17720.0
62.10	17360.0
63.10	13713.0
64.10	1512.0
65.10	1662.0
65.90	312.0
67.10	869.0
68.10	35072.0
69.10	34864.0
70.10	3051.0
70.90	100.0
72.10	2096.0
73.10	15537.0
74.10	60008.0
75.10	173056.0
76.10	15588.0
77.00	1888.0
78.00	1196.0
79.00	13692.0
80.00	3800.0
81.00	14134.0
82.00	3284.0
83.10	373.0
85.90	258.0
87.10	12797.0
88.00	12327.0
91.00	1961.0
92.10	10345.0
93.10	14083.0
94.10	38792.0
95.10	309248.0
96.10	21064.0
97.10	635.0
103.00	148.0
104.00	1664.0
105.10	441.0
106.00	1756.0
107.00	257.0
109.90	264.0
110.90	504.0
112.00	371.0
112.90	362.0
115.00	436.0
116.00	1252.0
117.00	2154.0
118.10	1614.0
119.00	1821.0
123.00	113.0
124.00	183.0
125.90	184.0
128.00	972.0
129.00	671.0
130.00	1307.0
131.00	409.0
134.90	637.0
135.90	187.0
137.00	493.0
140.00	236.0
141.00	2922.0
141.90	397.0
143.00	4134.0
143.80	203.0
145.10	628.0
146.00	522.0
146.90	259.0
148.00	934.0
149.10	203.0
149.90	256.0
151.90	151.0
153.00	208.0
154.00	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

155.00	661.0
156.00	241.0
157.10	417.0
159.00	427.0
161.00	316.0
169.80	162.0
171.20	378.0
172.10	1906.0
174.10	211968.0
175.10	16624.0
176.10	204480.0
177.10	13454.0
178.00	308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	4546.0
37.10	20160.0
38.10	18464.0
39.10	6826.0
40.00	598.0
43.10	154.0
44.00	3168.0
45.00	3363.0
46.00	372.0
47.00	5455.0
48.00	2639.0
49.10	17072.0
50.10	75752.0
51.10	23600.0
52.10	1043.0
53.00	216.0
55.00	1354.0
56.10	6668.0
57.10	10837.0
58.10	474.0
60.10	4090.0
61.10	19568.0
62.10	18560.0
63.10	14822.0
64.10	1625.0
65.10	1489.0
65.90	308.0
67.10	864.0
68.10	38840.0
69.10	37904.0
70.10	3568.0
72.10	2457.0
73.10	16944.0
74.10	65568.0
75.10	187904.0
76.10	16704.0
77.00	2306.0
78.00	1432.0
79.00	14630.0
80.00	4245.0
81.00	15489.0
82.00	3439.0
83.10	485.0
87.00	13994.0
88.00	12905.0
91.00	2045.0
92.10	11368.0
93.10	15591.0
94.10	43256.0
95.10	340544.0
96.10	21944.0
97.00	543.0
102.90	207.0
104.00	1974.0
105.00	488.0
106.00	1807.0
107.00	229.0
109.90	345.0
110.90	478.0
112.00	410.0
113.00	418.0
115.00	494.0
116.00	1351.0
117.00	2378.0
118.00	1839.0
119.00	1925.0
123.00	122.0
123.90	257.0
125.00	116.0
125.90	223.0
128.00	977.0
129.00	841.0
130.00	1476.0
131.00	452.0
135.00	641.0
136.00	196.0
137.00	646.0
140.00	266.0
141.00	3397.0
141.90	428.0
143.00	4297.0
143.80	227.0
145.10	529.0
146.00	584.0
146.90	224.0
148.00	1022.0
149.00	213.0
150.00	252.0
153.00	281.0
153.90	206.0
155.00	752.0
156.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

157.10	536.0
157.90	113.0
159.00	439.0
161.10	401.0
169.80	176.0
171.20	384.0
172.20	1888.0
174.10	237888.0
175.10	17784.0
176.10	230208.0
177.10	15197.0
178.10	392.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	4227.0
37.10	19984.0
38.10	17776.0
39.10	6660.0
40.00	574.0
43.20	148.0
44.10	3163.0
45.10	3412.0
46.00	363.0
47.00	5178.0
48.00	2610.0
49.10	16680.0
50.10	74240.0
51.10	23352.0
52.10	993.0
53.00	214.0
55.00	1356.0
56.10	6704.0
57.10	10513.0
58.00	447.0
60.10	4145.0
61.10	19232.0
62.10	18312.0
63.10	14240.0
64.10	1663.0
65.00	1277.0
65.90	243.0
66.30	112.0
67.00	858.0
68.10	37896.0
69.10	37672.0
70.10	3514.0
71.00	111.0
72.10	2461.0
73.10	16992.0
74.10	64528.0
75.10	184768.0
76.10	15839.0
77.00	2293.0
78.00	1404.0
79.00	14375.0
80.00	4371.0
81.00	15374.0
82.00	3200.0
83.10	494.0
87.10	13204.0
88.00	12431.0
91.00	1843.0
92.10	11104.0
93.10	15143.0
94.10	44296.0
95.10	339264.0
96.10	20600.0
97.10	488.0
102.80	237.0
104.00	2066.0
105.00	544.0
106.00	1577.0
107.00	224.0
109.90	351.0
110.90	385.0
112.00	339.0
113.00	459.0
115.00	505.0
116.00	1444.0
117.00	2331.0
118.00	1811.0
119.00	1939.0
123.90	288.0
125.00	100.0
125.80	210.0
127.90	995.0
128.90	860.0
130.00	1326.0
131.00	443.0
135.00	667.0
136.00	181.0
137.00	739.0
139.90	271.0
141.10	3537.0
141.90	411.0
143.00	4083.0
143.80	242.0
145.10	460.0
146.00	606.0
147.00	203.0
148.00	940.0
149.00	209.0
150.00	253.0
153.10	301.0
153.90	167.0
155.00	705.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

156.00	170.0
157.10	579.0
157.90	116.0
159.00	360.0
161.10	379.0
169.80	159.0
170.20	119.0
172.20	1870.0
174.10	242880.0
175.10	18008.0
176.10	234112.0
177.10	15580.0
178.10	413.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Scan 2874 (10.581 min): VU040287.D
BFB07

m/z	Abundance
40.00	189.0
44.10	424.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07