

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
 Data File : VU055526.D
 Acq On : 26 Sep 2023 19:03
 Operator : MD/SY
 Sample : 04530-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYJ02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	16	21	28	rBV2	20324	22536	2.00%	0.235%
2	1.602	87	97	119	rVB2	688228	842499	74.74%	8.784%
3	1.911	185	193	204	rBV	123745	158159	14.03%	1.649%
4	2.563	384	396	413	rBV	251781	417366	37.02%	4.352%
5	3.351	630	641	654	rVB3	10196	18969	1.68%	0.198%
6	4.627	1024	1038	1044	rBV	127522	287381	25.49%	2.996%
7	5.058	1156	1172	1197	rBV	217246	483890	42.92%	5.045%
8	5.721	1358	1378	1406	rBV2	427961	1127301	100.00%	11.754%
9	6.245	1528	1541	1573	rBV	331247	661405	58.67%	6.896%
10	6.541	1622	1633	1648	rVB8	10985	23489	2.08%	0.245%
11	6.685	1665	1678	1700	rBV	252207	508881	45.14%	5.306%
12	7.563	1940	1951	1977	rBV	123030	228554	20.27%	2.383%
13	7.897	2040	2055	2087	rBV	527545	949371	84.22%	9.899%
14	8.177	2130	2142	2164	rBV3	72962	131052	11.63%	1.366%
15	8.634	2271	2284	2325	rBV2	380034	912887	80.98%	9.518%
16	9.415	2514	2527	2554	rBV	502094	851196	75.51%	8.875%
17	10.753	2928	2943	2958	rBV2	191002	311893	27.67%	3.252%
18	11.810	3260	3272	3292	rBV	520221	858098	76.12%	8.947%
19	12.190	3377	3390	3414	rBV	472334	795988	70.61%	8.299%




Sum of corrected areas: 9590915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055526.D
Acq On : 26 Sep 2023 19:03
Operator : MD/SY
Sample : 04530-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYJ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

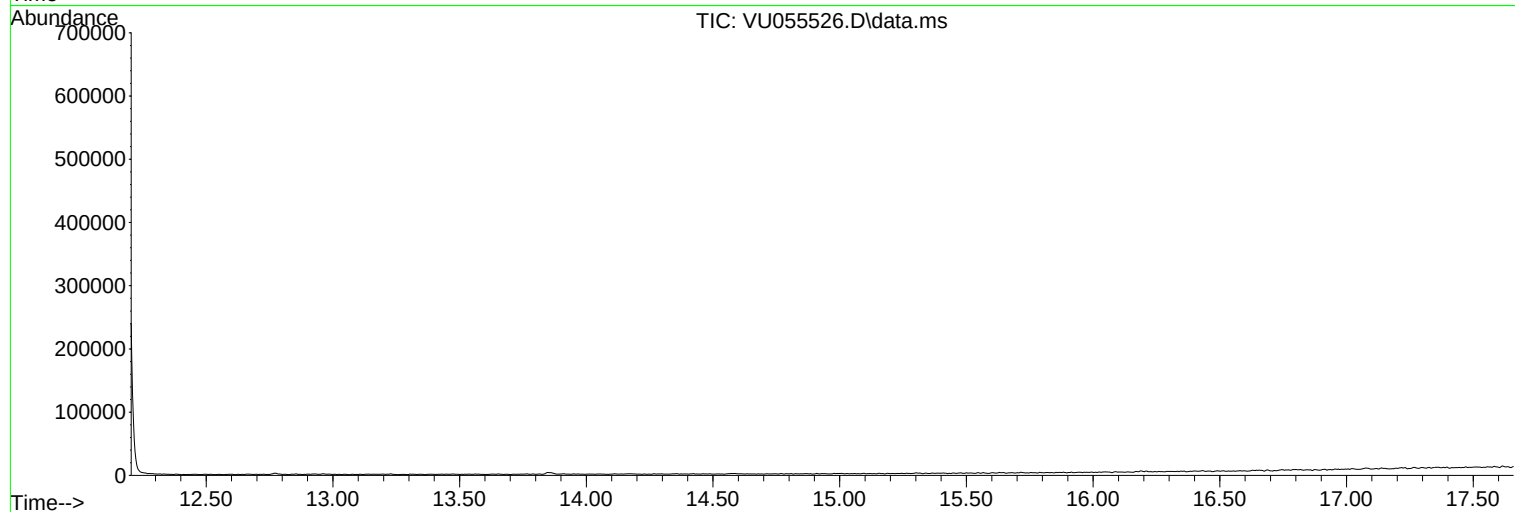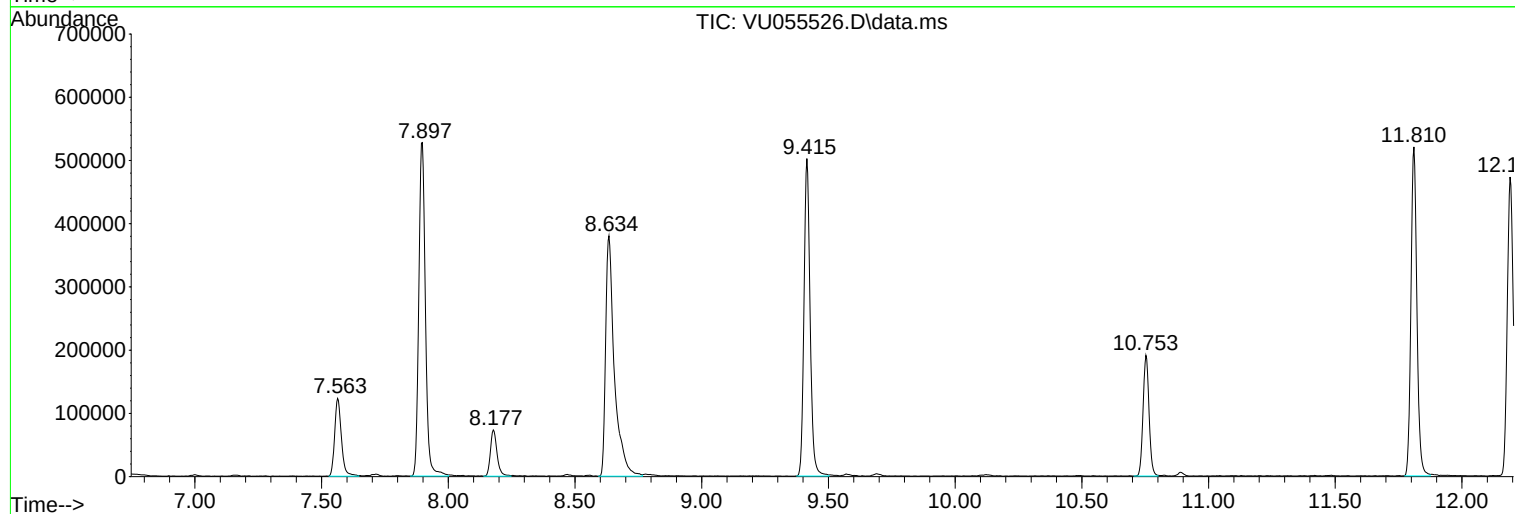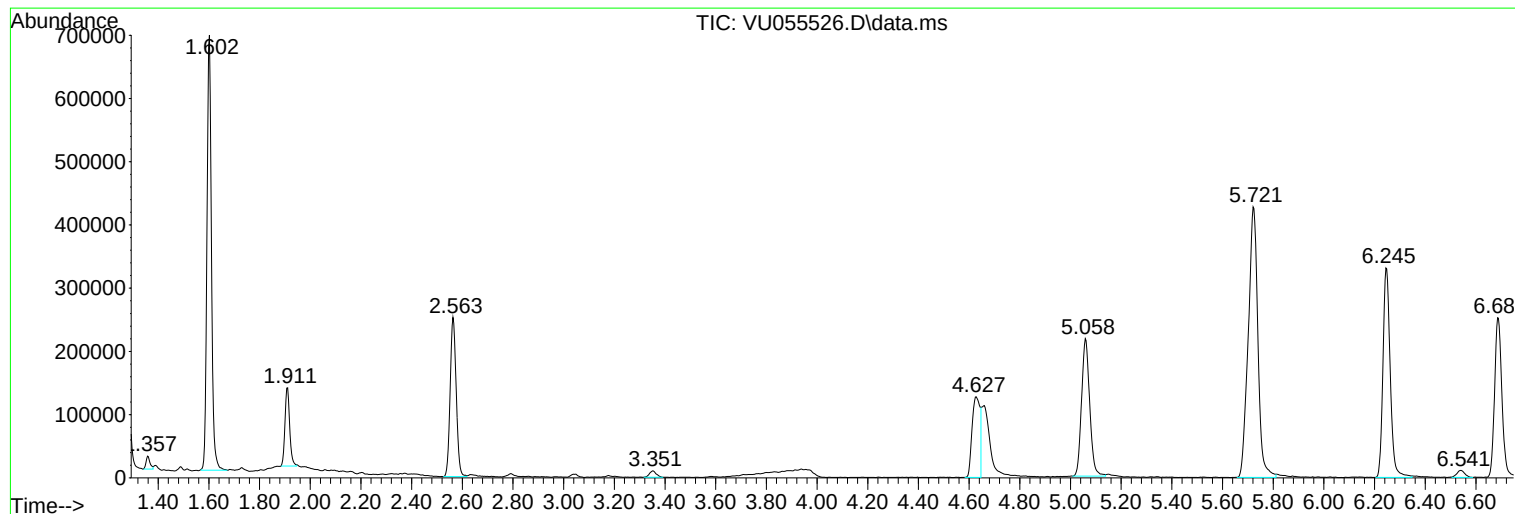

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055526.D
Acq On : 26 Sep 2023 19:03
Operator : MD/SY
Sample : 04530-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYJ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055526.D
Acq On : 26 Sep 2023 19:03
Operator : MD/SY
Sample : 04530-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYJ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc