

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
 Data File : VU055543.D
 Acq On : 27 Sep 2023 02:44
 Operator : MD/SY
 Sample : VIBLK145
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK145

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	106	rBV	146635	174477	15.94%	1.992%
2	1.911	185	193	211	rVB	102531	133355	12.18%	1.522%
3	2.563	384	396	415	rBV	245462	403606	36.86%	4.608%
4	2.792	456	467	476	rBV	9855	16956	1.55%	0.194%
5	3.042	531	545	563	rBV	98443	183695	16.78%	2.097%
6	3.181	575	588	609	rVB2	19899	45331	4.14%	0.518%
7	4.627	1024	1038	1076	rBV	118853	420206	38.38%	4.797%
8	5.058	1156	1172	1193	rBV	208977	465182	42.49%	5.311%
9	5.724	1358	1379	1414	rBV2	412061	1094857	100.00%	12.500%
10	6.245	1527	1541	1568	rBV	303876	598990	54.71%	6.839%
11	6.531	1618	1630	1646	rVB5	7877	17823	1.63%	0.203%
12	6.688	1658	1679	1696	rBV	249405	494900	45.20%	5.650%
13	7.563	1939	1951	1971	rBV2	113562	211276	19.30%	2.412%
14	7.894	2041	2054	2073	rBV	509020	908948	83.02%	10.377%
15	8.177	2131	2142	2165	rBV	67890	122080	11.15%	1.394%
16	8.634	2272	2284	2316	rBV3	357497	857141	78.29%	9.786%
17	9.415	2514	2527	2549	rBV	444135	772345	70.54%	8.818%
18	10.753	2931	2943	2961	rBV	172864	292881	26.75%	3.344%
19	11.810	3260	3272	3295	rBV	473737	779780	71.22%	8.903%
20	12.190	3376	3390	3416	rBV	459808	765255	69.90%	8.737%




Sum of corrected areas: 8759084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055543.D
Acq On : 27 Sep 2023 02:44
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

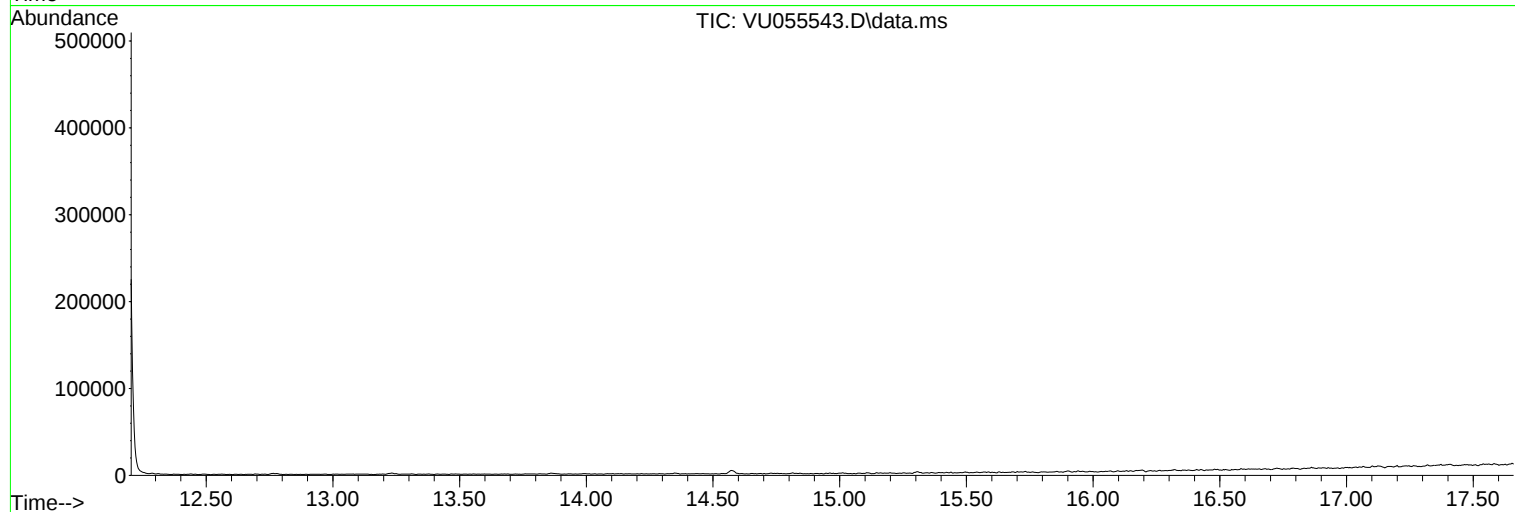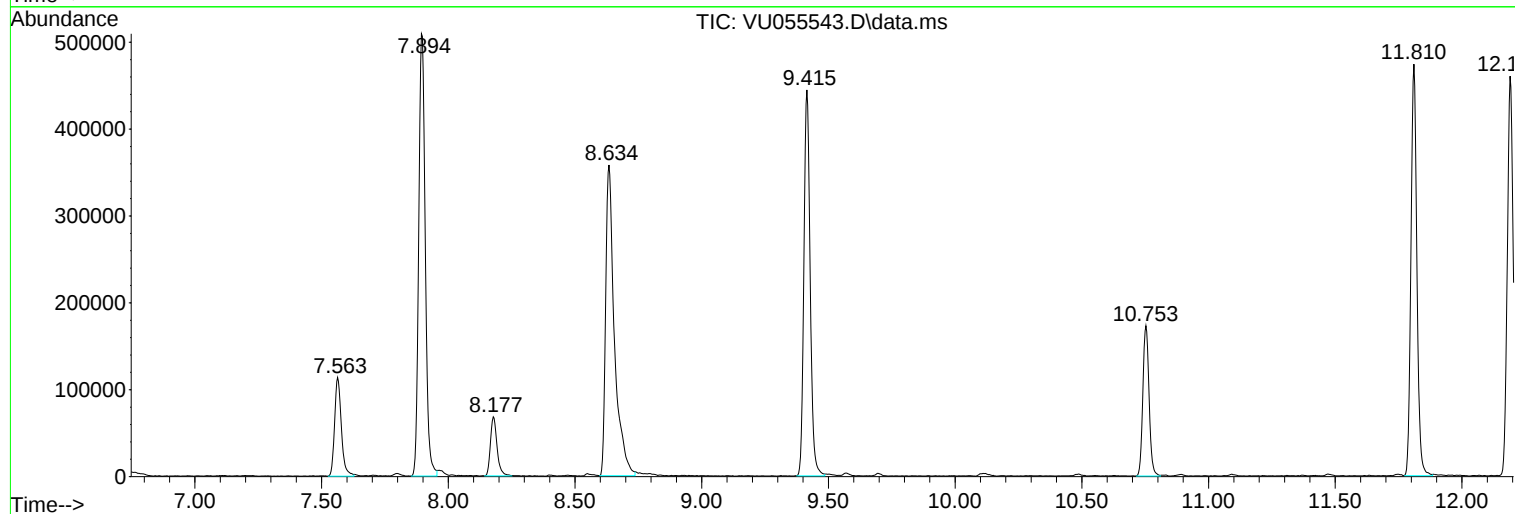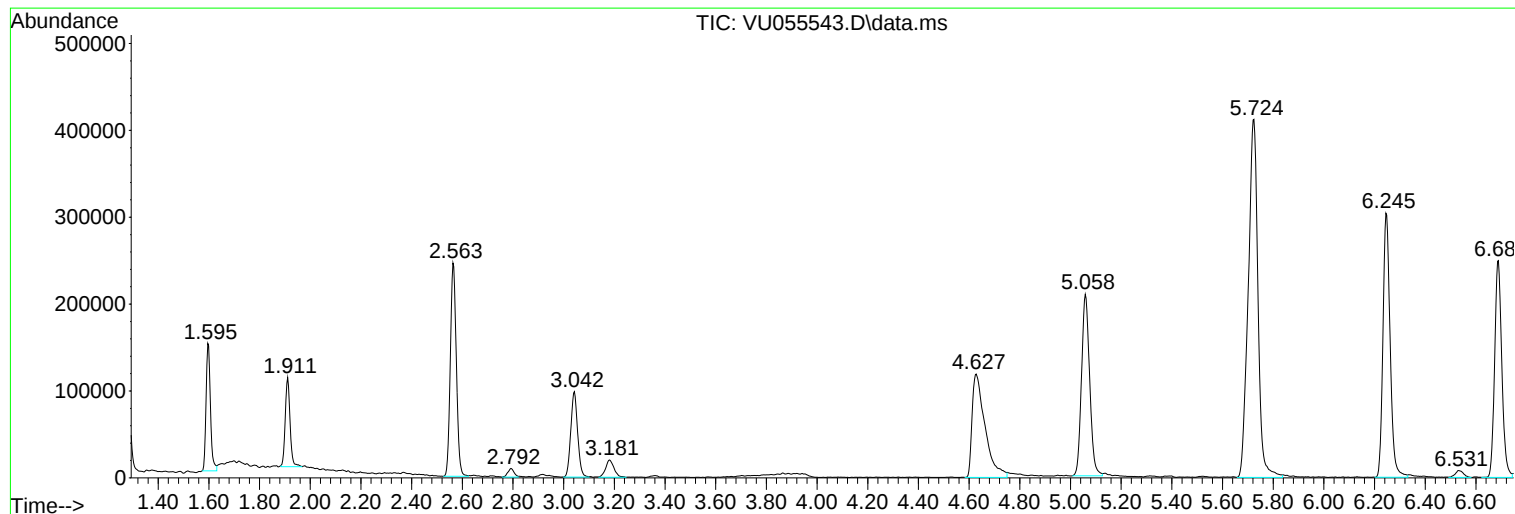

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055543.D
Acq On : 27 Sep 2023 02:44
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055543.D
Acq On : 27 Sep 2023 02:44
Operator : MD/SY
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------