


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092623\
Data File : VU055505.D
Acq On : 26 Sep 2023 09:16
Operator : MD/SY
Sample : BFB052
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB052

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 27 23:33:30 2023

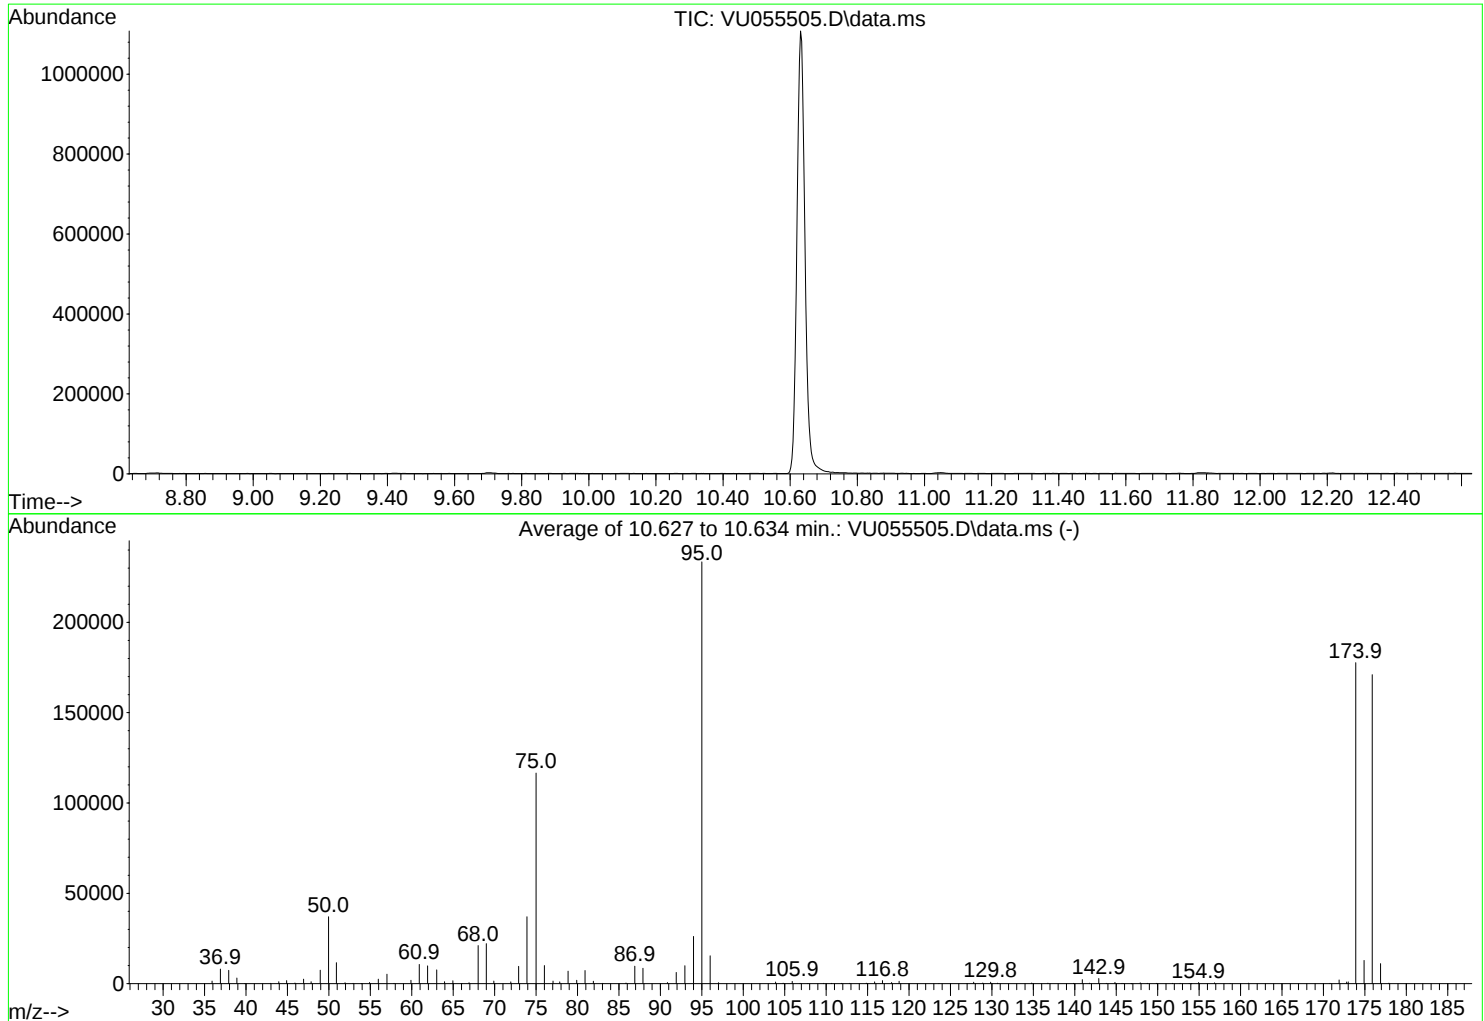

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	36984	PASS
75	95	30	80	49.9	116552	PASS
95	95	100	100	100.0	233493	PASS
96	95	5	9	6.6	15401	PASS
173	174	0.00	2	0.5	959	PASS
174	95	50	120	76.1	177685	PASS
175	174	5	9	7.2	12849	PASS
176	174	95	101	96.3	171072	PASS
177	176	5	9	6.5	11089	PASS

m/z	Abundance
39.80	281.0
44.00	550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	1336.0
36.90	8054.0
37.90	7410.0
38.90	3008.0
39.90	454.0
42.90	106.0
44.00	1417.0
44.90	1792.0
45.90	357.0
47.00	2559.0
47.90	1055.0
49.00	7331.0
49.90	36360.0
50.90	11178.0
52.00	444.0
52.90	128.0
54.90	589.0
56.00	2265.0
57.00	5074.0
57.90	157.0
59.90	1767.0
60.90	10431.0
61.90	9496.0
63.00	7690.0
63.90	1041.0
64.90	1476.0
66.10	123.0
66.90	498.0
68.00	20440.0
69.00	21376.0
69.90	1470.0
71.90	847.0
72.90	9444.0
73.90	35952.0
75.00	112824.0
76.00	9955.0
77.10	1304.0
77.90	831.0
78.80	6720.0
79.90	1822.0
80.90	6869.0
81.90	1304.0
83.10	168.0
85.90	284.0
86.90	9267.0
87.90	7974.0
90.80	727.0
91.90	5786.0
93.00	9741.0
94.00	25128.0
95.00	225088.0
96.00	15030.0
97.00	485.0
103.90	941.0
104.90	245.0
105.90	1091.0
106.90	173.0
109.70	198.0
110.70	119.0
111.80	128.0
112.90	139.0
114.90	246.0
115.80	958.0
116.80	1598.0
117.90	625.0
118.80	1208.0
127.80	711.0
128.90	349.0
129.80	767.0
130.70	292.0
134.80	381.0
136.80	227.0
139.80	143.0
140.90	1921.0
141.80	322.0
142.90	2776.0
143.80	268.0
144.80	708.0
145.70	231.0
147.90	407.0
148.70	177.0
149.80	195.0
151.70	229.0
152.70	104.0
153.80	165.0
155.00	529.0
156.80	474.0
158.70	165.0
160.90	246.0
170.80	185.0
171.90	1943.0
172.80	1245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

173.90	168256.0
174.90	12590.0
175.90	161856.0
176.90	10544.0
177.90	283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	1565.0
36.90	8311.0
37.90	7603.0
38.90	3266.0
39.90	414.0
43.00	156.0
43.90	1608.0
44.90	1789.0
45.90	447.0
46.90	2531.0
47.80	1085.0
49.00	7659.0
50.00	37960.0
50.90	12060.0
51.90	587.0
52.90	142.0
53.90	103.0
54.90	637.0
55.90	2507.0
57.00	5504.0
57.90	176.0
59.90	1896.0
60.90	10969.0
61.90	10151.0
63.00	7931.0
64.00	1038.0
65.00	1618.0
66.10	127.0
66.90	564.0
68.00	21504.0
69.00	22816.0
69.90	1411.0
71.90	932.0
72.90	9729.0
73.90	38360.0
75.00	119928.0
76.00	10196.0
77.00	1393.0
77.80	1041.0
78.90	7141.0
79.90	1944.0
80.90	7515.0
81.90	1361.0
83.10	169.0
85.90	323.0
86.90	9995.0
87.90	8633.0
90.90	638.0
91.90	6476.0
92.90	10139.0
94.00	26944.0
95.00	241088.0
96.00	15962.0
97.00	575.0
103.90	911.0
104.80	220.0
105.90	1356.0
106.80	201.0
107.80	117.0
109.70	186.0
110.60	141.0
111.90	190.0
112.80	157.0
114.90	286.0
115.80	951.0
116.80	1714.0
117.90	672.0
118.80	1375.0
123.60	145.0
127.00	104.0
127.80	763.0
128.90	344.0
129.90	860.0
130.70	324.0
134.80	369.0
136.70	327.0
139.80	197.0
140.90	2215.0
141.80	343.0
142.90	2919.0
143.80	186.0
144.90	801.0
145.70	310.0
147.90	447.0
148.80	158.0
149.90	165.0
151.80	171.0
152.70	162.0
153.80	146.0
154.90	684.0
156.80	453.0
158.70	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

161.00	285.0
170.80	209.0
171.90	2136.0
172.80	1305.0
173.00	1332.0
173.90	182976.0
174.90	13116.0
175.90	176768.0
176.90	11593.0
177.90	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	1507.0
36.90	7765.0
37.90	6963.0
38.90	3039.0
39.90	353.0
43.00	179.0
43.90	1744.0
44.90	1549.0
45.90	390.0
46.90	2336.0
47.80	983.0
48.90	7211.0
50.00	36632.0
50.90	11514.0
51.90	568.0
52.90	145.0
54.90	525.0
55.90	2621.0
57.00	5136.0
57.80	189.0
59.90	1869.0
60.90	10502.0
61.90	9833.0
63.00	7387.0
64.00	1018.0
65.00	1790.0
66.00	156.0
66.90	487.0
68.00	21272.0
69.00	22328.0
69.90	1398.0
72.00	1119.0
72.90	9422.0
73.90	36752.0
75.00	116904.0
76.00	9972.0
77.00	1474.0
77.80	1085.0
78.90	7006.0
79.90	1871.0
80.90	7367.0
81.90	1411.0
83.00	152.0
85.80	404.0
86.90	9834.0
87.90	8799.0
90.80	589.0
91.90	6466.0
92.90	9780.0
94.00	26256.0
95.00	234304.0
96.00	15210.0
97.00	574.0
103.90	882.0
104.70	305.0
105.90	1365.0
106.80	215.0
107.80	145.0
109.70	146.0
110.60	157.0
111.90	237.0
112.90	187.0
114.80	235.0
115.90	913.0
116.80	1762.0
117.90	665.0
118.80	1430.0
123.60	163.0
127.00	107.0
127.80	838.0
128.90	327.0
129.90	849.0
130.70	338.0
134.80	372.0
136.70	365.0
139.90	221.0
140.90	2394.0
141.80	286.0
142.90	2769.0
143.80	121.0
144.90	759.0
145.90	341.0
146.80	130.0
147.90	476.0
148.70	127.0
149.90	129.0
151.90	122.0
152.70	196.0
154.00	133.0
154.90	699.0
156.90	405.0
158.80	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

160.90	264.0
170.80	199.0
171.90	2089.0
173.00	1546.0
173.90	181824.0
174.90	12841.0
175.90	174592.0
176.90	11130.0
177.90	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052