

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092624\
 Data File : VU061020.D
 Acq On : 26 Sep 2024 15:05
 Operator : MD/SY
 Sample : P4186-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY080

Quant Time: Sep 27 04:53:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 27 04:49:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	140029	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	154493	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	57658	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	50370	3.999	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.907	69	45221	5.043	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%
11) 1,1-Dichloroethene-d2	2.560	65	18277	4.094	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.800%
20) 2-Butanone-d5	4.627	46	109365	54.090	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.180%
24) Chloroform-d	5.055	84	93162	4.839	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.695	65	47198	5.128	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.721	84	172032	4.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.682	67	63034	4.920	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.891	98	134252	3.556	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.200%
43) trans-1,3-Dichloroprop...	8.177	79	18008	3.905	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.627	63	83628	45.970	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.940%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	47465	4.729	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	49738	5.134	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds						
22) cis-1,2-Dichloroethene	4.666	96	2406	0.238	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092624\
Data File : VU061020.D
Acq On : 26 Sep 2024 15:05
Operator : MD/SY
Sample : P4186-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY080


Quant Time: Sep 27 04:53:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 27 04:49:19 2024
Response via : Initial Calibration

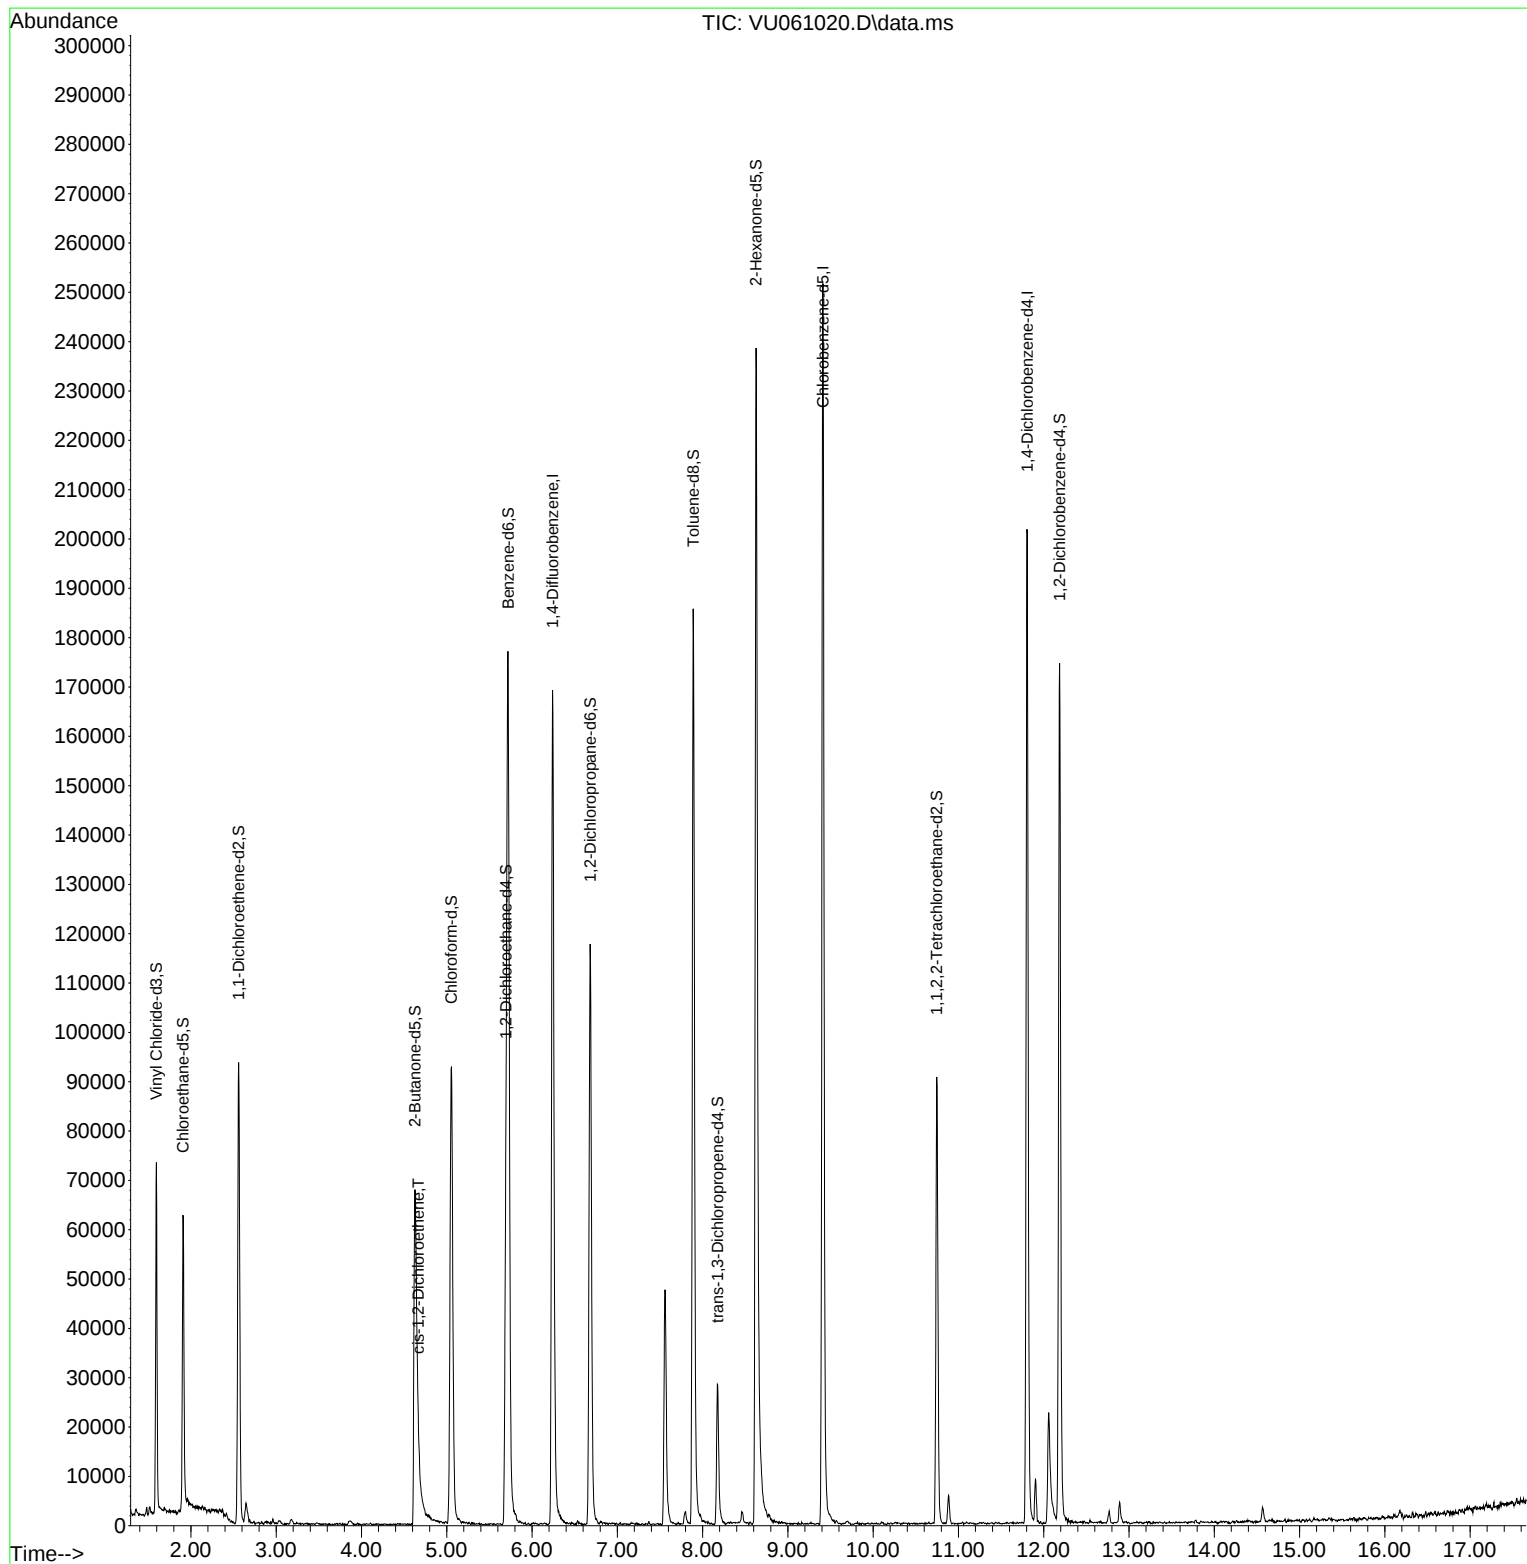

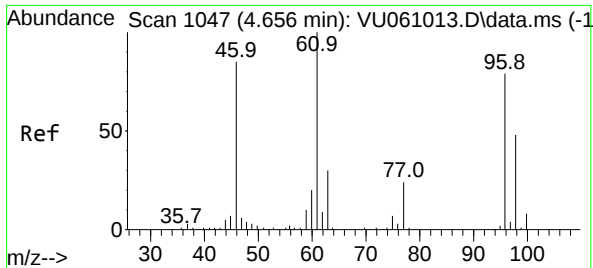

#22
 cis-1,2-Dichloroethene
 Concen: 0.238 ug/L
 RT: 4.666 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VU061020.D
 Acq: 26 Sep 2024 15:05

Instrument :
 MSVOA_U
 ClientSampleId :
 EY080

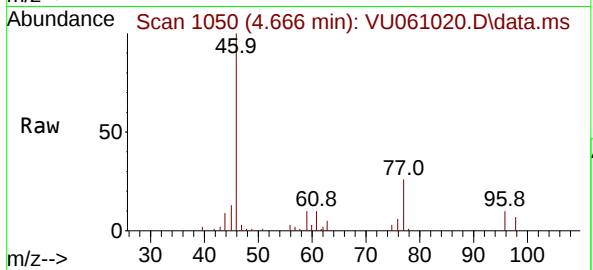

Tgt Ion:	96	Resp:	2406
Ion	Ratio	Lower	Upper
96	100		
61	115.4	89.7	166.5
98	65.4	45.1	83.9

