


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092624\
Data File : VU061012.D
Acq On : 26 Sep 2024 10:15
Operator : MD/SY
Sample : BFB006
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB006

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 27 04:49:19 2024

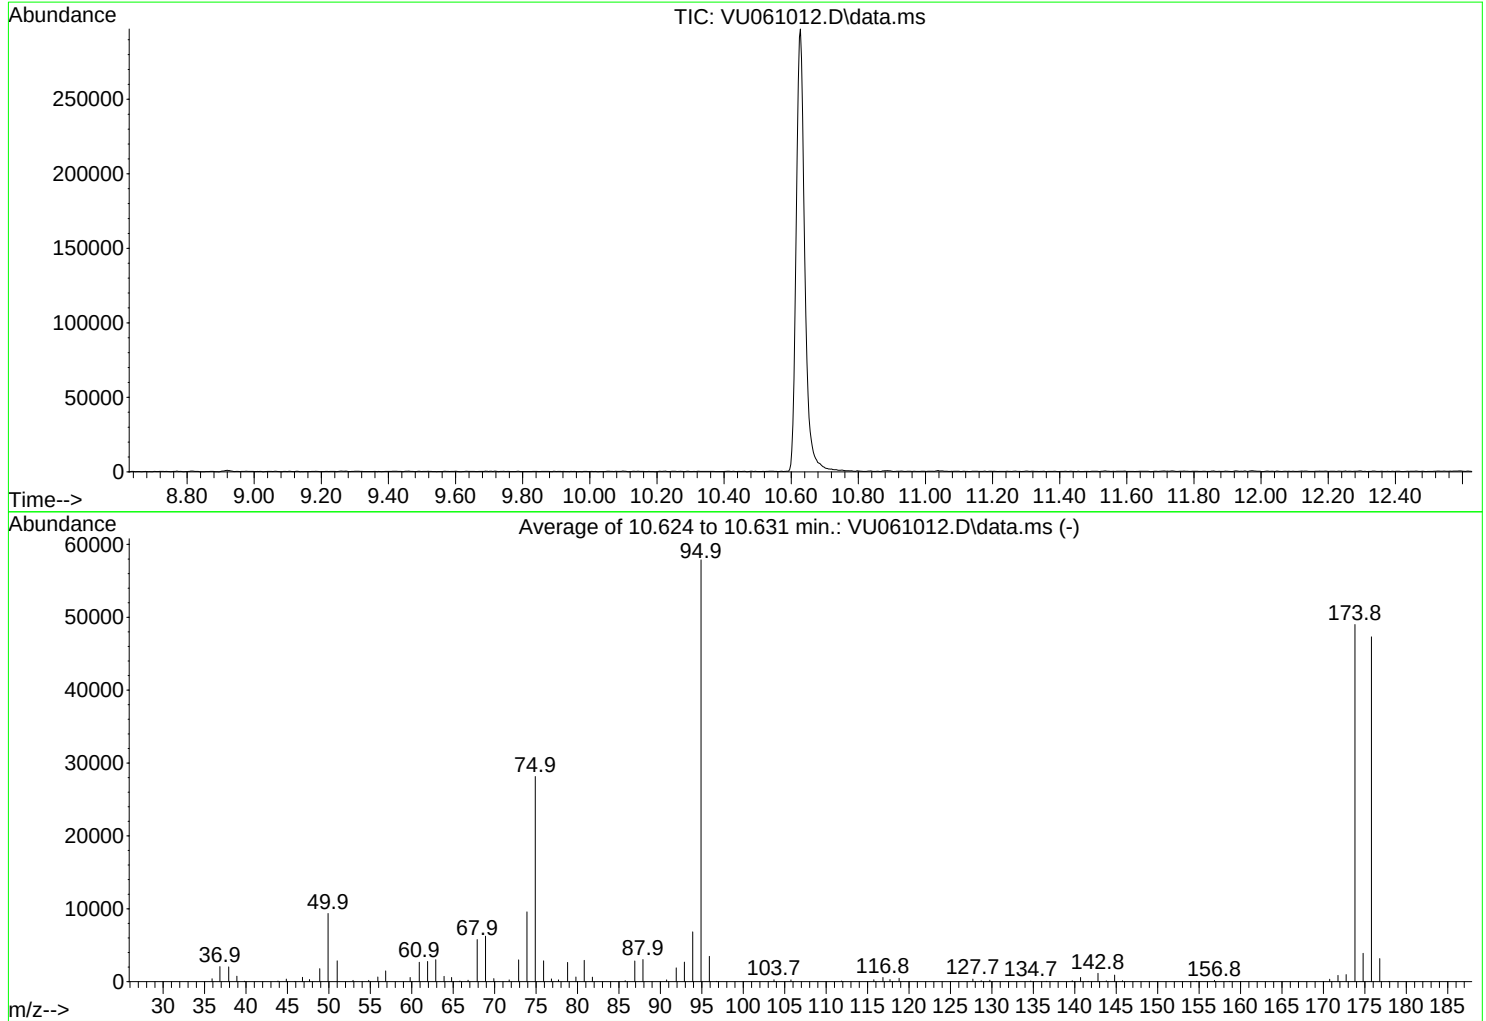

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	9348	PASS
75	95	30	80	48.6	28157	PASS
95	95	100	100	100.0	57885	PASS
96	95	5	9	6.0	3462	PASS
173	174	0.00	2	2.0	964	PASS
174	95	50	120	84.7	49003	PASS
175	174	5	9	7.9	3888	PASS
176	174	95	101	96.6	47328	PASS
177	176	5	9	6.7	3165	PASS

m/z	Abundance
39.90	108.0
43.90	365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.80	444.0
36.80	2151.0
37.90	2061.0
38.90	690.0
39.70	139.0
43.80	392.0
44.80	341.0
46.80	576.0
47.70	250.0
48.90	1994.0
49.90	9650.0
51.00	2905.0
52.90	193.0
54.80	192.0
55.90	659.0
56.90	1704.0
59.80	524.0
60.90	2871.0
61.90	2890.0
62.90	2870.0
63.90	789.0
64.80	557.0
65.80	110.0
66.90	219.0
67.90	5645.0
68.90	6104.0
69.90	458.0
71.70	231.0
72.90	2731.0
73.90	9835.0
74.90	28544.0
75.90	2944.0
76.80	441.0
77.70	261.0
78.80	2743.0
79.80	664.0
80.80	2991.0
81.80	649.0
85.70	167.0
86.90	2855.0
87.90	3062.0
90.70	235.0
91.90	1947.0
92.90	2869.0
93.90	7248.0
94.90	59248.0
95.90	3691.0
96.80	104.0
103.70	231.0
105.70	273.0
115.70	236.0
116.90	601.0
117.70	308.0
118.80	431.0
127.70	328.0
128.70	134.0
129.70	177.0
139.70	107.0
140.70	529.0
142.80	1117.0
143.80	187.0
144.80	819.0
145.70	143.0
156.90	145.0
170.80	282.0
171.70	769.0
172.80	920.0
173.80	48808.0
174.80	4005.0
175.80	46944.0
176.80	3189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.90	416.0
36.90	2158.0
37.90	2095.0
38.90	755.0
39.80	184.0
43.90	467.0
44.90	355.0
46.80	577.0
47.70	298.0
48.90	1783.0
49.90	9554.0
51.00	2959.0
52.90	194.0
54.80	176.0
55.90	622.0
56.90	1498.0
59.80	606.0
60.90	2699.0
61.90	2965.0
62.90	3127.0
63.90	752.0
64.80	562.0
65.80	124.0
66.80	187.0
67.90	5976.0
68.90	6458.0
69.90	428.0
71.70	251.0
72.90	3128.0
73.90	9802.0
74.90	28920.0
75.90	2992.0
76.90	376.0
77.70	269.0
78.80	2654.0
79.80	669.0
80.80	3039.0
81.80	647.0
85.70	131.0
86.90	2928.0
87.90	3150.0
90.80	228.0
91.90	1958.0
92.90	2785.0
93.90	7067.0
94.90	59480.0
95.90	3479.0
103.70	277.0
105.80	241.0
111.80	119.0
115.70	279.0
116.80	573.0
117.70	287.0
118.80	467.0
127.70	374.0
128.70	150.0
129.80	210.0
134.70	108.0
139.70	163.0
140.70	581.0
142.80	1156.0
143.80	121.0
144.80	960.0
145.70	129.0
156.80	185.0
170.70	345.0
171.70	876.0
172.80	997.0
173.80	50400.0
174.80	4040.0
175.80	48808.0
176.80	3245.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	356.0
36.80	1899.0
37.90	1883.0
38.90	804.0
39.80	198.0
43.90	505.0
44.90	365.0
45.90	135.0
46.80	632.0
47.60	284.0
48.90	1577.0
49.90	8841.0
51.00	2700.0
52.90	124.0
54.80	132.0
55.90	603.0
56.80	1183.0
59.80	555.0
60.90	2429.0
61.90	2479.0
62.90	3009.0
63.90	653.0
64.80	566.0
66.70	176.0
67.90	5728.0
68.90	6116.0
69.90	376.0
71.80	232.0
72.90	3109.0
73.90	9106.0
74.90	27008.0
75.90	2607.0
76.90	306.0
77.70	191.0
78.80	2510.0
79.80	609.0
80.80	2753.0
81.80	567.0
85.80	105.0
86.90	2716.0
87.90	2902.0
90.70	242.0
91.90	1762.0
92.90	2372.0
93.90	6181.0
94.90	54928.0
95.90	3215.0
103.70	267.0
105.80	204.0
111.90	122.0
115.80	288.0
116.80	521.0
117.70	282.0
118.80	460.0
127.70	329.0
128.70	115.0
129.80	190.0
134.70	137.0
136.60	121.0
139.70	153.0
140.70	585.0
141.60	101.0
142.80	1142.0
144.80	894.0
145.80	119.0
154.70	107.0
156.80	187.0
158.70	105.0
170.70	349.0
171.80	911.0
172.70	976.0
173.80	47800.0
174.80	3620.0
175.80	46232.0
176.80	3062.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006