

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
 Data File : VU063652.D
 Acq On : 25 Sep 2025 19:58
 Operator : MD/SY
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
 Title : SW846 8260

Signal : TIC: VU063652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	57	59	66	rVB2	1025	725	1.16%	0.130%
2	1.515	66	70	78	rBV3	2198	2515	4.03%	0.452%
3	1.595	85	95	101	rBV4	4728	7324	11.74%	1.315%
4	1.775	138	151	157	rBV2	21049	34188	54.78%	6.140%
5	1.843	164	172	181	rBV7	3751	6022	9.65%	1.082%
6	2.467	364	366	371	rVB3	982	690	1.11%	0.124%
7	2.566	389	397	406	rVB4	3966	5663	9.07%	1.017%
8	2.624	412	415	424	rVB4	1038	1157	1.85%	0.208%
9	2.708	435	441	448	rBV6	888	1482	2.37%	0.266%
10	2.779	453	463	476	rBV2	6013	10037	16.08%	1.803%
11	2.914	500	505	510	rBV4	1051	1100	1.76%	0.198%
12	3.033	533	542	552	rBV6	4752	8787	14.08%	1.578%
13	3.174	574	586	603	rBV2	11679	26379	42.27%	4.738%
14	3.348	628	640	653	rBV7	4774	10108	16.20%	1.815%
15	4.666	1041	1050	1057	rBV6	2000	4442	7.12%	0.798%
16	4.981	1141	1148	1153	rVB6	1241	1710	2.74%	0.307%
17	5.078	1168	1178	1182	rBV5	1205	1861	2.98%	0.334%
18	5.287	1233	1243	1249	rBV4	957	1689	2.71%	0.303%
19	5.367	1261	1268	1269	rBV2	1567	1399	2.24%	0.251%
20	5.380	1269	1272	1279	rVV5	2319	2361	3.78%	0.424%
21	5.454	1283	1295	1306	rBV6	1368	2953	4.73%	0.530%
22	5.525	1307	1317	1327	rVV7	2082	3733	5.98%	0.670%
23	5.701	1365	1372	1374	rBV3	994	1115	1.79%	0.200%
24	5.772	1387	1394	1396	rBV4	1013	1325	2.12%	0.238%
25	6.537	1624	1632	1647	rBV4	3790	7111	11.39%	1.277%
26	6.750	1692	1698	1704	rBV4	1471	2263	3.63%	0.406%
27	6.910	1744	1748	1759	rVB4	1599	2347	3.76%	0.422%
28	7.097	1801	1806	1808	rBV2	890	749	1.20%	0.135%
29	7.560	1946	1950	1958	rVV2	528	744	1.19%	0.134%
30	7.605	1958	1964	1973	rVV3	1355	2314	3.71%	0.416%
31	7.795	2014	2023	2037	rBV5	4104	9036	14.48%	1.623%
32	7.894	2043	2054	2067	rVV5	2912	6047	9.69%	1.086%
33	7.968	2069	2077	2091	rVV3	2426	4229	6.78%	0.760%
34	8.216	2139	2154	2164	rBV5	1648	2930	4.69%	0.526%
35	8.547	2249	2257	2268	rBV9	4126	7881	12.63%	1.415%
36	8.698	2294	2304	2320	rBV2	4941	12936	20.73%	2.323%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
 Data File : VU063652.D
 Acq On : 25 Sep 2025 19:58
 Operator : MD/SY
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
 Title : SW846 8260

37	8.798	2330	2335	2343	rBV7	495	635	1.02%	0.114%
38	8.846	2345	2350	2356	rVV3	1038	1265	2.03%	0.227%
39	9.418	2518	2528	2533	rBV3	5877	10386	16.64%	1.865%
40	9.573	2566	2576	2586	rBV2	3325	6071	9.73%	1.090%
41	9.695	2605	2614	2632	rVB3	6474	12080	19.36%	2.170%
42	10.103	2732	2741	2742	rBV4	2527	2779	4.45%	0.499%
43	10.122	2742	2747	2762	rVV8	3284	7463	11.96%	1.340%
44	10.335	2803	2813	2821	rBV5	2303	4616	7.40%	0.829%
45	10.483	2850	2859	2866	rBV5	2845	4159	6.66%	0.747%
46	10.634	2899	2906	2919	rBV3	5214	9006	14.43%	1.617%
47	10.782	2944	2952	2961	rBV6	4765	8662	13.88%	1.556%
48	10.904	2982	2990	3004	rBV	6109	10452	16.75%	1.877%
49	10.987	3008	3016	3024	rBV6	3229	5110	8.19%	0.918%
50	11.097	3039	3050	3066	rBV6	7348	16041	25.70%	2.881%
51	11.415	3140	3149	3156	rBV5	2945	4267	6.84%	0.766%
52	11.466	3156	3165	3175	rVB2	4195	6156	9.86%	1.106%
53	11.640	3209	3219	3231	rVB3	4945	8990	14.41%	1.615%
54	11.749	3244	3253	3259	rBV3	7518	11701	18.75%	2.101%
55	11.817	3259	3274	3296	rVB6	13870	49323	79.03%	8.858%
56	12.212	3386	3397	3414	rBV5	17641	34550	55.36%	6.205%
57	13.444	3771	3780	3795	rBV2	9700	15689	25.14%	2.818%
58	13.843	3895	3904	3919	rBV3	14743	25383	40.67%	4.559%
59	14.013	3949	3957	3968	rVB7	6070	8482	13.59%	1.523%
60	14.090	3968	3981	4005	rBV	28027	62407	100.00%	11.208%
61	14.328	4044	4055	4072	rBV3	17715	30390	48.70%	5.458%
62	14.958	4246	4251	4257	rVB3	556	646	1.04%	0.116%
63	16.051	4586	4591	4596	rBV4	629	777	1.25%	0.140%
64	16.826	4829	4832	4836	rBV3	985	760	1.22%	0.136%
65	17.614	5074	5077	5081	rBV4	1242	1196	1.92%	0.215%




Sum of corrected areas: 556794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
Data File : VU063652.D
Acq On : 25 Sep 2025 19:58
Operator : MD/SY
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

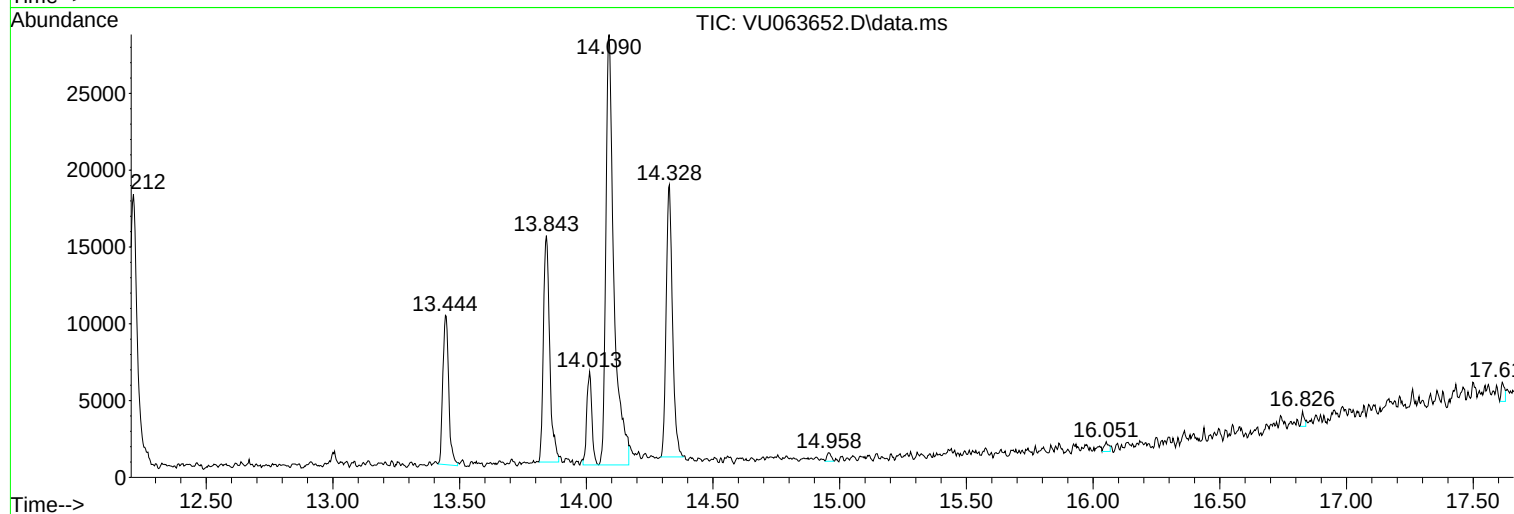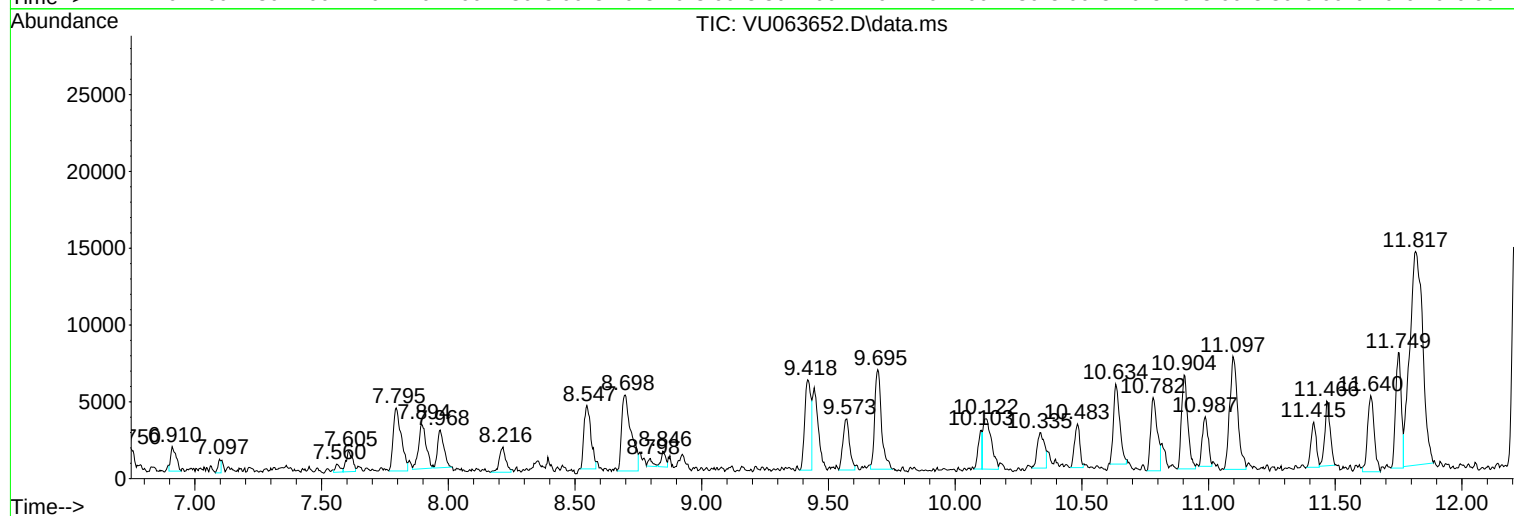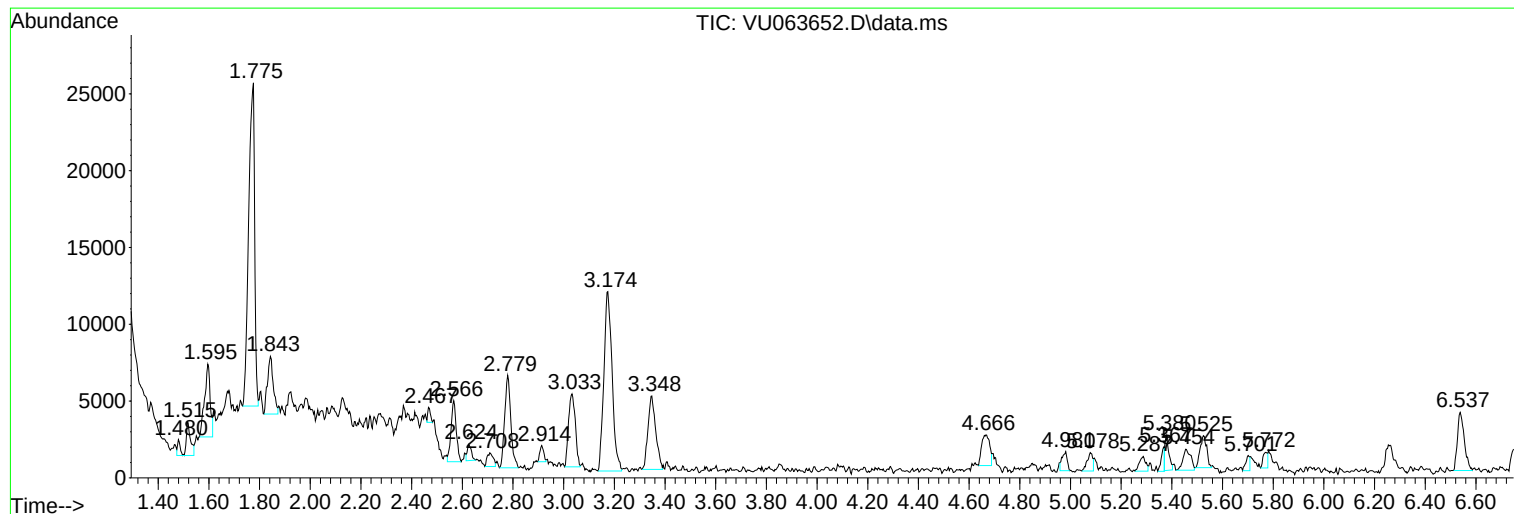

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
Data File : VU063652.D
Acq On : 25 Sep 2025 19:58
Operator : MD/SY
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
Data File : VU063652.D
Acq On : 25 Sep 2025 19:58
Operator : MD/SY
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------