


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092625\
Data File : VU063645.D
Acq On : 25 Sep 2025 15:50
Operator : MD/SY
Sample : BFB
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092625W.M
Title : SW846 8260
Last Update : Sat Sep 27 00:59:58 2025

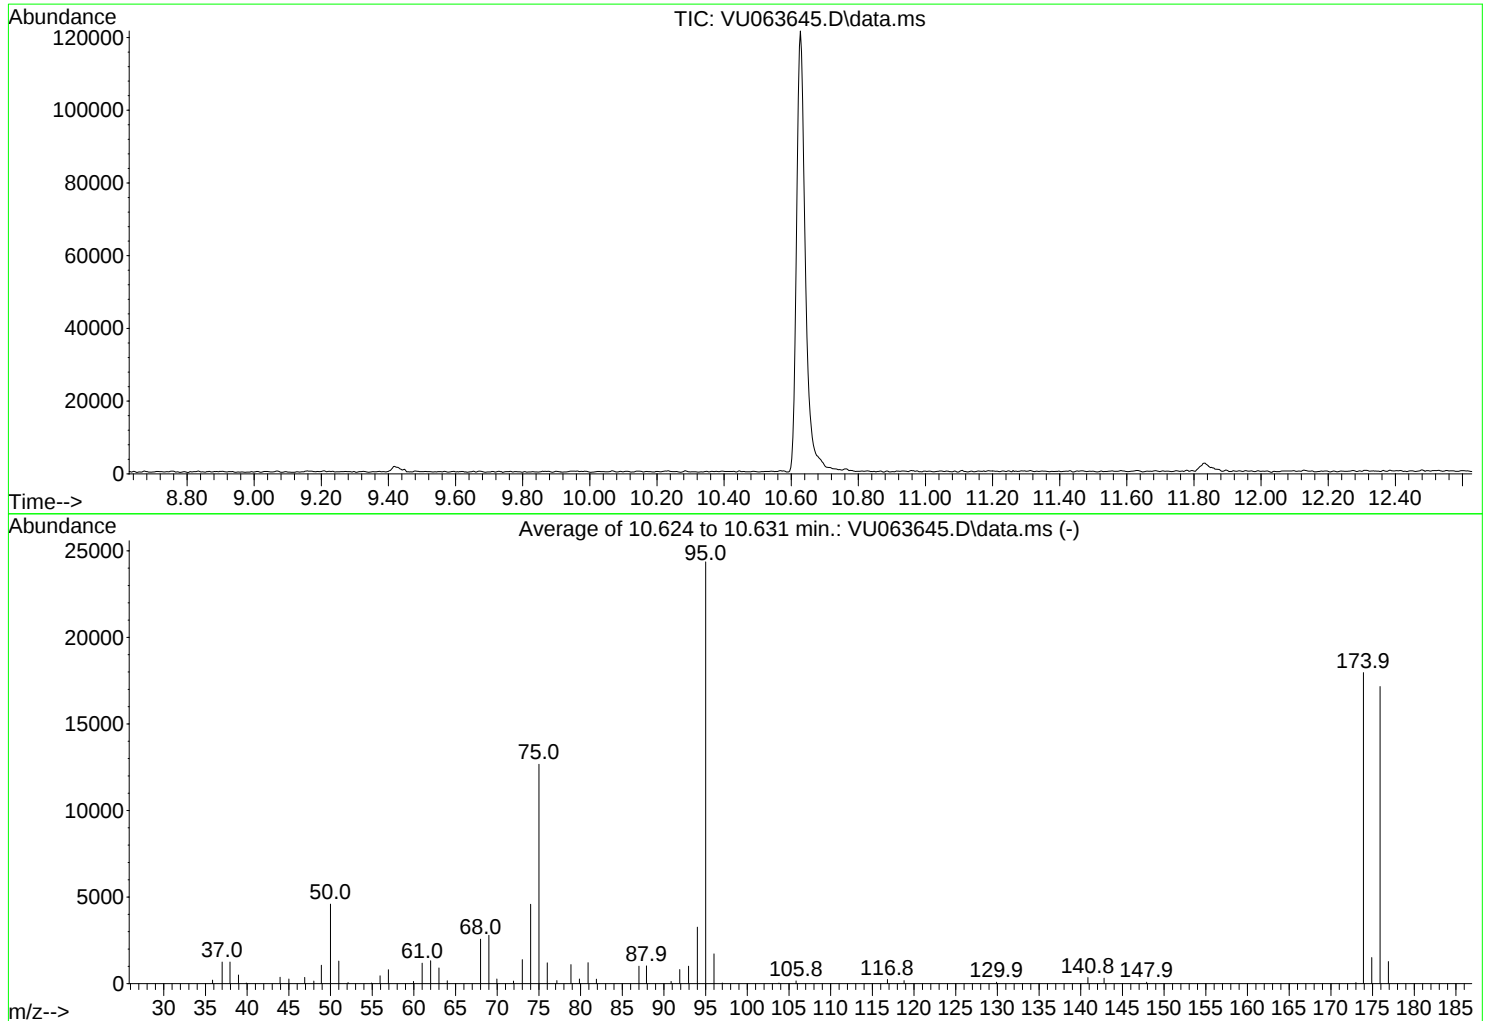

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4596	PASS
75	95	30	60	52.0	12674	PASS
95	95	100	100	100.0	24365	PASS
96	95	5	9	7.1	1719	PASS
173	174	0.00	2	0.4	66	PASS
174	95	50	100	73.8	17971	PASS
175	174	5	9	8.4	1508	PASS
176	174	95	101	95.5	17168	PASS
177	176	5	9	7.4	1276	PASS