


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092719\
 Data File : VU034843.D
 Acq On : 26 Sep 2019 14:07
 Operator : JC/SP
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Sep 28 00:27:34 2019

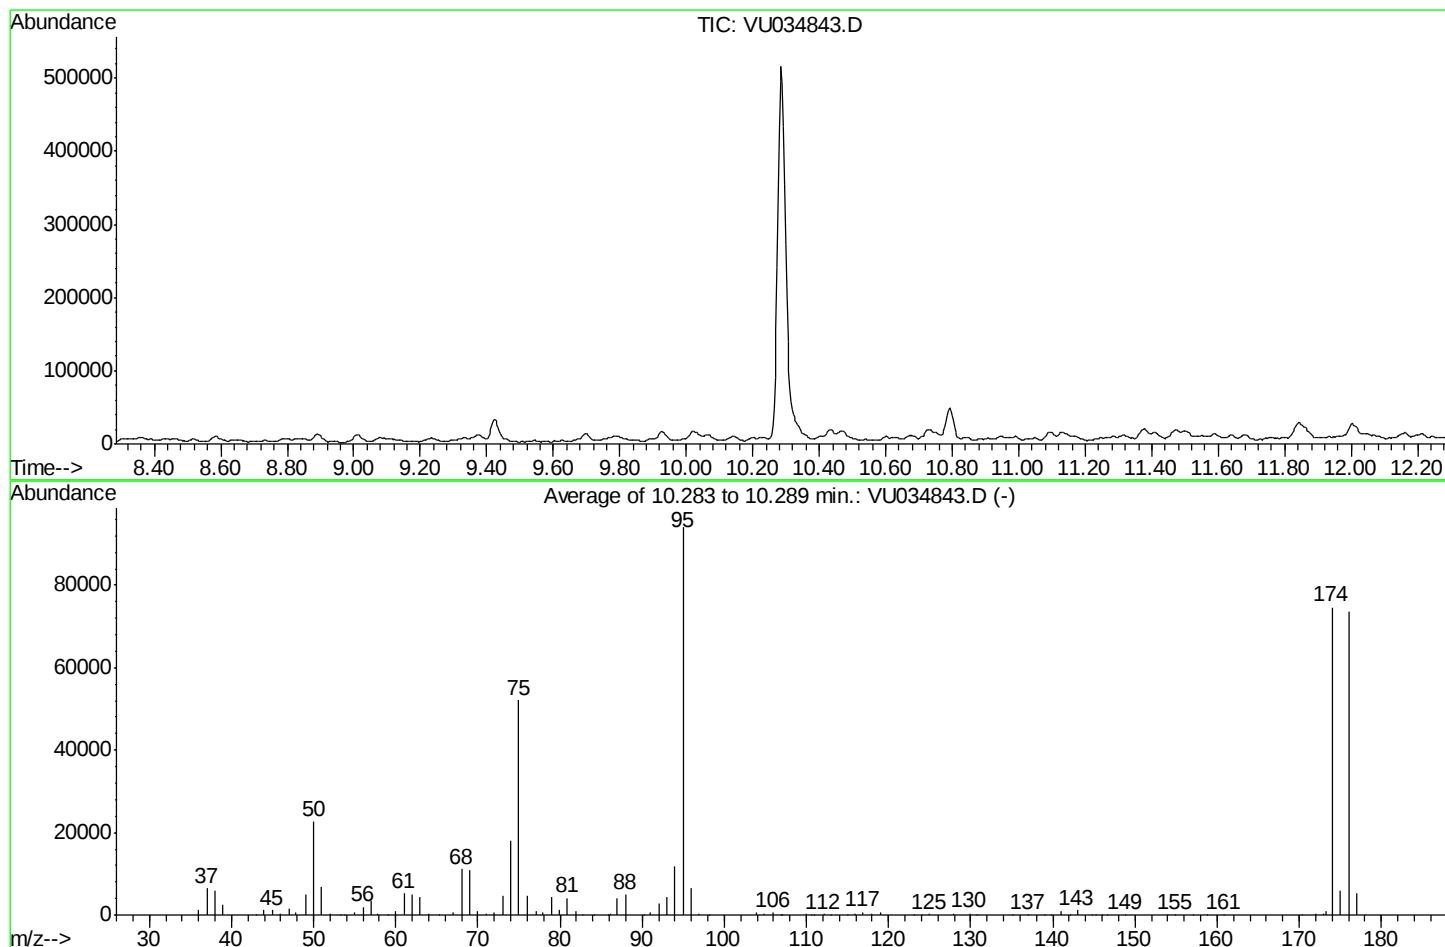

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	22605	PASS
75	95	30	80	55.3	52048	PASS
95	95	100	100	100.0	94074	PASS
96	95	5	9	7.1	6663	PASS
173	174	0.00	2	1.1	848	PASS
174	95	50	120	79.4	74669	PASS
175	174	5	9	8.1	6032	PASS
176	174	95	101	98.7	73720	PASS
177	176	5	9	7.1	5205	PASS

m/z	Abundance
36.00	1111.0
37.00	6563.0
38.00	5751.0
39.00	2833.0
40.00	442.0
40.90	728.0
43.00	1080.0
44.00	1922.0
45.00	1254.0
45.90	230.0
47.10	1524.0
47.90	708.0
49.00	5280.0
50.00	22880.0
51.00	7010.0
52.10	365.0
55.00	924.0
56.10	2086.0
57.00	3776.0
58.00	208.0
59.10	140.0
60.00	1134.0
61.00	5123.0
62.00	5002.0
63.00	3854.0
63.90	377.0
65.30	227.0
67.10	474.0
68.00	10935.0
69.00	11008.0
70.00	1148.0
71.00	499.0
71.90	600.0
73.00	4503.0
74.00	18096.0
75.00	51528.0
76.00	4558.0
77.10	981.0
77.90	582.0
78.90	4362.0
79.90	1156.0
80.90	4152.0
81.90	1073.0
82.70	145.0
84.20	507.0
85.10	430.0
85.80	137.0
86.20	186.0
86.90	3959.0
88.00	5151.0
90.20	122.0
91.00	470.0
92.00	2778.0
93.00	3890.0
94.00	12030.0
95.00	93584.0
96.00	6783.0
96.90	280.0
98.20	170.0
104.00	464.0
104.90	314.0
105.90	587.0
107.10	145.0
110.00	189.0
110.60	124.0
112.10	150.0
113.00	139.0
115.80	384.0
116.90	686.0
117.90	347.0
119.00	570.0
124.90	273.0
127.90	324.0
129.90	405.0
130.80	148.0
135.10	151.0
141.00	1064.0
143.00	1171.0
146.00	121.0
154.00	127.0
170.40	125.0
172.00	301.0
172.90	939.0
174.00	73328.0
175.00	5931.0
176.00	71912.0
177.00	4992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1150.0
37.00	6756.0
38.00	6305.0
39.00	2603.0
40.10	494.0
41.00	724.0
41.80	136.0
43.00	1157.0
44.00	1989.0
45.00	1270.0
45.90	245.0
47.00	1650.0
47.90	580.0
49.00	5294.0
50.00	23232.0
51.00	6956.0
52.00	317.0
53.30	112.0
55.10	1052.0
56.10	2076.0
57.00	4421.0
57.80	194.0
59.10	150.0
60.00	1021.0
61.00	5473.0
62.00	5070.0
63.00	4441.0
64.00	427.0
65.30	205.0
67.10	447.0
68.00	11475.0
69.00	11186.0
70.00	1174.0
71.00	610.0
72.00	631.0
73.00	4714.0
74.00	18736.0
75.00	53664.0
76.00	4691.0
77.10	1112.0
77.90	709.0
78.90	4542.0
79.90	1365.0
80.90	4142.0
82.00	996.0
82.80	102.0
84.20	412.0
85.10	329.0
86.10	194.0
86.90	4121.0
88.00	5066.0
90.20	128.0
91.10	577.0
92.00	2958.0
93.00	4555.0
94.00	12372.0
95.00	97368.0
96.00	6976.0
96.90	273.0
98.20	157.0
104.00	464.0
104.90	297.0
105.90	515.0
107.10	158.0
109.90	151.0
110.80	142.0
112.20	182.0
115.00	109.0
115.80	448.0
116.90	751.0
118.00	307.0
119.00	570.0
123.10	127.0
124.00	115.0
125.00	231.0
127.90	443.0
129.90	491.0
130.70	126.0
137.00	120.0
140.90	1018.0
142.10	109.0
143.00	1142.0
146.60	107.0
148.80	106.0
154.90	156.0
157.10	117.0
158.80	160.0
170.30	123.0
172.00	314.0
173.20	1343.0
174.00	76832.0
175.00	6406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

176.0076096.0

177.005434.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1126.0
37.00	6575.0
38.00	5918.0
39.00	2228.0
40.00	511.0
41.00	732.0
41.90	175.0
43.00	1479.0
44.00	1978.0
45.00	1234.0
45.90	212.0
47.00	1542.0
47.80	566.0
49.00	4759.0
50.00	21704.0
51.00	6278.0
52.00	220.0
53.30	173.0
53.80	101.0
55.10	1063.0
56.00	2018.0
57.00	4836.0
57.80	226.0
59.10	111.0
60.00	925.0
61.00	5212.0
62.00	4814.0
63.00	4491.0
64.00	422.0
66.90	364.0
67.10	373.0
68.00	10831.0
69.00	10234.0
70.00	1173.0
71.00	646.0
72.00	562.0
73.00	4580.0
74.00	17592.0
75.00	50952.0
76.00	4434.0
77.00	895.0
77.90	633.0
78.90	4611.0
79.90	1338.0
80.90	4224.0
81.90	874.0
82.80	112.0
84.20	296.0
85.10	260.0
86.10	207.0
87.00	4001.0
88.00	4332.0
91.10	578.0
92.00	3106.0
93.00	4882.0
94.00	11426.0
95.00	91272.0
96.00	6532.0
96.90	243.0
98.20	168.0
103.90	538.0
104.80	345.0
106.00	491.0
106.80	123.0
109.90	183.0
110.90	210.0
112.10	202.0
114.90	192.0
115.90	452.0
116.90	713.0
117.90	346.0
118.90	521.0
123.00	159.0
124.00	130.0
125.00	147.0
127.90	423.0
129.90	477.0
135.00	147.0
136.90	192.0
138.90	105.0
139.70	105.0
140.90	1022.0
142.10	151.0
143.00	1045.0
144.80	156.0
145.20	103.0
154.90	256.0
157.00	107.0
158.80	157.0
160.80	152.0
171.80	338.0
173.20	1203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

174.00	73848.0
175.00	6062.0
176.00	73152.0
177.00	5191.0
177.90	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
37.20	136.0
38.80	202.0
40.00	529.0
41.00	915.0
42.00	126.0
43.10	1135.0
43.90	831.0
45.00	100.0
55.00	411.0
55.80	221.0
56.20	176.0
57.10	806.0
69.90	113.0
71.00	331.0
84.10	249.0
85.10	349.0
96.20	100.0
97.90	339.0
109.70	103.0
175.00	101.0
207.10	168.0
288.90	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10