


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092719\
Data File : VU034863.D
Acq On : 27 Sep 2019 09:55
Operator : JC/SP
Sample : BFB11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091819WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Sep 28 00:27:34 2019

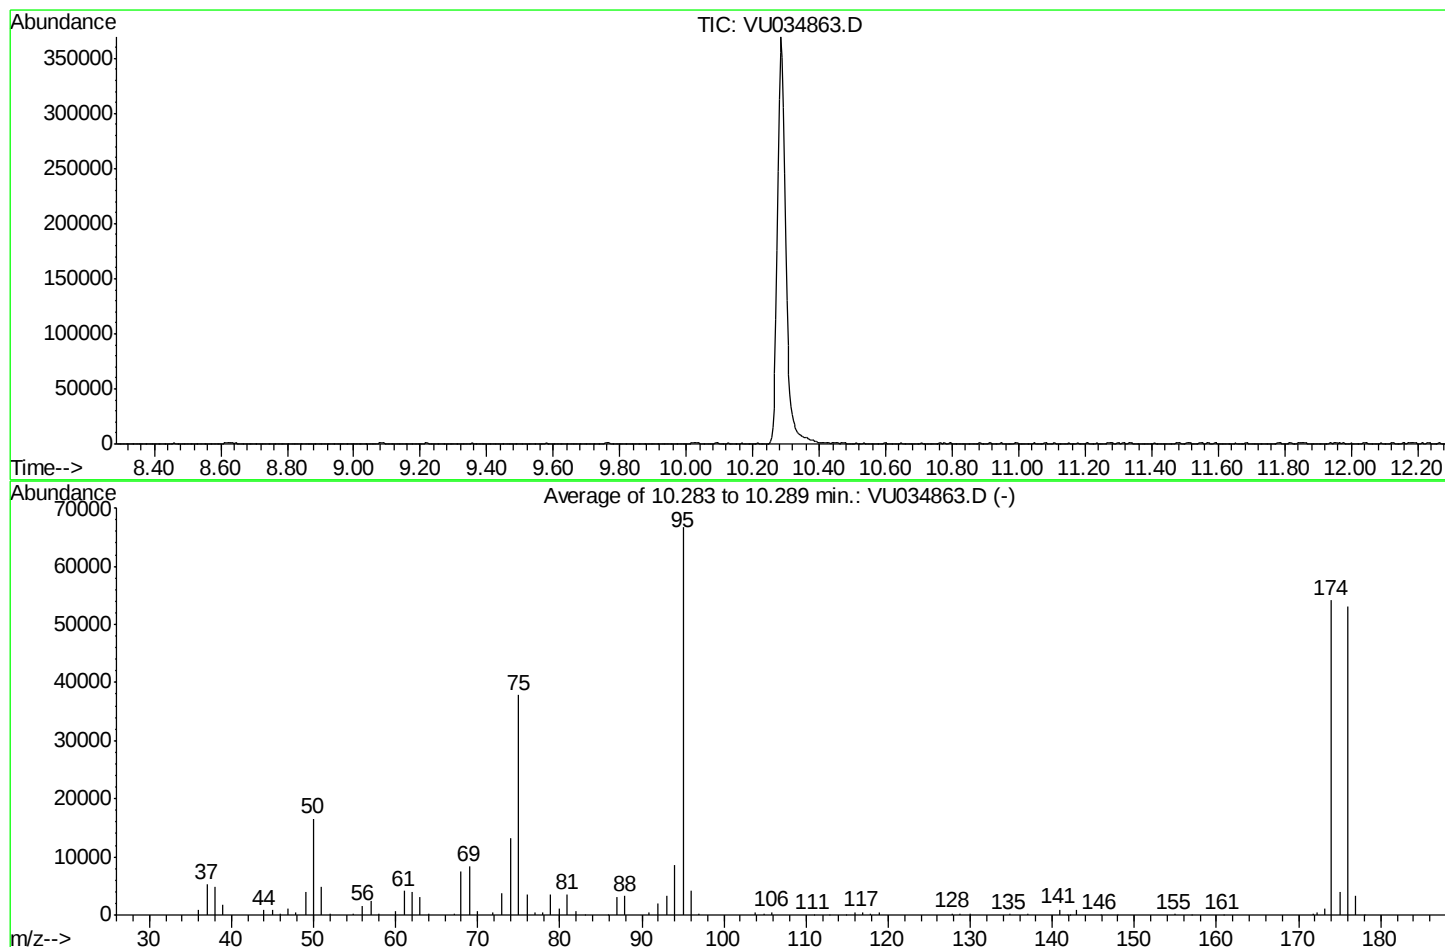

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	16581	PASS
75	95	30	80	56.6	37784	PASS
95	95	100	100	100.0	66698	PASS
96	95	5	9	6.2	4154	PASS
173	174	0.00	2	2.0	1071	PASS
174	95	50	120	81.1	54080	PASS
175	174	5	9	7.4	3981	PASS
176	174	95	101	98.2	53085	PASS
177	176	5	9	6.4	3400	PASS

m/z	Abundance
36.00	983.0
37.00	5387.0
38.00	4678.0
39.00	1823.0
39.80	147.0
44.00	1104.0
45.00	803.0
45.90	147.0
47.00	1059.0
47.90	661.0
49.00	3908.0
50.00	16976.0
51.00	4825.0
52.10	162.0
54.90	152.0
56.00	1647.0
57.00	2550.0
57.90	118.0
60.00	797.0
61.00	4277.0
62.00	4144.0
63.00	3209.0
64.00	272.0
67.20	297.0
68.00	7694.0
69.00	8091.0
70.00	704.0
71.90	513.0
73.00	3902.0
74.00	13132.0
75.00	37712.0
76.10	3536.0
77.00	429.0
77.90	376.0
78.90	3637.0
79.90	1094.0
80.90	3450.0
81.90	843.0
83.00	110.0
85.80	115.0
87.00	2880.0
87.90	3067.0
90.90	331.0
92.00	2025.0
93.00	3158.0
94.00	8406.0
95.00	66520.0
96.00	4221.0
97.00	134.0
103.80	372.0
104.90	143.0
105.90	495.0
110.90	118.0
115.90	370.0
116.90	494.0
117.90	317.0
118.90	381.0
127.80	230.0
128.80	143.0
129.90	223.0
134.70	187.0
136.90	136.0
140.90	933.0
142.90	819.0
154.90	140.0
156.90	114.0
160.80	116.0
171.70	273.0
172.30	326.0
173.20	1056.0
174.00	53000.0
175.00	3940.0
176.00	51632.0
177.00	3465.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	949.0
37.00	5476.0
38.00	5006.0
39.00	1893.0
39.80	146.0
44.00	1154.0
45.00	789.0
45.90	141.0
47.00	1111.0
47.90	571.0
49.00	3987.0
50.00	16944.0
51.00	5077.0
52.10	179.0
54.90	161.0
56.00	1673.0
57.00	2559.0
57.90	130.0
60.00	715.0
61.00	4260.0
62.00	4070.0
63.00	3283.0
64.00	278.0
67.10	296.0
68.00	7673.0
69.00	8639.0
70.00	731.0
71.90	480.0
73.00	3946.0
74.00	13506.0
75.00	39040.0
76.10	3631.0
77.00	448.0
77.90	385.0
78.90	3700.0
79.90	1170.0
80.90	3548.0
81.90	795.0
83.00	114.0
85.80	122.0
87.00	3078.0
87.90	3385.0
90.90	359.0
92.00	2082.0
93.00	3474.0
94.00	8703.0
95.00	68472.0
96.10	4323.0
97.00	137.0
103.90	448.0
104.90	143.0
105.90	528.0
110.90	107.0
112.80	111.0
114.80	116.0
115.90	401.0
116.80	538.0
117.90	312.0
118.90	438.0
127.90	315.0
128.80	147.0
129.90	216.0
134.70	153.0
136.90	178.0
140.90	941.0
141.80	112.0
142.90	881.0
145.90	156.0
147.80	116.0
154.90	126.0
160.90	107.0
171.80	278.0
172.30	373.0
173.10	1105.0
174.00	55680.0
175.00	4057.0
176.00	54824.0
177.00	3521.0
178.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	845.0
37.00	4978.0
38.00	4812.0
39.00	1791.0
39.90	173.0
44.00	1164.0
45.00	792.0
45.90	130.0
46.90	1076.0
47.90	441.0
49.00	3704.0
50.00	15825.0
51.00	4813.0
52.10	210.0
54.90	170.0
56.00	1562.0
57.00	2420.0
57.90	118.0
60.00	646.0
61.00	3999.0
62.00	3914.0
63.00	3073.0
64.00	287.0
67.10	285.0
68.00	7334.0
69.00	8150.0
70.00	673.0
71.90	462.0
73.00	3631.0
74.00	12809.0
75.00	36600.0
76.00	3224.0
76.90	404.0
77.90	369.0
78.90	3556.0
79.90	1079.0
80.90	3382.0
81.90	682.0
87.00	2985.0
87.90	3328.0
90.90	368.0
91.90	2027.0
93.00	3472.0
94.00	8460.0
95.00	65104.0
96.10	3918.0
97.00	125.0
103.90	485.0
104.80	133.0
105.90	483.0
114.80	129.0
115.90	376.0
116.80	521.0
117.90	319.0
118.90	418.0
127.90	352.0
128.80	140.0
130.00	218.0
134.80	122.0
137.00	183.0
140.90	879.0
141.80	124.0
142.20	143.0
142.90	901.0
145.90	155.0
147.90	142.0
154.90	136.0
172.20	337.0
173.10	1053.0
174.00	53560.0
175.00	3947.0
176.00	52800.0
177.00	3216.0
178.00	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Scan 2847 (10.244 min): VU034863.D
BFB11

m/z	Abundance
39.80	156.0
43.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11