

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
 Data File : VU044894.D
 Acq On : 27 Sep 2021 17:19
 Operator : SY/MD
 Sample : M3888-06DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 20897DL

Quant Time: Sep 27 17:40:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 25 09:30:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.375	168	199669	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	350545	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	333879	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	167506	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	158877	45.592	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.180%	
35) Dibromofluoromethane	5.292	113	108618	45.167	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.340%	
50) Toluene-d8	7.899	98	447447	49.265	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.540%	
62) 4-Bromofluorobenzene	10.635	95	178008	52.768	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.540%	
Target Compounds						Qvalue
3) Chloromethane	1.517	50	1107	0.305	ug/l	90
5) Bromomethane	1.832	94	629	Below Cal		89
11) Tert butyl alcohol	3.192	59	3232	3.178	ug/l #	72
16) Acetone	2.633	43	8839	4.497	ug/l	99
17) Carbon Disulfide	2.787	76	1716	0.254	ug/l #	89
18) Methyl Acetate	2.954	43	6865	1.045	ug/l	95
20) Methylene Chloride	3.047	84	2137	0.672	ug/l	95
25) 2-Butanone	4.723	43	2536	0.850	ug/l #	87
31) Cyclohexane	5.375	56	5351	1.070	ug/l #	10
36) 1,1-Dichloropropene	5.375	75	19210	5.165	ug/l #	49
38) Carbon Tetrachloride	5.375	117	20981	6.310	ug/l #	15
40) Benzene	5.777	78	744707	65.673	ug/l	99
42) 1,2-Dichloroethane	5.777	62	7339	1.645	ug/l #	75
52) Toluene	7.973	92	420412	62.011	ug/l	99
53) t-1,3-Dichloropropene	7.970	75	5208	1.246	ug/l #	1
55) 1,1,2-Trichloroethane	8.275	97	8301	2.864	ug/l #	17
56) Ethyl methacrylate	8.275	69	503	1.979	ug/l #	16
59) 2-Hexanone	8.693	43	989	0.226	ug/l	87
67) Ethyl Benzene	9.574	91	64286	5.196	ug/l	100
68) m/p-Xylenes	9.697	106	137921	29.148	ug/l	98
69) o-Xylene	10.105	106	107443	23.483	ug/l	97
70) Styrene	10.118	104	51062	6.862	ug/l #	70
76) 1,2,3-Trichloropropane	10.635	75	97377	19.198	ug/l #	41
78) n-propylbenzene	10.909	91	5159	0.358	ug/l	100
79) 2-Chlorotoluene	11.002	91	3468	0.395	ug/l #	43
80) 1,3,5-Trimethylbenzene	11.092	105	14120	1.402	ug/l	97
81) trans-1,4-Dichloro-2-b...	10.635	75	97377	62.190	ug/l #	9
83) tert-Butylbenzene	11.471	119	6165	0.635	ug/l #	57
84) 1,2,4-Trimethylbenzene	11.471	105	55295	5.570	ug/l	97
85) sec-Butylbenzene	11.471	105	55295	4.402	ug/l #	58
89) n-Butylbenzene	12.214	91	500	1.322	ug/l #	53
90) Hexachloroethane	12.623	117	490	0.266	ug/l #	15
95) Naphthalene	14.089	128	451934	35.455	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_U
ClientSampleId :
20897DL

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044894.D
Acq On : 27 Sep 2021 17:19
Operator : SY/MD
Sample : M3888-06DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
20897DL

Quant Time: Sep 27 17:40:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 25 09:30:46 2021
Response via : Initial Calibration




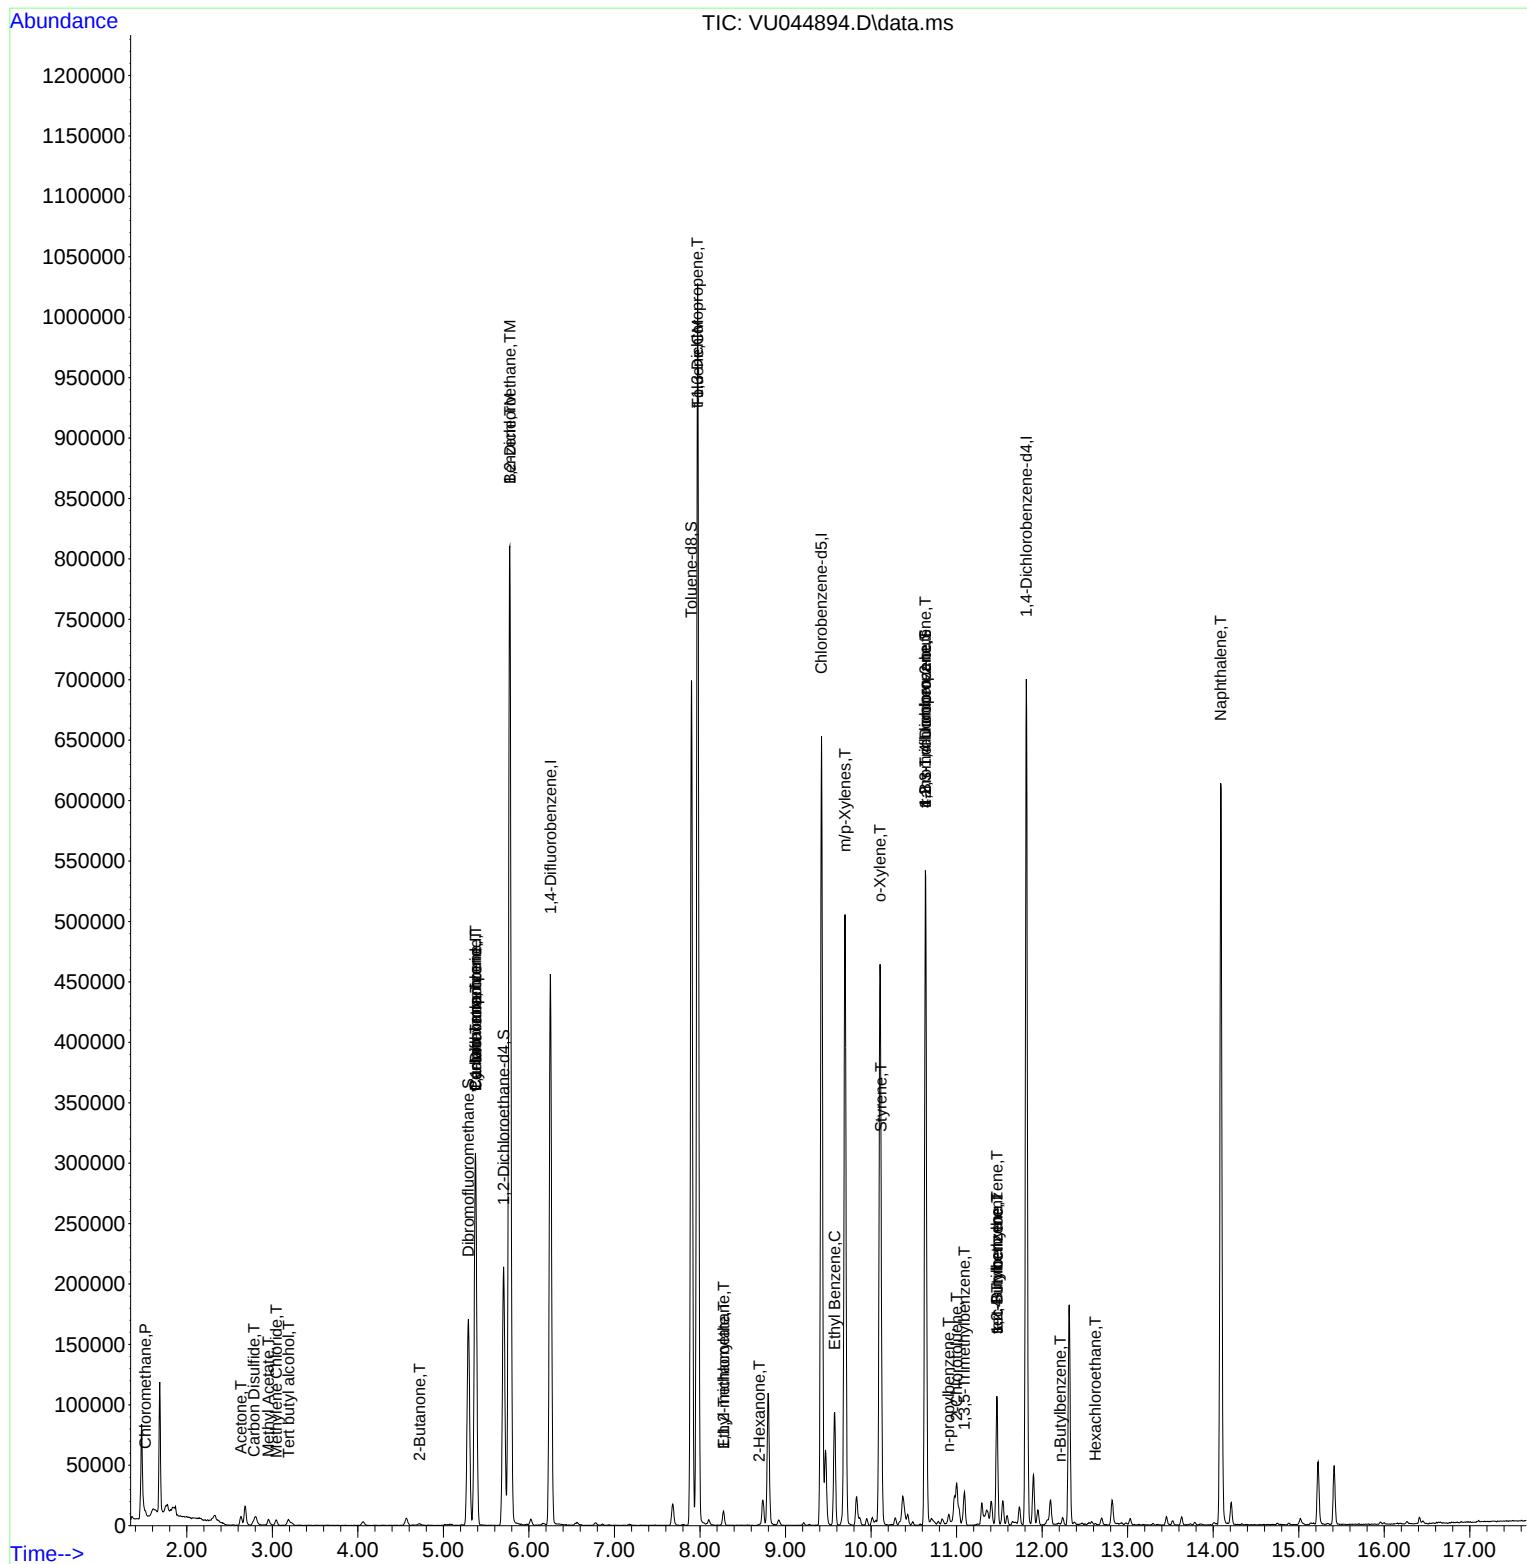


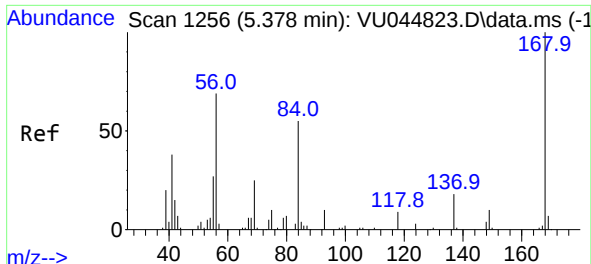

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampleId :
20897DL


Tgt Ion:168 Resp: 199669
Ion Ratio Lower Upper
168 100
99 63.6 51.4 77.0

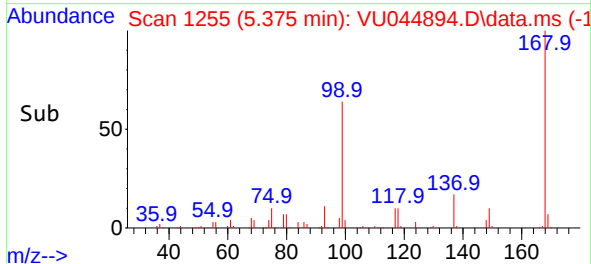

#3
Chloromethane
Concen: 0.305 ug/l
RT: 1.517 min Scan# 55
Delta R.T. -0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 50 Resp: 1107
Ion Ratio Lower Upper
50 100
52 27.0 26.3 39.5


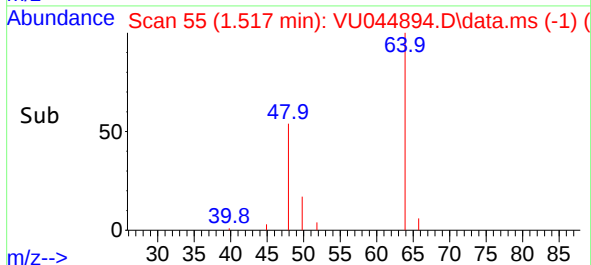

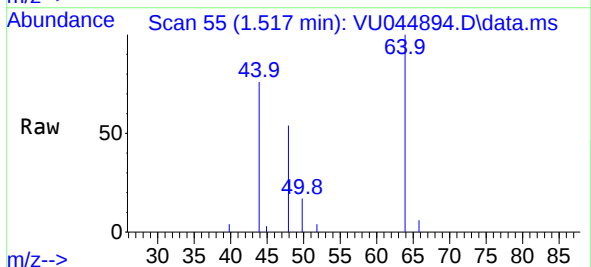




#5
Bromomethane
Concen: Below Cal
RT: 1.832 min Scan# 153
Delta R.T. -0.016 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 94 Resp: 629
Ion Ratio Lower Upper
94 100
96 82.3 74.5 111.7



#11
Tert butyl alcohol
Concen: 3.178 ug/l
RT: 3.192 min Scan# 576
Delta R.T. -0.013 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 59 Resp: 3232
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


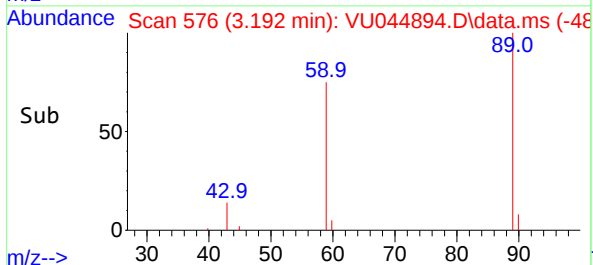

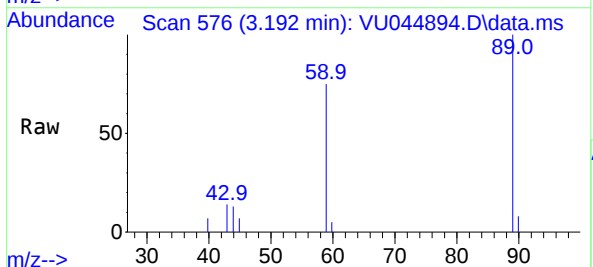




#16
Acetone
Concen: 4.497 ug/l
RT: 2.633 min Scan# 402
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 43 Resp: 8839
Ion Ratio Lower Upper
43 100
58 32.1 25.2 37.8

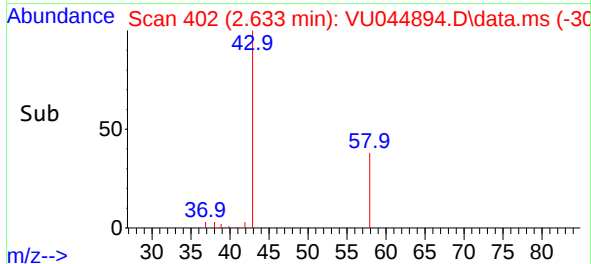

#17
Carbon Disulfide
Concen: 0.254 ug/l
RT: 2.787 min Scan# 450
Delta R.T. -0.010 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 76 Resp: 1716
Ion Ratio Lower Upper
76 100
78 13.3 7.4 11.0#



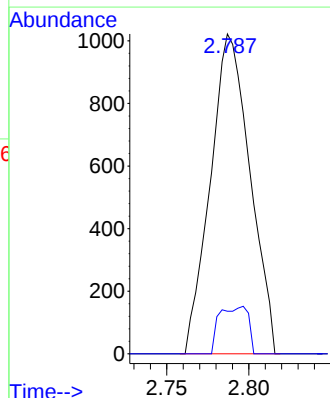
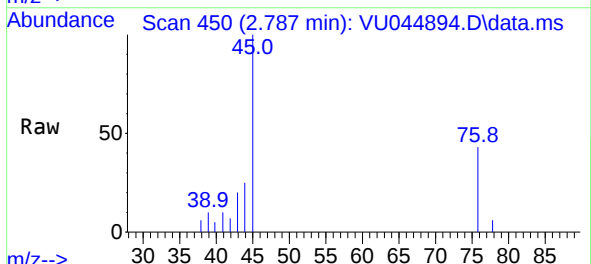




#18
Methyl Acetate
Concen: 1.045 ug/l
RT: 2.954 min Scan# 502
Delta R.T. 0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 43 Resp: 6865
Ion Ratio Lower Upper
43 100
74 21.2 19.0 28.6

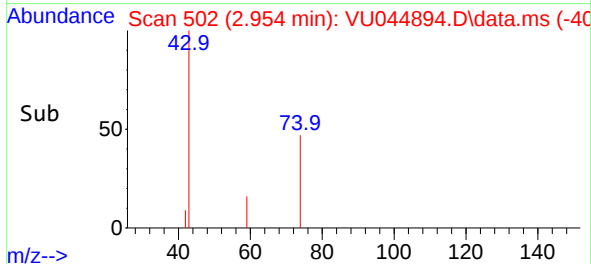

#20
Methylene Chloride
Concen: 0.672 ug/l
RT: 3.047 min Scan# 531
Delta R.T. -0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 84 Resp: 2137
Ion Ratio Lower Upper
84 100
49 136.9 104.9 157.3
51 34.6 31.8 47.8
86 65.7 49.8 74.6

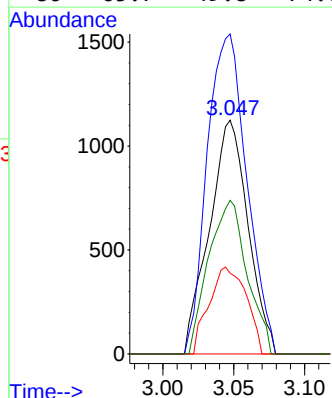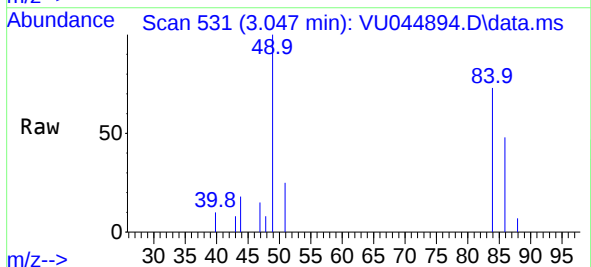







#25

2-Butanone
Concen: 0.850 ug/l
RT: 4.723 min Scan# 1052
Delta R.T. 0.013 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Instrument :
MSVOA_U
ClientSampled :
20897DL




Tgt Ion: 43 Resp: 2536
Ion Ratio Lower Upper
43 100
72 19.9 21.3 31.9#

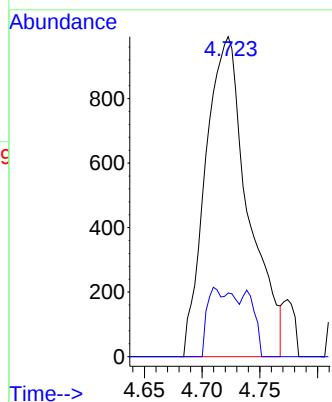


#31

Cyclohexane
Concen: 1.070 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.019 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 56 Resp: 5351
Ion Ratio Lower Upper
56 100
69 157.4 25.2 37.8#
84 117.6 66.4 99.6#

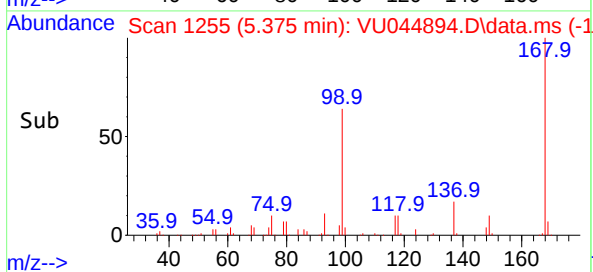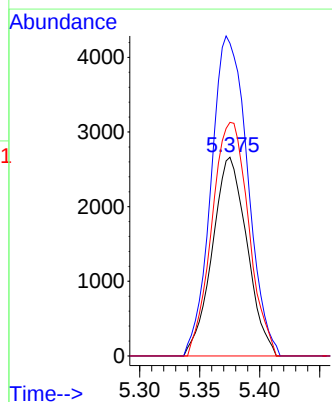







#33

1,2-Dichloroethane-d4
Concen: 45.592 ug/l
RT: 5.703 min Scan# 1357
Delta R.T. -0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Instrument :
MSVOA_U
ClientSampled :
20897DL




Tgt Ion: 65 Resp: 158877
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.8

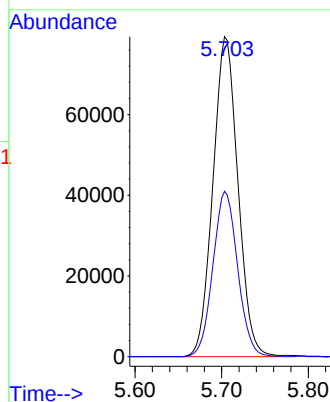


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.253 min Scan# 1528
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 114 Resp: 350545
Ion Ratio Lower Upper
114 100
63 23.1 0.0 47.8
88 16.8 0.0 32.8









#35
Dibromofluoromethane
Concen: 45.167 ug/l
RT: 5.292 min Scan# 1229
Delta R.T. -0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion:113 Resp: 108618
Ion Ratio Lower Upper
113 100
111 103.4 84.1 126.1
192 17.8 14.8 22.2



#36
1,1-Dichloropropene
Concen: 5.165 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.154 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19


Tgt Ion: 75 Resp: 19210
Ion Ratio Lower Upper
75 100
110 6.6 16.3 48.9#
77 0.0 25.0 37.4#

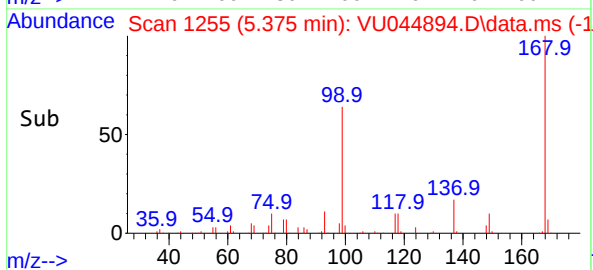






#38
Carbon Tetrachloride
Concen: 6.310 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.154 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19


Instrument :
MSVOA_U
ClientSampled :
20897DL





Tgt Ion:117 Resp: 20981
Ion Ratio Lower Upper
117 100
119 5.0 77.4 116.2#
121 0.0 24.5 36.7#




#40
Benzene
Concen: 65.673 ug/l
RT: 5.777 min Scan# 1380
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

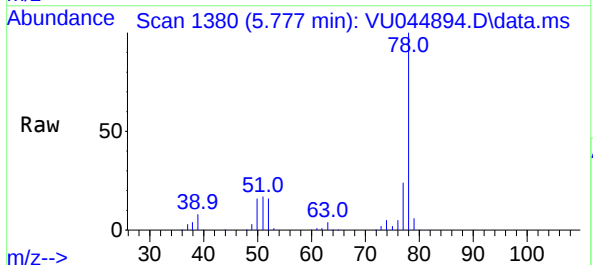

Tgt Ion: 78 Resp: 744707
Ion Ratio Lower Upper
78 100
77 24.2 19.1 28.7

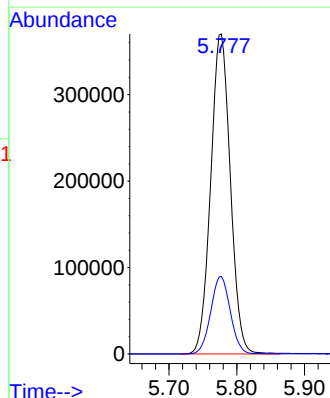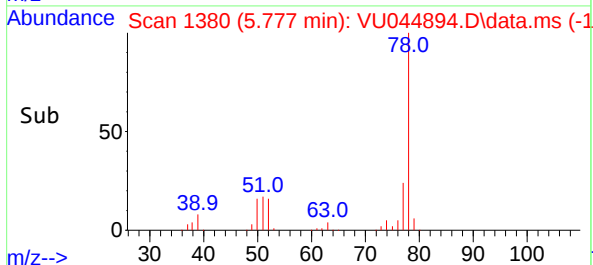



#42

1,2-Dichloroethane

Concen: 1.645 ug/l

RT: 5.777 min Scan# 1380

Delta R.T. -0.023 min

Lab File: VU044894.D





Acq: 27 Sep 2021 17:19

Tgt Ion: 62 Resp: 7339

Ion Ratio Lower Upper

62 100

98 0.0 0.0 17.8



#50

Toluene-d8

Concen: 49.265 ug/l

RT: 7.899 min Scan# 2040

Delta R.T. -0.003 min

Lab File: VU044894.D




Acq: 27 Sep 2021 17:19


Tgt Ion: 98 Resp: 447447

Ion Ratio Lower Upper

98 100

100 64.6 52.5 78.7



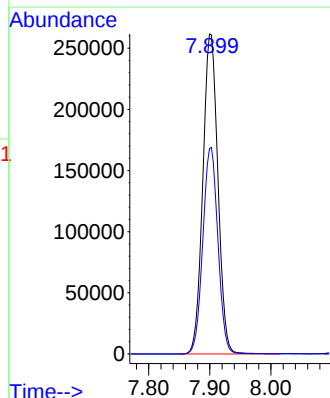





#52
Toluene
Concen: 62.011 ug/l
RT: 7.973 min Scan# 2063
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampleId :
20897DL


Tgt Ion: 92 Resp: 420412
Ion Ratio Lower Upper
92 100
91 169.7 136.9 205.3

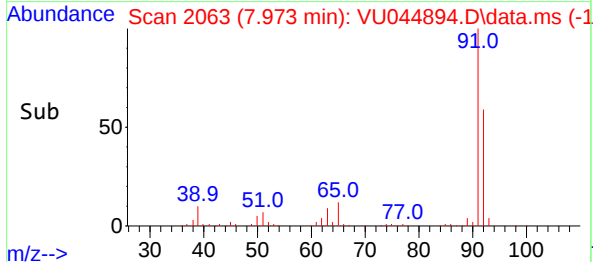

#53
t-1,3-Dichloropropene
Concen: 1.246 ug/l
RT: 7.970 min Scan# 2062
Delta R.T. -0.244 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 75 Resp: 5208
Ion Ratio Lower Upper
75 100
77 141.2 25.6 38.4#


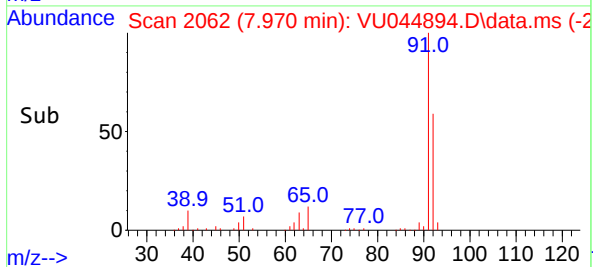

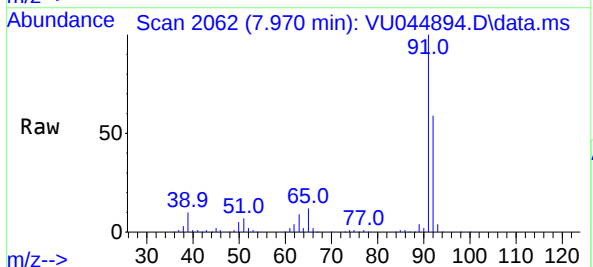




#55
1,1,2-Trichloroethane
Concen: 2.864 ug/l
RT: 8.275 min Scan# 2157
Delta R.T. -0.129 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 97	Resp:	8301
Ion	Ratio	Lower Upper
97	100	
83	0.0	69.7 104.5#
85	0.0	44.8 67.2#
99	6.4	49.3 73.9#



#56
Ethyl methacrylate
Concen: 1.979 ug/l
RT: 8.275 min Scan# 2157
Delta R.T. -0.062 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 69	Resp:	503
Ion	Ratio	Lower Upper
69	100	
41	0.0	53.5 80.3#
39	91.1	31.1 46.7#


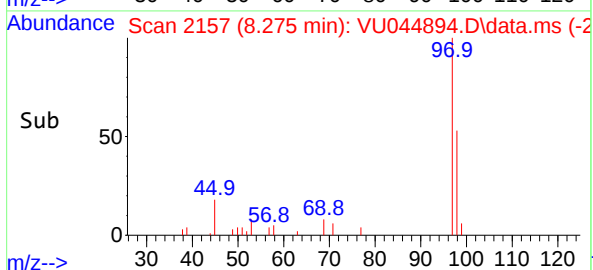
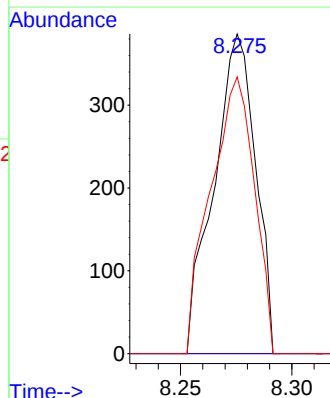





#59
2-Hexanone
Concen: 0.226 ug/l
RT: 8.693 min Scan# 2287
Delta R.T. 0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 43 Resp: 989
Ion Ratio Lower Upper
43 100
58 46.3 28.0 84.0

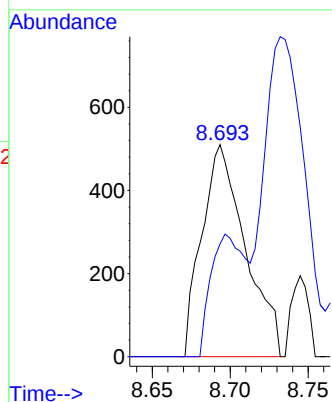

#62
4-Bromofluorobenzene
Concen: 52.768 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 95 Resp: 178008
Ion Ratio Lower Upper
95 100
174 71.6 0.0 146.6
176 68.5 0.0 141.2


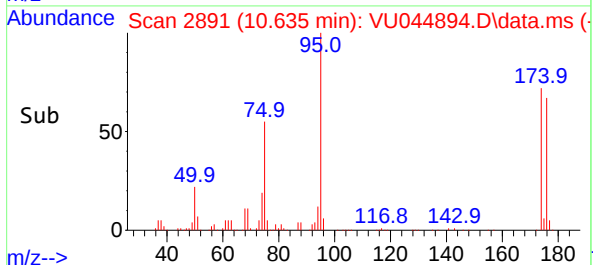

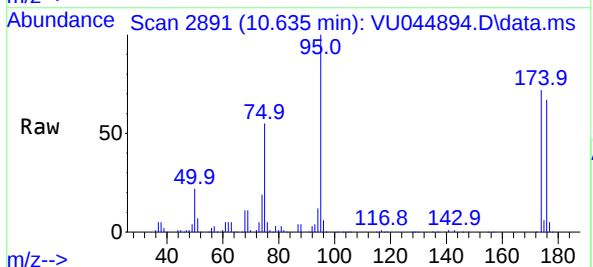




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampleId :
20897DL


Tgt Ion:117 Resp: 333879
Ion Ratio Lower Upper
117 100
82 60.6 47.8 71.8
119 32.3 25.8 38.6

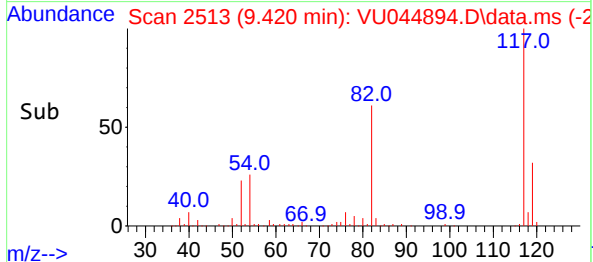

#67
Ethyl Benzene
Concen: 5.196 ug/l
RT: 9.574 min Scan# 2561
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 91 Resp: 64286
Ion Ratio Lower Upper
91 100
106 30.6 24.3 36.5


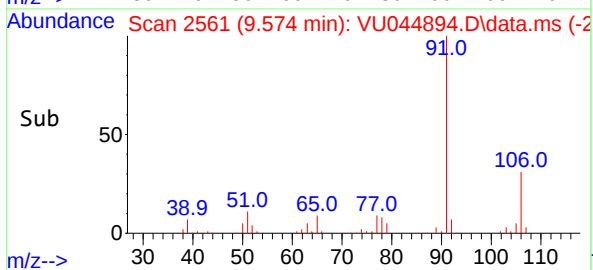






#68
m/p-Xylenes
Concen: 29.148 ug/l
RT: 9.697 min Scan# 2599
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampleId :
20897DL


Tgt Ion:106 Resp: 137921
Ion Ratio Lower Upper
106 100
91 209.0 164.2 246.2

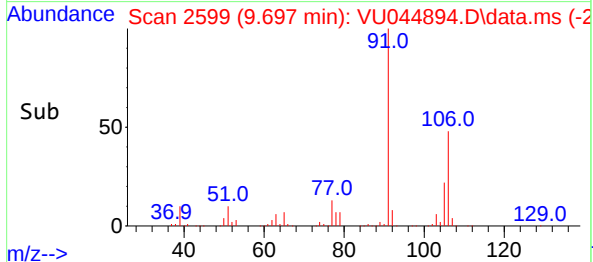

#69
o-Xylene
Concen: 23.483 ug/l
RT: 10.105 min Scan# 2726
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion:106 Resp: 107443
Ion Ratio Lower Upper
106 100
91 222.7 108.9 326.7


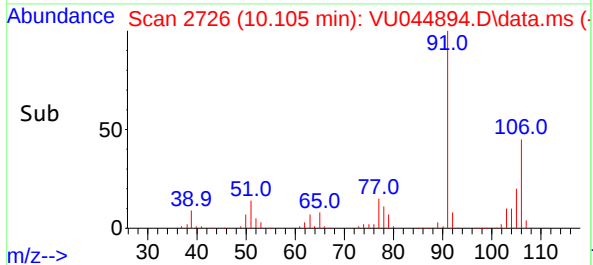

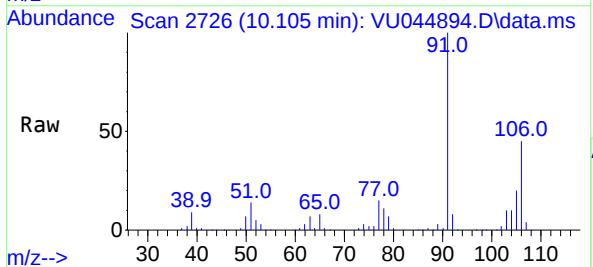




#70
Styrene
Concen: 6.862 ug/l
RT: 10.118 min Scan# 2730
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion:104 Resp: 51062
Ion Ratio Lower Upper
104 100
78 74.2 41.4 62.0#
103 74.0 43.5 65.3#

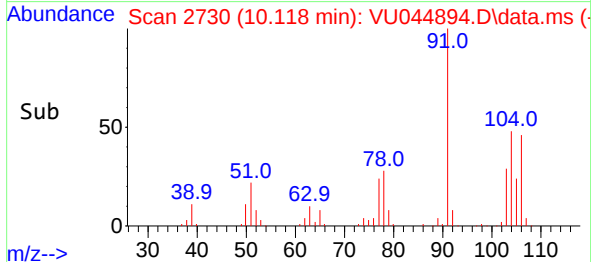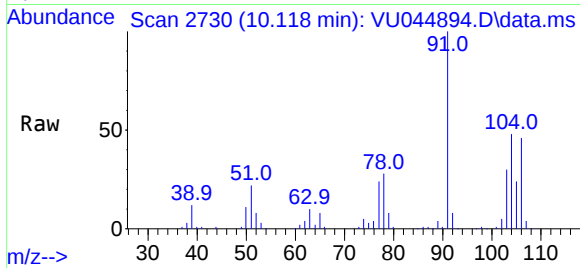

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.816 min Scan# 3258
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion:152 Resp: 167506
Ion Ratio Lower Upper
152 100
115 62.5 43.5 130.7
150 155.8 0.0 350.0


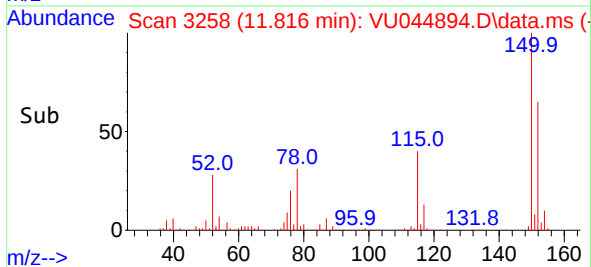

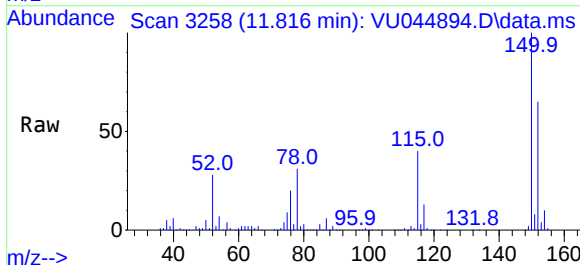




#76
1,2,3-Trichloropropane
Concen: 19.198 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.193 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 75 Resp: 97377
Ion Ratio Lower Upper
75 100
77 1.1 17.9 53.7#

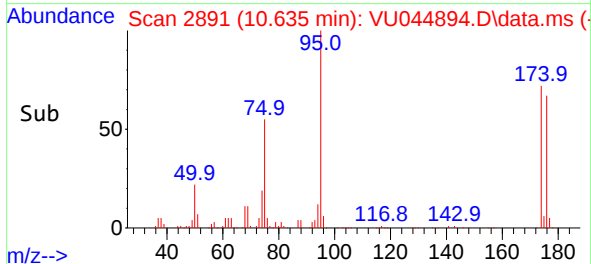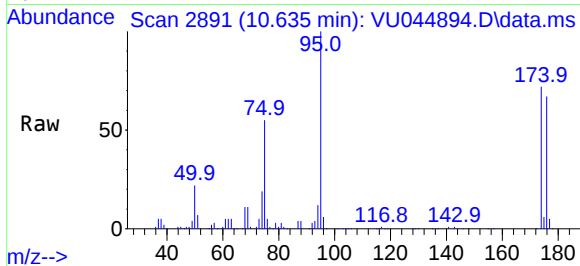

#78
n-propylbenzene
Concen: 0.358 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 91 Resp: 5159
Ion Ratio Lower Upper
91 100
120 21.6 10.8 32.4


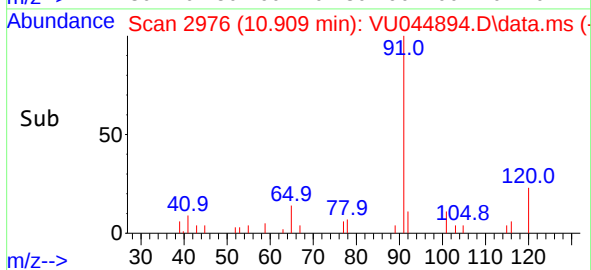

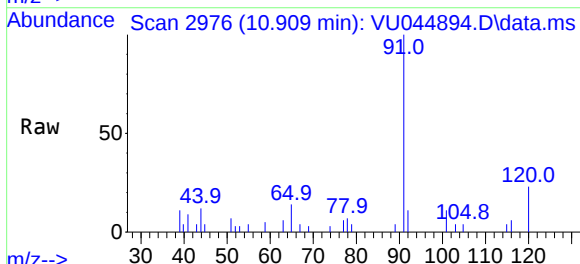




#79
2-Chlorotoluene
Concen: 0.395 ug/l
RT: 11.002 min Scan# 3005
Delta R.T. 0.013 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 91 Resp: 3468
Ion Ratio Lower Upper
91 100
126 0.0 15.7 47.0#

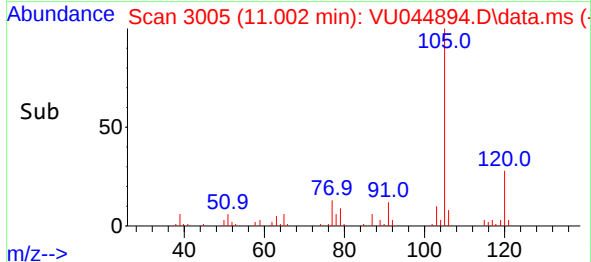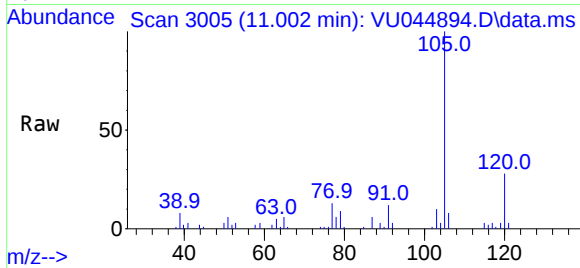

#80
1,3,5-Trimethylbenzene
Concen: 1.402 ug/l
RT: 11.092 min Scan# 3033
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 105 Resp: 14120
Ion Ratio Lower Upper
105 100
120 50.1 24.1 72.2


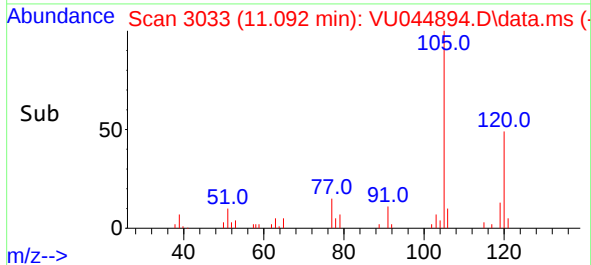

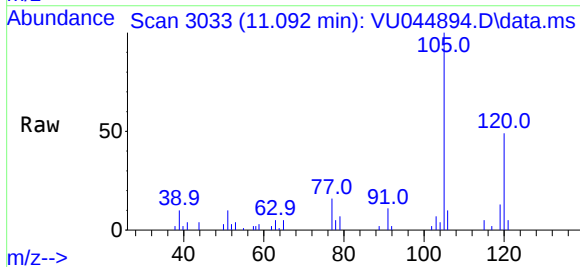




#81
trans-1,4-Dichloro-2-butene
Concen: 62.190 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. 0.084 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampleId :
20897DL


Tgt Ion: 75 Resp: 97377
Ion Ratio Lower Upper
75 100
53 0.1 82.0 123.0#
89 0.0 34.2 51.4#

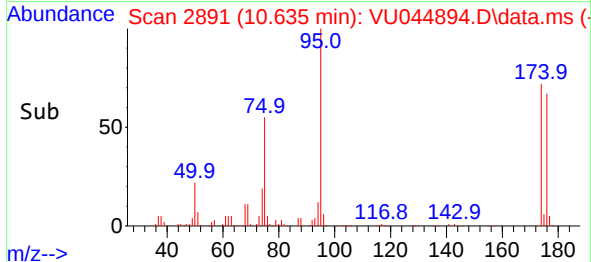

#83
tert-Butylbenzene
Concen: 0.635 ug/l
RT: 11.471 min Scan# 3151
Delta R.T. 0.048 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 119 Resp: 6165
Ion Ratio Lower Upper
119 100
91 92.1 30.4 91.2#
134 0.0 11.5 34.5#


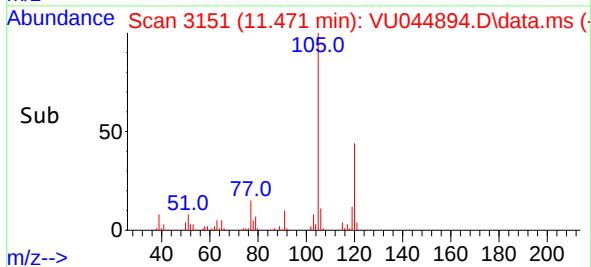

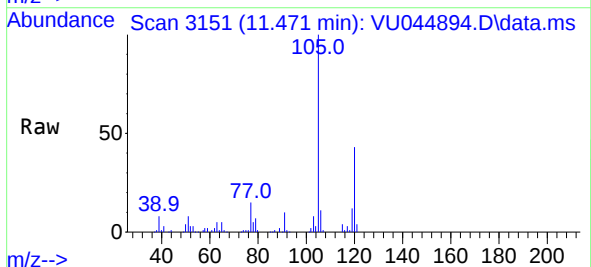




#84
1,2,4-Trimethylbenzene
Concen: 5.570 ug/l
RT: 11.471 min Scan# 3151
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion:105 Resp: 55295
Ion Ratio Lower Upper
105 100
120 42.7 22.4 67.3

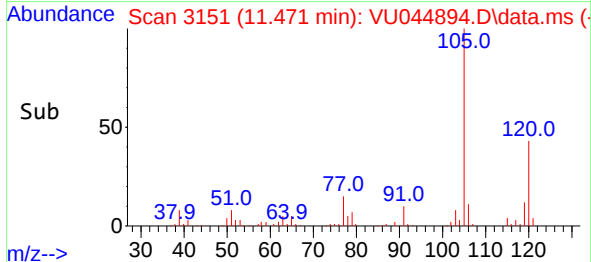

#85
sec-Butylbenzene
Concen: 4.402 ug/l
RT: 11.471 min Scan# 3151
Delta R.T. -0.177 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion:105 Resp: 55295
Ion Ratio Lower Upper
105 100
134 0.0 9.3 28.0#


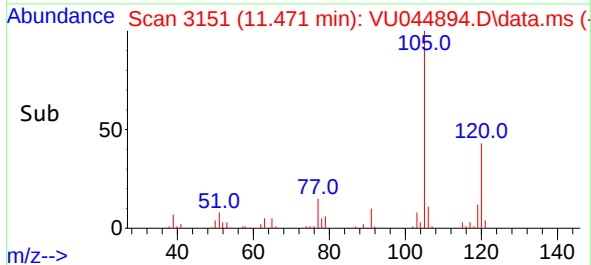

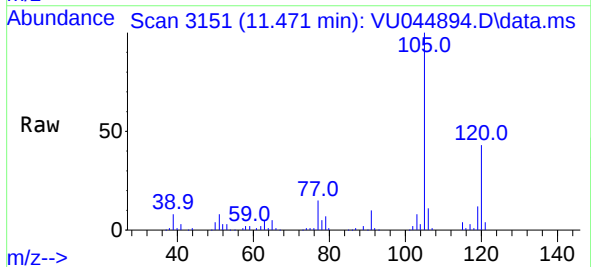




#89
n-Butylbenzene
Concen: 1.322 ug/l
RT: 12.214 min Scan# 3382
Delta R.T. 0.003 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19




Instrument :
MSVOA_U
ClientSampled :
20897DL


Tgt Ion: 91 Resp: 500
Ion Ratio Lower Upper
91 100
92 29.2 26.8 80.4
134 60.6 11.8 35.4#

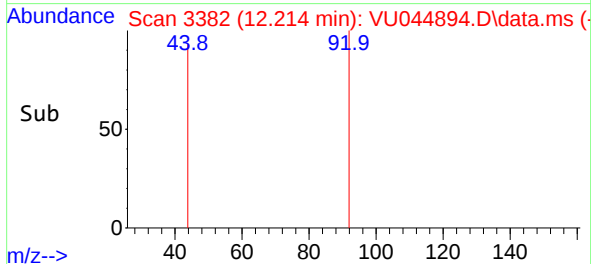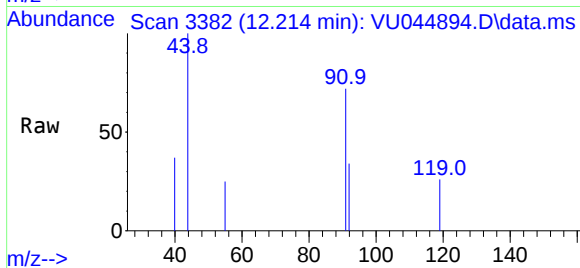

#90
Hexachloroethane
Concen: 0.266 ug/l
RT: 12.623 min Scan# 3509
Delta R.T. 0.145 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Tgt Ion: 117 Resp: 490
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.3#

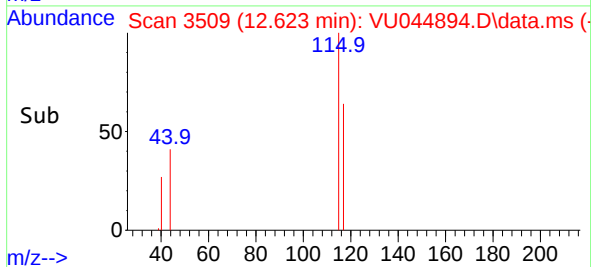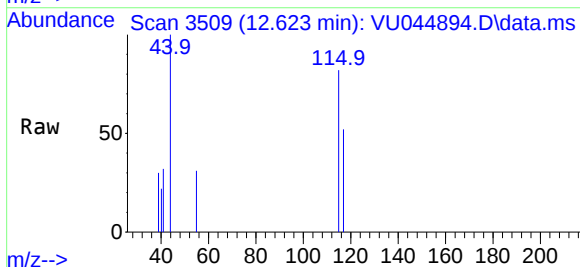



#95
Naphthalene
Concen: 35.455 ug/l
RT: 14.089 min Scan# 3965
Delta R.T. -0.000 min
Lab File: VU044894.D
Acq: 27 Sep 2021 17:19

Instrument :
MSVOA_U
ClientSampleId :
20897DL

Tgt Ion:128 Resp: 451934

Ion	Ratio	Lower	Upper
128	100		
127	13.1	10.4	15.6
129	10.9	8.6	13.0

