

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
 Data File : VU044916.D
 Acq On : 28 Sep 2021 03:04
 Operator : SY/MD
 Sample : M3829-07DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RE108D2-20210917DL

Quant Time: Sep 28 06:31:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 25 09:30:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.375	168	198574	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	353765	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	319235	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.815	152	153811	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	158945	45.863	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.720%	
35) Dibromofluoromethane	5.292	113	108394	44.664	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.320%	
50) Toluene-d8	7.902	98	439748	47.977	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.960%	
62) 4-Bromofluorobenzene	10.635	95	160295	47.085	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.160%	
Target Compounds						
44) Trichloroethene	6.546	130	126053	45.831	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044916.D
Acq On : 28 Sep 2021 03:04
Operator : SY/MD
Sample : M3829-07DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE108D2-20210917DL


Quant Time: Sep 28 06:31:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 25 09:30:46 2021
Response via : Initial Calibration

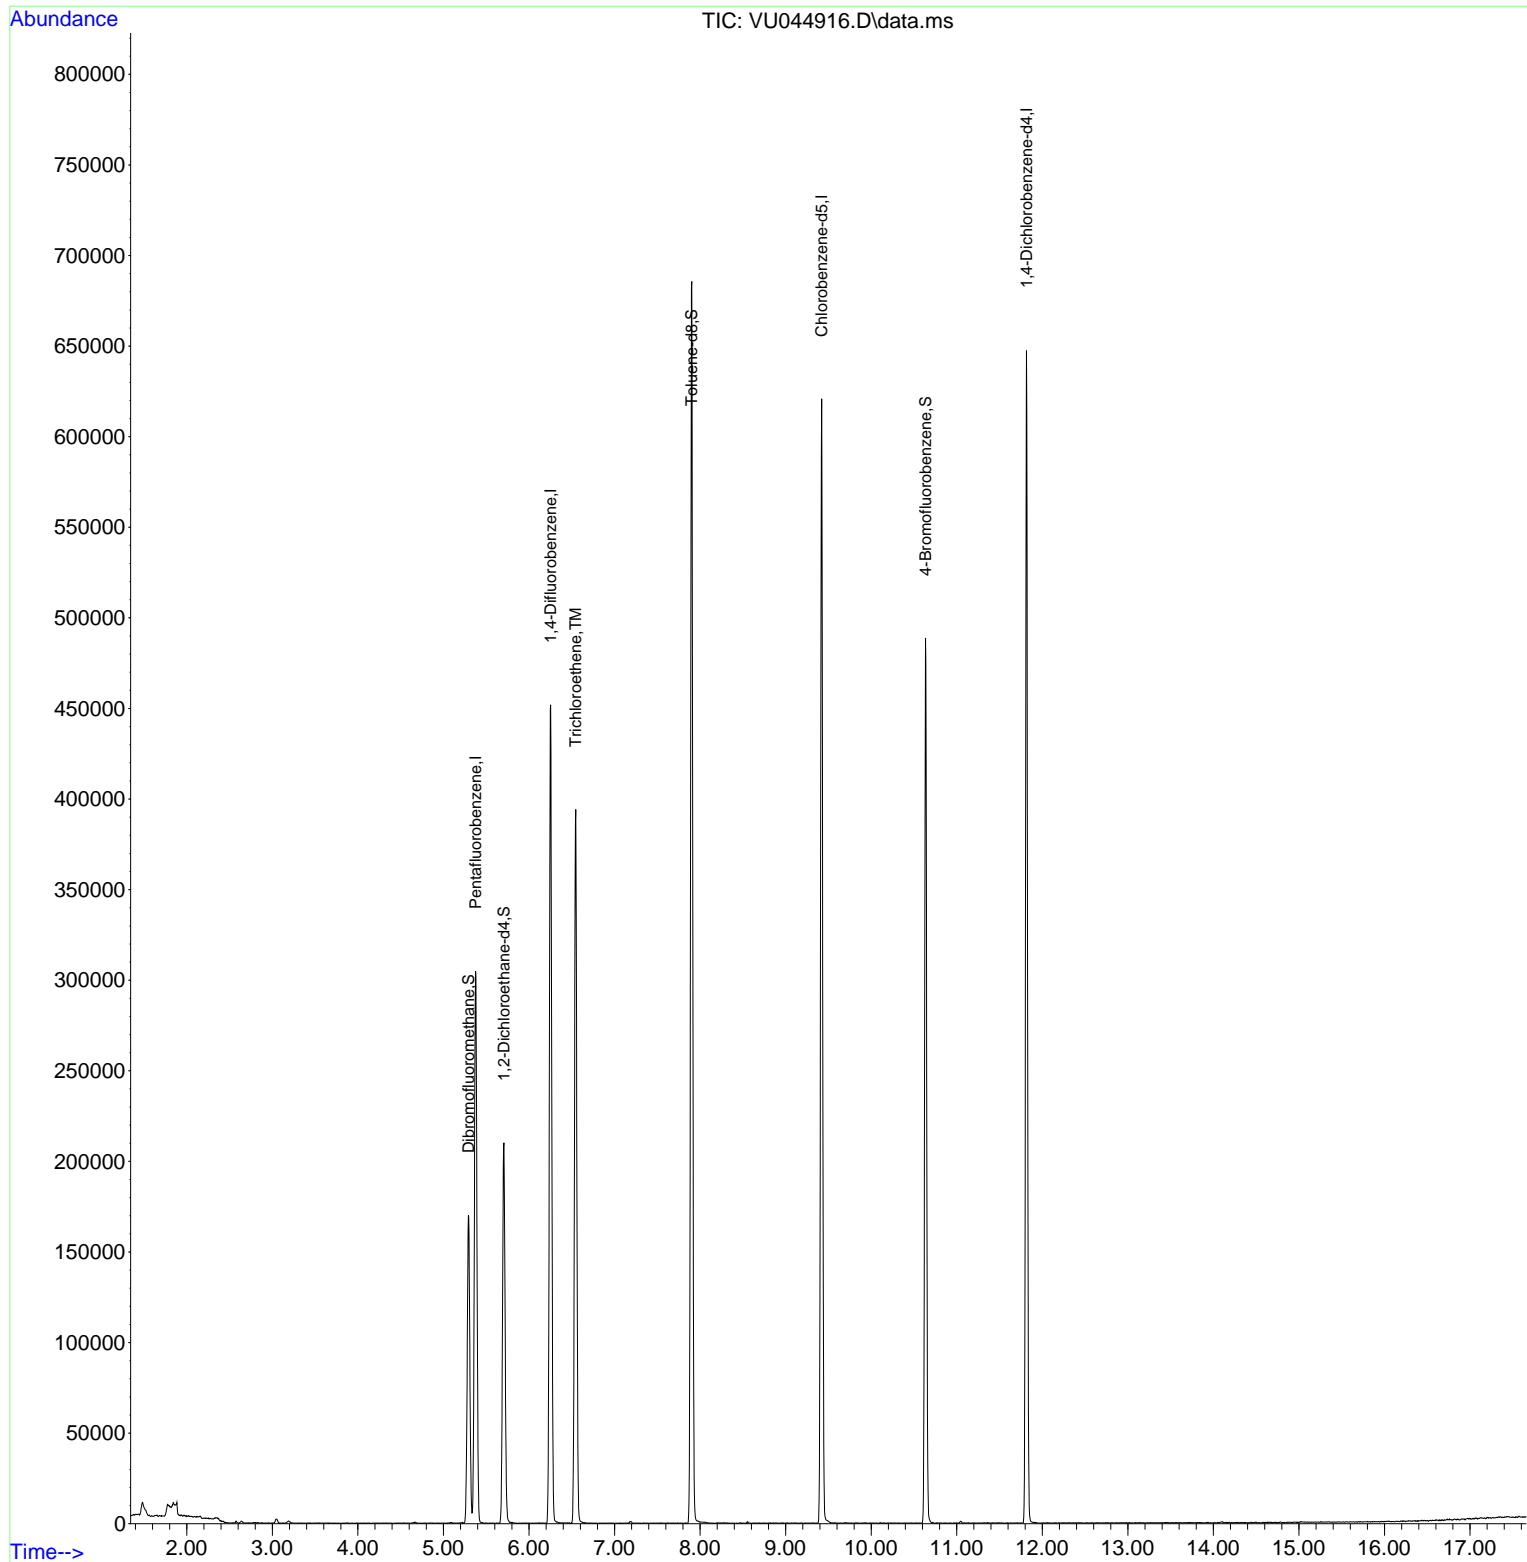



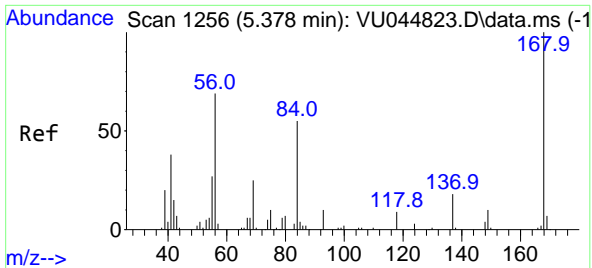


#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.375 min Scan# 1255
 Delta R.T. -0.003 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04


Instrument : MSVOA_U
 ClientSampled : RE108D2-20210917DL

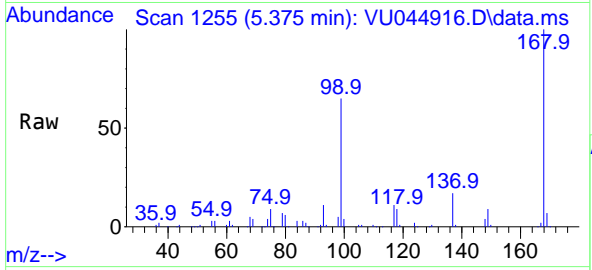



Tgt Ion:168 Resp: 198574
 Ion Ratio Lower Upper
 168 100
 99 64.6 51.4 77.0

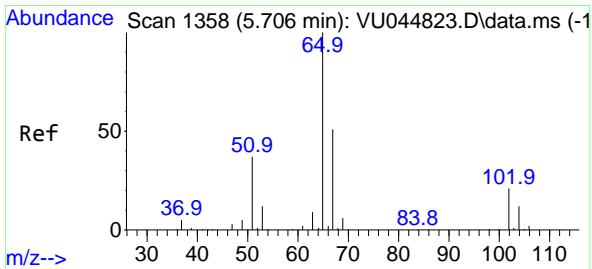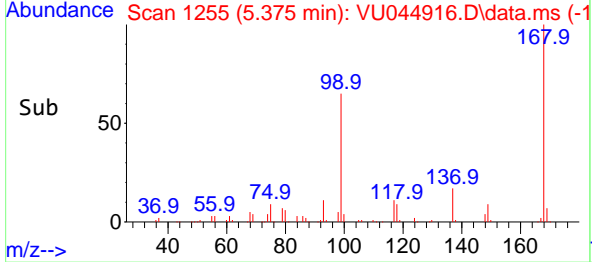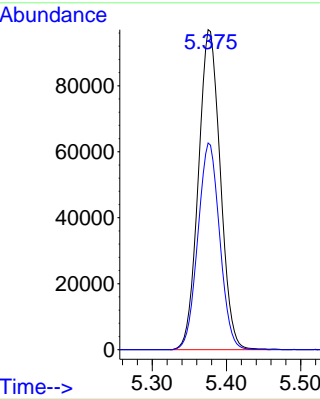


#33
 1,2-Dichloroethane-d4
 Concen: 45.863 ug/l
 RT: 5.706 min Scan# 1358
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

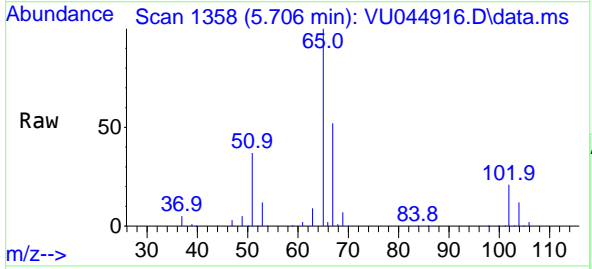


Tgt Ion: 65 Resp: 158945
 Ion Ratio Lower Upper
 65 100
 67 51.4 0.0 104.8

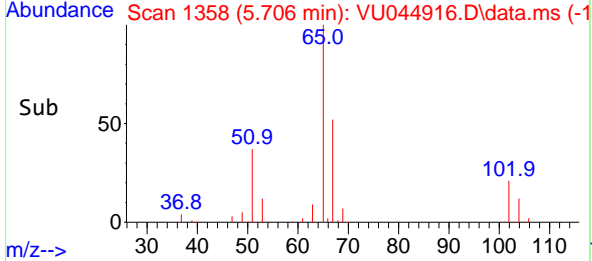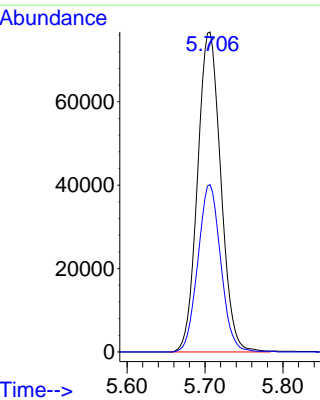

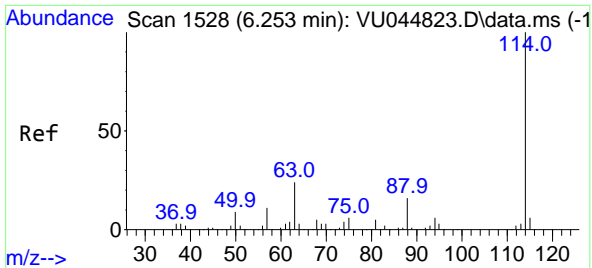




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.253 min Scan# 1528
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

Instrument :
 MSVOA_U
 ClientSampled :
 RE108D2-20210917DL

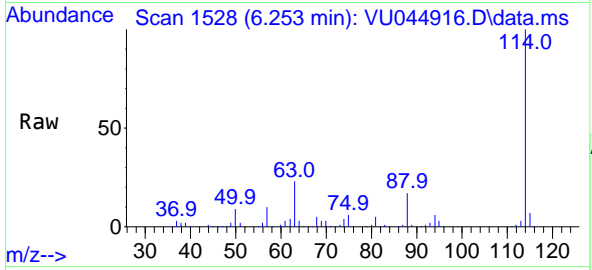


Tgt Ion:114 Resp: 353765

Ion	Ratio	Lower	Upper
114	100		
63	22.6	0.0	47.8
88	16.9	0.0	32.8

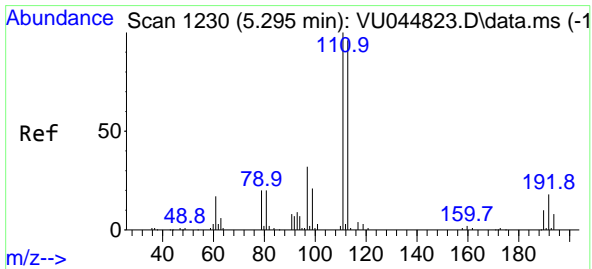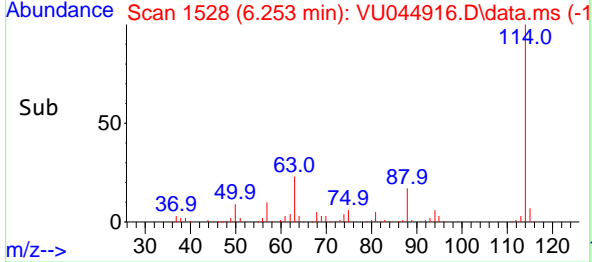
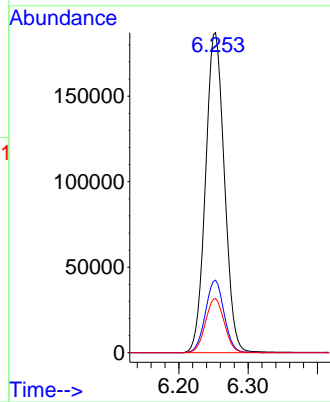



#35
 Dibromofluoromethane
 Concen: 44.664 ug/l
 RT: 5.292 min Scan# 1229
 Delta R.T. -0.003 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

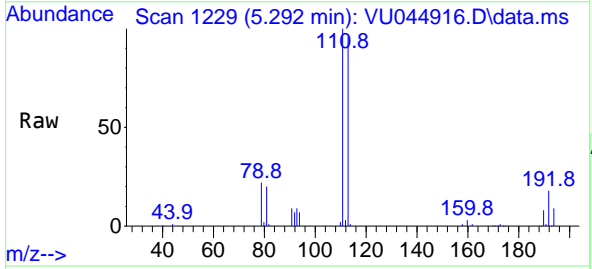

Tgt Ion:113 Resp: 108394


Ion	Ratio	Lower	Upper
113	100		
111	103.0	84.1	126.1
192	18.1	14.8	22.2

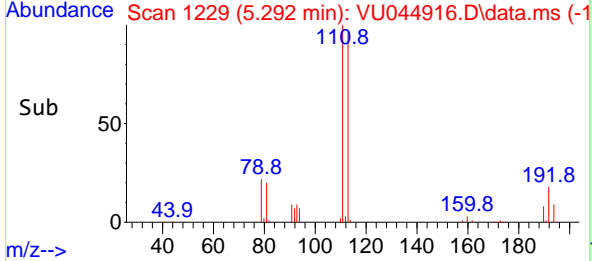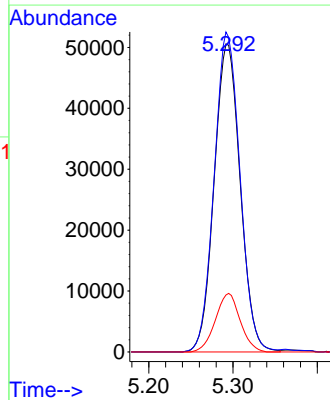



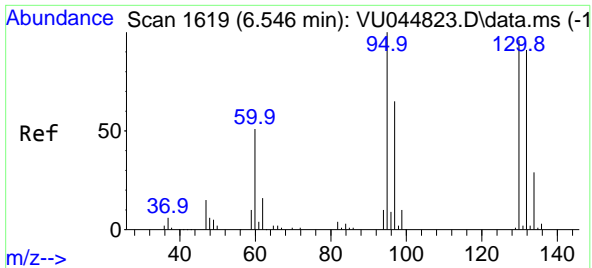


#44
 Trichloroethene
 Concen: 45.831 ug/l
 RT: 6.546 min Scan# 1619
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04


Instrument :
 MSVOA_U
ClientSampled :
 RE108D2-20210917DL

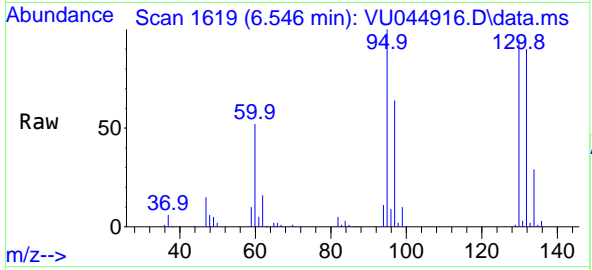



Tgt Ion:130 Resp: 126053
 Ion Ratio Lower Upper
 130 100
 95 104.9 0.0 209.0

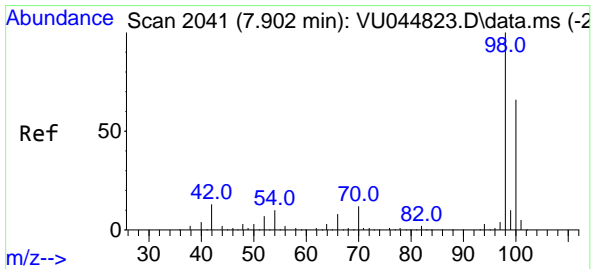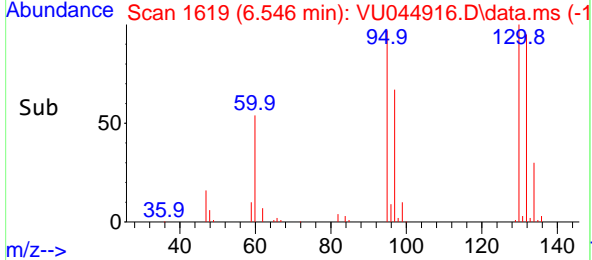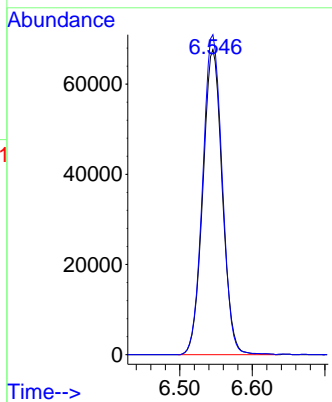


#50
 Toluene-d8
 Concen: 47.977 ug/l
 RT: 7.902 min Scan# 2041
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

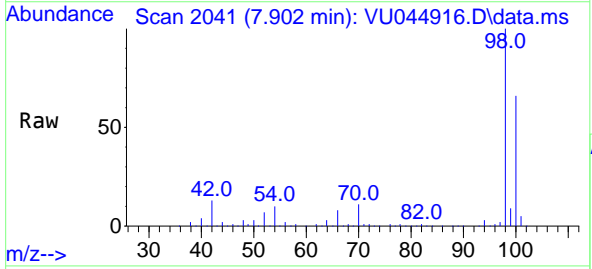


Tgt Ion: 98 Resp: 439748
 Ion Ratio Lower Upper
 98 100
 100 65.2 52.5 78.7

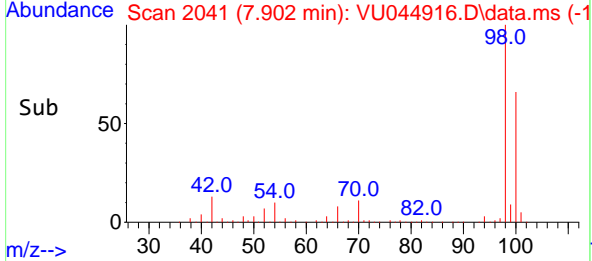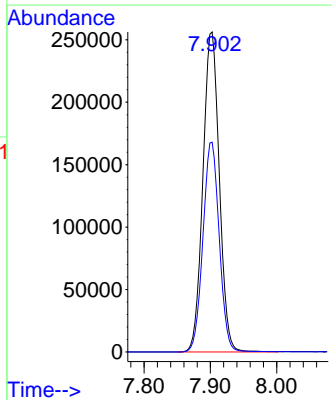



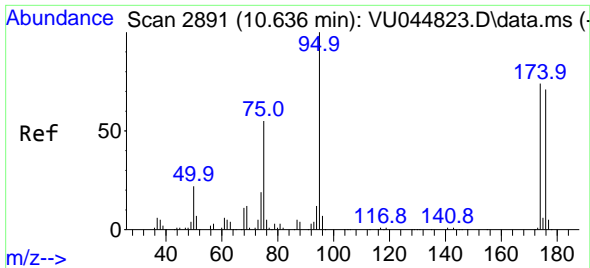


#62
 4-Bromofluorobenzene
 Concen: 47.085 ug/l
 RT: 10.635 min Scan# 2891
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04


Instrument :
 MSVOA_U
ClientSampled :
 RE108D2-20210917DL

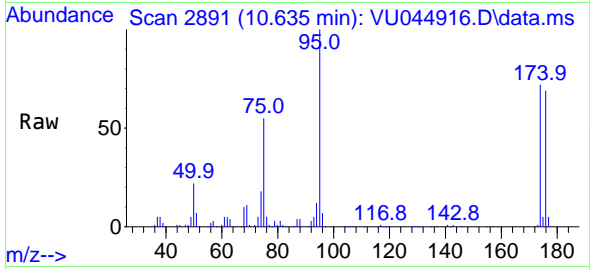



Tgt Ion: 95 Resp: 160295
 Ion Ratio Lower Upper
 95 100
 174 72.7 0.0 146.6
 176 69.2 0.0 141.2

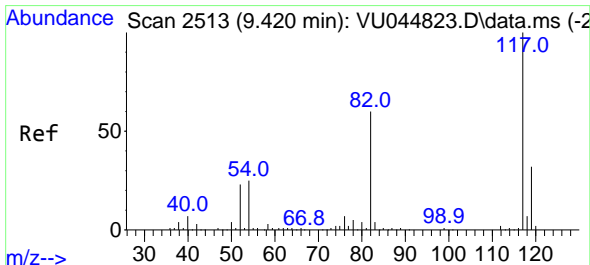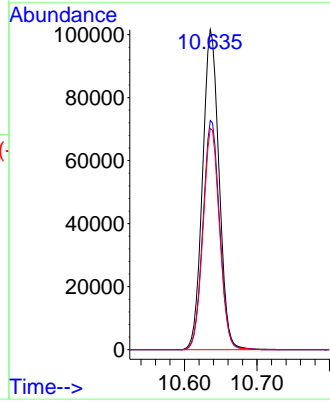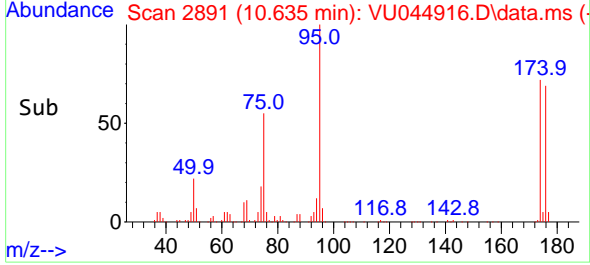


#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 9.420 min Scan# 2513
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

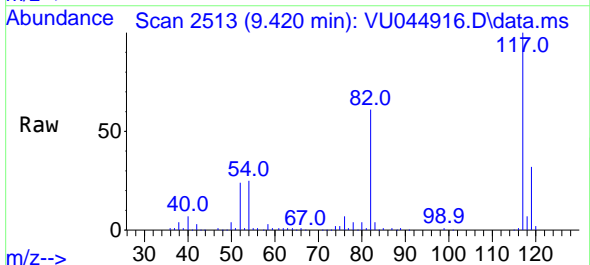


Tgt Ion: 117 Resp: 319235
 Ion Ratio Lower Upper
 117 100
 82 60.8 47.8 71.8
 119 31.6 25.8 38.6

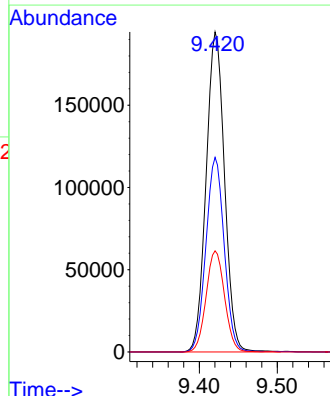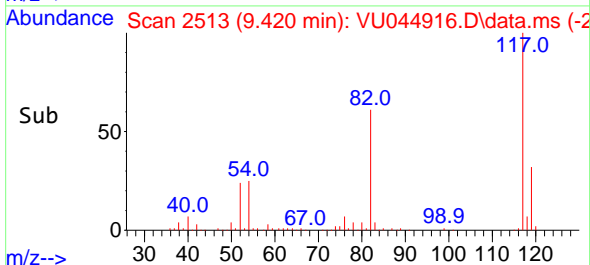

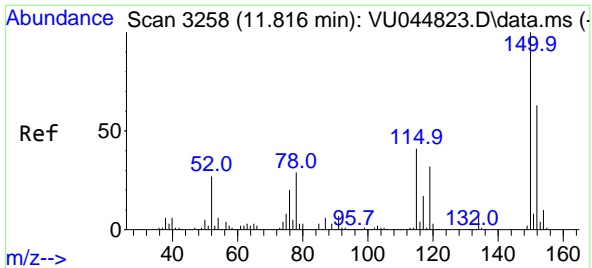

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.815 min Scan# 3258
 Delta R.T. -0.000 min
 Lab File: VU044916.D
 Acq: 28 Sep 2021 03:04

Instrument :
 MSVOA_U
ClientSampled :
 RE108D2-20210917DL

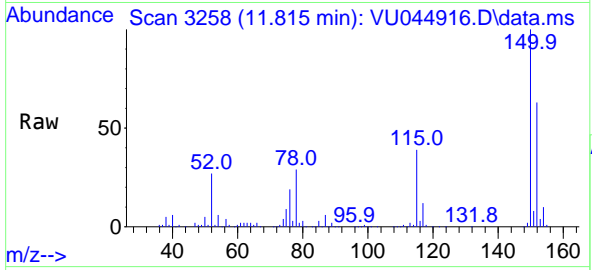

Tgt Ion:152 Resp: 153811
 Ion Ratio Lower Upper
 152 100
 115 61.6 43.5 130.7
 150 157.4 0.0 350.0

