

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
 Data File : VU044897.D
 Acq On : 27 Sep 2021 18:29
 Operator : SY/MD
 Sample : M3888-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 20898

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Title : SW846 8260

Signal : TIC: VU044897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.462	30	38	68	rBV	39511	79471	6.50%	0.583%
2	1.588	72	77	98	rVV3	10350	19042	1.56%	0.140%
3	1.684	101	107	116	rVB	21007	24508	2.00%	0.180%
4	2.353	307	315	325	rVB	12114	23543	1.92%	0.173%
5	2.633	390	402	434	rBV	279156	533999	43.64%	3.918%
6	2.832	438	464	487	rVV	55911	162084	13.25%	1.189%
7	2.951	489	501	522	rVB	100790	184691	15.09%	1.355%
8	3.253	562	595	618	rBV2	53639	169842	13.88%	1.246%
9	4.446	951	966	984	rBV2	35482	87646	7.16%	0.643%
10	4.713	1035	1049	1081	rBV2	60201	167759	13.71%	1.231%
11	5.038	1132	1150	1178	rBV4	12409	34197	2.79%	0.251%
12	5.292	1213	1229	1242	rBV	173755	367494	30.04%	2.697%
13	5.375	1242	1255	1276	rVB	308301	633971	51.81%	4.652%
14	5.703	1341	1357	1369	rBV	217025	436100	35.64%	3.200%
15	5.774	1369	1379	1398	rVB	104187	213991	17.49%	1.570%
16	6.250	1514	1527	1566	rVB	466712	897595	73.36%	6.586%
17	6.552	1607	1621	1642	rBV	18157	56238	4.60%	0.413%
18	6.783	1679	1693	1708	rBV2	80836	180757	14.77%	1.326%
19	7.475	1896	1908	1922	rVB	24004	42237	3.45%	0.310%
20	7.726	1978	1986	1998	rVB3	8800	15838	1.29%	0.116%
21	7.806	2000	2011	2022	rBV3	6934	12522	1.02%	0.092%
22	7.899	2026	2040	2053	rBV	716652	1223542	100.00%	8.978%
23	7.973	2053	2063	2075	rVB	147757	250195	20.45%	1.836%
24	8.558	2235	2245	2261	rVB2	11039	20674	1.69%	0.152%
25	8.697	2275	2288	2290	rBV4	9183	13058	1.07%	0.096%
26	8.732	2290	2299	2310	rVV	48566	87200	7.13%	0.640%
27	8.799	2310	2320	2343	rVB3	34665	69283	5.66%	0.508%
28	8.922	2345	2358	2371	rBV3	9857	18746	1.53%	0.138%
29	9.420	2499	2513	2525	rBV	665845	1111318	90.83%	8.155%
30	9.574	2552	2561	2577	rVB	18781	35886	2.93%	0.263%
31	9.664	2577	2589	2591	rVV2	44018	59373	4.85%	0.436%
32	9.697	2592	2599	2611	rVB	111334	187275	15.31%	1.374%
33	9.832	2632	2641	2648	rBV2	17311	29845	2.44%	0.219%
34	9.925	2660	2670	2685	rVB	49552	79808	6.52%	0.586%
35	10.118	2715	2730	2746	rBV5	103997	308902	25.25%	2.267%
36	10.221	2747	2762	2764	rBV2	38356	57191	4.67%	0.420%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
 Data File : VU044897.D
 Acq On : 27 Sep 2021 18:29
 Operator : SY/MD
 Sample : M3888-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 20898

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
 Title : SW846 8260

37	10.369	2797	2808	2816	rBV6	13615	25125	2.05%	0.184%
38	10.639	2879	2892	2903	rBV	579929	922373	75.39%	6.768%
39	10.690	2903	2908	2919	rVV2	19855	33919	2.77%	0.249%
40	10.748	2920	2926	2938	rVB4	10230	17143	1.40%	0.126%
41	10.918	2967	2979	2989	rBV2	20050	33535	2.74%	0.246%
42	11.240	3066	3079	3085	rBV3	19974	36063	2.95%	0.265%
43	11.291	3086	3095	3109	rVB6	19148	47893	3.91%	0.351%
44	11.378	3115	3122	3140	rVB5	13426	29549	2.42%	0.217%
45	11.471	3141	3151	3163	rVB	61216	94188	7.70%	0.691%
46	11.542	3163	3173	3180	rBV	27210	44823	3.66%	0.329%
47	11.613	3190	3195	3222	rVB4	24301	52546	4.29%	0.386%
48	11.732	3223	3232	3246	rBV7	12887	29334	2.40%	0.215%
49	11.815	3246	3258	3275	rVB	739154	1178246	96.30%	8.646%
50	11.899	3275	3284	3293	rBV	25759	38840	3.17%	0.285%
51	11.954	3293	3301	3318	rVB6	9588	18969	1.55%	0.139%
52	12.063	3321	3335	3363	rBV	377984	725971	59.33%	5.327%
53	12.317	3402	3414	3429	rVB	281224	433959	35.47%	3.184%
54	12.510	3466	3474	3485	rVB7	14583	23006	1.88%	0.169%
55	12.819	3549	3570	3583	rBV	52143	105403	8.61%	0.773%
56	13.452	3753	3767	3780	rVB4	9305	17599	1.44%	0.129%
57	13.523	3780	3789	3802	rBV3	25968	41398	3.38%	0.304%
58	13.629	3812	3822	3835	rVB2	27063	45445	3.71%	0.333%
59	13.860	3881	3894	3910	rBV2	7386	15451	1.26%	0.113%
60	14.008	3928	3940	3953	rBV4	17403	29333	2.40%	0.215%
61	14.089	3953	3965	3980	rBV	670223	1066143	87.14%	7.823%
62	14.214	3994	4004	4019	rVB5	50430	97644	7.98%	0.716%
63	15.224	4307	4318	4335	rVB	117804	194565	15.90%	1.428%
64	15.413	4365	4377	4392	rBV	101719	168739	13.79%	1.238%
65	15.957	4537	4546	4553	rBV2	10178	15247	1.25%	0.112%
66	16.265	4633	4642	4663	rVB6	8198	16057	1.31%	0.118%
67	16.413	4679	4688	4694	rBV2	17703	27328	2.23%	0.201%
68	16.452	4695	4700	4710	rVB5	10759	15716	1.28%	0.115%
69	16.767	4787	4798	4817	rBV	48943	90654	7.41%	0.665%


Sum of corrected areas: 13628025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044897.D
Acq On : 27 Sep 2021 18:29
Operator : SY/MD
Sample : M3888-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
20898

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

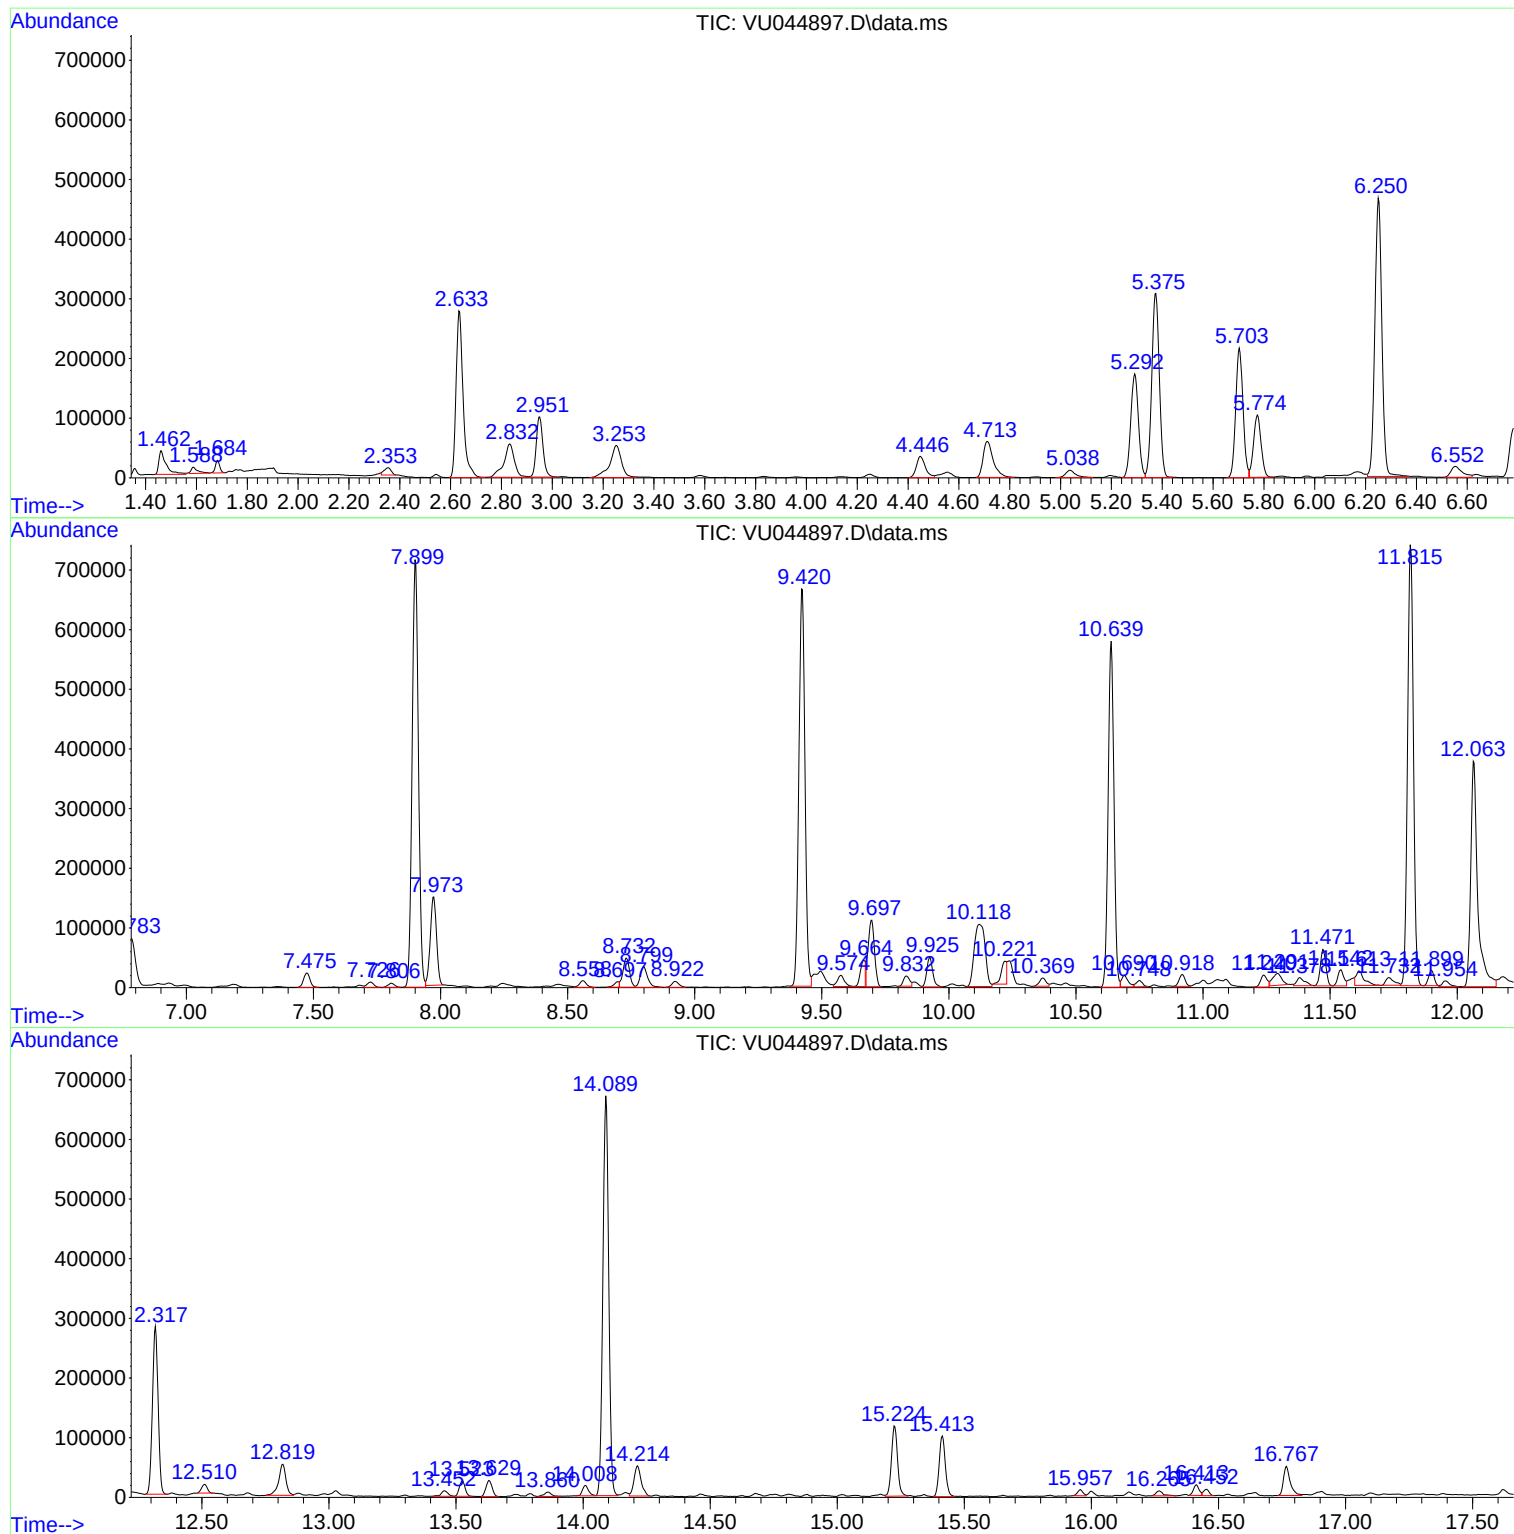

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044897.D
Acq On : 27 Sep 2021 18:29
Operator : SY/MD
Sample : M3888-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
20898

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044897.D
Acq On : 27 Sep 2021 18:29
Operator : SY/MD
Sample : M3888-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
20898

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
