


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092721\
Data File : VU044904.D
Acq On : 27 Sep 2021 21:37
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092421W.M
Title : SW846 8260
Last Update : Tue Sep 28 11:39:06 2021

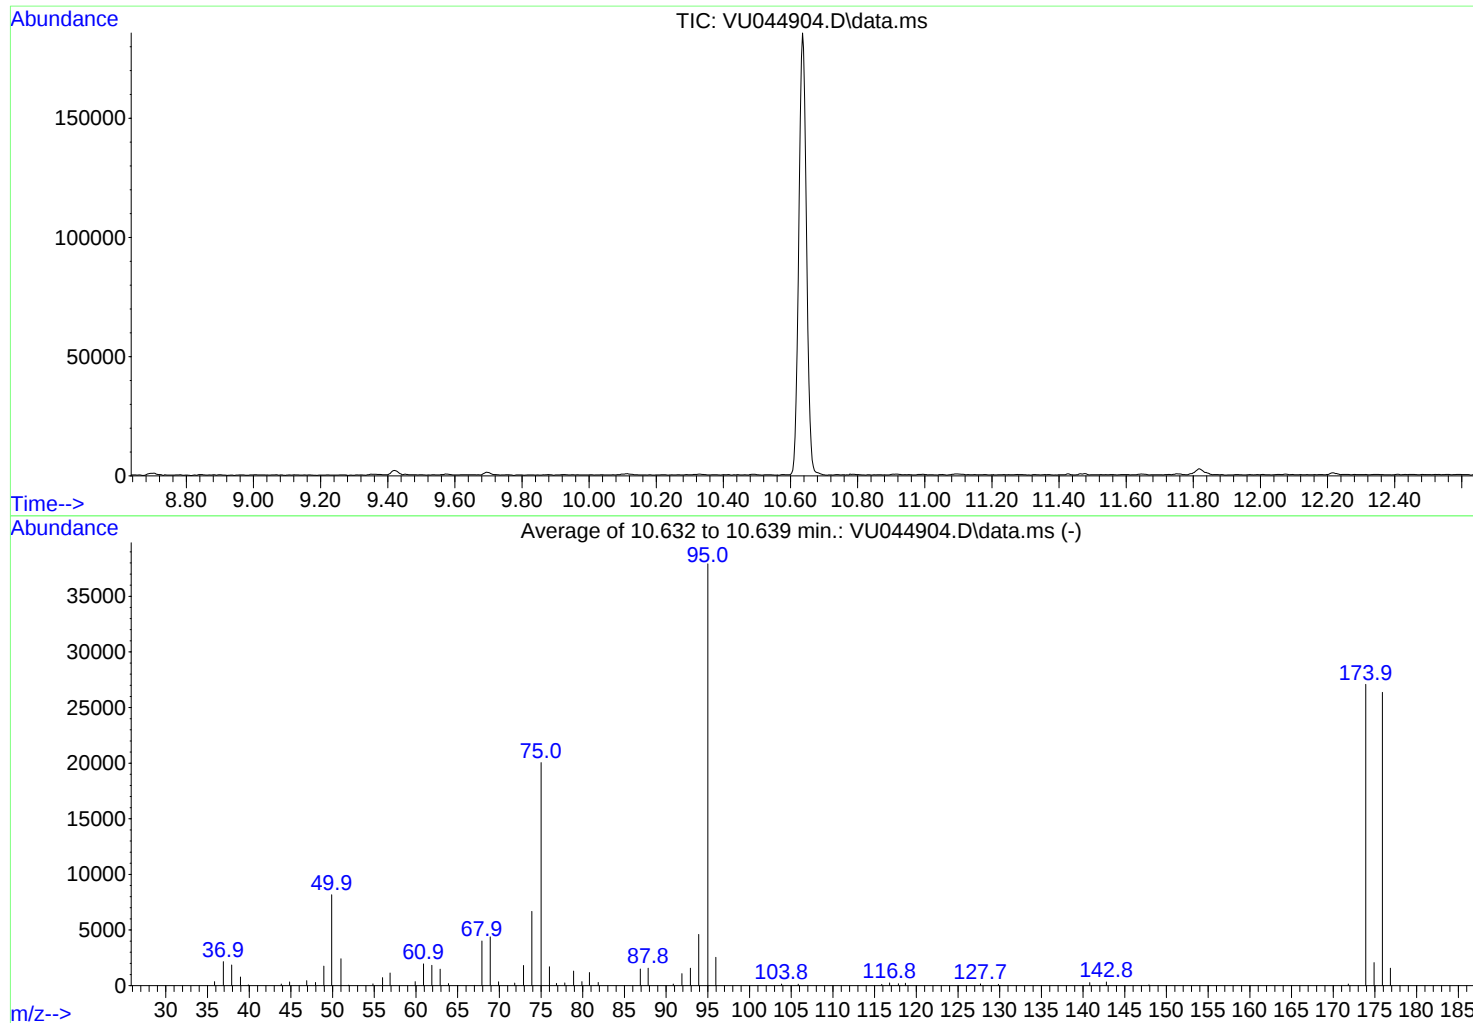

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	8170	PASS
75	95	30	60	52.9	20059	PASS
95	95	100	100	100.0	37920	PASS
96	95	5	9	6.7	2548	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.4	27083	PASS
175	174	5	9	7.6	2066	PASS
176	174	95	101	97.4	26368	PASS
177	176	5	9	6.0	1570	PASS