

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092723\
 Data File : VU055562.D
 Acq On : 27 Sep 2023 19:37
 Operator : MD/SY
 Sample : 04530-05DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHY3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.602	87	97	111	rVB2	422003	510521	52.85%	6.156%
2	1.911	185	193	209	rVB	116266	153025	15.84%	1.845%
3	2.563	384	396	412	rBV	201099	332019	34.37%	4.004%
4	3.042	534	545	558	rBV2	14241	26277	2.72%	0.317%
5	3.181	577	588	603	rBV2	9049	20573	2.13%	0.248%
6	3.351	628	641	652	rBV4	6025	11556	1.20%	0.139%
7	4.660	1024	1048	1077	rBV3	243697	834807	86.42%	10.067%
8	5.058	1157	1172	1195	rVB	184411	416973	43.16%	5.028%
9	5.724	1357	1379	1419	rBV2	353287	966028	100.00%	11.649%
10	6.248	1527	1542	1564	rBV	240905	475524	49.22%	5.734%
11	6.541	1621	1633	1647	rBV8	9030	20308	2.10%	0.245%
12	6.689	1664	1679	1697	rBV	218792	439594	45.51%	5.301%
13	7.563	1938	1951	1975	rBV2	101173	193176	20.00%	2.329%
14	7.894	2040	2054	2074	rBV	430559	771455	79.86%	9.303%
15	8.177	2130	2142	2163	rBV	60706	111163	11.51%	1.340%
16	8.634	2272	2284	2320	rBV4	316834	777577	80.49%	9.377%
17	9.415	2514	2527	2547	rBV	378512	641686	66.43%	7.738%
18	10.753	2928	2943	2962	rBV	166392	274201	28.38%	3.307%
19	11.810	3260	3272	3296	rBV	388316	647753	67.05%	7.811%
20	12.190	3376	3390	3408	rBV	400558	668493	69.20%	8.061%




Sum of corrected areas: 8292709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092723\
Data File : VU055562.D
Acq On : 27 Sep 2023 19:37
Operator : MD/SY
Sample : 04530-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

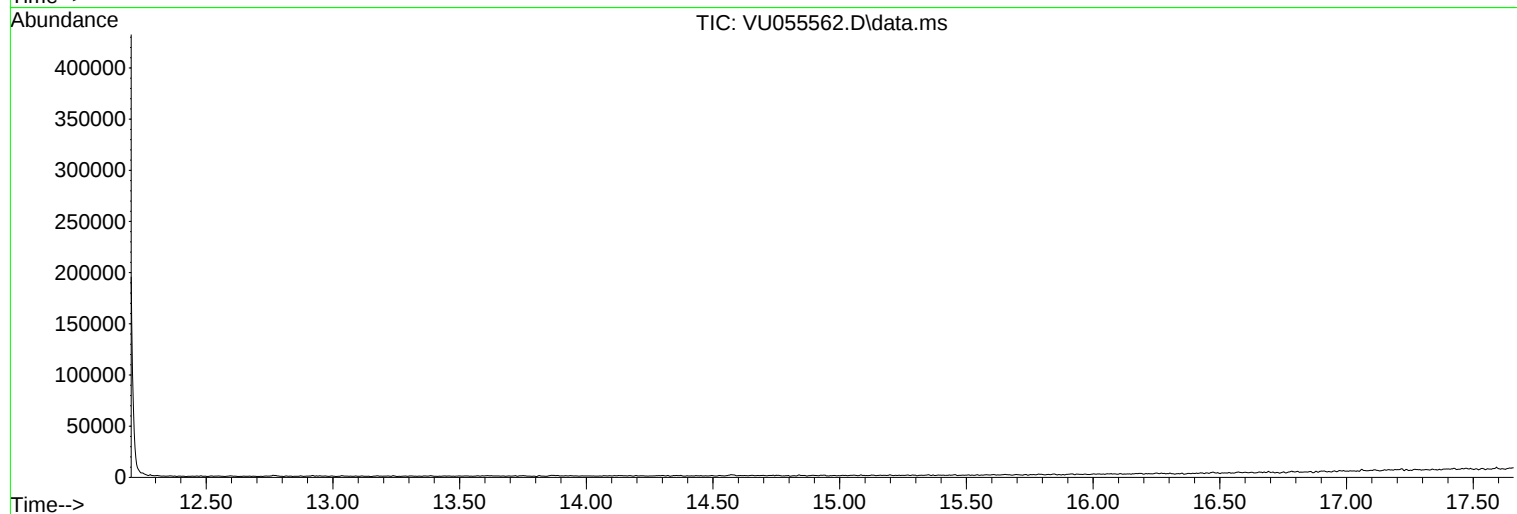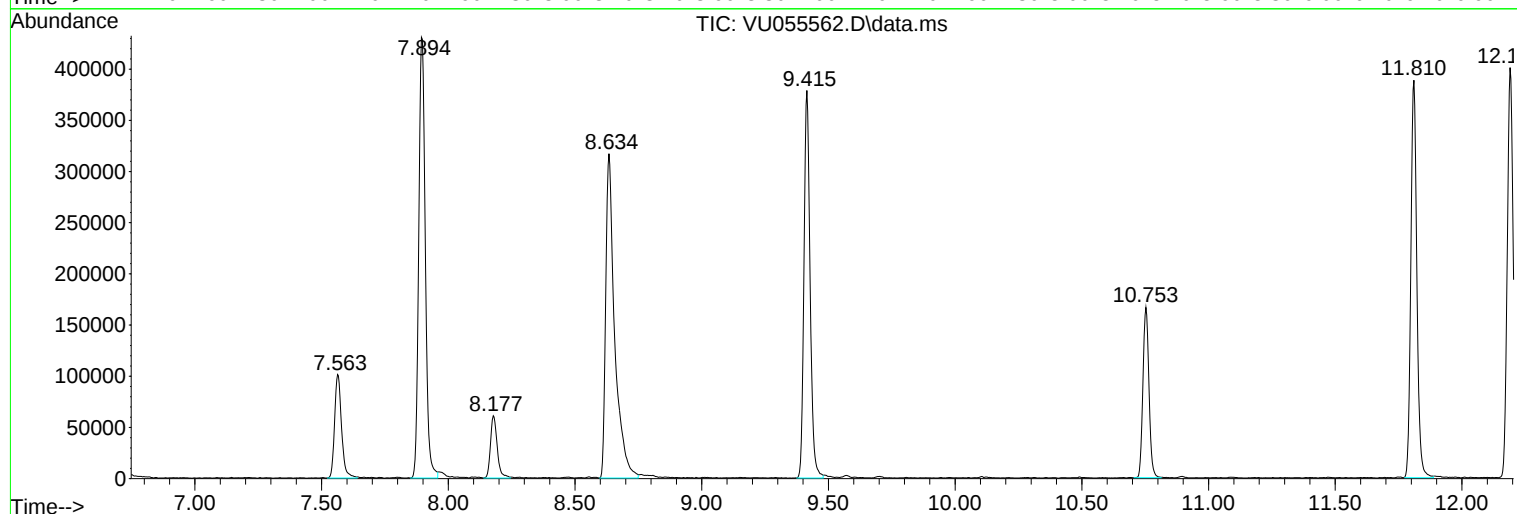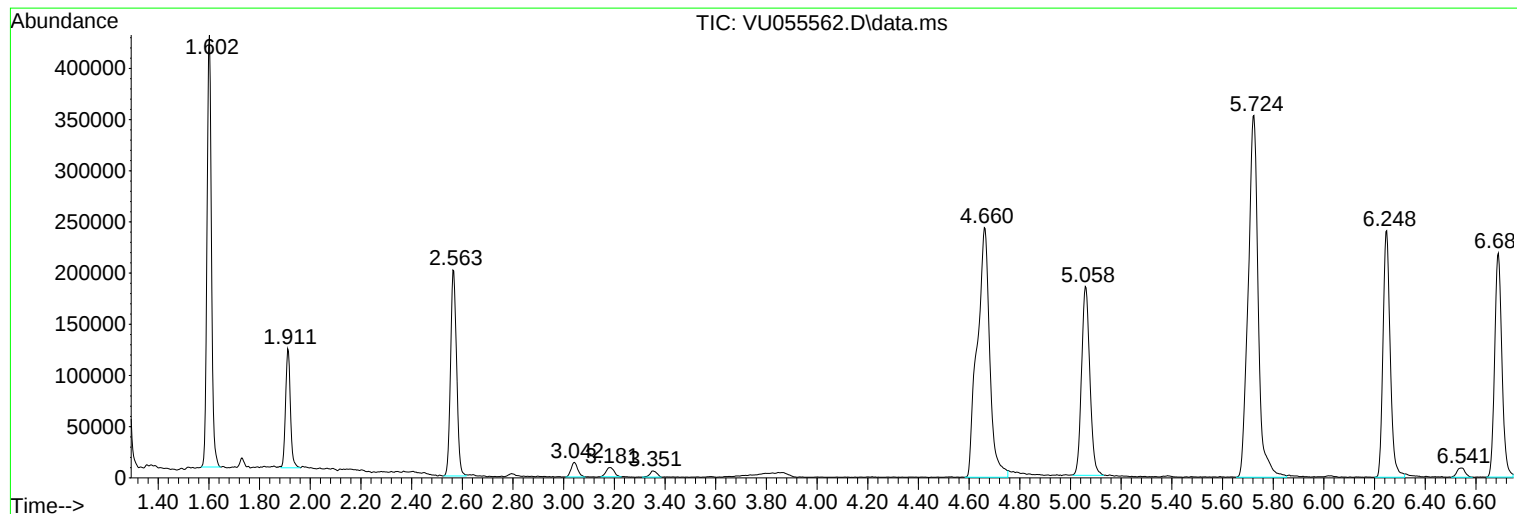

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092723\
Data File : VU055562.D
Acq On : 27 Sep 2023 19:37
Operator : MD/SY
Sample : 04530-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092723\
Data File : VU055562.D
Acq On : 27 Sep 2023 19:37
Operator : MD/SY
Sample : 04530-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc