


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092723\
Data File : VU055545.D
Acq On : 27 Sep 2023 10:56
Operator : MD/SY
Sample : BFB053
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB053

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 27 23:33:30 2023

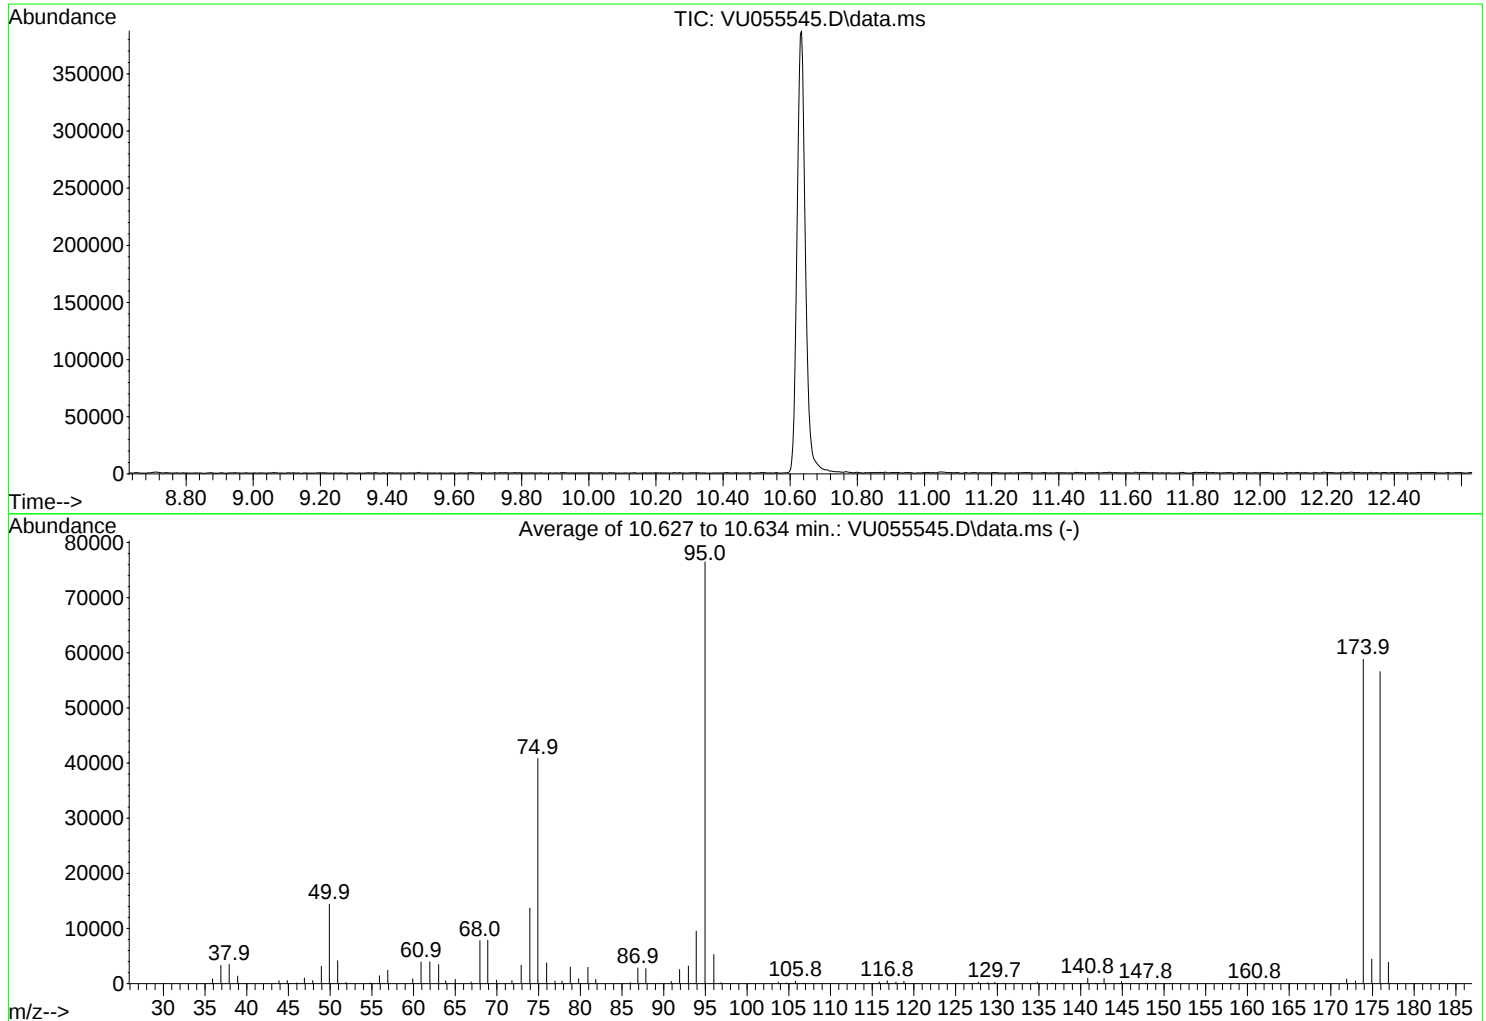

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	14406	PASS
75	95	30	80	53.4	40843	PASS
95	95	100	100	100.0	76493	PASS
96	95	5	9	6.9	5279	PASS
173	174	0.00	2	0.8	499	PASS
174	95	50	120	76.9	58829	PASS
175	174	5	9	7.5	4438	PASS
176	174	95	101	96.2	56587	PASS
177	176	5	9	6.8	3853	PASS

Scan 2891 (10.585 min): VU055545.D\data.ms
BFB053

m/z	Abundance
39.80	280.0
43.80	664.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	837.0
36.90	3342.0
37.90	3295.0
38.90	1348.0
39.80	201.0
43.90	1119.0
44.80	458.0
46.00	112.0
46.90	918.0
47.90	484.0
48.90	2888.0
49.90	14108.0
50.90	4216.0
51.90	232.0
54.80	167.0
55.90	1309.0
56.90	2157.0
59.90	736.0
60.90	3626.0
62.00	3627.0
63.00	3446.0
63.90	464.0
65.00	773.0
66.90	223.0
68.00	7728.0
68.90	7531.0
70.00	621.0
71.80	643.0
72.90	3107.0
74.00	12900.0
74.90	38800.0
76.00	3655.0
77.00	461.0
77.80	402.0
78.80	2754.0
79.80	801.0
80.90	2660.0
81.80	734.0
86.00	181.0
86.90	2472.0
87.80	2520.0
90.90	354.0
91.90	2347.0
92.90	3038.0
93.90	8979.0
94.90	72256.0
96.00	4871.0
96.80	157.0
103.70	259.0
104.70	138.0
105.80	522.0
115.90	300.0
116.80	529.0
117.90	213.0
118.80	395.0
127.70	293.0
128.80	204.0
129.70	295.0
134.80	210.0
140.90	928.0
142.80	929.0
144.90	384.0
147.70	110.0
160.80	133.0
171.90	661.0
172.90	476.0
173.90	53864.0
174.90	4272.0
175.90	52536.0
176.90	3713.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	904.0
36.90	3337.0
37.90	3562.0
38.90	1426.0
39.80	278.0
43.90	1208.0
44.90	553.0
46.00	151.0
46.90	1091.0
47.90	585.0
49.00	3194.0
49.90	14666.0
50.90	4253.0
51.90	246.0
54.80	132.0
55.90	1425.0
56.90	2534.0
59.90	918.0
60.90	4057.0
61.90	4053.0
63.00	3539.0
63.90	534.0
65.00	785.0
66.90	347.0
68.00	7998.0
68.90	8163.0
70.00	661.0
71.80	576.0
72.90	3316.0
74.00	13935.0
74.90	41992.0
75.90	3908.0
77.00	513.0
77.80	489.0
78.80	3035.0
79.80	893.0
80.90	3027.0
81.90	812.0
86.00	190.0
86.90	2840.0
87.80	2849.0
90.90	405.0
91.90	2599.0
92.90	3161.0
93.90	9851.0
95.00	78856.0
96.00	5397.0
96.90	177.0
103.70	284.0
104.70	163.0
105.80	486.0
106.70	111.0
115.80	326.0
116.80	529.0
117.90	273.0
118.80	436.0
127.80	240.0
128.80	192.0
129.70	265.0
130.70	121.0
134.80	297.0
136.60	147.0
140.80	1026.0
141.80	128.0
142.80	922.0
144.90	373.0
147.80	101.0
160.90	132.0
171.90	838.0
172.90	486.0
173.90	60432.0
174.90	4491.0
175.90	58424.0
176.90	4019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	845.0
36.90	3232.0
37.90	3587.0
38.90	1326.0
39.80	326.0
43.90	1212.0
44.90	646.0
46.00	145.0
46.90	1062.0
47.90	581.0
48.90	3313.0
49.90	14445.0
50.90	3999.0
51.90	248.0
54.80	154.0
55.90	1525.0
56.90	2551.0
59.90	983.0
60.90	4136.0
61.90	4176.0
63.00	3366.0
63.80	548.0
65.00	823.0
66.90	421.0
67.90	7740.0
68.90	7888.0
69.90	626.0
71.80	464.0
72.90	3571.0
73.90	14281.0
74.90	41736.0
75.90	3752.0
76.90	475.0
77.80	540.0
78.80	3211.0
79.80	1014.0
80.90	3238.0
81.90	801.0
86.00	142.0
86.90	3228.0
87.90	2839.0
90.90	430.0
91.90	2675.0
93.00	3371.0
93.90	9772.0
95.00	78368.0
96.00	5570.0
96.80	208.0
103.80	313.0
104.70	112.0
105.80	422.0
106.70	129.0
115.80	349.0
116.80	522.0
117.80	300.0
118.80	486.0
127.80	267.0
128.90	148.0
129.70	251.0
130.70	120.0
134.80	329.0
136.60	169.0
140.80	1005.0
141.80	162.0
142.80	964.0
144.90	341.0
147.90	132.0
149.90	109.0
156.70	105.0
158.80	126.0
160.90	121.0
171.90	1043.0
173.00	534.0
173.90	62192.0
174.90	4552.0
175.90	58800.0
176.90	3826.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053