
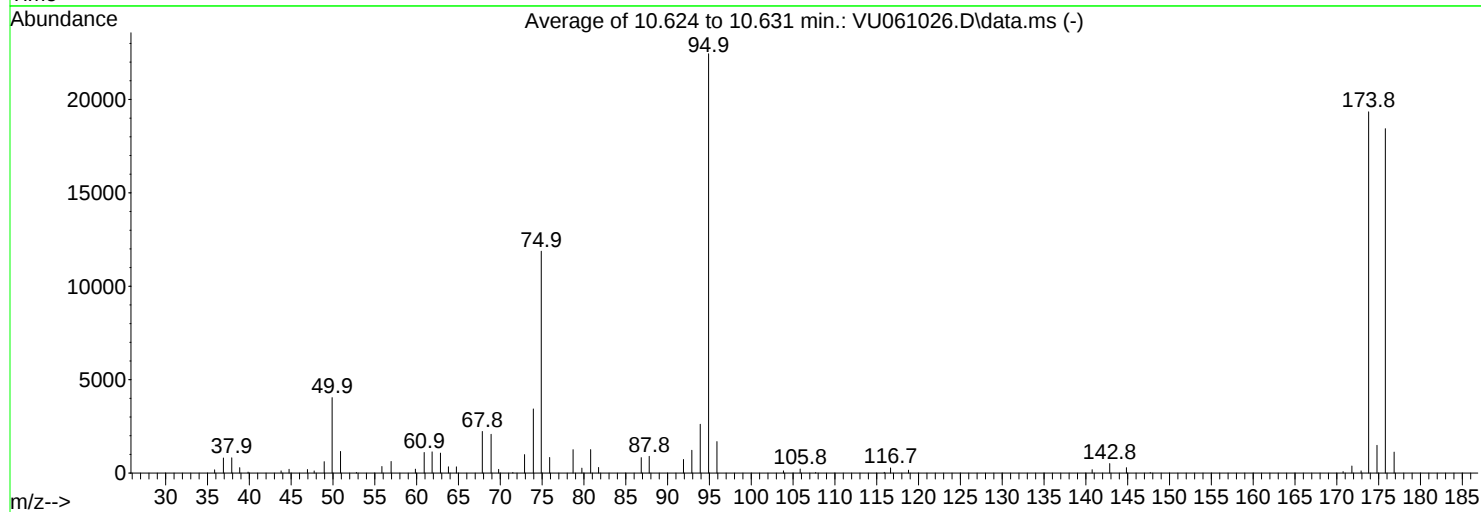


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092724\
Data File : VU061026.D
Acq On : 27 Sep 2024 08:51
Operator : MD/SY
Sample : BFB007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB007

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 28 04:04:44 2024

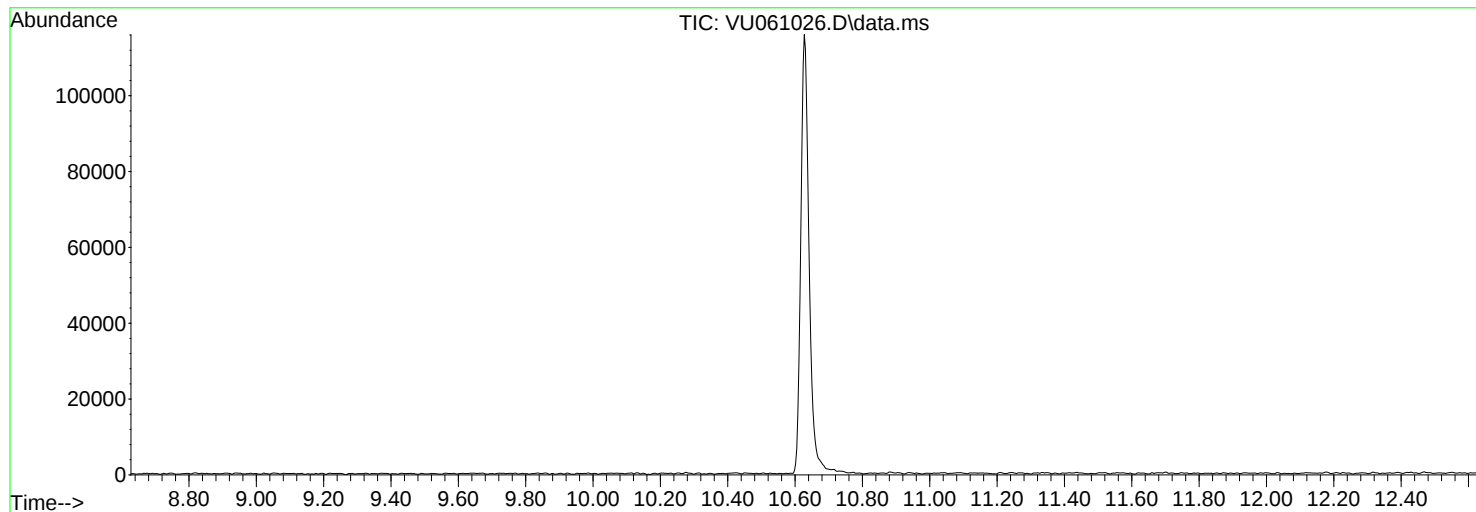

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	4040	PASS
75	95	30	80	52.9	11877	PASS
95	95	100	100	100.0	22448	PASS
96	95	5	9	7.5	1686	PASS
173	174	0.00	2	0.6	119	PASS
174	95	50	120	86.2	19339	PASS
175	174	5	9	7.7	1486	PASS
176	174	95	101	95.3	18437	PASS
177	176	5	9	6.1	1123	PASS

m/z	Abundance
39.80	135.0
43.90	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.80	187.0
36.90	735.0
37.90	792.0
38.90	339.0
39.90	182.0
43.80	343.0
44.80	204.0
46.90	199.0
48.90	538.0
49.90	3522.0
50.90	1239.0
52.80	106.0
55.90	401.0
57.00	626.0
59.90	247.0
60.90	1120.0
61.90	1098.0
62.90	1023.0
63.80	361.0
64.80	390.0
67.90	2136.0
68.90	2035.0
69.80	153.0
72.90	976.0
73.90	3306.0
74.90	11416.0
75.90	847.0
78.70	1146.0
79.70	271.0
80.80	1147.0
81.80	270.0
86.80	835.0
87.80	908.0
91.90	826.0
92.90	1162.0
93.90	2567.0
94.90	22016.0
95.90	1578.0
103.90	112.0
105.80	217.0
115.90	121.0
116.60	250.0
118.90	150.0
140.80	164.0
142.90	475.0
144.90	275.0
147.70	103.0
171.80	327.0
173.80	18720.0
174.80	1466.0
175.80	17616.0
176.80	1061.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	195.0
36.90	821.0
37.90	873.0
38.80	293.0
40.00	198.0
43.80	416.0
44.80	220.0
46.90	196.0
47.70	141.0
48.90	627.0
49.90	4241.0
50.90	1169.0
55.90	351.0
57.00	633.0
59.90	216.0
60.90	1141.0
61.90	1180.0
62.80	1115.0
63.80	353.0
64.80	340.0
67.80	2321.0
68.90	2127.0
69.80	214.0
72.90	1033.0
74.00	3510.0
74.90	12363.0
75.90	847.0
78.70	1327.0
79.80	251.0
80.80	1293.0
81.70	316.0
86.90	849.0
87.80	953.0
91.90	732.0
92.90	1298.0
93.90	2702.0
94.90	23136.0
95.90	1766.0
103.80	128.0
105.90	253.0
107.70	104.0
116.60	289.0
118.80	153.0
140.70	174.0
142.80	524.0
144.90	284.0
170.80	118.0
171.80	406.0
173.80	20064.0
174.80	1572.0
175.80	19088.0
176.80	1168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	142.0
36.90	862.0
37.90	786.0
38.80	242.0
40.00	189.0
43.80	506.0
44.70	189.0
47.00	172.0
47.80	203.0
49.00	670.0
49.90	4358.0
50.90	1068.0
55.70	301.0
56.90	606.0
59.80	168.0
60.90	1047.0
61.80	1130.0
62.80	1071.0
63.80	297.0
64.70	274.0
67.80	2231.0
68.90	2062.0
69.80	228.0
71.50	111.0
72.90	959.0
74.00	3481.0
74.90	11853.0
75.90	809.0
78.70	1292.0
79.80	269.0
80.80	1331.0
81.80	313.0
86.90	798.0
87.80	833.0
91.90	619.0
92.90	1204.0
93.90	2566.0
94.90	22192.0
95.90	1715.0
103.80	121.0
105.90	183.0
116.70	290.0
118.70	171.0
140.70	209.0
142.80	530.0
144.80	314.0
170.70	120.0
171.80	402.0
172.90	357.0
173.80	19232.0
174.80	1421.0
175.80	18608.0
176.90	1139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007