

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092818\
 Data File : VU027302.D
 Acq On : 29 Sep 2018 03:52
 Operator : MD/SY
 Sample : J4777-34
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A

Quant Time: Sep 29 07:04:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 22 01:31:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	108086	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	184496	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	177366	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	84643	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	107244	49.30	ug/l	0.00
Spiked Amount			Recovery	=	98.60%	
35) Dibromofluoromethane	4.88	113	74739	46.73	ug/l	0.00
Spiked Amount			Recovery	=	93.46%	
50) Toluene-d8	7.57	98	292477	47.99	ug/l	0.00
Spiked Amount			Recovery	=	95.98%	
62) 4-Bromofluorobenzene	10.31	95	98958	47.32	ug/l	0.00
Spiked Amount			Recovery	=	94.64%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	2.83	59	163	0.327	ug/l #	72
14) Allyl chloride	2.70	41	15124	4.995	ug/l #	23
16) Acetone	2.32	43	11434	Below Cal		93
18) Methyl Acetate	2.62	43	3149	1.017	ug/l	93
20) Methylene Chloride	2.70	84	298439	153.183	ug/l	98
25) 2-Butanone	4.29	43	1807	0.988	ug/l	99
29) Tetrahydrofuran	4.65	42	543	0.491	ug/l #	55
30) Chloroform	4.68	83	4049	1.223	ug/l	95
31) Cyclohexane	4.98	56	2836	0.303	ug/l #	1
36) 1,1-Dichloropropene	4.98	75	10044	4.079	ug/l #	50
37) Ethyl Acetate	4.29	43	1807	0.542	ug/l #	70
38) Carbon Tetrachloride	4.99	117	11287	4.817	ug/l #	17
43) Isopropyl Acetate	5.55	43	105124	21.625	ug/l	98
47) Bromodichloromethane	6.76	83	1083	0.416	ug/l #	81
48) Methyl methacrylate	6.54	41	3890	2.452	ug/l #	22
51) 4-Methyl-2-Pentanone	7.47	43	711	0.217	ug/l	95
56) Ethyl methacrylate	7.84	69	64	2.213	ug/l #	1
59) 2-Hexanone	8.31	43	1472	0.575	ug/l #	26
68) m/p-Xylenes	9.38	106	462	1.646	ug/l	85
76) 1,2,3-Trichloropropane	10.31	75	52379	20.370	ug/l #	36
80) 1,3,5-Trimethylbenzene	10.77	105	1328	0.250	ug/l	94
81) trans-1,4-Dichloro-2-buten	10.31	75	52379	65.186	ug/l #	100
84) 1,2,4-Trimethylbenzene	11.15	105	1516	0.280	ug/l	99
86) p-Isopropyltoluene	11.48	119	132	0.949	ug/l #	1
89) n-Butylbenzene	11.88	91	350	2.450	ug/l #	18
95) Naphthalene	13.75	128	9155	2.951	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092818\
Data File : VU027302.D
Acq On : 29 Sep 2018 03:52
Operator : MD/SY
Sample : J4777-34
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A

Quant Time: Sep 29 07:04:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 22 01:31:57 2018
Response via : Initial Calibration

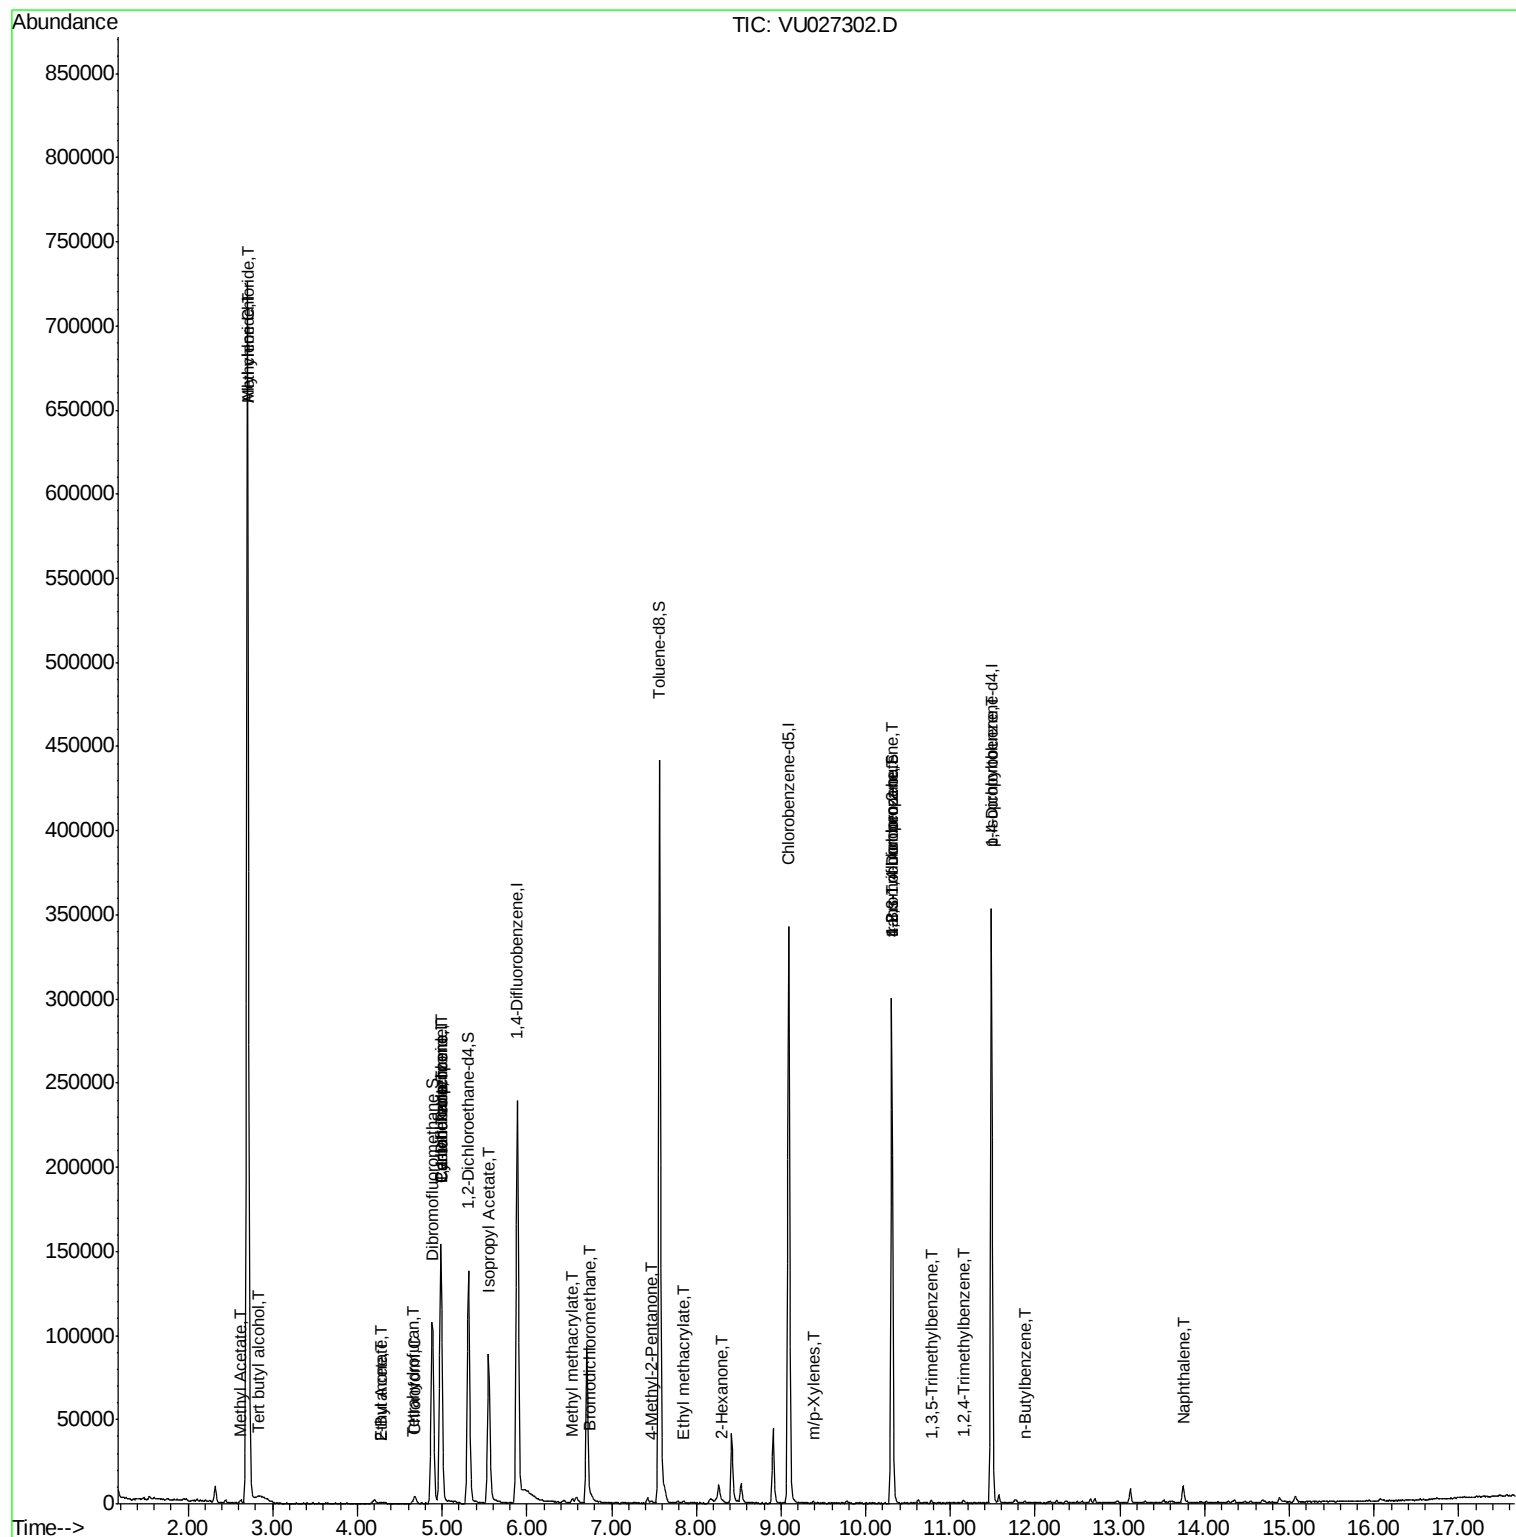



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. -0.00 min

Lab File: VU027302.D

Acq: 29 Sep 2018 03:52

Instrument :

MSVOA_U

ClientSampleId :


PL-01-092718-A

Tgt Ion:168 Resp: 108086

Ion Ratio Lower Upper

168 100

99 62.0 48.1 72.1

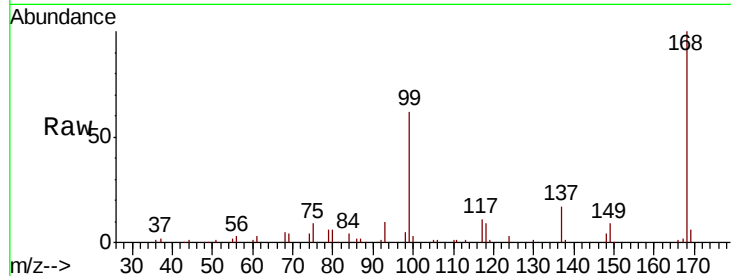

Abundance Ion 167.90 (167.60 to 168.60): VU026969.D (-1169) (-)

Ion 98.90 (98.60 to 99.60): VU026969.D (-1169) (-)

4.99

50000

40000

30000



20000

10000

0

4.90 4.95 5.00 5.05 5.10

Time-->

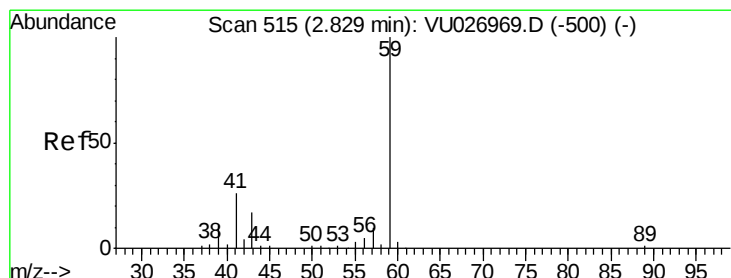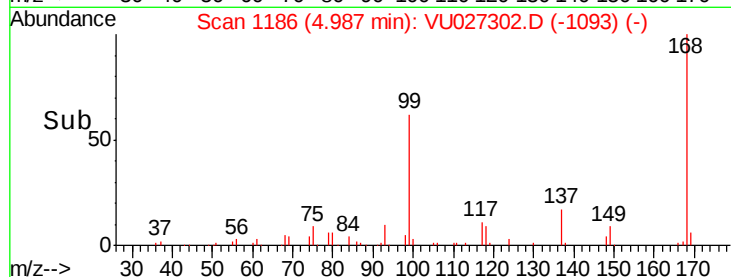

#11

Tert butyl alcohol

Concen: 0.327 ug/l

RT: 2.83 min Scan# 514

Delta R.T. -0.00 min

Lab File: VU027302.D


Acq: 29 Sep 2018 03:52

Tgt Ion: 59 Resp: 163

Ion Ratio Lower Upper

59 100

57 0.0 8.5 12.7#

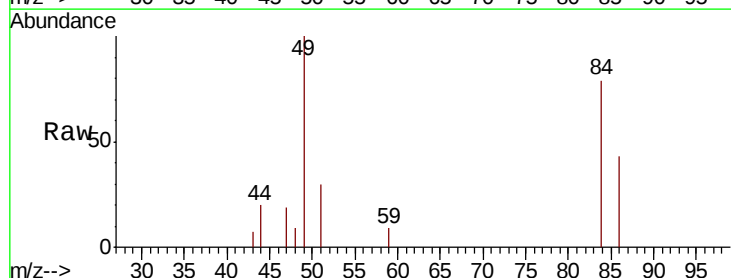

Abundance Ion 59.00 (58.70 to 59.70): VU026969.D (-500) (-)

Ion 57.00 (56.70 to 57.70): VU026969.D (-500) (-)

2.83

150


100


50

0

2.80 2.81 2.82 2.83 2.84

Time-->




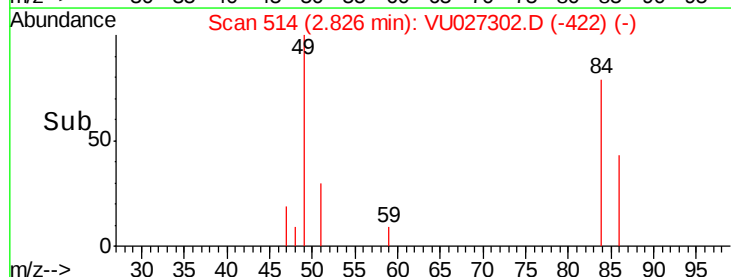




#14
 Allyl chloride
 Concen: 4.995 ug/l
 RT: 2.70 min Scan# 475
 Delta R.T. 0.11 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion: 41 Resp: 15124
 Ion Ratio Lower Upper
 41 100
 39 0.0 55.7 83.5#
 76 0.0 26.5 39.7#

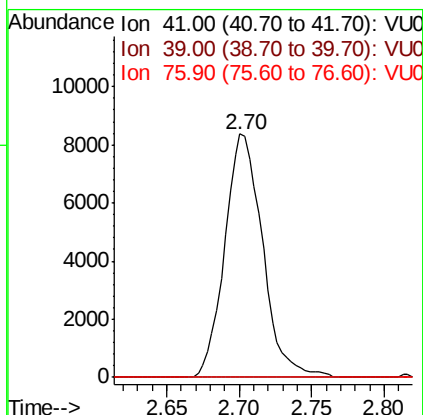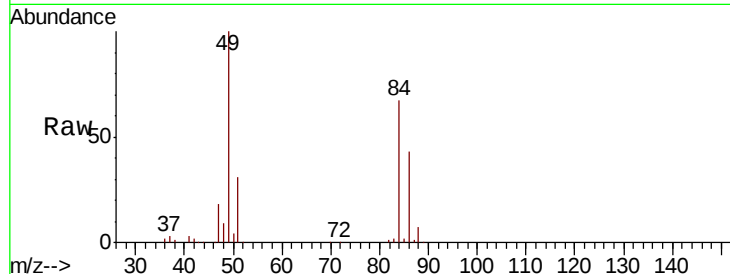

#16
 Acetone
 Concen: Below Cal
 RT: 2.32 min Scan# 357
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 43 Resp: 11434
 Ion Ratio Lower Upper
 43 100
 58 27.0 24.6 36.8









#18
Methyl Acetate
Concen: 1.017 ug/l
RT: 2.62 min Scan# 450
Delta R.T. 0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52




Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A


Tgt Ion: 43 Resp: 3149
Ion Ratio Lower Upper
43 100
74 17.4 16.6 25.0

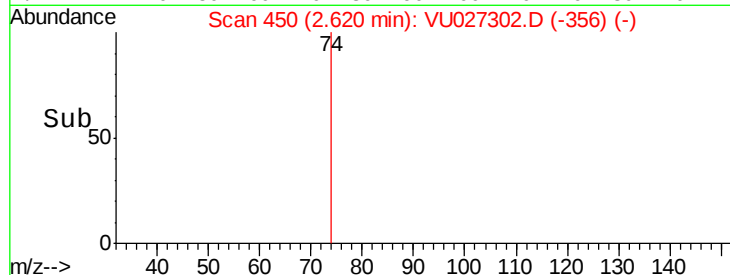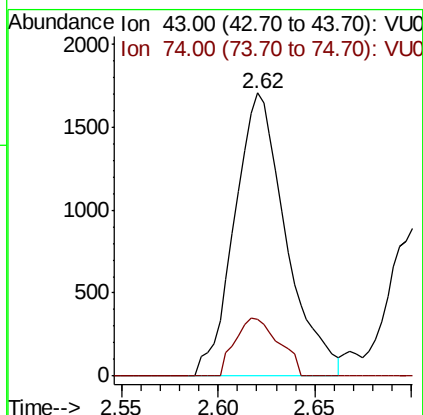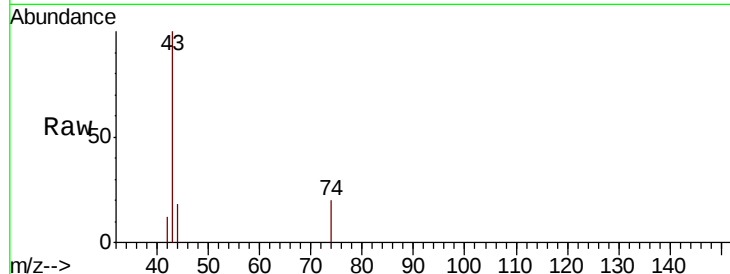

#20
Methylene Chloride
Concen: 153.183 ug/l
RT: 2.70 min Scan# 476
Delta R.T. -0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 84 Resp: 298439
Ion Ratio Lower Upper
84 100
49 148.1 114.9 172.3
51 45.4 35.8 53.8
86 64.2 51.3 76.9

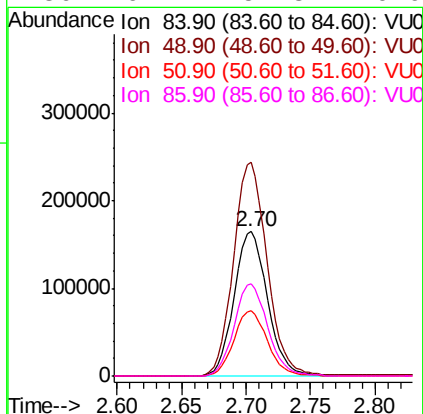

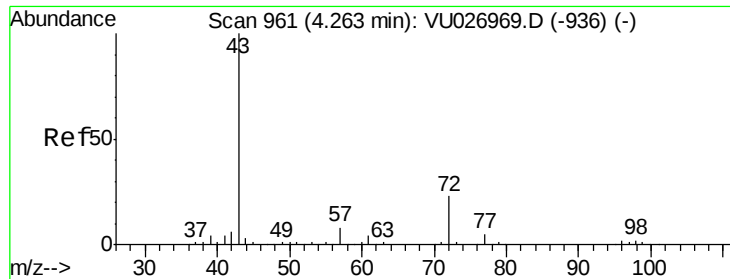

#25

2-Butanone

Concen: 0.988 ug/l

RT: 4.29 min Scan# 968

Delta R.T. 0.02 min

Lab File: VU027302.D

Acq: 29 Sep 2018 03:52

Instrument :

MSVOA_U

ClientSampleId :


PL-01-092718-A

Tgt Ion: 43 Resp: 1807




Ion Ratio Lower Upper

43 100

72 22.6 18.4 27.6



Abundance Ion 43.00 (42.70 to 43.70): VU026969.D (-936) (-)

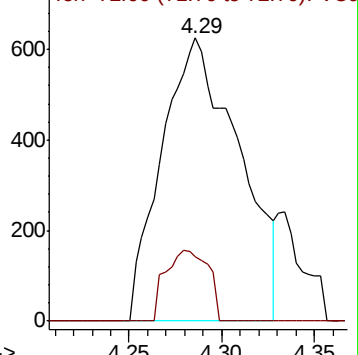

#29

Tetrahydrofuran

Concen: 0.491 ug/l

RT: 4.65 min Scan# 1082

Delta R.T. 0.01 min

Lab File: VU027302.D

Acq: 29 Sep 2018 03:52


Tgt Ion: 42 Resp: 543

Ion Ratio Lower Upper



42 100


72 0.0 31.7 47.5#

71 22.1 29.6 44.4#



Abundance Ion 42.00 (41.70 to 42.70): VU026969.D (-1062) (-)




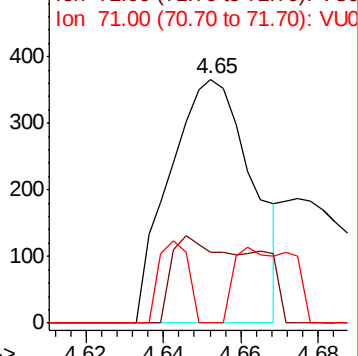




#30
Chloroform
Concen: 1.223 ug/l
RT: 4.68 min Scan# 1091
Delta R.T. 0.01 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52




Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A


Tgt Ion: 83 Resp: 4049
Ion Ratio Lower Upper
83 100
85 60.1 51.5 77.3



#31
Cyclohexane
Concen: 0.303 ug/l
RT: 4.98 min Scan# 1185
Delta R.T. -0.02 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 56 Resp: 2836
Ion Ratio Lower Upper
56 100
69 151.2 23.0 34.4#
84 141.0 61.4 92.2#







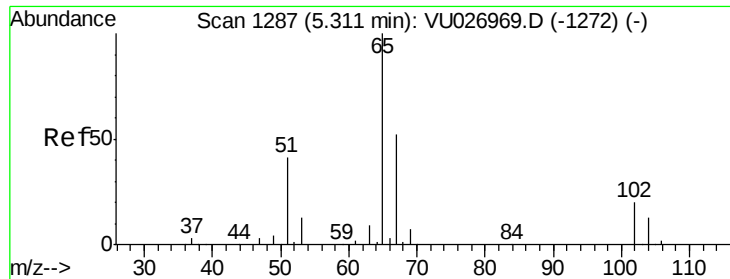

#33
 1,2-Dichloroethane-d4
 Concen: 49.298 ug/l
 RT: 5.31 min Scan# 1287
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion: 65 Resp: 107244
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 105.6

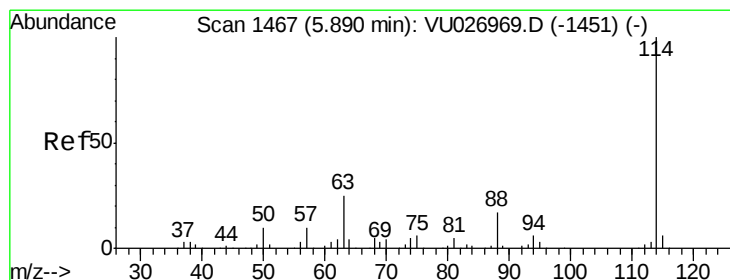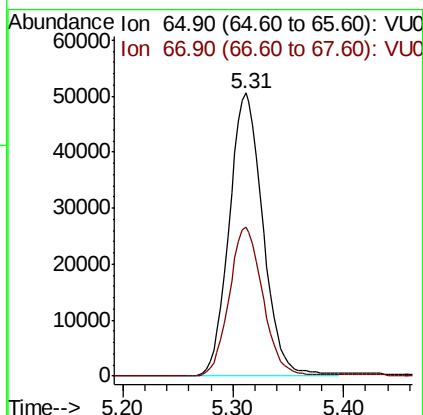

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 114 Resp: 184496
 Ion Ratio Lower Upper
 114 100
 63 24.7 0.0 49.2
 88 16.9 0.0 33.8









#35
 Dibromofluoromethane
 Concen: 46.735 ug/l
 RT: 4.88 min Scan# 1154
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion:113 Resp: 74739
 Ion Ratio Lower Upper
 113 100
 111 102.7 82.2 123.4
 192 18.8 15.2 22.8

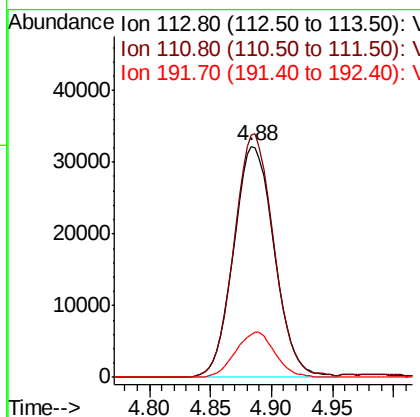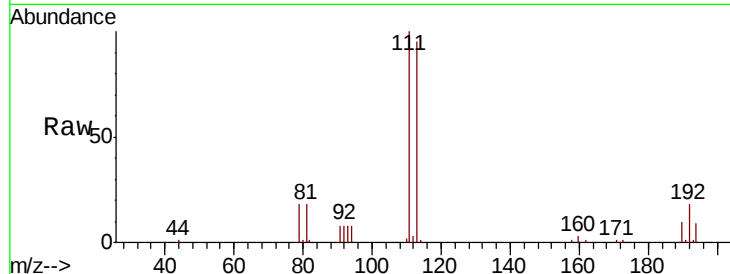

#36
 1,1-Dichloropropene
 Concen: 4.079 ug/l
 RT: 4.98 min Scan# 1185
 Delta R.T. -0.15 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 75 Resp: 10044
 Ion Ratio Lower Upper
 75 100
 110 7.7 16.1 48.2#
 77 0.0 24.6 36.8#



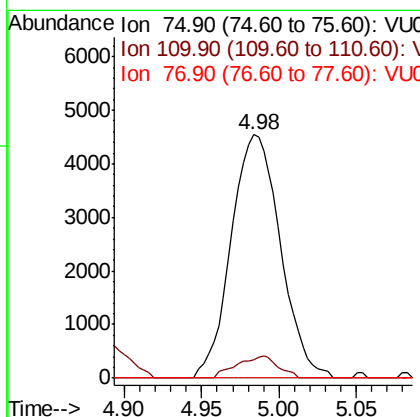



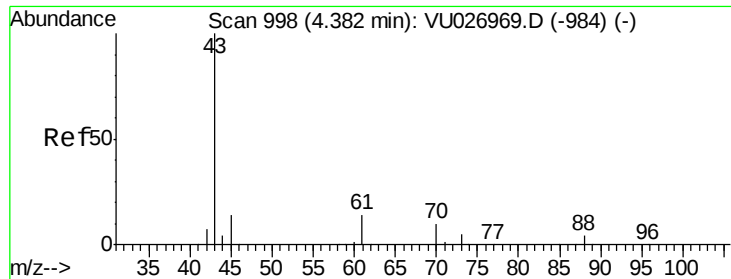

#37
Ethyl Acetate
Concen: 0.542 ug/l
RT: 4.29 min Scan# 968
Delta R.T. -0.10 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52




Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A


Tgt Ion: 43 Resp: 1807
Ion Ratio Lower Upper
43 100
61 0.0 10.5 15.7#
70 0.0 7.4 11.0#

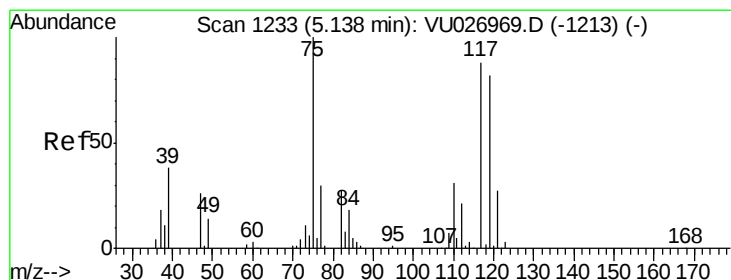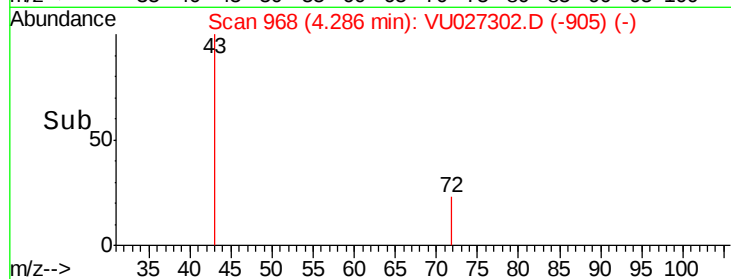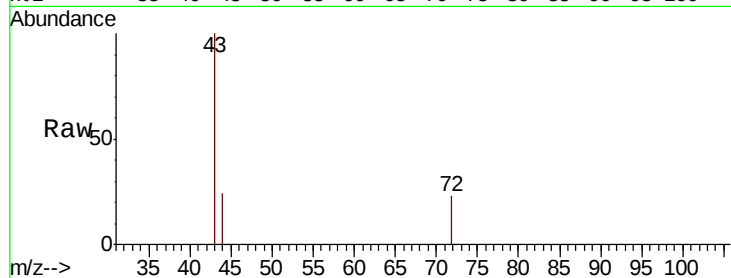

#38
Carbon Tetrachloride
Concen: 4.817 ug/l
RT: 4.99 min Scan# 1186
Delta R.T. -0.15 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 117 Resp: 11287
Ion Ratio Lower Upper
117 100
119 4.7 74.4 111.6#
121 0.0 24.2 36.4#


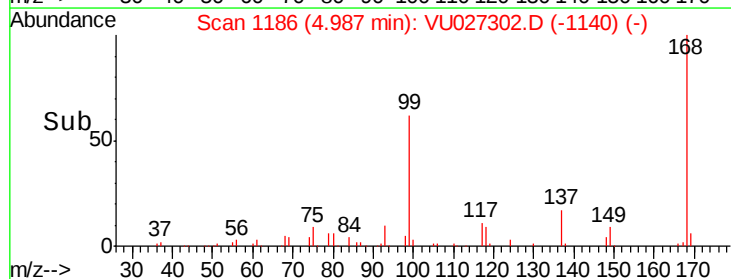

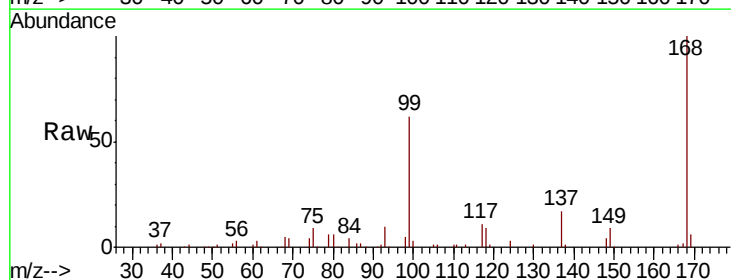


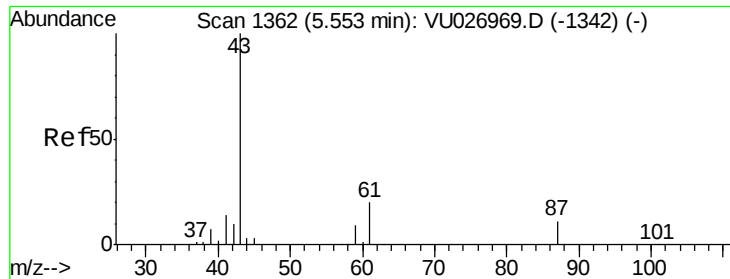

#43
Isopropyl Acetate
Concen: 21.625 ug/l
RT: 5.55 min Scan# 1361
Delta R.T. -0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52




Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A


Tgt Ion: 43 Resp: 105124
Ion Ratio Lower Upper
43 100
61 18.4 15.7 23.5
87 10.5 9.0 13.4

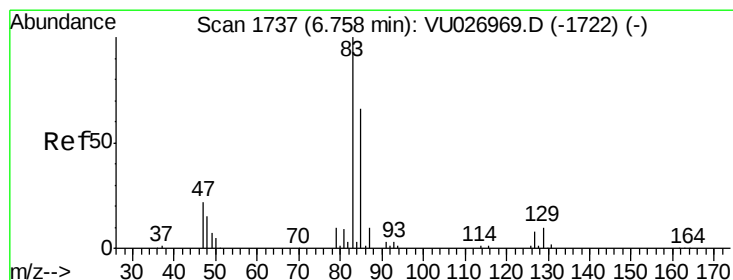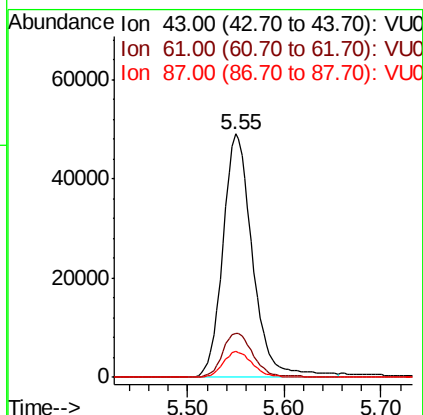

#47
Bromodichloromethane
Concen: 0.416 ug/l
RT: 6.76 min Scan# 1737
Delta R.T. -0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 83 Resp: 1083
Ion Ratio Lower Upper
83 100
85 50.8 52.5 78.7#
127 0.0 6.3 9.5#

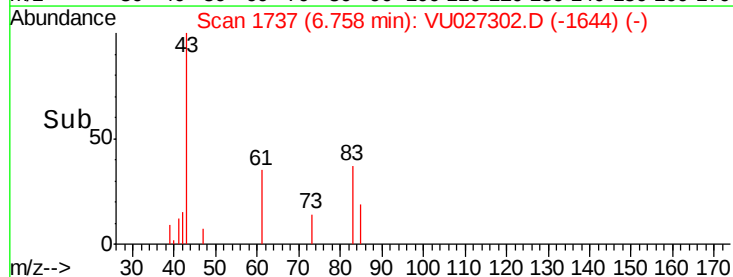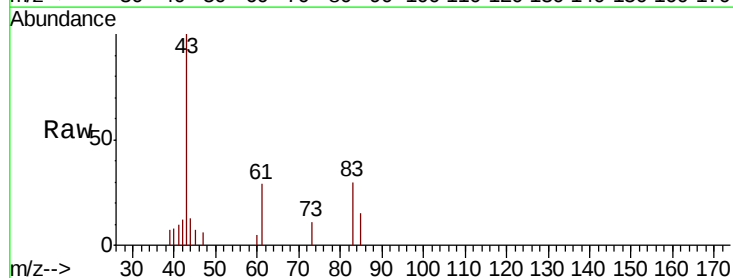



#48

Methyl methacrylate

Concen: 2.452 ug/l

RT: 6.54 min Scan# 1669

Delta R.T. -0.08 min

Lab File: VU027302.D

Acq: 29 Sep 2018 03:52

Instrument :

MSVOA_U

ClientSampleId :

PL-01-092718-A


Tgt Ion: 41 Resp: 3890

Ion Ratio Lower Upper

41 100

69 0.0 60.6 90.8#




39 8.6 42.8 64.2#



Abundance Ion 41.00 (40.70 to 41.70): VU027302.D (-1602) (-)

Ion 69.00 (68.70 to 69.70): VU027302.D (-1602) (-)

Ion 39.00 (38.70 to 39.70): VU027302.D (-1602) (-)

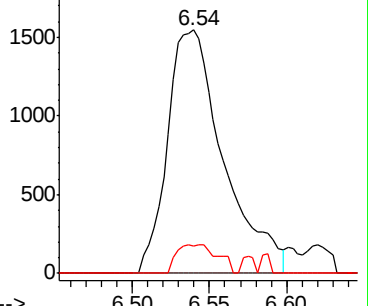

#50

Toluene-d8

Concen: 47.989 ug/l

RT: 7.57 min Scan# 1988

Delta R.T. -0.00 min

Lab File: VU027302.D


Acq: 29 Sep 2018 03:52

Tgt Ion: 98 Resp: 292477

Ion Ratio Lower Upper



98 100


100 65.0 52.1 78.1



Abundance Ion 98.00 (97.70 to 98.70): VU027302.D (-1896) (-)

Ion 100.00 (99.70 to 100.70): VU027302.D (-1896) (-)



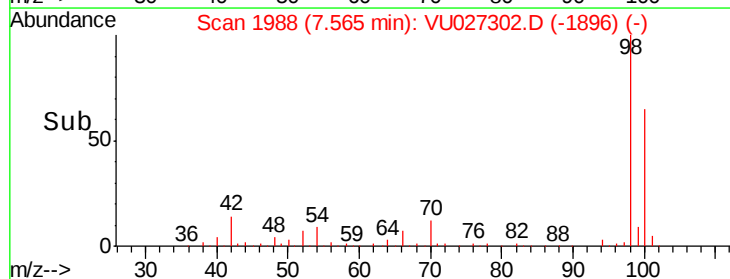
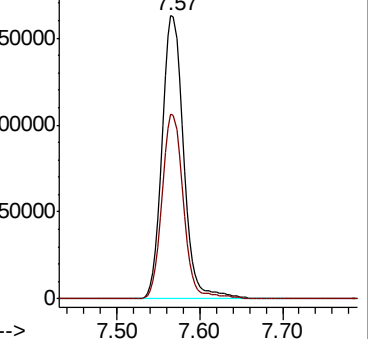




#51
 4-Methyl-2-Pentanone
 Concen: 0.217 ug/l
 RT: 7.47 min Scan# 1957
 Delta R.T. 0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion: 43 Resp: 711
 Ion Ratio Lower Upper
 43 100
 58 34.2 29.8 44.6

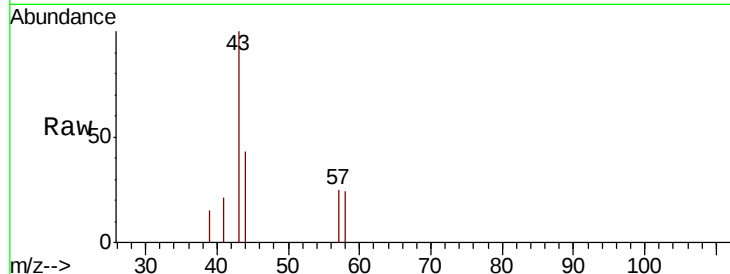

#56
 Ethyl methacrylate
 Concen: 2.213 ug/l
 RT: 7.84 min Scan# 2073
 Delta R.T. -0.18 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 69 Resp: 64
 Ion Ratio Lower Upper
 69 100
 41 445.3 59.0 88.4#
 39 217.2 30.2 45.4#







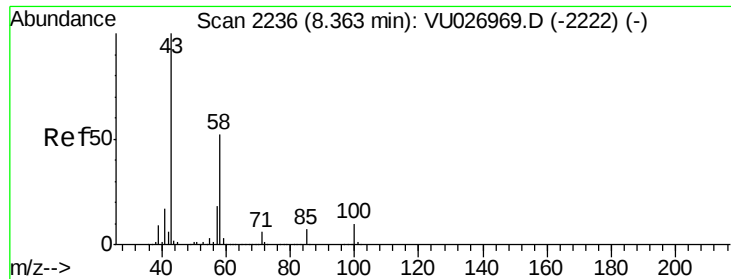

#59
 2-Hexanone
 Concen: 0.575 ug/l
 RT: 8.31 min Scan# 2221
 Delta R.T. -0.05 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion: 43 Resp: 1472
 Ion Ratio Lower Upper
 43 100
 58 0.0 26.1 78.2#

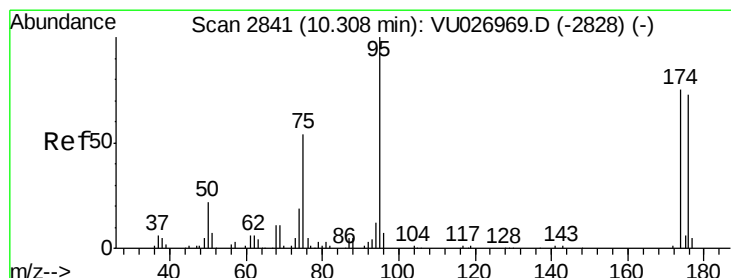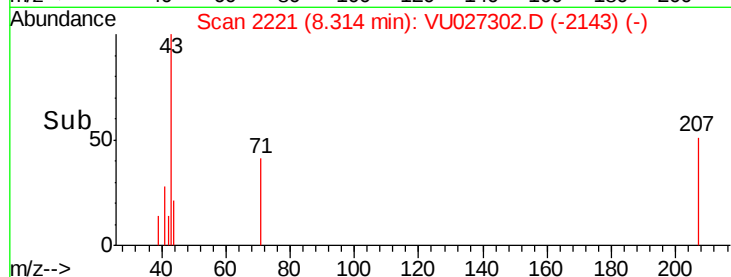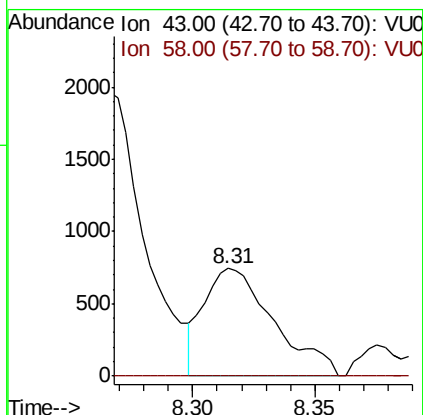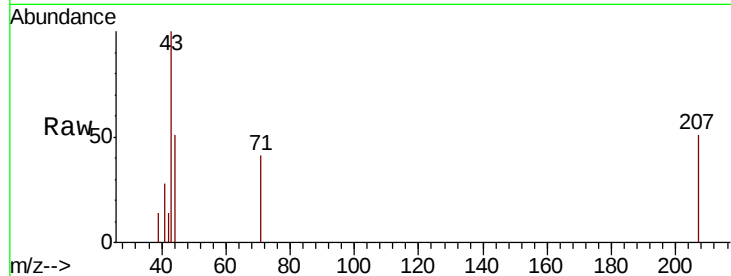

#62
 4-Bromofluorobenzene
 Concen: 47.320 ug/l
 RT: 10.31 min Scan# 2841
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 95 Resp: 98958
 Ion Ratio Lower Upper
 95 100
 174 73.6 0.0 150.2
 176 70.4 0.0 145.2

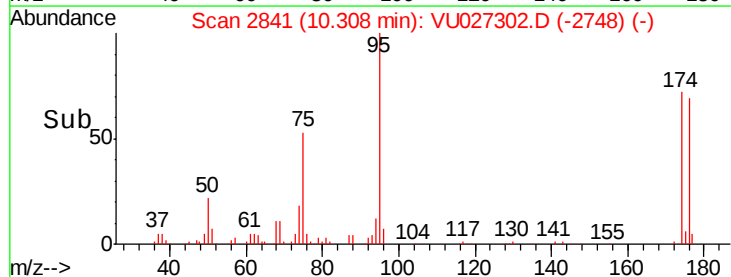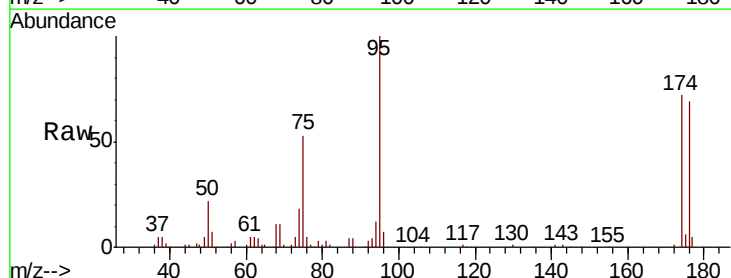


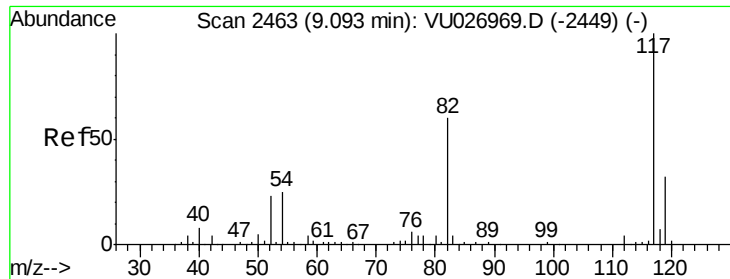




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2463
Delta R.T. -0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A

Tgt Ion:117 Resp: 177366
Ion Ratio Lower Upper
117 100
82 61.1 48.0 72.0
119 32.4 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

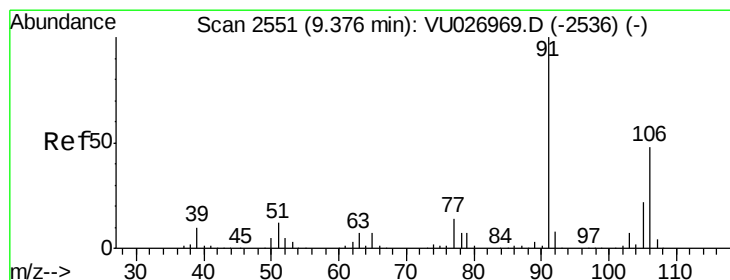
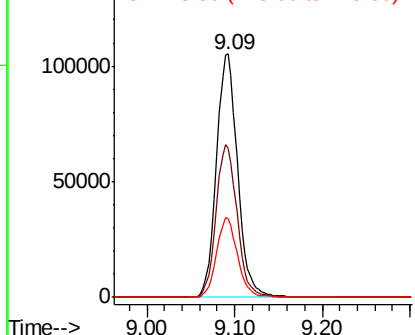



#68
m/p-Xylenes
Concen: 1.646 ug/l
RT: 9.38 min Scan# 2551
Delta R.T. 0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion:106 Resp: 462
Ion Ratio Lower Upper
106 100
91 231.6 166.5 249.7



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0

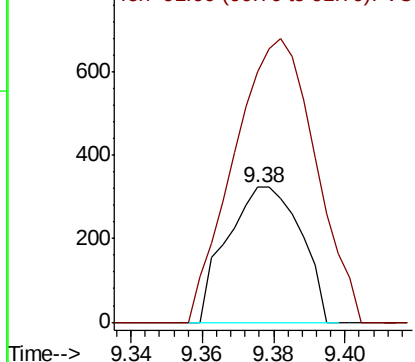

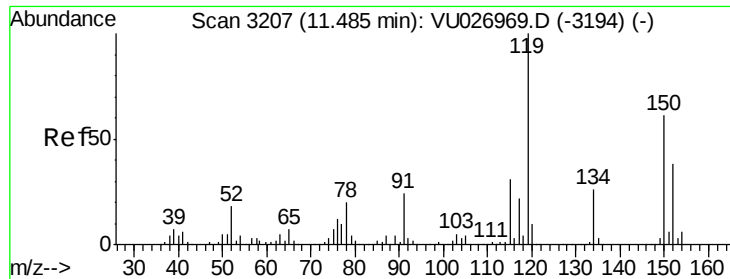


#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3207
Delta R.T. -0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A

Tgt Ion: 152 Resp: 84643
Ion Ratio Lower Upper
152 100
115 61.3 44.9 134.5
150 157.5 0.0 355.8




Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

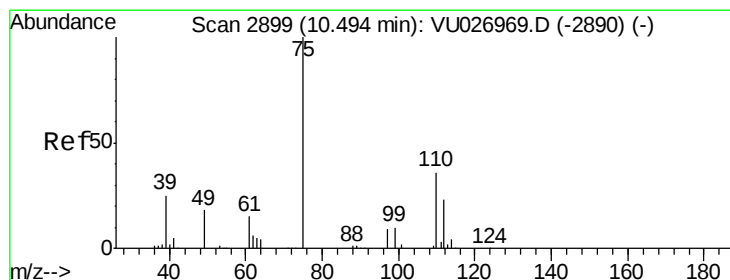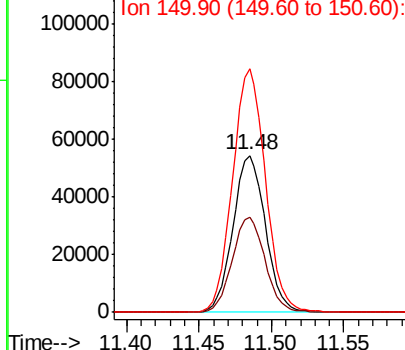



#76


1,2,3-Trichloropropane
Concen: 20.370 ug/l
RT: 10.31 min Scan# 2841
Delta R.T. -0.19 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 75 Resp: 52379
Ion Ratio Lower Upper
75 100
77 1.2 20.9 62.8#



Abundance Ion 74.90 (74.60 to 75.60): VU0
Ion 77.00 (76.70 to 77.70): VU0



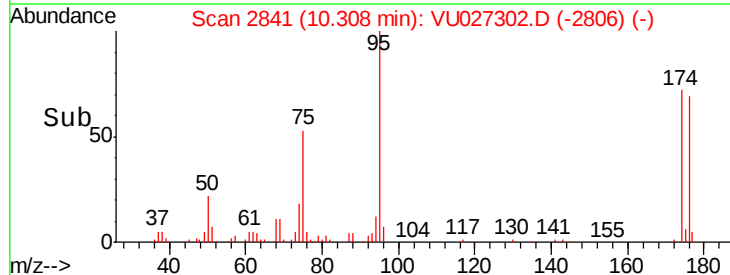
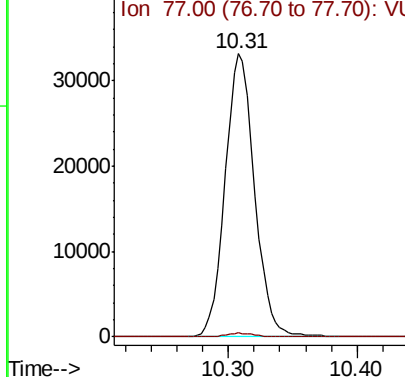


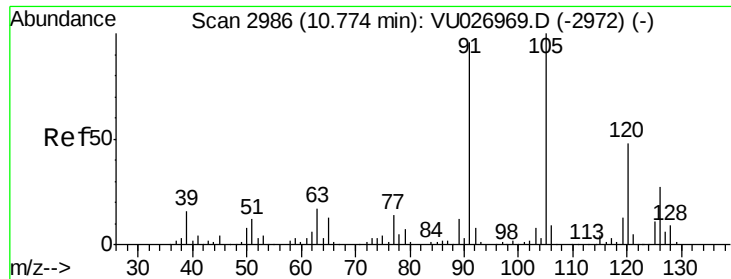

#80
 1,3,5-Trimethylbenzene
 Concen: 0.250 ug/l
 RT: 10.77 min Scan# 2985
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion: 105 Resp: 1328
 Ion Ratio Lower Upper
 105 100
 120 43.5 23.9 71.7

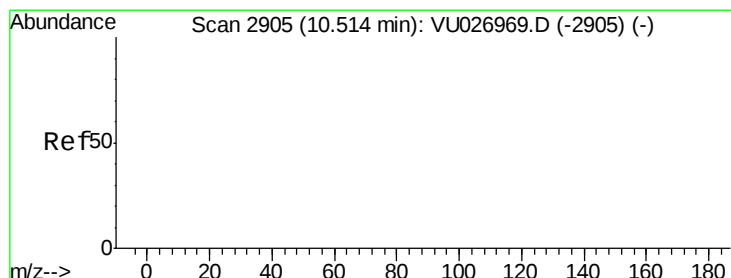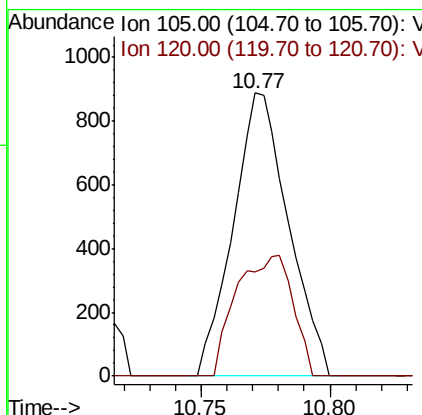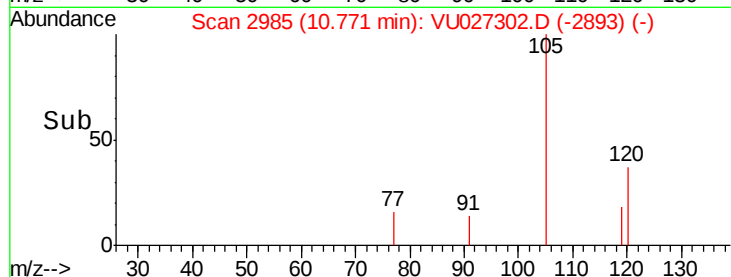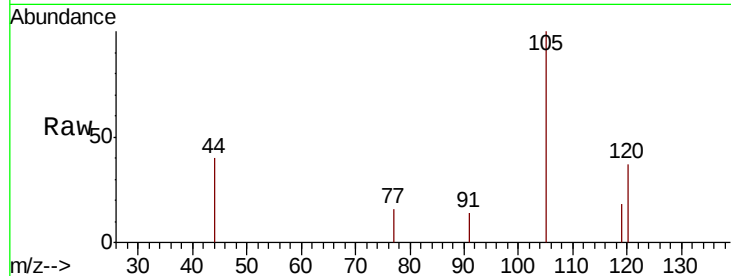

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.186 ug/l
 RT: 10.31 min Scan# 2841
 Delta R.T. -0.21 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion: 75 Resp: 52379
 Ion Ratio Lower Upper
 75 100
 53 0.0 0.0 0.0
 89 0.0 0.0 0.0


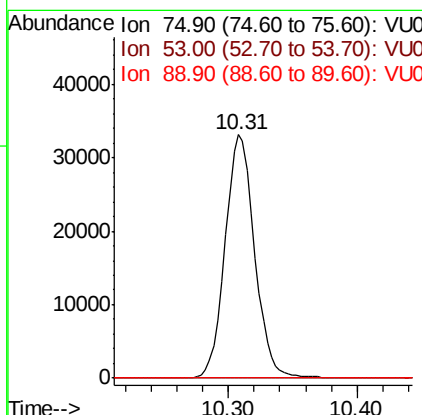
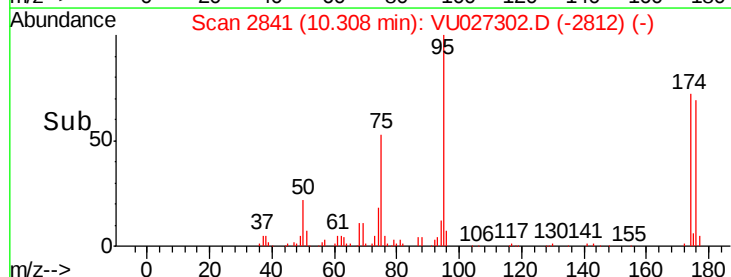
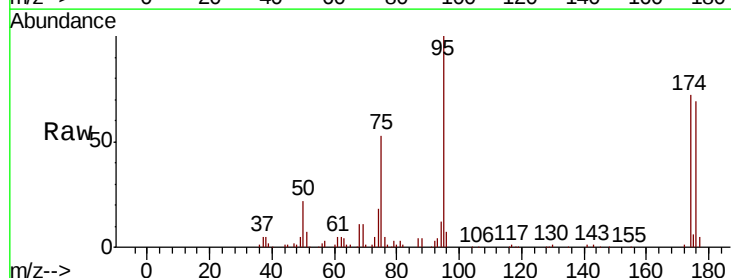


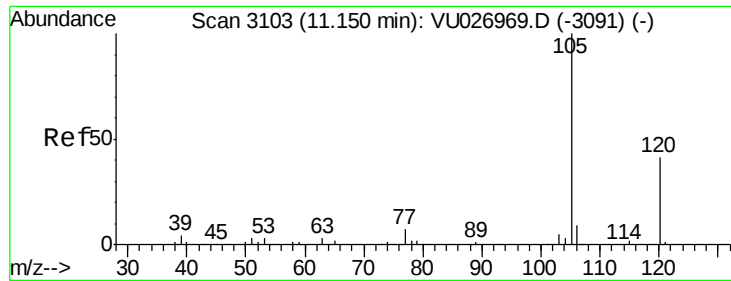

#84
 1,2,4-Trimethylbenzene
 Concen: 0.280 ug/l
 RT: 11.15 min Scan# 3104
 Delta R.T. 0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52




Instrument :
 MSVOA_U
 ClientSampleId :
 PL-01-092718-A


Tgt Ion:105 Resp: 1516
 Ion Ratio Lower Upper
 105 100
 120 44.2 22.4 67.2

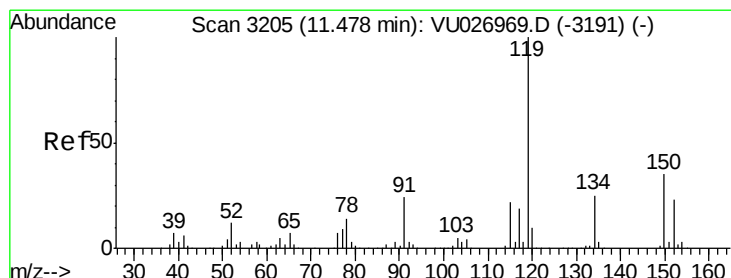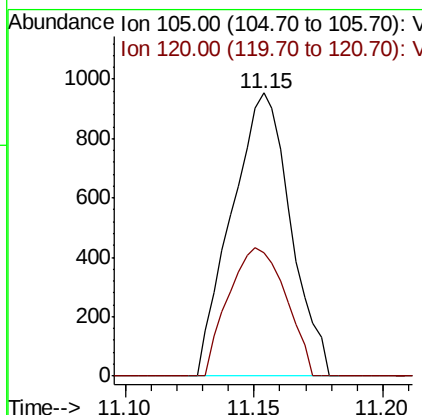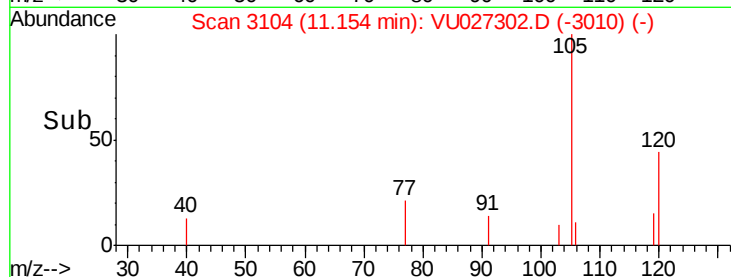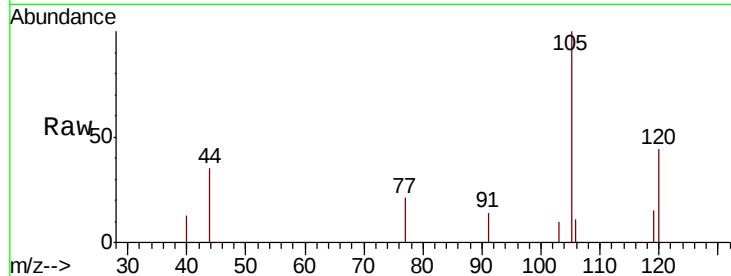

#86
 p-Isopropyltoluene
 Concen: 0.949 ug/l
 RT: 11.48 min Scan# 3204
 Delta R.T. -0.00 min
 Lab File: VU027302.D
 Acq: 29 Sep 2018 03:52

Tgt Ion:119 Resp: 132
 Ion Ratio Lower Upper
 119 100
 134 65.9 12.8 38.3#
 91 224.2 12.3 36.8#


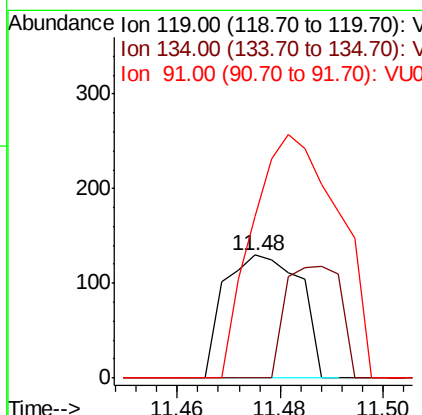
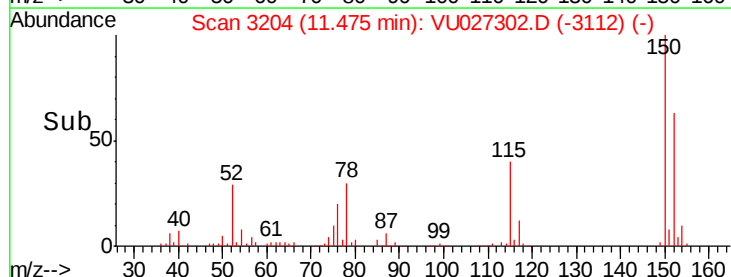
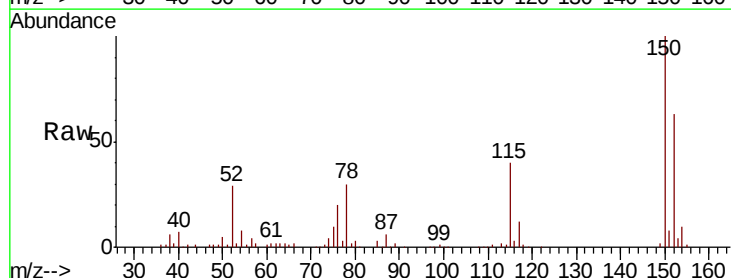


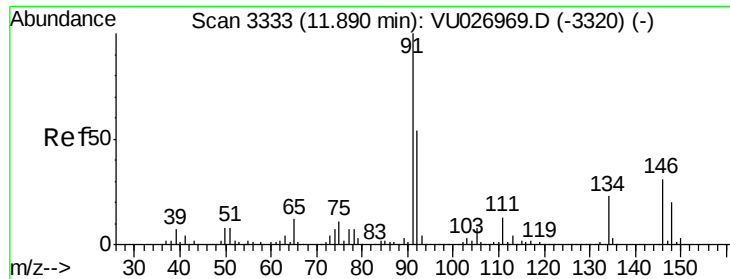

#89
n-Butylbenzene
Concen: 2.450 ug/l
RT: 11.88 min Scan# 3330
Delta R.T. -0.01 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Instrument :
MSVOA_U
ClientSampleId :
PL-01-092718-A

Tgt Ion: 91 Resp: 350
Ion Ratio Lower Upper
91 100
92 0.0 27.1 81.2#
134 70.3 11.7 35.0#

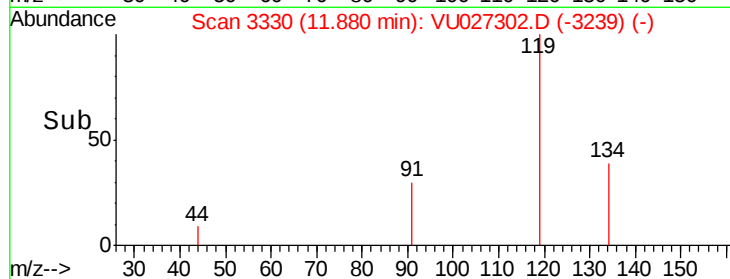

#95
Naphthalene
Concen: 2.951 ug/l
RT: 13.75 min Scan# 3910
Delta R.T. 0.00 min
Lab File: VU027302.D
Acq: 29 Sep 2018 03:52

Tgt Ion: 128 Resp: 9155
Ion Ratio Lower Upper
128 100
127 12.0 10.6 15.8
129 9.6 8.6 12.8

