


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092818\
 Data File : VU027228.D
 Acq On : 27 Sep 2018 16:32
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
 Title : SW846 8260
 Last Update : Sat Sep 22 01:31:57 2018

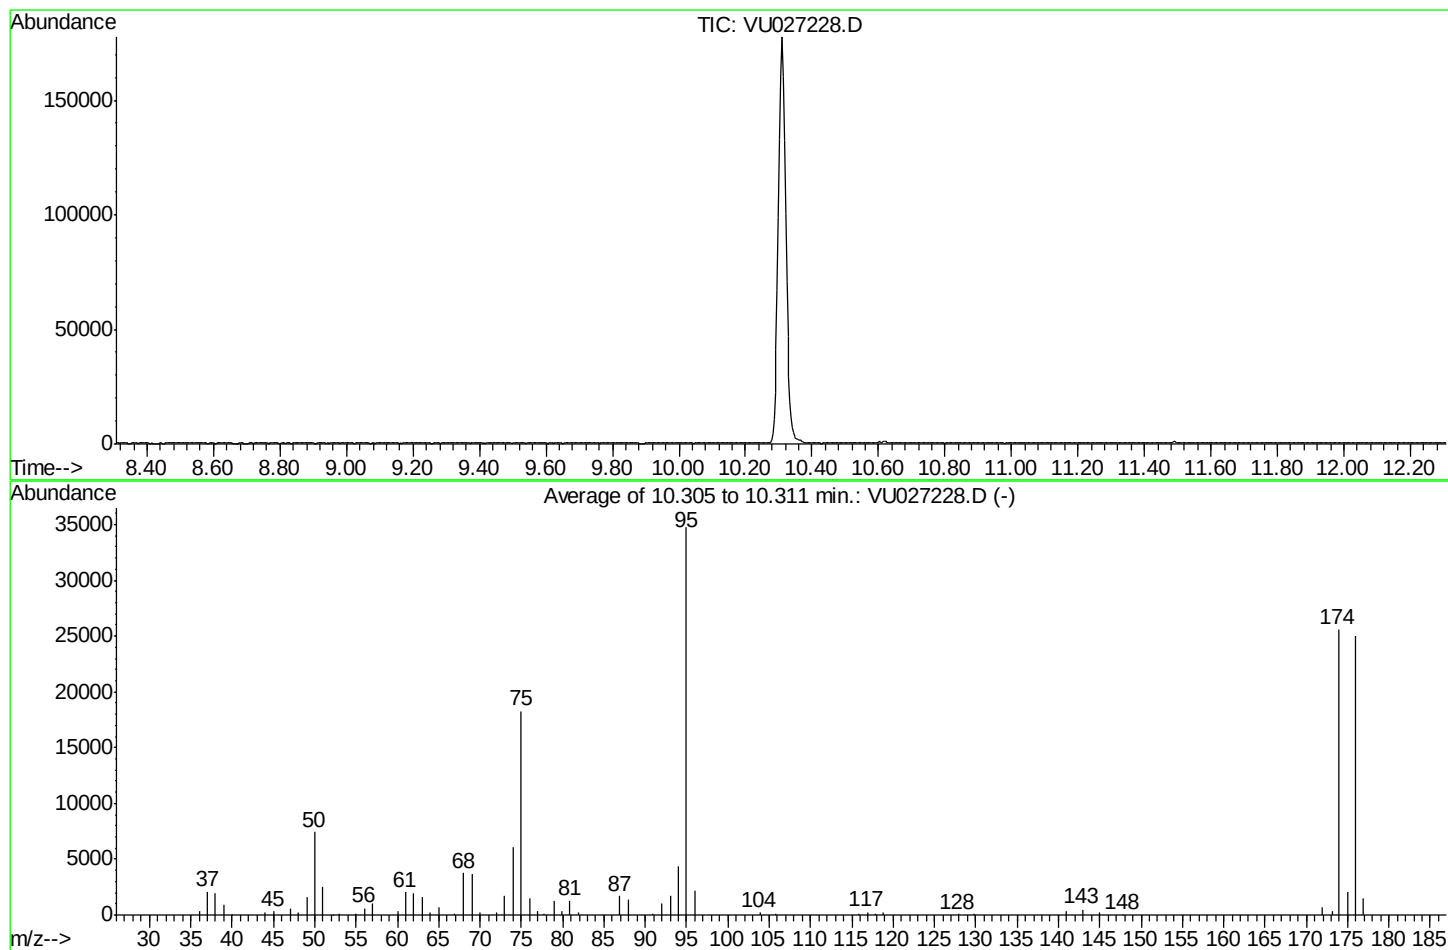

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	7423	PASS
75	95	30	60	52.5	18248	PASS
95	95	100	100	100.0	34749	PASS
96	95	5	9	6.4	2240	PASS
173	174	0.00	2	1.4	359	PASS
174	95	50	100	73.5	25536	PASS
175	174	5	9	8.1	2066	PASS
176	174	95	101	98.0	25032	PASS
177	176	5	9	5.9	1475	PASS