


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092818\
Data File : VU027254.D
Acq On : 28 Sep 2018 07:38
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

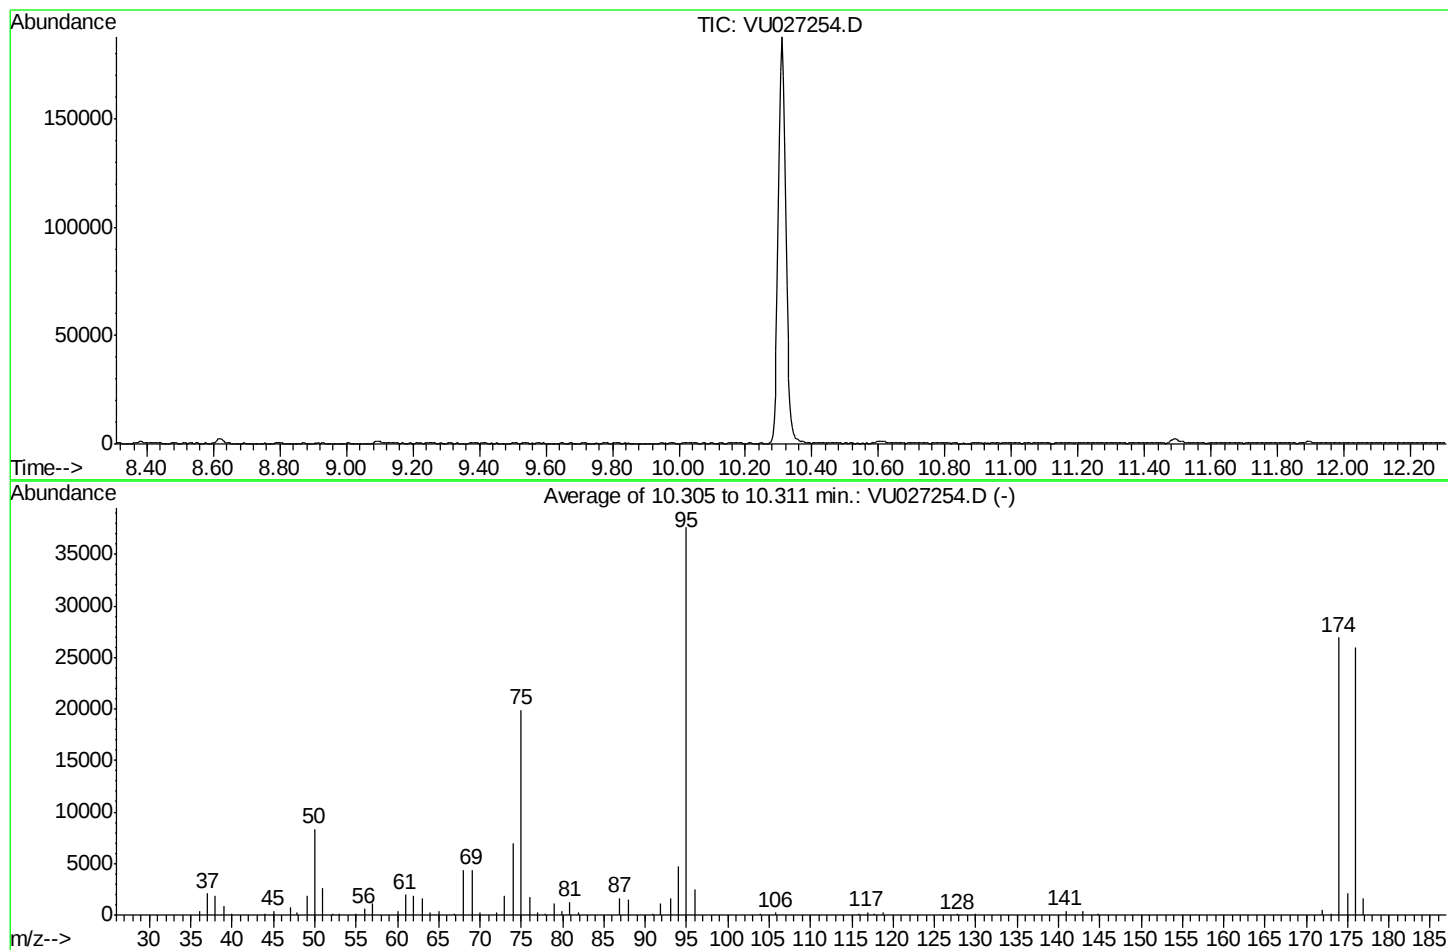

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	8345	PASS
75	95	30	60	52.9	19885	PASS
95	95	100	100	100.0	37621	PASS
96	95	5	9	6.5	2445	PASS
173	174	0.00	2	0.6	173	PASS
174	95	50	100	71.5	26912	PASS
175	174	5	9	7.9	2133	PASS
176	174	95	101	96.5	25957	PASS
177	176	5	9	6.4	1653	PASS