


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092820\
Data File : VU040324.D
Acq On : 28 Sep 2020 09:13
Operator : SY/MD
Sample : BFB08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Sep 29 07:18:40 2020

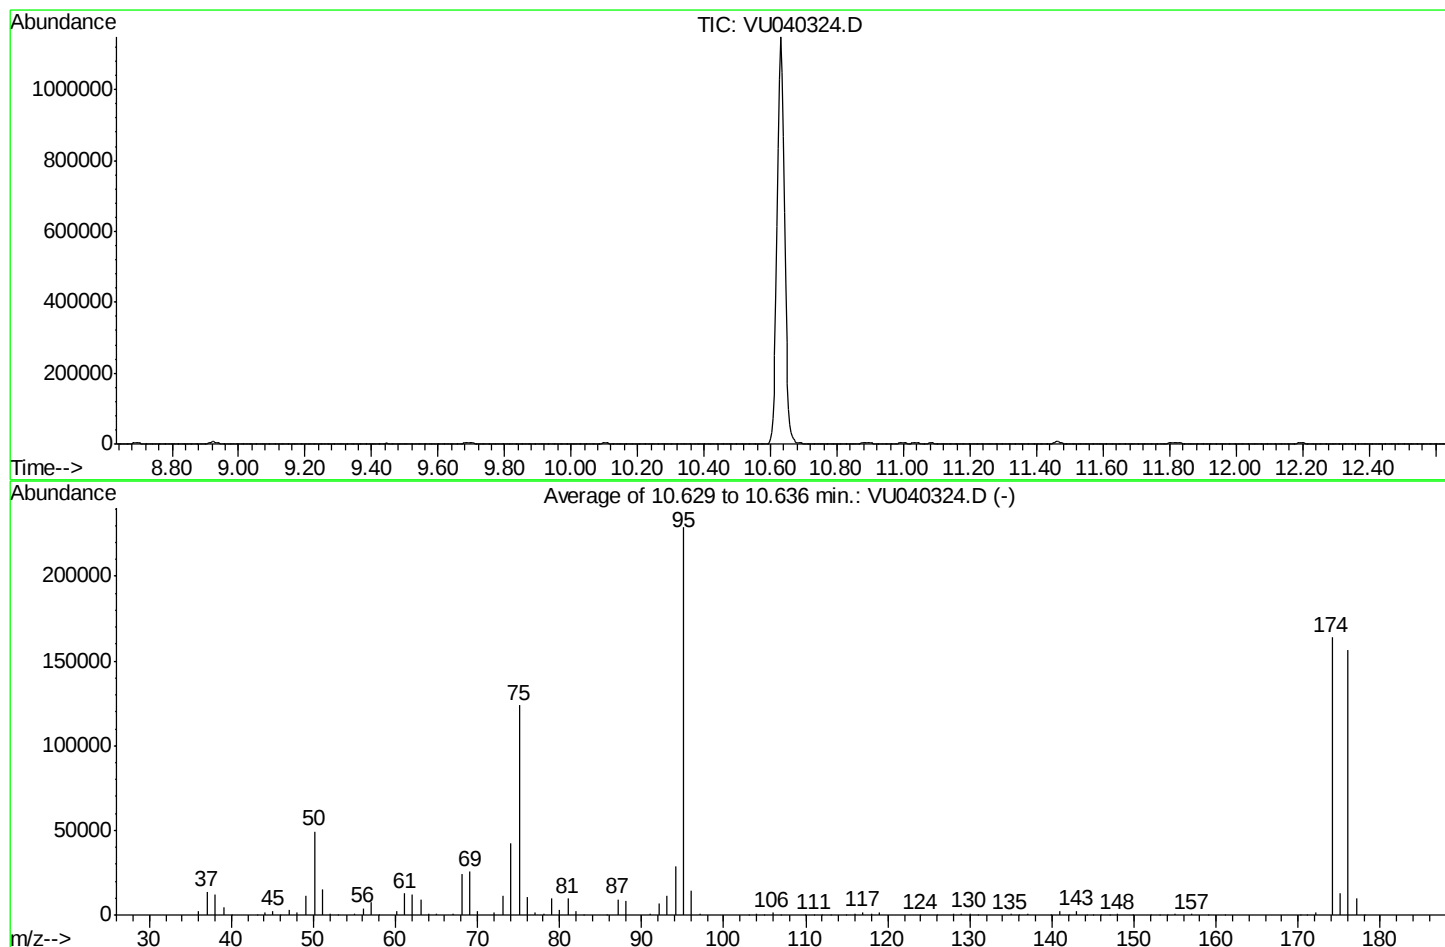

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	49234	PASS
75	95	30	80	54.1	123794	PASS
95	95	100	100	100.0	228928	PASS
96	95	5	9	6.1	14076	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.5	163776	PASS
175	174	5	9	7.6	12514	PASS
176	174	95	101	95.4	156309	PASS
177	176	5	9	6.3	9907	PASS

m/z	Abundance
36.00	2376.0
37.10	14590.0
38.10	12419.0
39.10	4932.0
40.00	434.0
43.00	189.0
44.10	1883.0
45.10	2390.0
46.00	297.0
47.00	3303.0
48.00	1481.0
49.10	11918.0
50.10	51424.0
51.10	16272.0
52.00	623.0
53.00	120.0
55.00	680.0
56.10	4215.0
57.10	7846.0
58.00	303.0
60.10	2272.0
61.10	12998.0
62.10	12465.0
63.10	9528.0
64.00	1213.0
65.00	947.0
67.00	742.0
68.10	25576.0
69.10	26328.0
70.00	2361.0
72.00	1618.0
73.10	11969.0
74.10	44240.0
75.10	128248.0
76.10	10655.0
77.10	1354.0
78.00	1092.0
79.00	10122.0
80.00	2785.0
81.00	9989.0
82.00	2303.0
82.90	194.0
87.10	9649.0
88.00	8545.0
91.00	1003.0
92.10	6476.0
93.10	11472.0
94.10	30448.0
95.10	235776.0
96.10	14591.0
97.10	519.0
103.00	156.0
104.00	1123.0
105.00	373.0
106.00	1381.0
107.00	275.0
109.90	132.0
111.00	263.0
111.90	245.0
112.90	167.0
114.80	233.0
116.00	899.0
117.00	1601.0
118.00	1017.0
119.00	1522.0
124.00	178.0
126.00	129.0
128.00	735.0
129.00	461.0
130.00	828.0
131.00	306.0
135.00	567.0
137.00	449.0
140.00	153.0
141.00	2590.0
142.00	250.0
143.00	2658.0
144.10	179.0
145.00	432.0
146.00	292.0
146.90	147.0
148.00	577.0
149.90	241.0
152.00	176.0
154.10	147.0
155.00	496.0
157.00	538.0
159.00	196.0
161.00	168.0
170.30	108.0
171.10	202.0
172.10	1331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

174.10	163584.0
175.10	12514.0
176.10	157632.0
177.10	10137.0
178.10	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	2437.0
37.00	14430.0
38.00	12295.0
39.10	4559.0
40.00	385.0
43.10	171.0
44.10	1885.0
45.10	2319.0
46.00	286.0
47.00	3105.0
48.00	1485.0
49.10	11555.0
50.10	50656.0
51.10	15789.0
52.00	568.0
53.00	137.0
55.00	636.0
56.10	4338.0
57.10	7809.0
58.00	346.0
60.10	2274.0
61.10	13057.0
62.10	12590.0
63.10	9272.0
64.00	1062.0
65.00	858.0
67.10	750.0
68.10	25240.0
69.10	26328.0
70.00	2358.0
72.10	1523.0
73.10	11618.0
74.10	44136.0
75.10	127576.0
76.10	10617.0
77.00	1279.0
78.10	1025.0
79.00	9995.0
80.00	2785.0
81.00	9950.0
82.00	2176.0
82.90	175.0
87.10	9504.0
88.00	8857.0
91.00	923.0
92.10	6699.0
93.10	11536.0
94.10	29568.0
95.10	236288.0
96.10	14499.0
97.10	487.0
103.00	151.0
104.00	1202.0
105.00	377.0
105.90	1294.0
107.00	249.0
109.90	194.0
111.10	295.0
111.90	217.0
113.00	179.0
114.90	254.0
116.00	959.0
117.00	1670.0
118.00	1081.0
119.00	1661.0
124.00	161.0
126.00	103.0
128.00	733.0
128.90	599.0
130.00	805.0
131.00	308.0
134.90	574.0
136.00	112.0
137.00	480.0
139.90	149.0
141.00	2559.0
142.00	296.0
143.00	2693.0
144.10	211.0
145.00	367.0
145.90	311.0
146.90	140.0
148.00	584.0
149.90	175.0
151.90	154.0
153.10	110.0
154.00	116.0
155.00	499.0
157.10	498.0
159.00	226.0
161.00	191.0
170.30	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

171.10	167.0
172.10	1281.0
174.10	169472.0
175.10	12934.0
176.10	161216.0
177.10	10270.0
178.00	299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	2294.0
37.00	12716.0
38.00	11094.0
39.10	3876.0
40.00	335.0
43.20	187.0
44.10	1816.0
45.10	2139.0
46.00	229.0
47.10	2764.0
48.00	1380.0
49.10	10289.0
50.10	45624.0
51.10	13938.0
52.00	522.0
52.90	107.0
55.00	559.0
56.10	3899.0
57.10	7087.0
58.00	334.0
60.10	2089.0
61.10	11724.0
62.10	11530.0
63.10	8373.0
64.10	892.0
65.10	735.0
67.10	679.0
68.10	22648.0
69.10	23768.0
70.00	1982.0
72.10	1328.0
73.10	10193.0
74.10	39584.0
75.10	115560.0
76.10	9707.0
77.00	1095.0
78.10	760.0
79.00	8949.0
80.00	2571.0
81.00	8967.0
82.00	1878.0
82.90	145.0
85.80	204.0
87.10	8608.0
88.00	8334.0
91.00	875.0
92.10	6378.0
93.10	10331.0
94.10	26136.0
95.10	214720.0
96.10	13140.0
97.10	376.0
103.00	122.0
104.00	1113.0
104.90	333.0
106.00	1137.0
107.00	191.0
109.90	222.0
111.00	265.0
111.90	181.0
113.00	165.0
114.90	224.0
116.00	1004.0
117.00	1544.0
118.00	966.0
119.00	1498.0
124.00	135.0
128.00	610.0
128.90	627.0
130.00	717.0
131.00	265.0
135.00	458.0
137.00	412.0
139.80	153.0
141.00	2304.0
142.00	296.0
143.00	2542.0
144.20	160.0
145.00	284.0
145.90	311.0
147.00	138.0
148.00	507.0
149.90	124.0
151.90	128.0
153.10	127.0
155.00	449.0
157.00	439.0
159.00	230.0
161.00	217.0
170.30	103.0
171.10	160.0
172.10	1147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

174.10	158272.0
175.10	12096.0
176.10	150080.0
177.10	9316.0
178.00	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

Scan 2874 (10.581 min): VU040324.D
BFB08

m/z	Abundance
40.00	170.0
44.00	310.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08