

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
 Data File : VU044964.D
 Acq On : 29 Sep 2021 00:58
 Operator : SY/MD
 Sample : M3926-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EP-1-MW-3R-0921DL

Quant Time: Sep 29 05:49:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 28 12:32:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.379	168	191199	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	341759	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	333229	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	167996	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	157853	49.596	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 99.200%			
35) Dibromofluoromethane	5.295	113	110510	51.259	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.520%			
50) Toluene-d8	7.903	98	436369	51.226	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.460%			
62) 4-Bromofluorobenzene	10.636	95	168453	47.899	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 95.800%			
Target Compounds						Qvalue
5) Bromomethane	1.867	94	352	0.293	ug/l	98
11) Tert butyl alcohol	3.186	59	538	0.589	ug/l #	72
16) Acetone	2.633	43	1613	0.854	ug/l #	83
20) Methylene Chloride	3.051	84	973	0.342	ug/l #	85
31) Cyclohexane	5.375	56	5088	1.052	ug/l #	1
36) 1,1-Dichloropropene	5.379	75	17547	4.910	ug/l #	50
38) Carbon Tetrachloride	5.375	117	20344	6.578	ug/l #	16
39) Methylcyclohexane	6.771	83	1293	0.295	ug/l #	80
48) Methyl methacrylate	7.044	41	2088	0.603	ug/l #	45
51) 4-Methyl-2-Pentanone	7.796	43	1149	0.222	ug/l	98
55) 1,1,2-Trichloroethane	8.372	97	777	0.280	ug/l #	15
56) Ethyl methacrylate	8.340	69	39	1.828	ug/l #	24
59) 2-Hexanone	8.690	43	1528	0.362	ug/l	92
60) Dibromochloromethane	8.565	129	91	2.206	ug/l #	10
67) Ethyl Benzene	9.574	91	43620	3.393	ug/l	100
68) m/p-Xylenes	9.697	106	36100	7.228	ug/l	95
69) o-Xylene	10.105	106	6186	1.248	ug/l	93
73) Isopropylbenzene	10.488	105	83209	6.651	ug/l	99
74) N-amyl acetate	10.330	43	1528	0.243	ug/l #	68
76) 1,2,3-Trichloropropane	10.636	75	91942	18.763	ug/l #	41
78) n-propylbenzene	10.909	91	150487	9.871	ug/l	99
79) 2-Chlorotoluene	10.909	91	150487	15.747	ug/l #	43
80) 1,3,5-Trimethylbenzene	11.092	105	28119	2.566	ug/l	99
81) trans-1,4-Dichloro-2-b...	10.636	75	91942	52.071	ug/l #	9
82) 4-Chlorotoluene	10.909	91	150487	13.932	ug/l #	47
83) tert-Butylbenzene	11.423	119	9502	0.891	ug/l	90
84) 1,2,4-Trimethylbenzene	11.472	105	664932	61.326	ug/l	100
85) sec-Butylbenzene	11.645	105	47866	3.487	ug/l	100
86) p-Isopropyltoluene	11.748	119	12671	1.147	ug/l	97
89) n-Butylbenzene	12.211	91	25184	2.476	ug/l #	80
90) Hexachloroethane	12.468	117	2894	1.451	ug/l #	15
93) 1,2,4-Trichlorobenzene	13.844	180	926	0.281	ug/l #	72
95) Naphthalene	14.092	128	8793	0.709	ug/l	99
96) 1,2,3-Trichlorobenzene	14.336	180	928	0.280	ug/l	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
Data File : VU044964.D
Acq On : 29 Sep 2021 00:58
Operator : SY/MD
Sample : M3926-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL

Quant Time: Sep 29 05:49:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 12:32:13 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
Data File : VU044964.D
Acq On : 29 Sep 2021 00:58
Operator : SY/MD
Sample : M3926-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Quant Time: Sep 29 05:49:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 12:32:13 2021
Response via : Initial Calibration

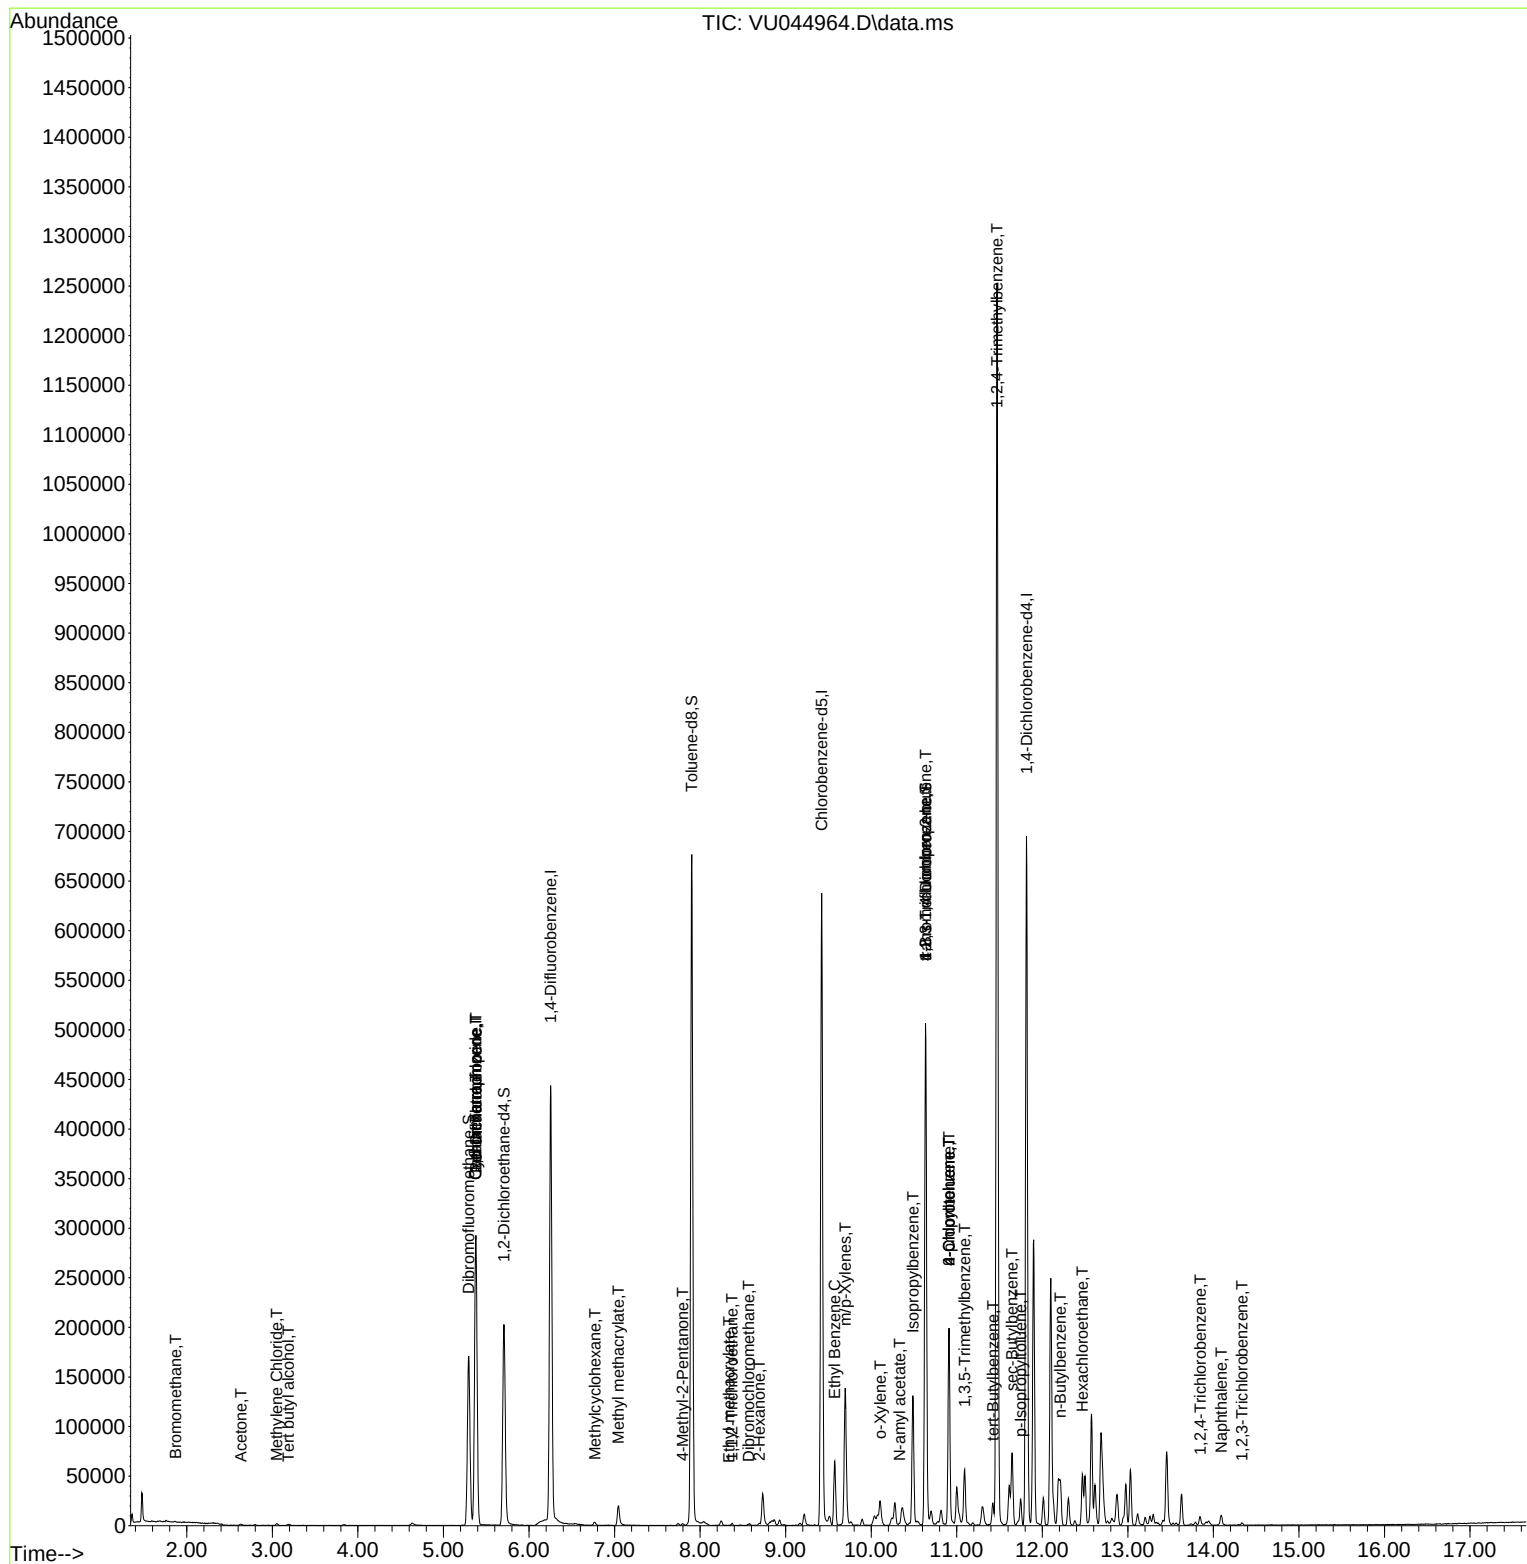






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 11
Delta R.T. 0.004 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL







Tgt Ion:168 Resp: 191199
Ion Ratio Lower Upper
168 100
99 66.0 51.4 77.0

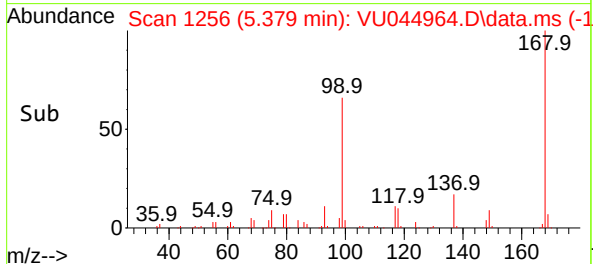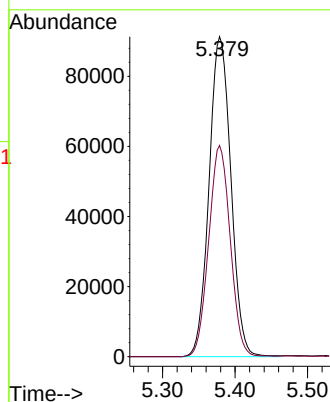

#5
Bromomethane
Concen: 0.293 ug/l
RT: 1.867 min Scan# 164
Delta R.T. 0.035 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 94 Resp: 352
Ion Ratio Lower Upper
94 100
96 91.2 74.5 111.7

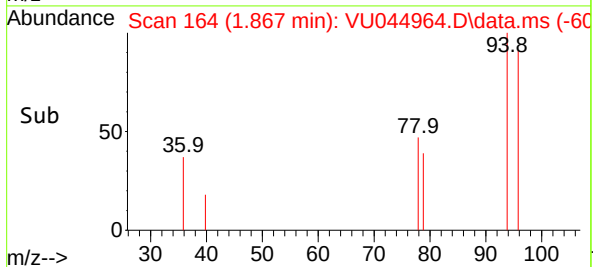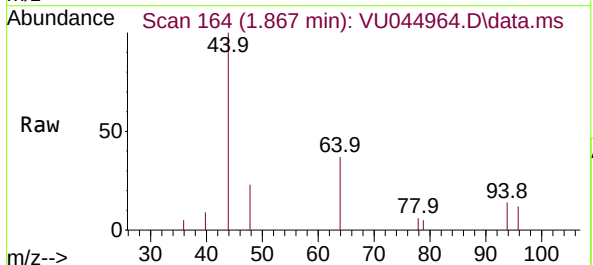

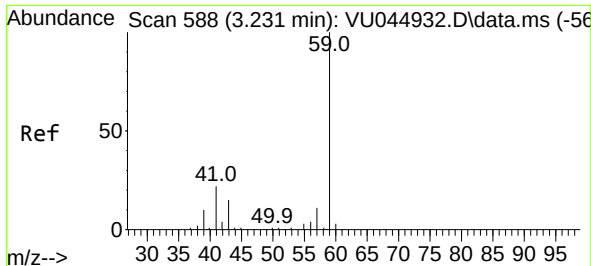

#11

Tert butyl alcohol

Concen: 0.589 ug/l

RT: 3.186 min Scan# 511

Delta R.T. -0.045 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Instrument :

MSVOA_U

ClientSampleId :





EP-1-MW-3R-0921DL

Tgt Ion: 59 Resp: 538

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

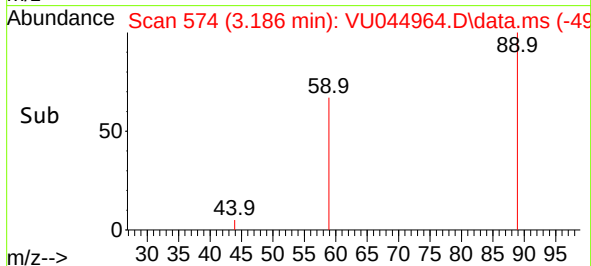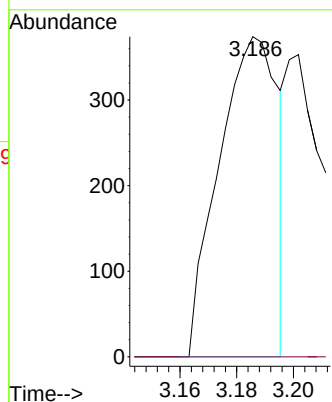

#16

Acetone

Concen: 0.854 ug/l

RT: 2.633 min Scan# 402

Delta R.T. 0.001 min

Lab File: VU044964.D




Acq: 29 Sep 2021 00:58


Tgt Ion: 43 Resp: 1613

Ion Ratio Lower Upper

43 100

58 22.2 25.2 37.8#


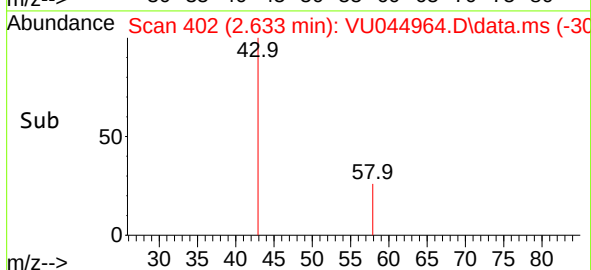

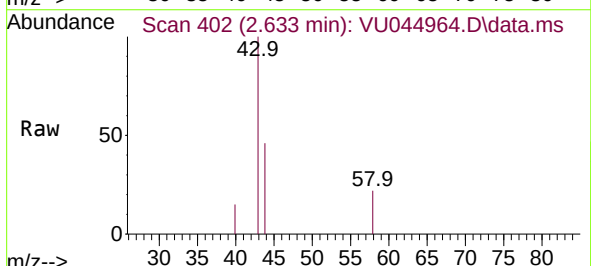




#20
Methylene Chloride
Concen: 0.342 ug/l
RT: 3.051 min Scan# 51
Delta R.T. 0.004 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:	84	Resp:	973
Ion	Ratio	Lower	Upper
84	100		
49	117.9	104.9	157.3
51	33.5	31.8	47.8
86	43.3	49.8	74.6#

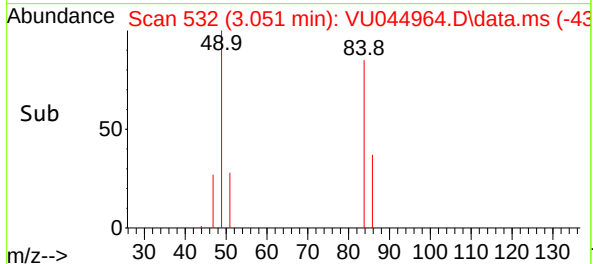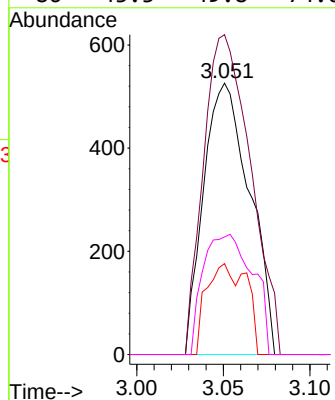

#31
Cyclohexane
Concen: 1.052 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.013 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:	56	Resp:	5088
Ion	Ratio	Lower	Upper
56	100		
69	160.2	25.2	37.8#
84	127.1	66.4	99.6#

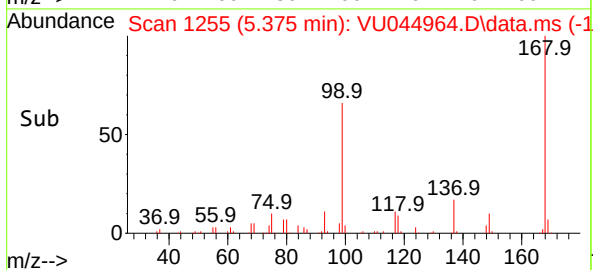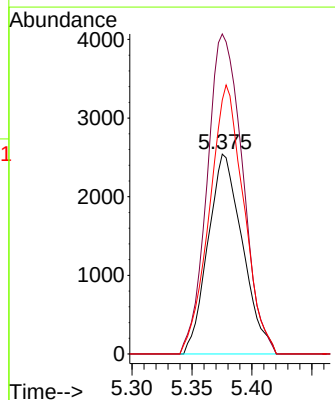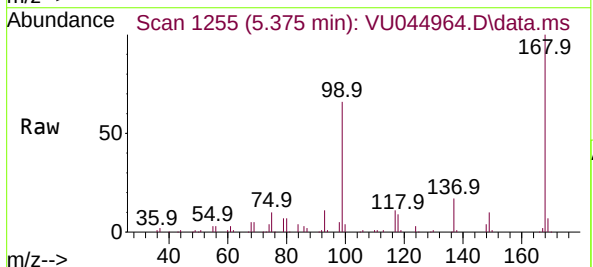



#33

1,2-Dichloroethane-d4

Concen: 49.596 ug/l

RT: 5.706 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Instrument :

MSVOA_U

ClientSampleId :





EP-1-MW-3R-0921DL

Tgt Ion: 65 Resp: 157853

Ion Ratio Lower Upper

65 100

67 50.5 0.0 104.8

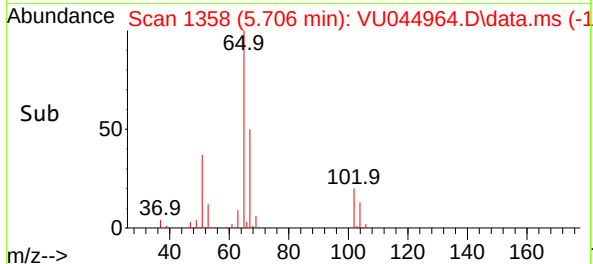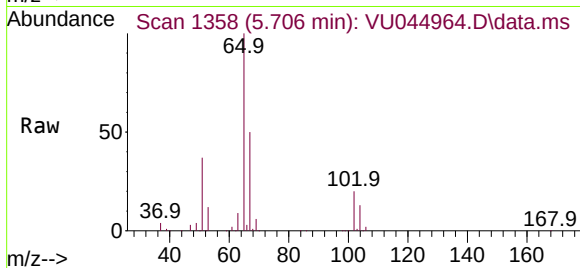

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1528

Delta R.T. 0.000 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58




Tgt Ion: 114 Resp: 341759


Ion Ratio Lower Upper

114 100

63 22.8 0.0 47.8

88 16.7 0.0 32.8

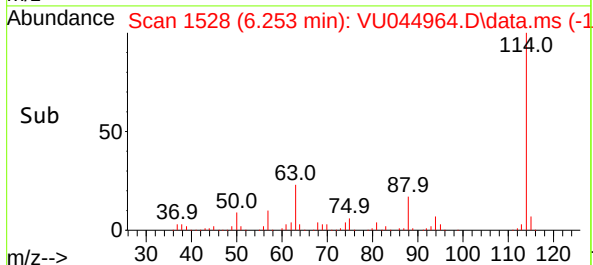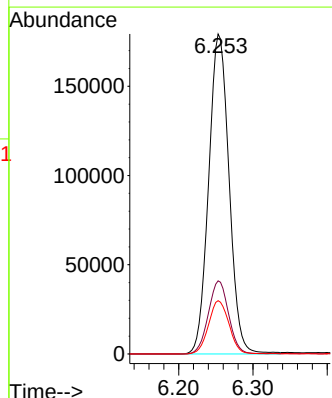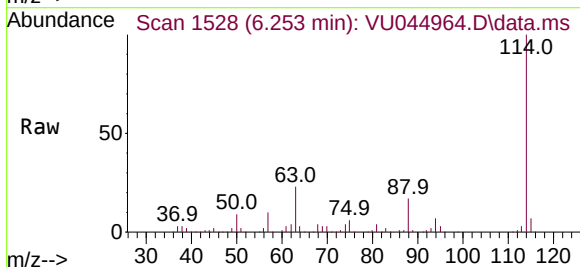



#35

Dibromofluoromethane

Concen: 51.259 ug/l

RT: 5.295 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Instrument :

MSVOA_U

ClientSampleId :

EP-1-MW-3R-0921DL





Tgt Ion:113 Resp: 110510

Ion Ratio Lower Upper

113 100

111 101.4 84.1 126.1

192 18.4 14.8 22.2

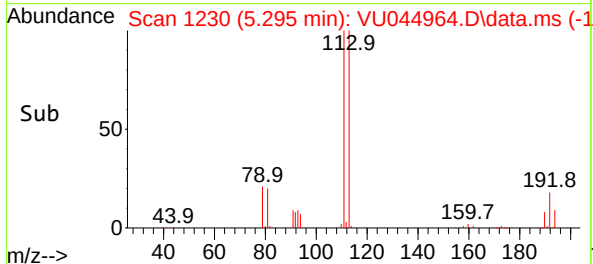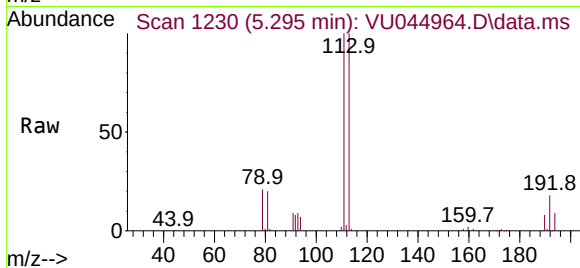

#36

1,1-Dichloropropene

Concen: 4.910 ug/l

RT: 5.379 min Scan# 1256

Delta R.T. -0.147 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58




Tgt Ion: 75 Resp: 17547


Ion Ratio Lower Upper

75 100

110 8.4 16.3 48.9#


77 0.0 25.0 37.4#

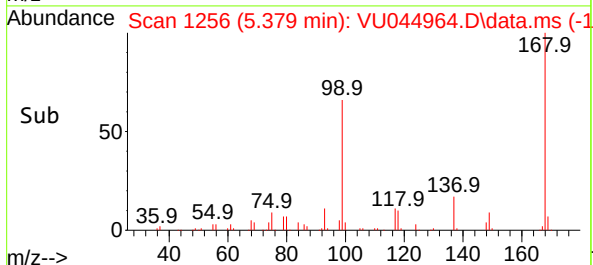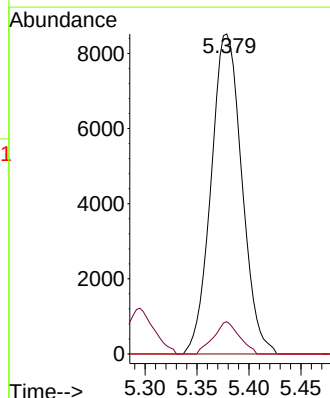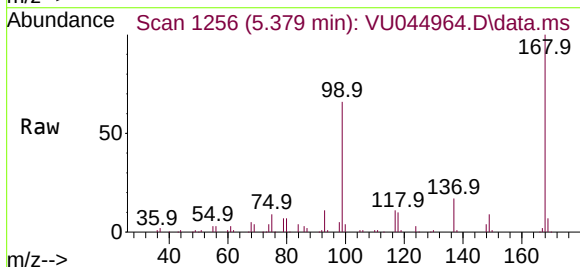






#38
Carbon Tetrachloride
Concen: 6.578 ug/l
RT: 5.375 min Scan# 117
Delta R.T. -0.151 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL







Tgt Ion:117 Resp: 20344
Ion Ratio Lower Upper
117 100
119 6.3 77.4 116.2#
121 0.0 24.5 36.7#

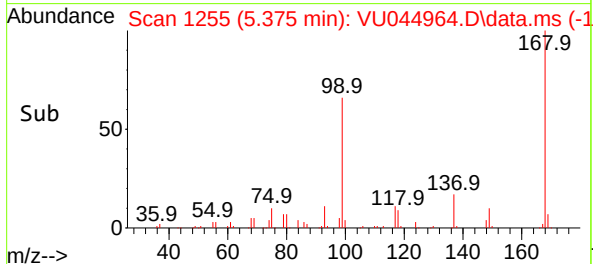

#39
Methylcyclohexane
Concen: 0.295 ug/l
RT: 6.771 min Scan# 1689
Delta R.T. 0.007 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 83 Resp: 1293
Ion Ratio Lower Upper
83 100
55 56.7 66.2 99.4#
98 49.5 37.5 56.3

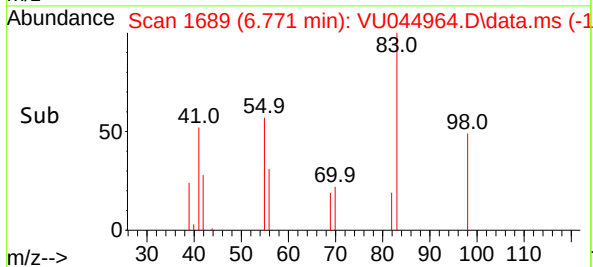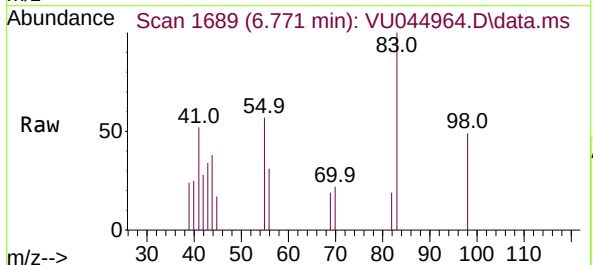



#48

Methyl methacrylate

Concen: 0.603 ug/l

RT: 7.044 min Scan# 1

Delta R.T. 0.080 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Instrument :

MSVOA_U

ClientSampleId :

EP-1-MW-3R-0921DL





Tgt Ion: 41 Resp: 2088

Ion Ratio Lower Upper

41 100

69 0.0 65.6 98.4#

39 59.5 46.2 69.4

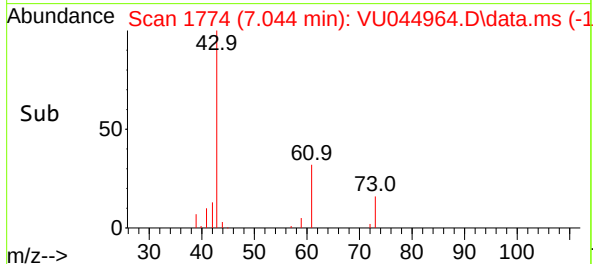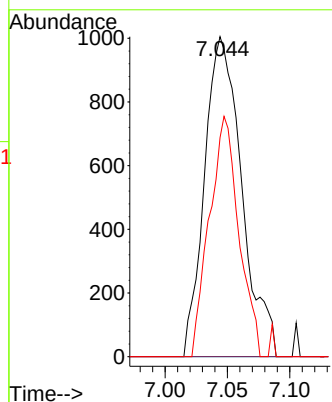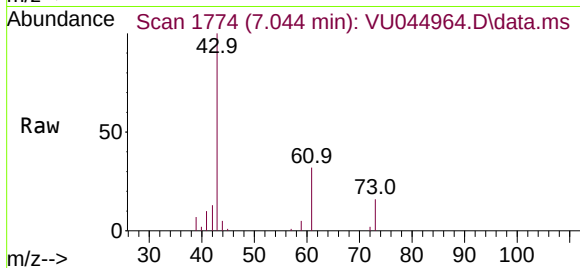

#50

Toluene-d8

Concen: 51.226 ug/l

RT: 7.903 min Scan# 2041

Delta R.T. 0.001 min

Lab File: VU044964.D




Acq: 29 Sep 2021 00:58


Tgt Ion: 98 Resp: 436369

Ion Ratio Lower Upper

98 100

100 65.2 52.5 78.7

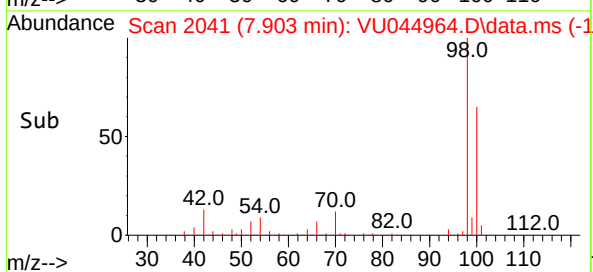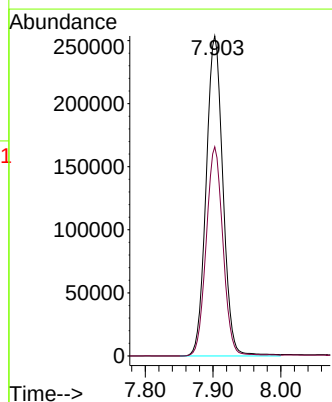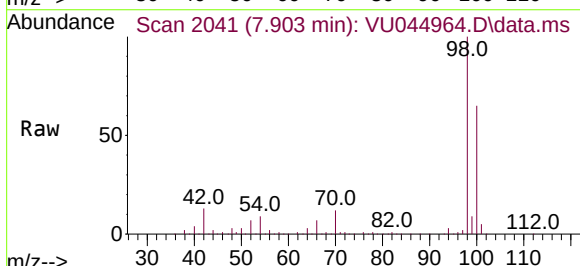



#51

4-Methyl-2-Pentanone

Concen: 0.222 ug/l

RT: 7.796 min Scan# 2009

Delta R.T. -0.003 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Instrument :

MSVOA_U

ClientSampleId :





EP-1-MW-3R-0921DL

Tgt Ion: 43 Resp: 1149

Ion Ratio Lower Upper

43 100

58 39.4 32.4 48.6

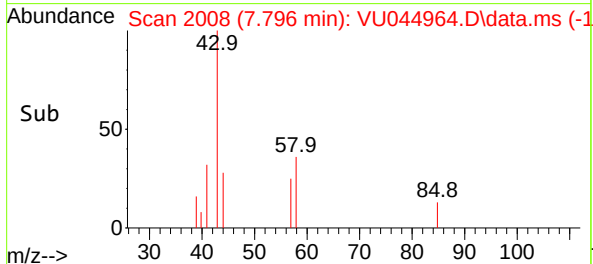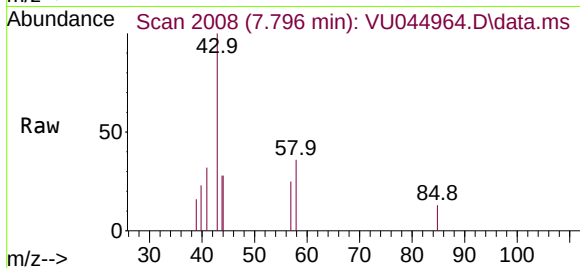

#55

1,1,2-Trichloroethane

Concen: 0.280 ug/l

RT: 8.372 min Scan# 2187

Delta R.T. -0.032 min

Lab File: VU044964.D

Acq: 29 Sep 2021 00:58

Tgt Ion: 97 Resp: 777




Ion Ratio Lower Upper


97 100

83 0.0 69.7 104.5#

85 0.0 44.8 67.2#

99 0.0 49.3 73.9#


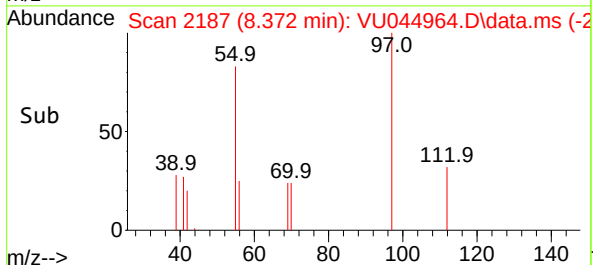
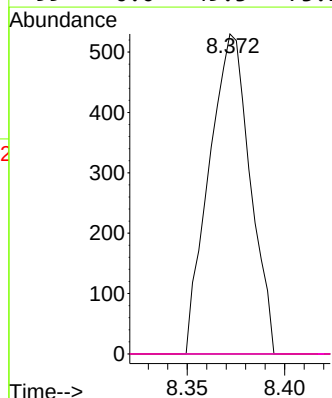
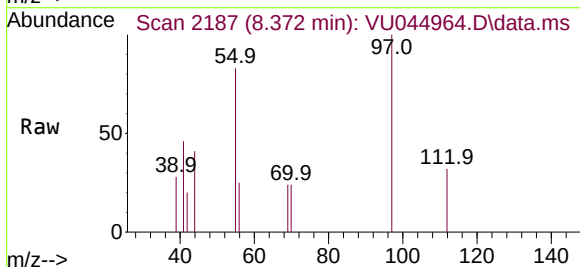




#56
Ethyl methacrylate
Concen: 1.828 ug/l
RT: 8.340 min Scan# 2177
Delta R.T. -0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:	69	Resp:	39
Ion	Ratio	Lower	Upper
69	100		
41	0.0	53.5	80.3#
39	0.0	31.1	46.7#

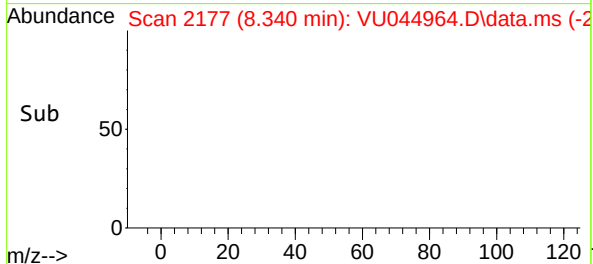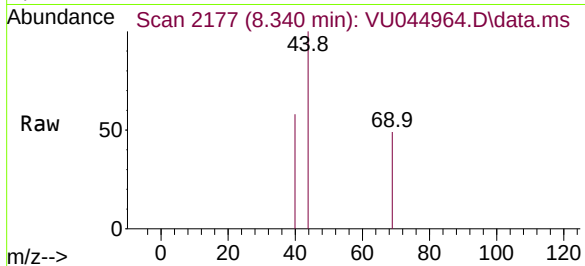

#59
2-Hexanone
Concen: 0.362 ug/l
RT: 8.690 min Scan# 2286
Delta R.T. -0.003 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:	43	Resp:	1528
Ion	Ratio	Lower	Upper
43	100		
58	50.5	28.0	84.0


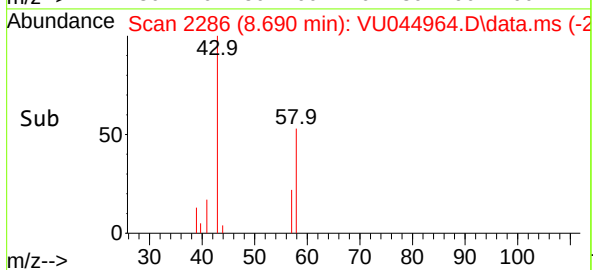

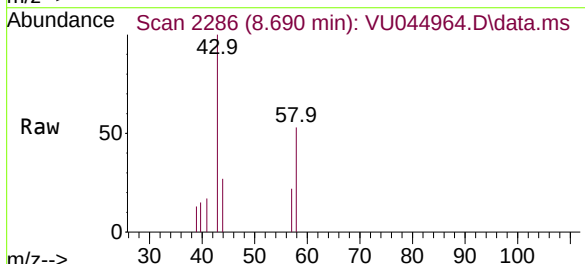




#60
Dibromochloromethane
Concen: 2.206 ug/l
RT: 8.565 min Scan# 211
Delta R.T. -0.251 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:129 Resp: 91
Ion Ratio Lower Upper
129 100
127 0.0 39.0 117.0#

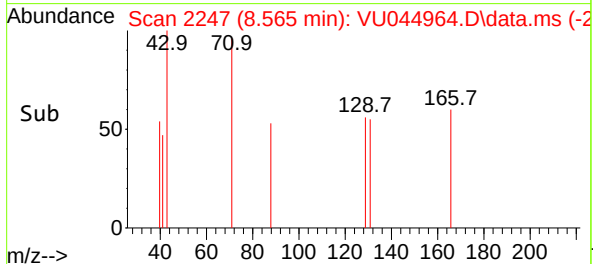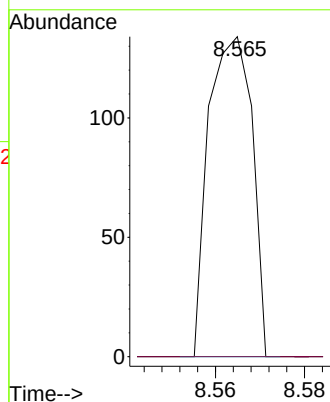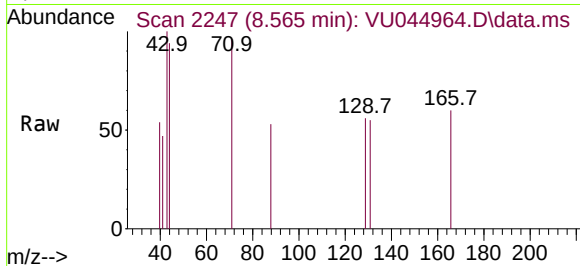

#62
4-Bromofluorobenzene
Concen: 47.899 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.001 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 95 Resp: 168453
Ion Ratio Lower Upper
95 100
174 72.0 0.0 146.6
176 68.6 0.0 141.2


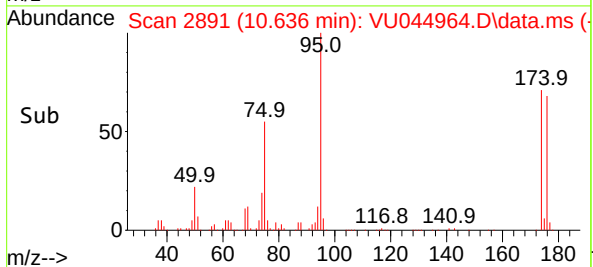

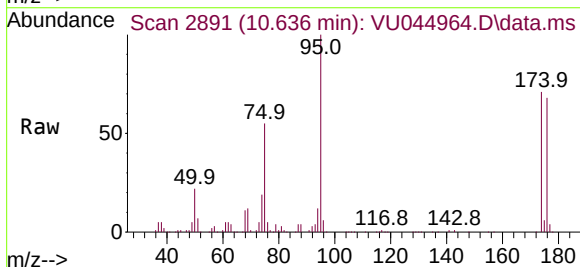




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:117 Resp: 333229
Ion Ratio Lower Upper
117 100
82 59.3 47.8 71.8
119 31.9 25.8 38.6

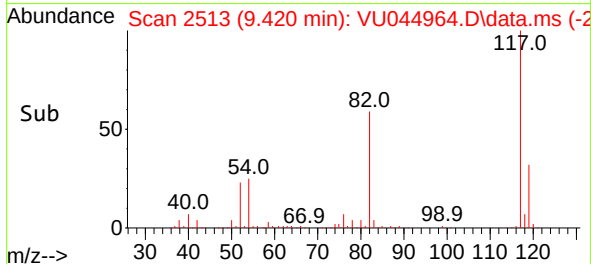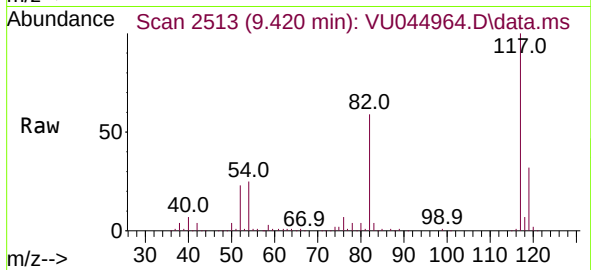

#67
Ethyl Benzene
Concen: 3.393 ug/l
RT: 9.574 min Scan# 2561
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 91 Resp: 43620
Ion Ratio Lower Upper
91 100
106 30.6 24.3 36.5




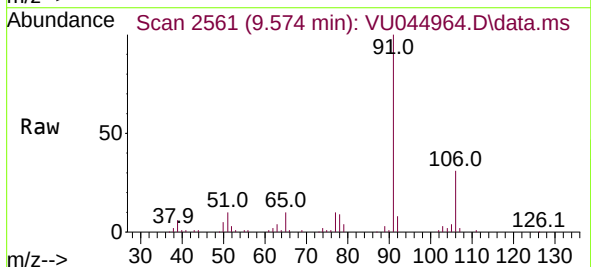




#68
m/p-Xylenes
Concen: 7.228 ug/l
RT: 9.697 min Scan# 2599
Delta R.T. -0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:106 Resp: 36100
Ion Ratio Lower Upper
106 100
91 213.1 164.2 246.2

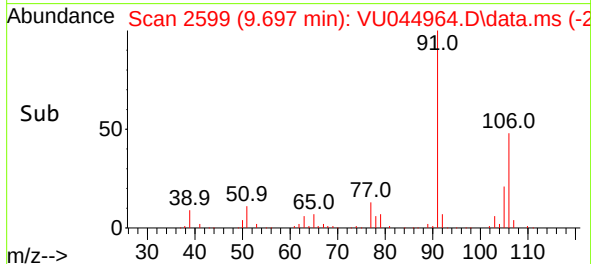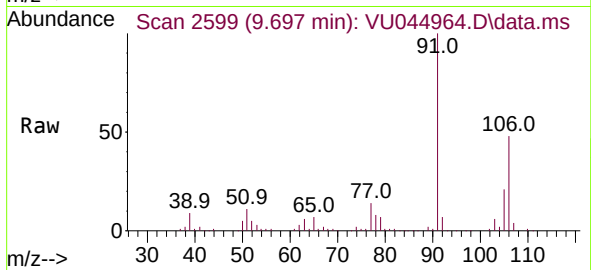

#69
o-Xylene
Concen: 1.248 ug/l
RT: 10.105 min Scan# 2726
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:106 Resp: 6186
Ion Ratio Lower Upper
106 100
91 229.6 108.9 326.7


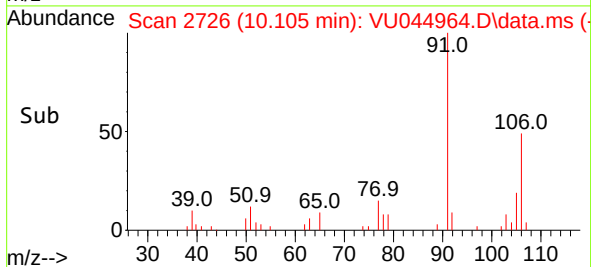

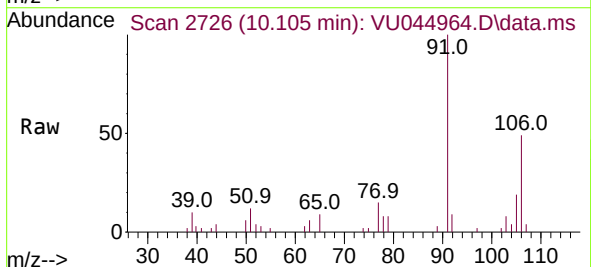




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.816 min Scan# 31
Delta R.T. 0.001 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:152 Resp: 167996
Ion Ratio Lower Upper
152 100
115 62.1 43.5 130.7
150 157.0 0.0 350.0

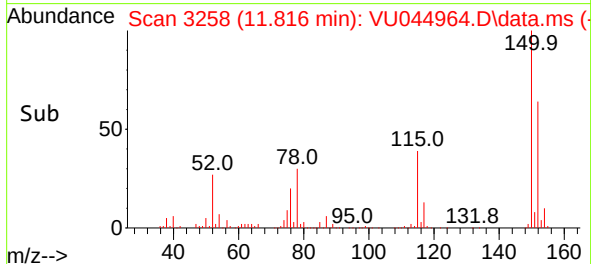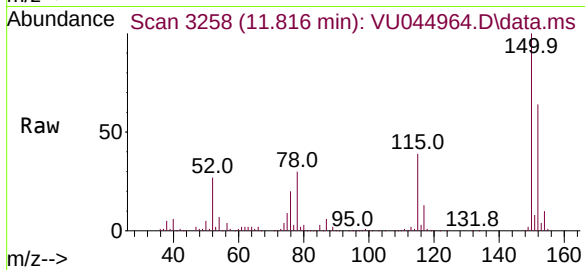

#73
Isopropylbenzene
Concen: 6.651 ug/l
RT: 10.488 min Scan# 2845
Delta R.T. 0.001 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:105 Resp: 83209
Ion Ratio Lower Upper
105 100
120 25.2 12.8 38.3


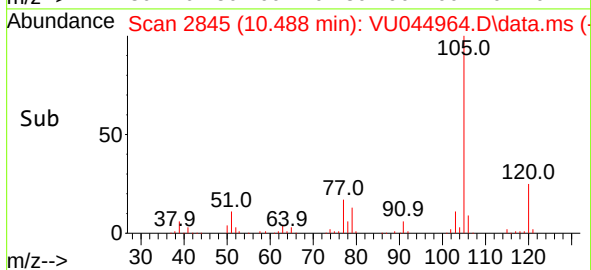

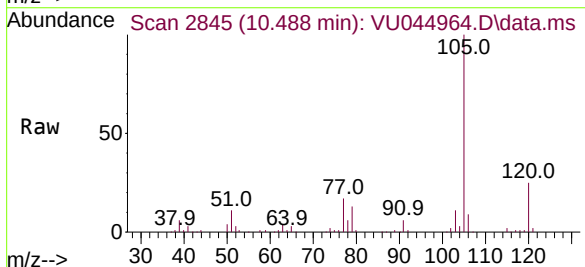


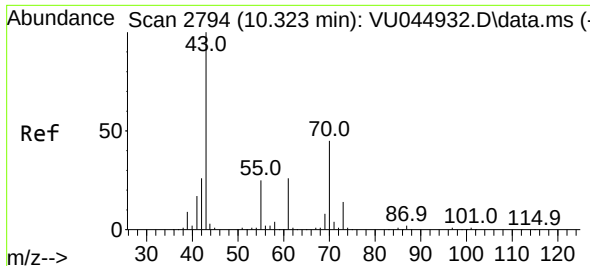

#74
N-amy1 acetate
Concen: 0.243 ug/l
RT: 10.330 min Scan# 21
Delta R.T. 0.007 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion: 43	Resp: 1528
Ion Ratio	Lower Upper
43	100
70	31.0 35.1 52.7#
55	0.0 20.5 30.7#
61	6.9 19.6 29.4#

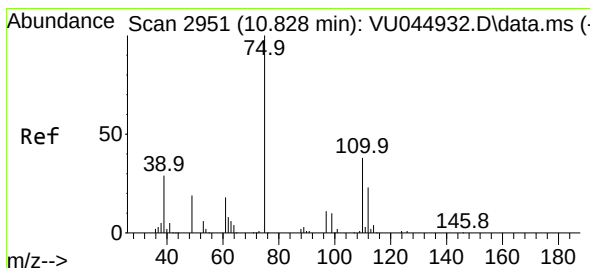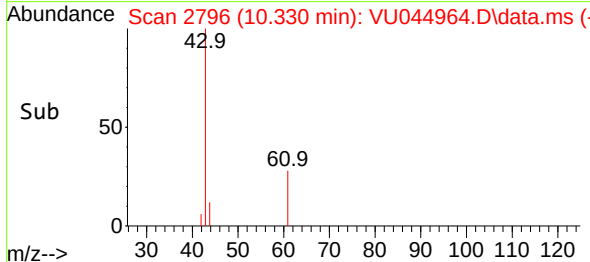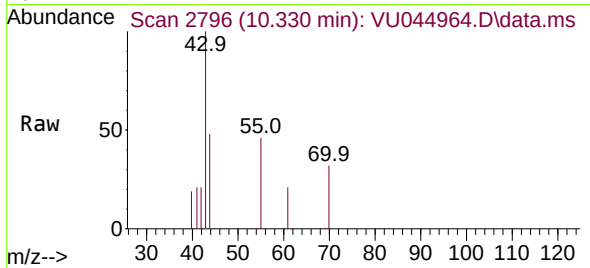

#76
1,2,3-Trichloropropane
Concen: 18.763 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. -0.192 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 75	Resp: 91942
Ion Ratio	Lower Upper
75	100
77	1.1 17.9 53.7#


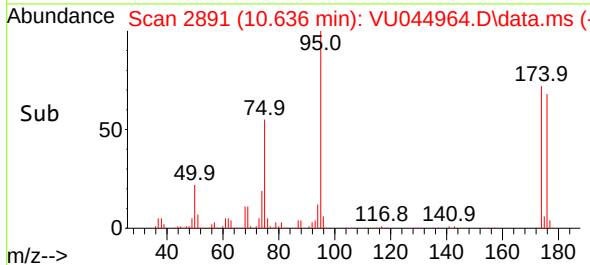

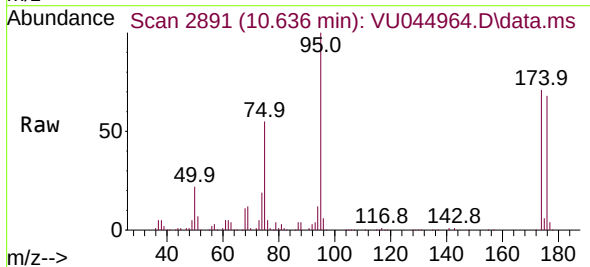


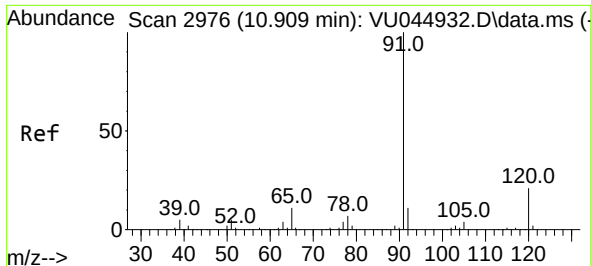

#78
n-propylbenzene
Concen: 9.871 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. -0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion: 91 Resp: 150487
Ion Ratio Lower Upper
91 100
120 21.1 10.8 32.4

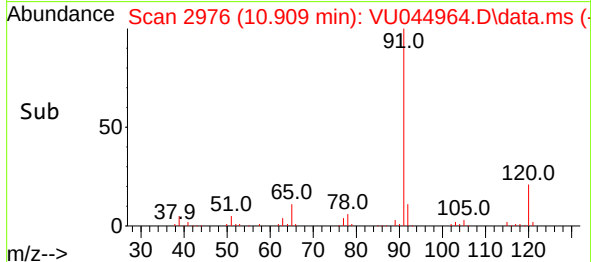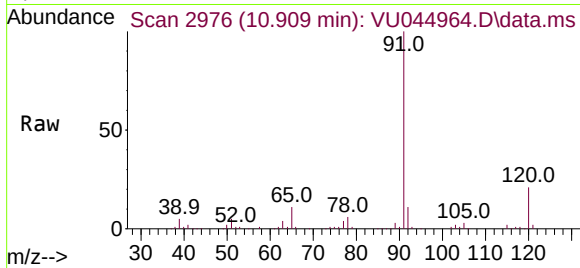

#79
2-Chlorotoluene
Concen: 15.747 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. -0.080 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 91 Resp: 150487
Ion Ratio Lower Upper
91 100
126 0.0 15.7 47.0#


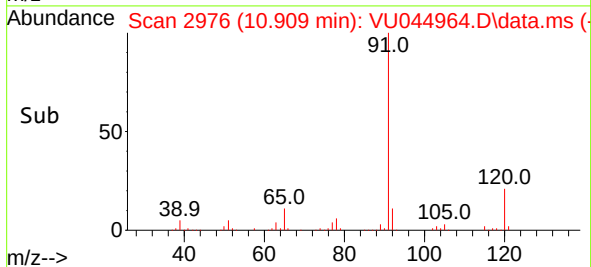

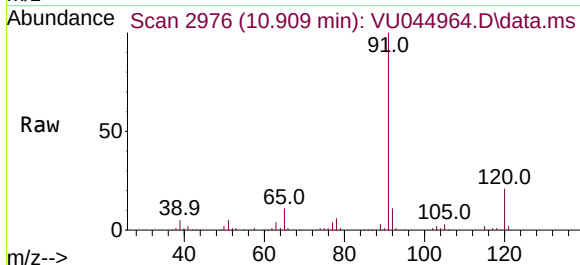


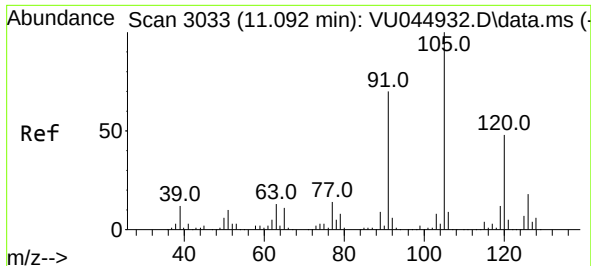

#80
1,3,5-Trimethylbenzene
Concen: 2.566 ug/l
RT: 11.092 min Scan# 3033
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:105 Resp: 28119
Ion Ratio Lower Upper
105 100
120 47.7 24.1 72.2

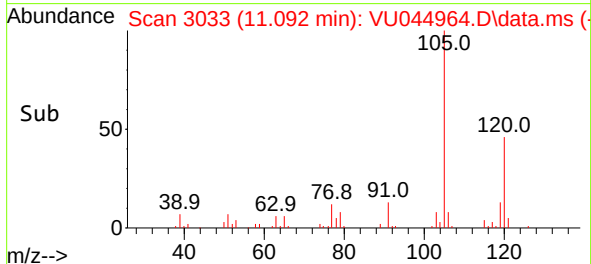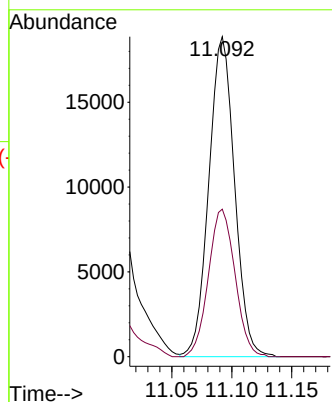

#81
trans-1,4-Dichloro-2-butene
Concen: 52.071 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.084 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 75 Resp: 91942
Ion Ratio Lower Upper
75 100
53 0.0 82.0 123.0#
89 0.0 34.2 51.4#


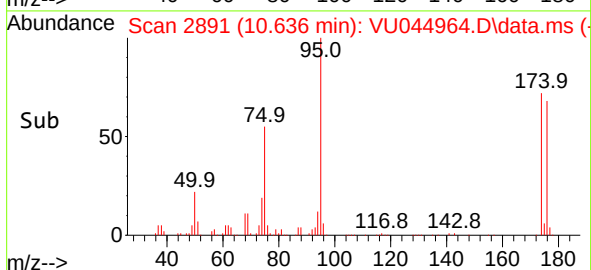

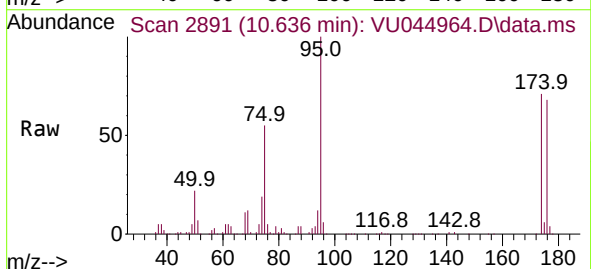


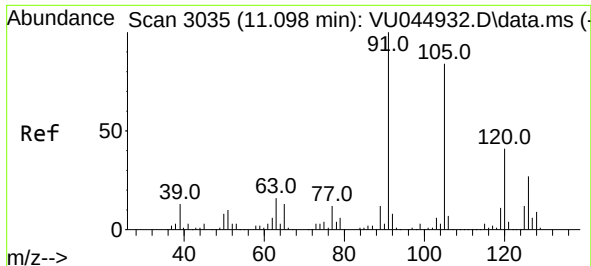

#82
4-Chlorotoluene
Concen: 13.932 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. -0.189 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion: 91 Resp: 150487
Ion Ratio Lower Upper
91 100
126 0.0 13.8 41.4#

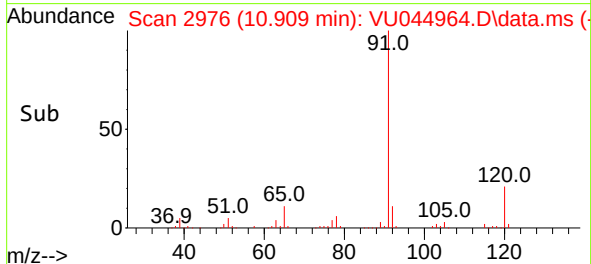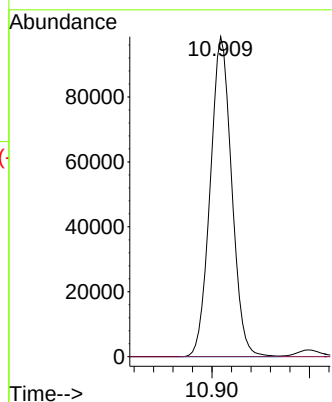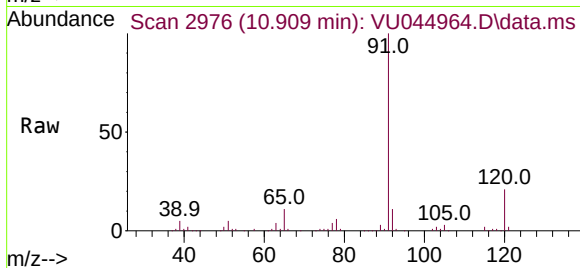

#83
tert-Butylbenzene
Concen: 0.891 ug/l
RT: 11.423 min Scan# 3136
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 119 Resp: 9502
Ion Ratio Lower Upper
119 100
91 69.5 30.4 91.2
134 25.4 11.5 34.5


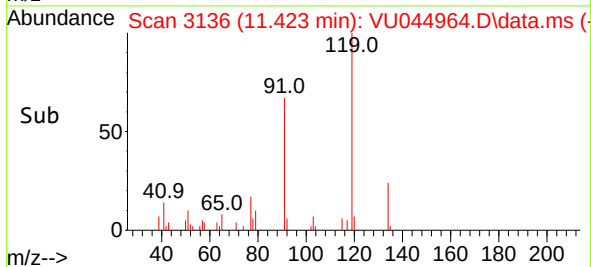

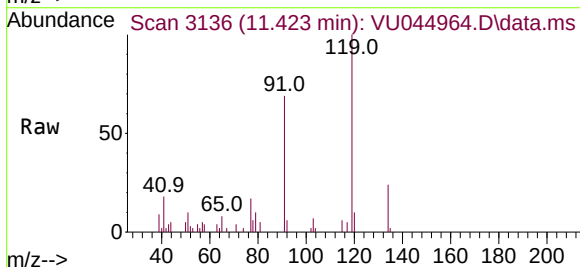


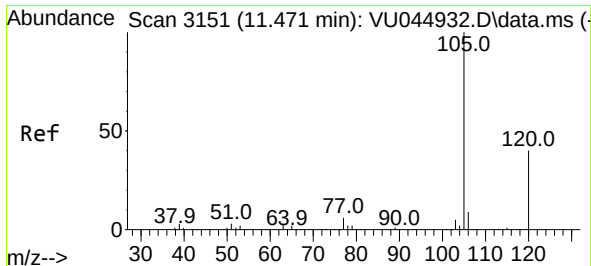

#84
1,2,4-Trimethylbenzene
Concen: 61.326 ug/l
RT: 11.472 min Scan# 3151
Delta R.T. 0.001 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:105 Resp: 664932
Ion Ratio Lower Upper
105 100
120 44.7 22.4 67.3

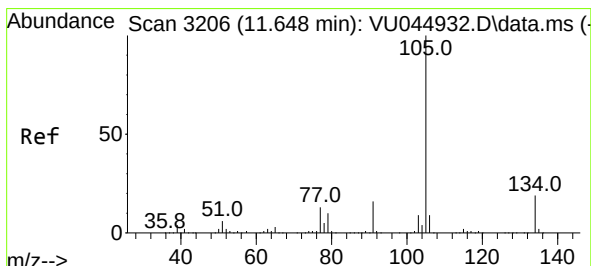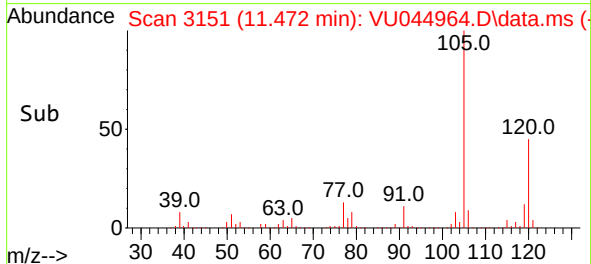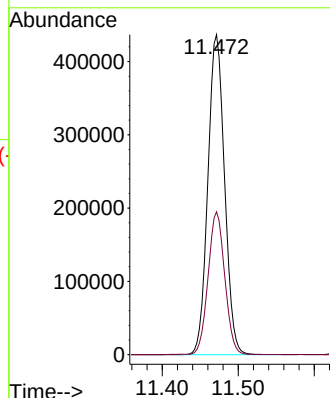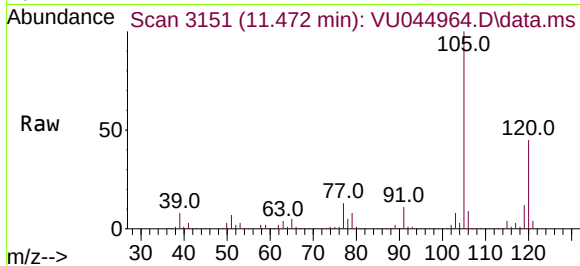

#85
sec-Butylbenzene
Concen: 3.487 ug/l
RT: 11.645 min Scan# 3205
Delta R.T. -0.003 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:105 Resp: 47866
Ion Ratio Lower Upper
105 100
134 18.6 9.3 28.0


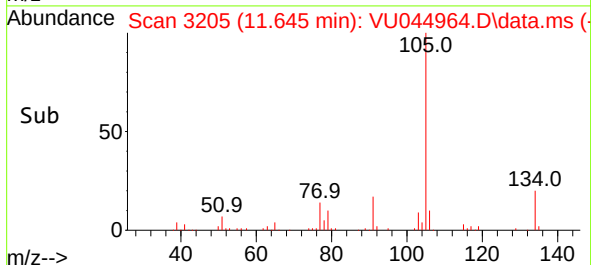

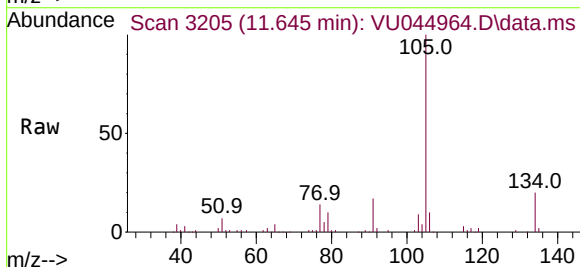


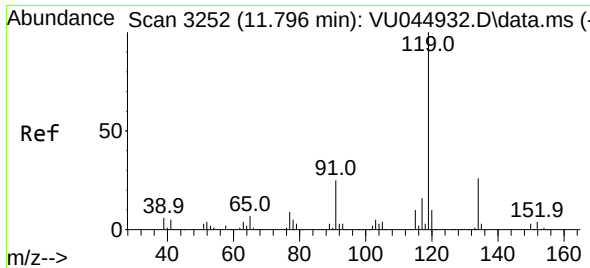

#86
p-Isopropyltoluene
Concen: 1.147 ug/l
RT: 11.748 min Scan# 31
Delta R.T. -0.048 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion: 119 Resp: 12671
Ion Ratio Lower Upper
119 100
134 27.8 12.8 38.3
91 25.4 12.2 36.6

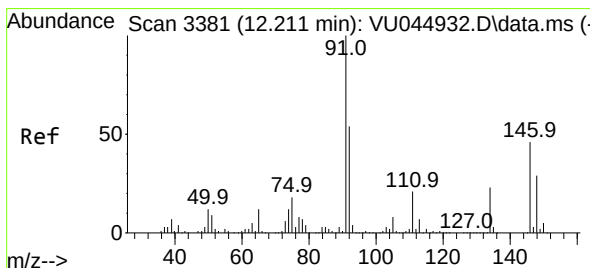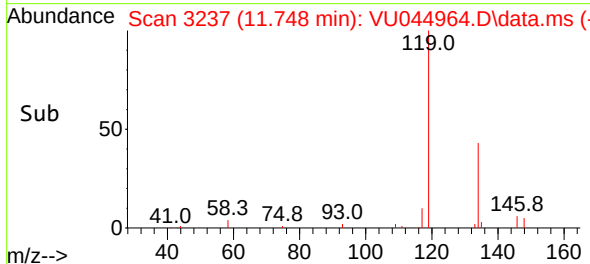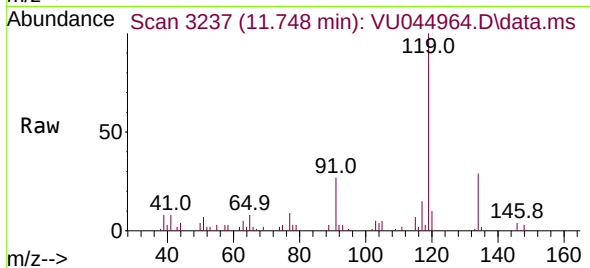

#89
n-Butylbenzene
Concen: 2.476 ug/l
RT: 12.211 min Scan# 3381
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion: 91 Resp: 25184
Ion Ratio Lower Upper
91 100
92 45.4 26.8 80.4
134 43.4 11.8 35.4#


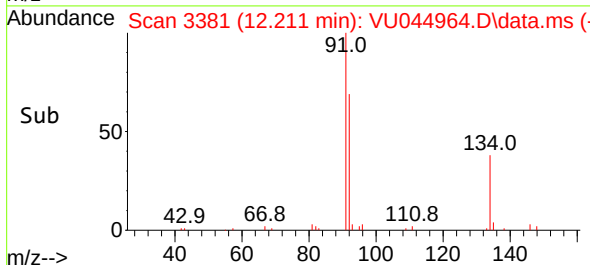
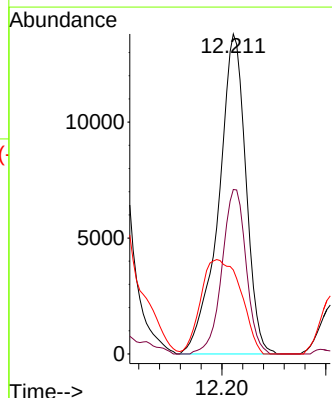
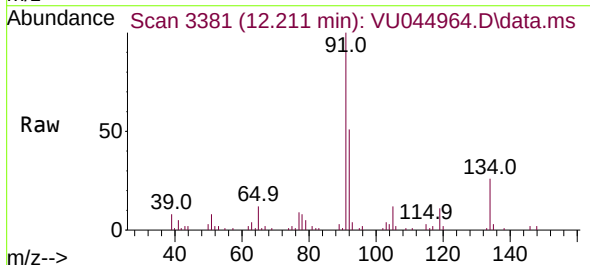




#90
Hexachloroethane
Concen: 1.451 ug/l
RT: 12.468 min Scan# 3464
Delta R.T. -0.010 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58




Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL


Tgt Ion:117 Resp: 2894
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.3#

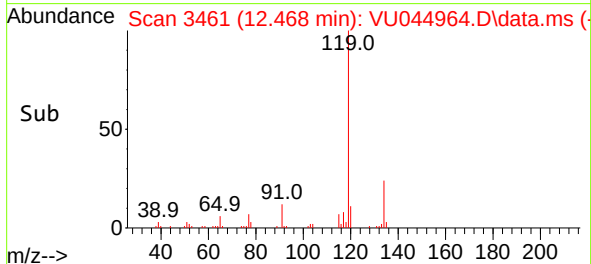

#93
1,2,4-Trichlorobenzene
Concen: 0.281 ug/l
RT: 13.844 min Scan# 3889
Delta R.T. 0.000 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:180 Resp: 926
Ion Ratio Lower Upper
180 100
182 101.3 47.4 142.3
145 82.4 15.4 46.2#


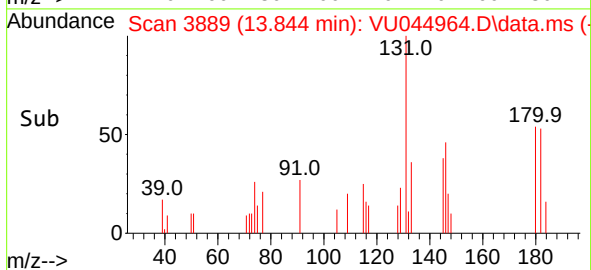

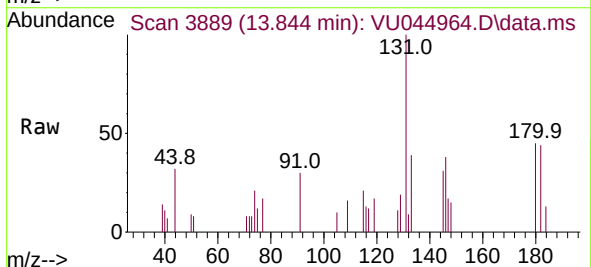


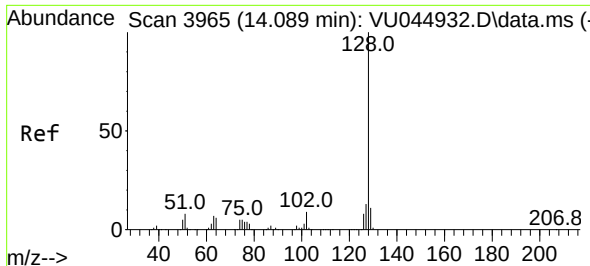

#95
Naphthalene
Concen: 0.709 ug/l
RT: 14.092 min Scan# 3965
Delta R.T. 0.003 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Instrument :
MSVOA_U
ClientSampleId :
EP-1-MW-3R-0921DL

Tgt Ion:128	Resp:	8793
Ion Ratio	Lower	Upper
128	100	
127	12.0	10.4 15.6
129	10.9	8.6 13.0

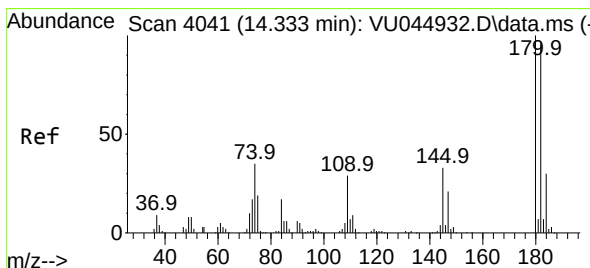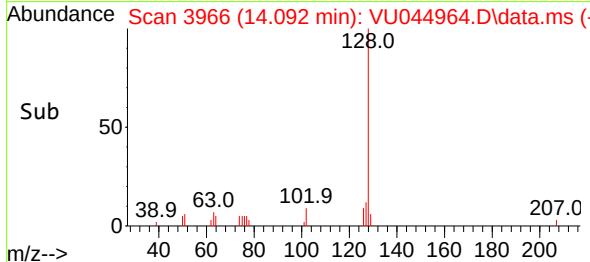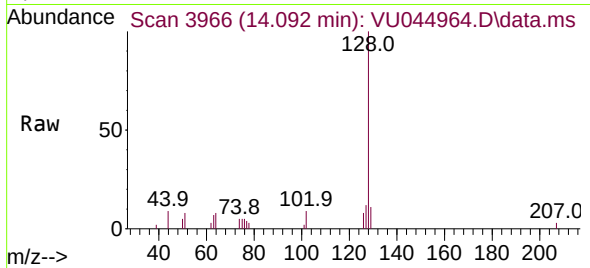

#96
1,2,3-Trichlorobenzene
Concen: 0.280 ug/l
RT: 14.336 min Scan# 4042
Delta R.T. 0.003 min
Lab File: VU044964.D
Acq: 29 Sep 2021 00:58

Tgt Ion:180	Resp:	928
Ion Ratio	Lower	Upper
180	100	
182	87.7	47.1 141.4
145	41.6	16.4 49.2

