



Acrolein

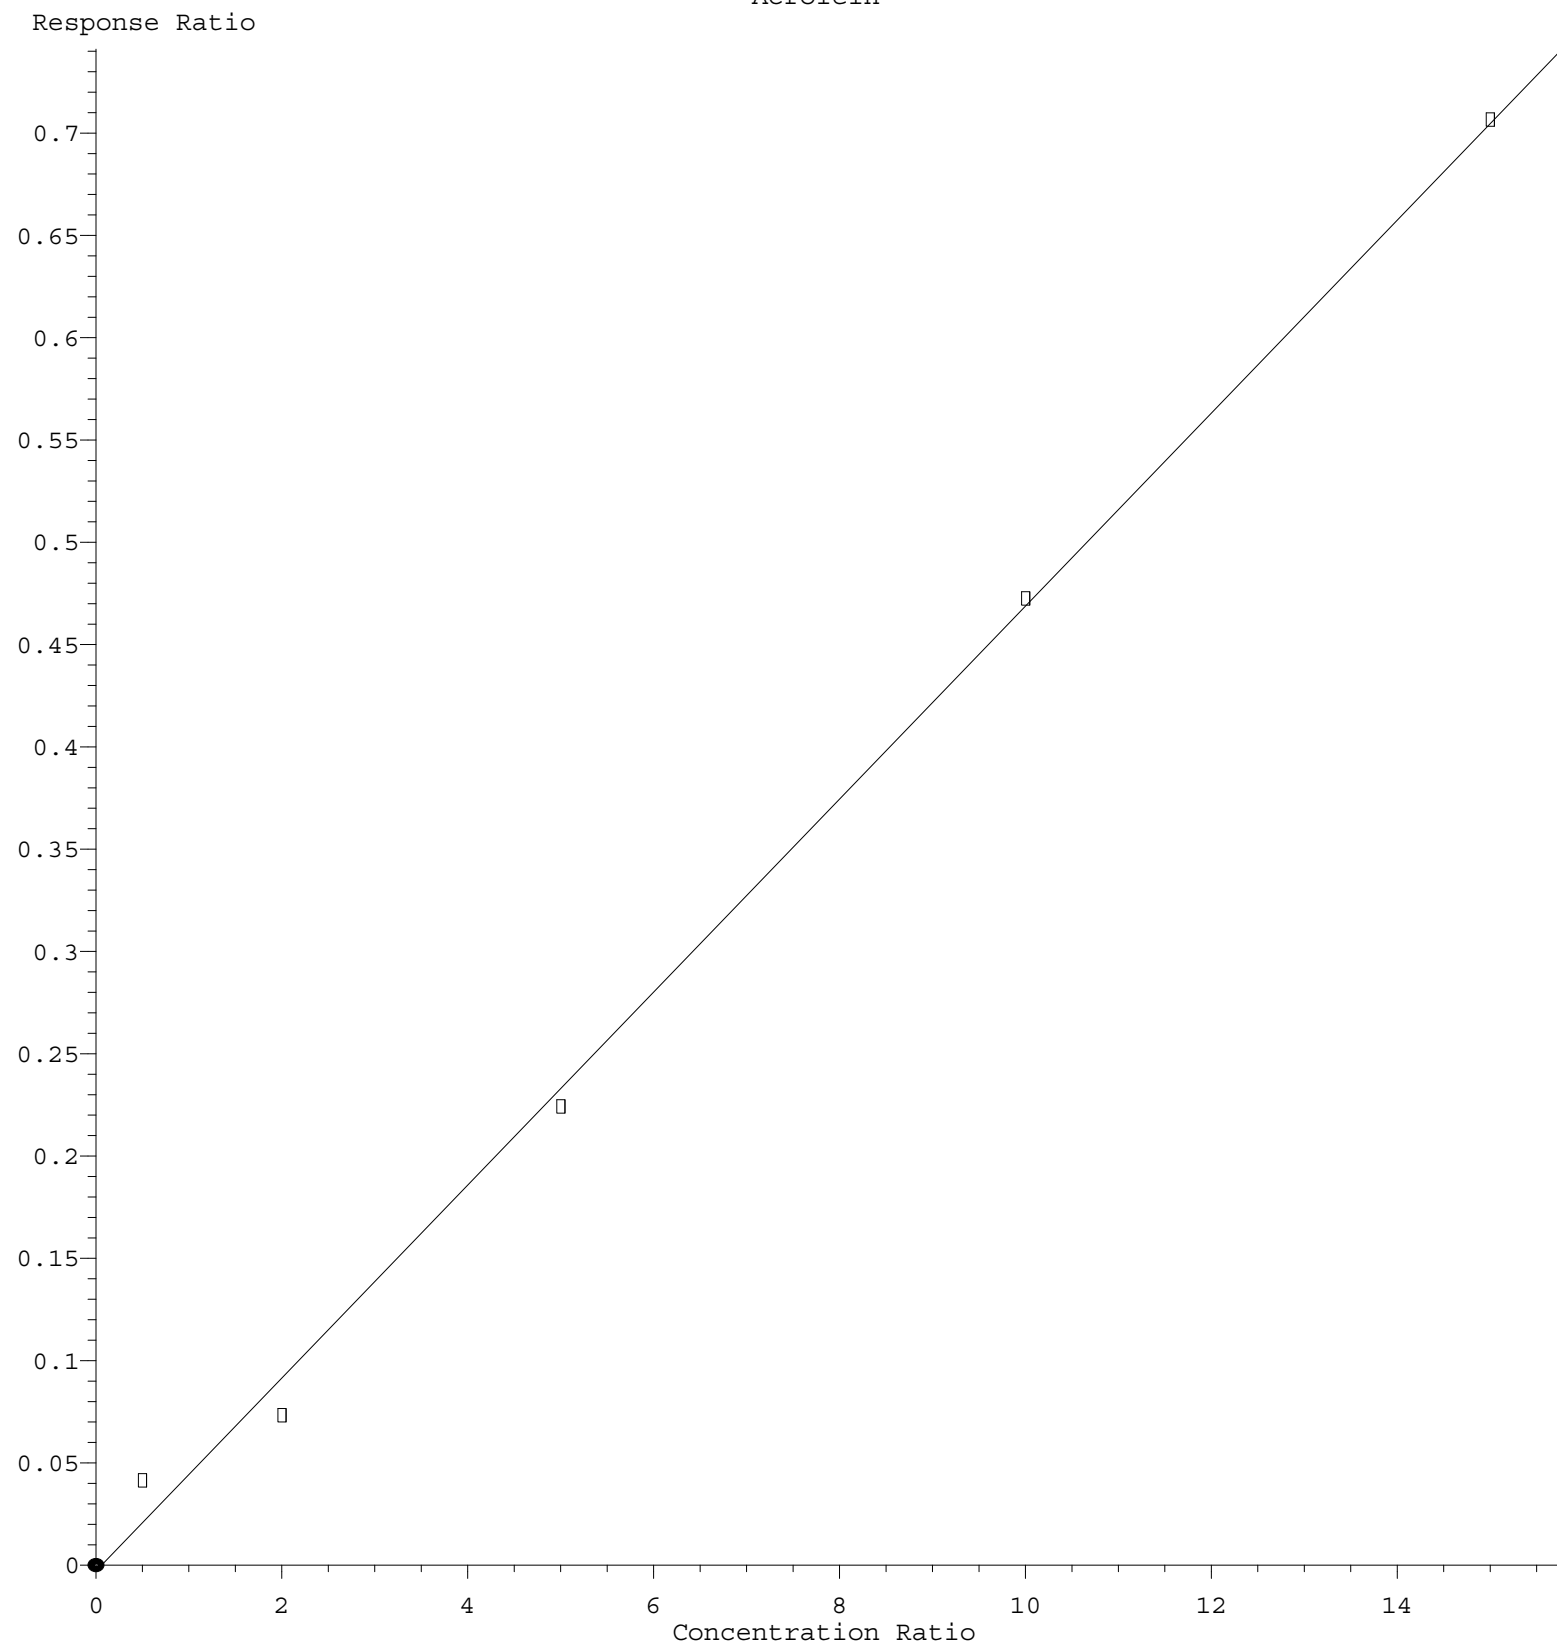

Response = $4.717 \times 10^{-2} \times \text{Amt} - 2.948 \times 10^{-3}$
 Coef of Det (r^2) = 0.997322 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M
 Calibration Table Last Updated: Tue Sep 28 12:32:13 2021


1,4-Dioxane

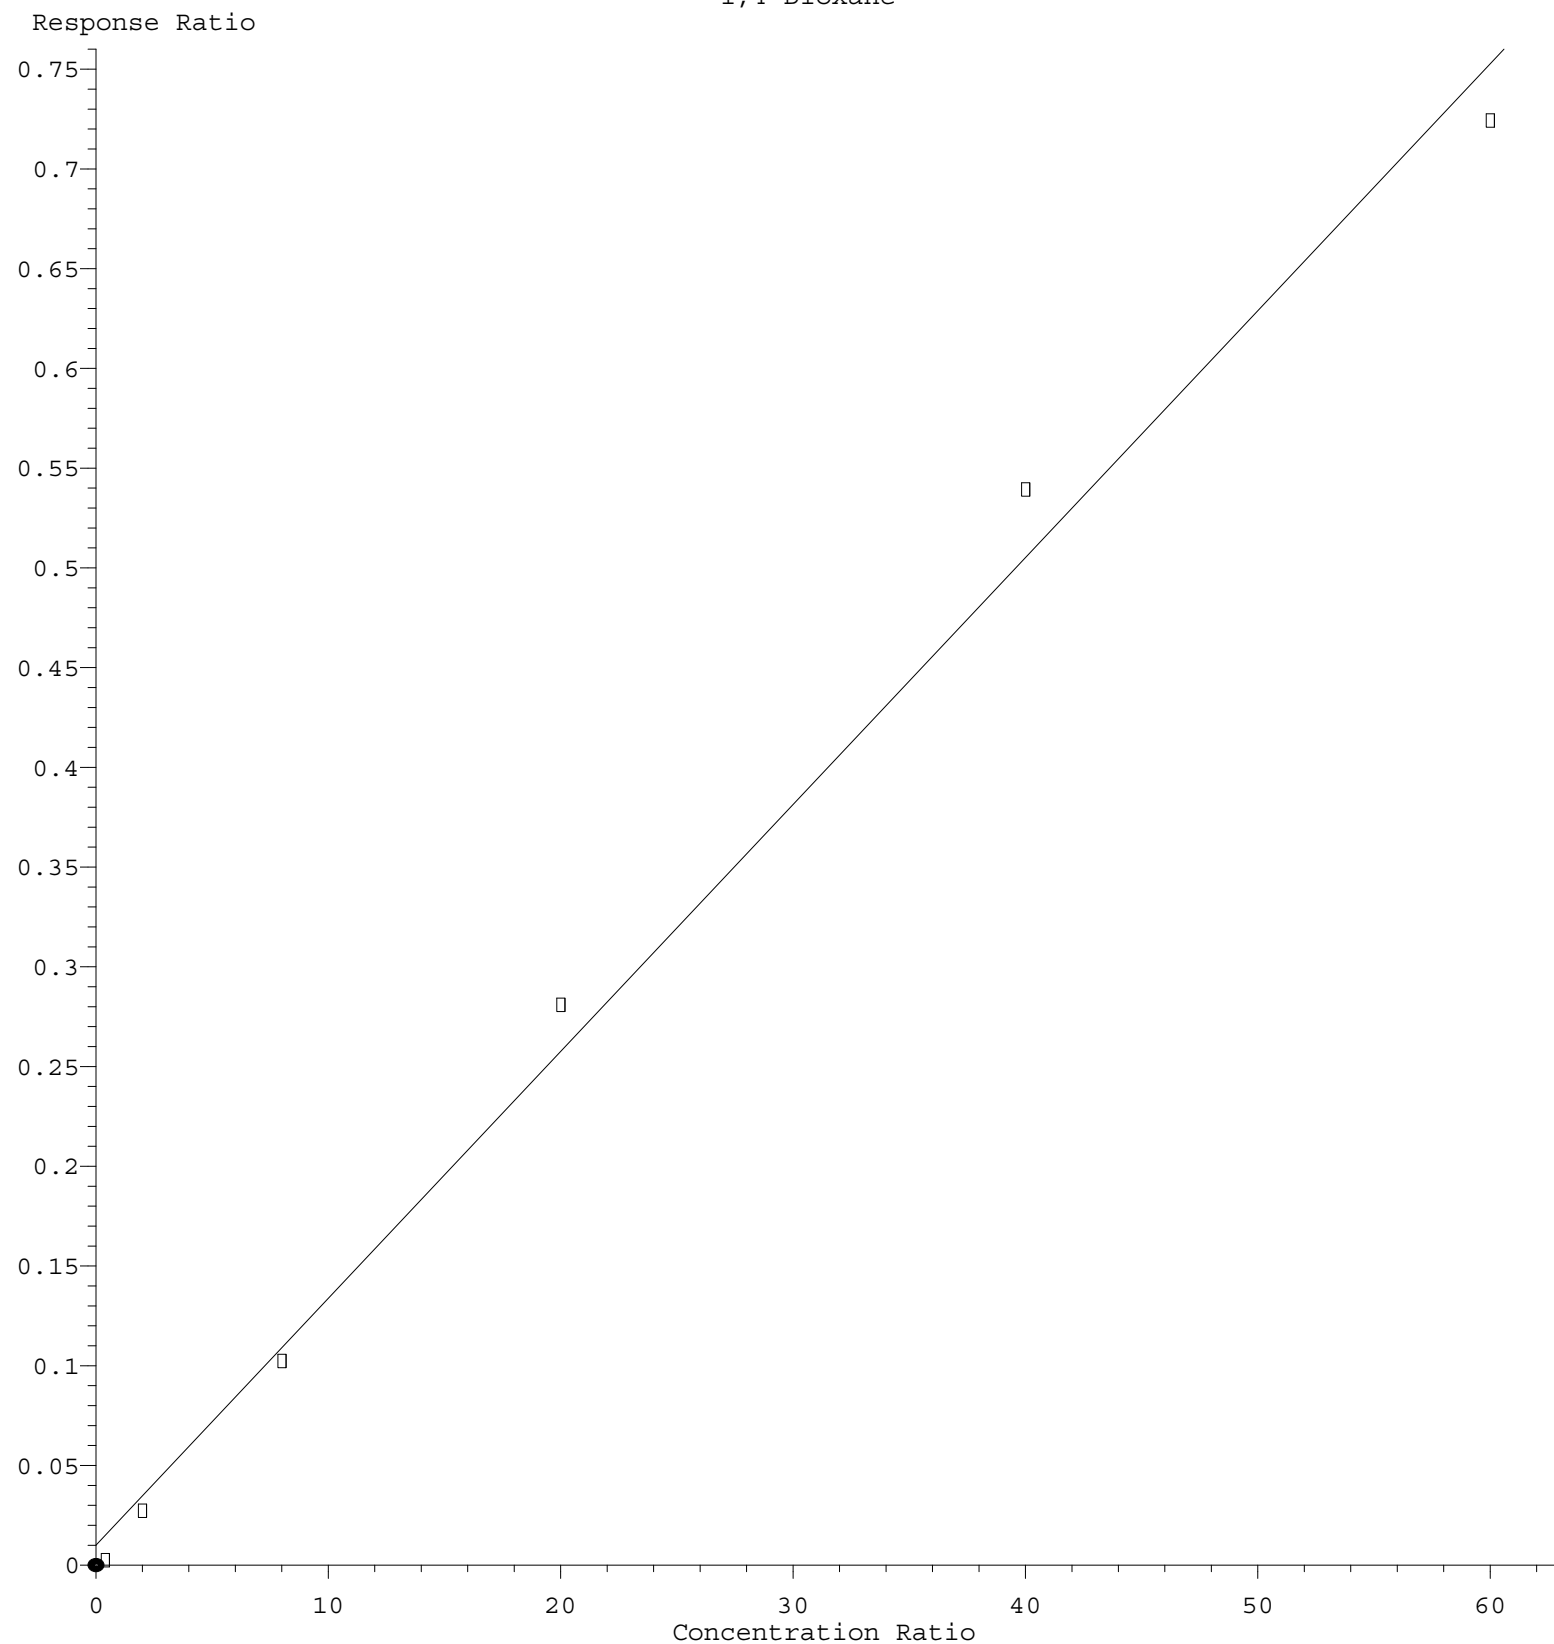

Response = 1.238e-002 * Amt + 1.040e-002
 Coef of Det (r^2) = 0.993651 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M
 Calibration Table Last Updated: Tue Sep 28 12:32:13 2021

Ethyl methacrylate

Response Ratio

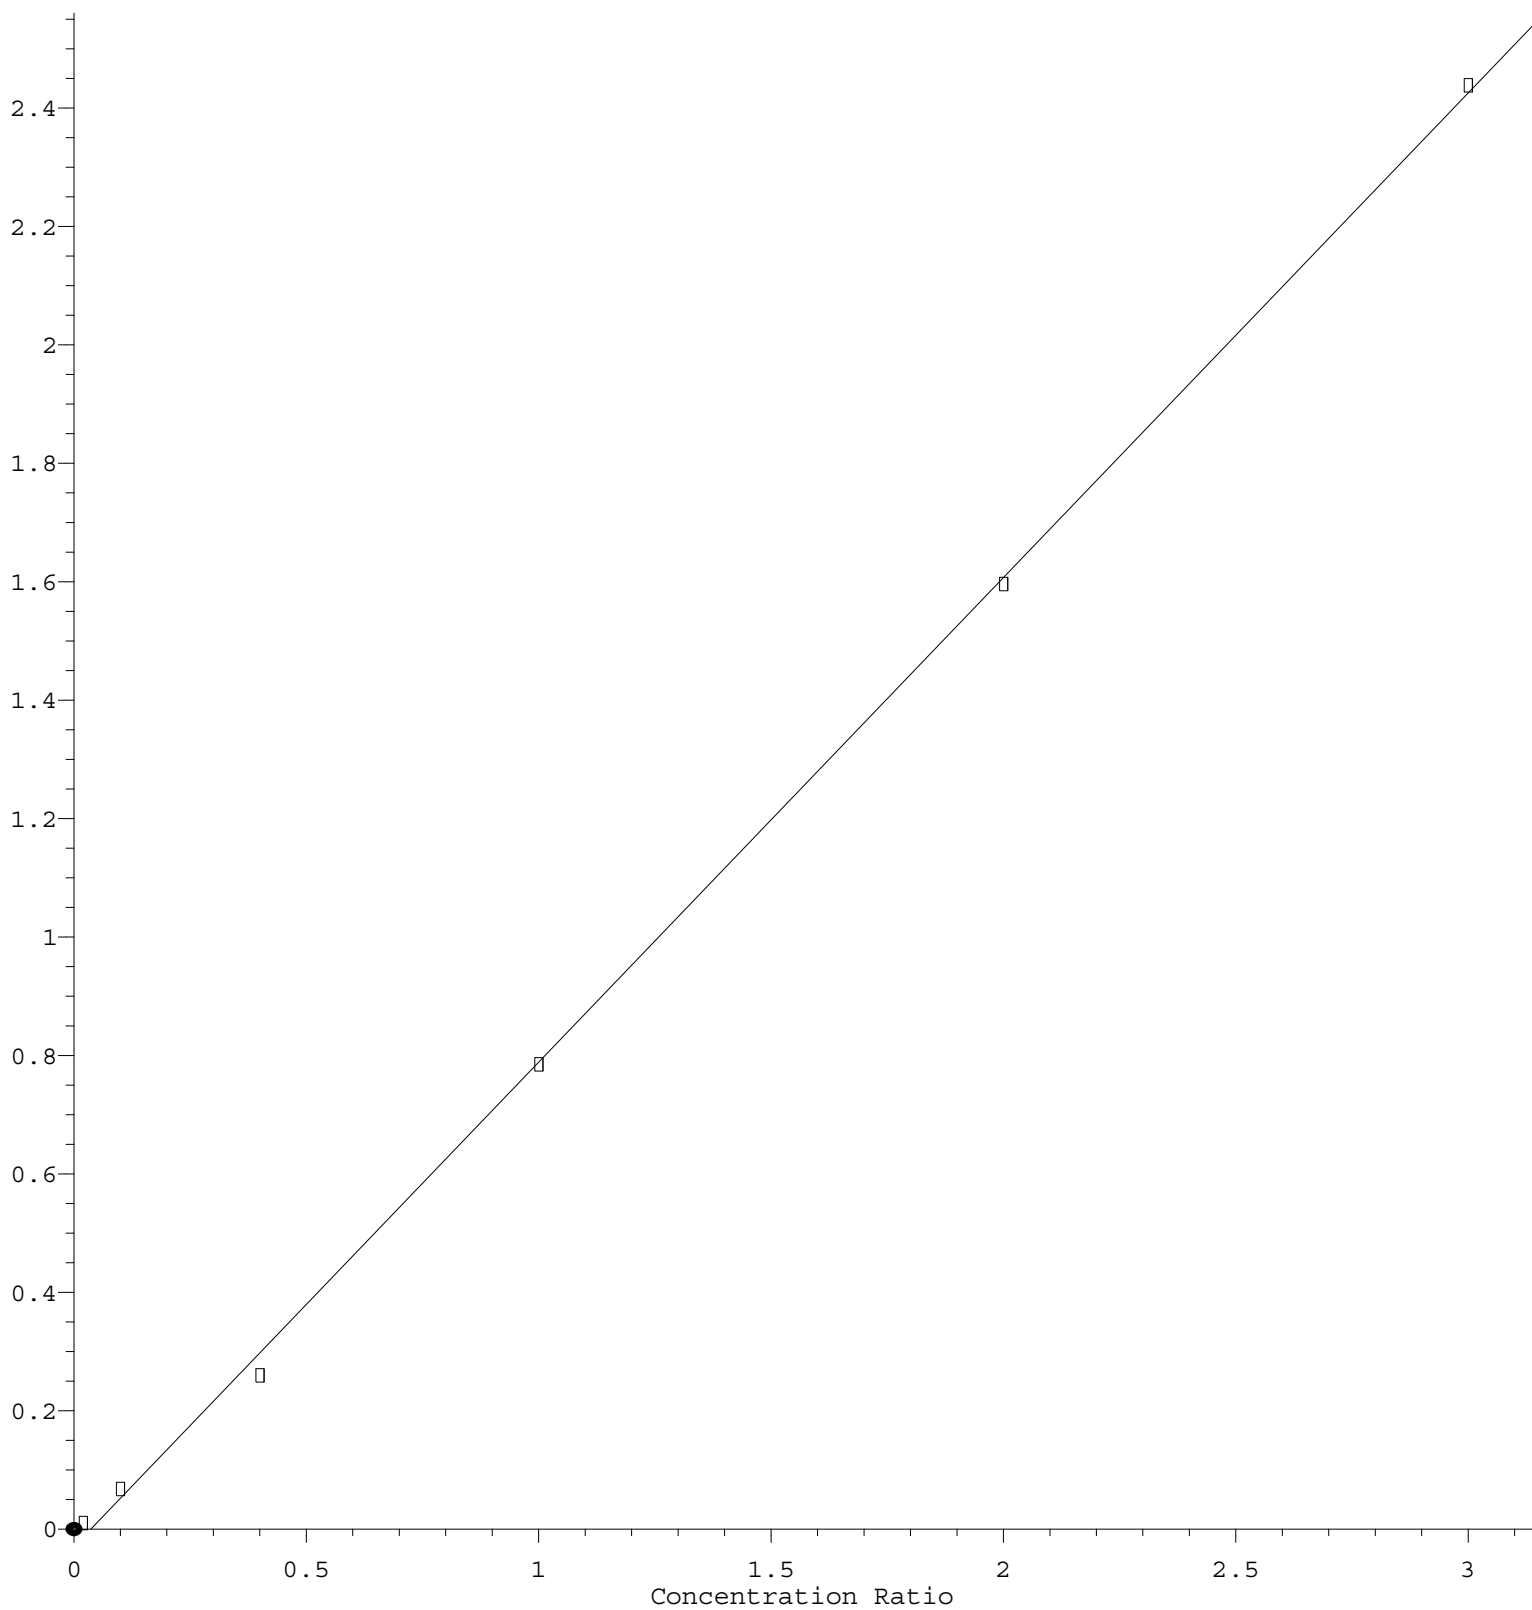

$$\text{Response} = 8.184\text{e-}001 * \text{Amt} - 2.980\text{e-}002$$


Coef of Det (r^2) = 0.999459 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M

Calibration Table Last Updated: Tue Sep 28 12:32:13 2021

2-Chloroethyl Vinyl ether


Response Ratio

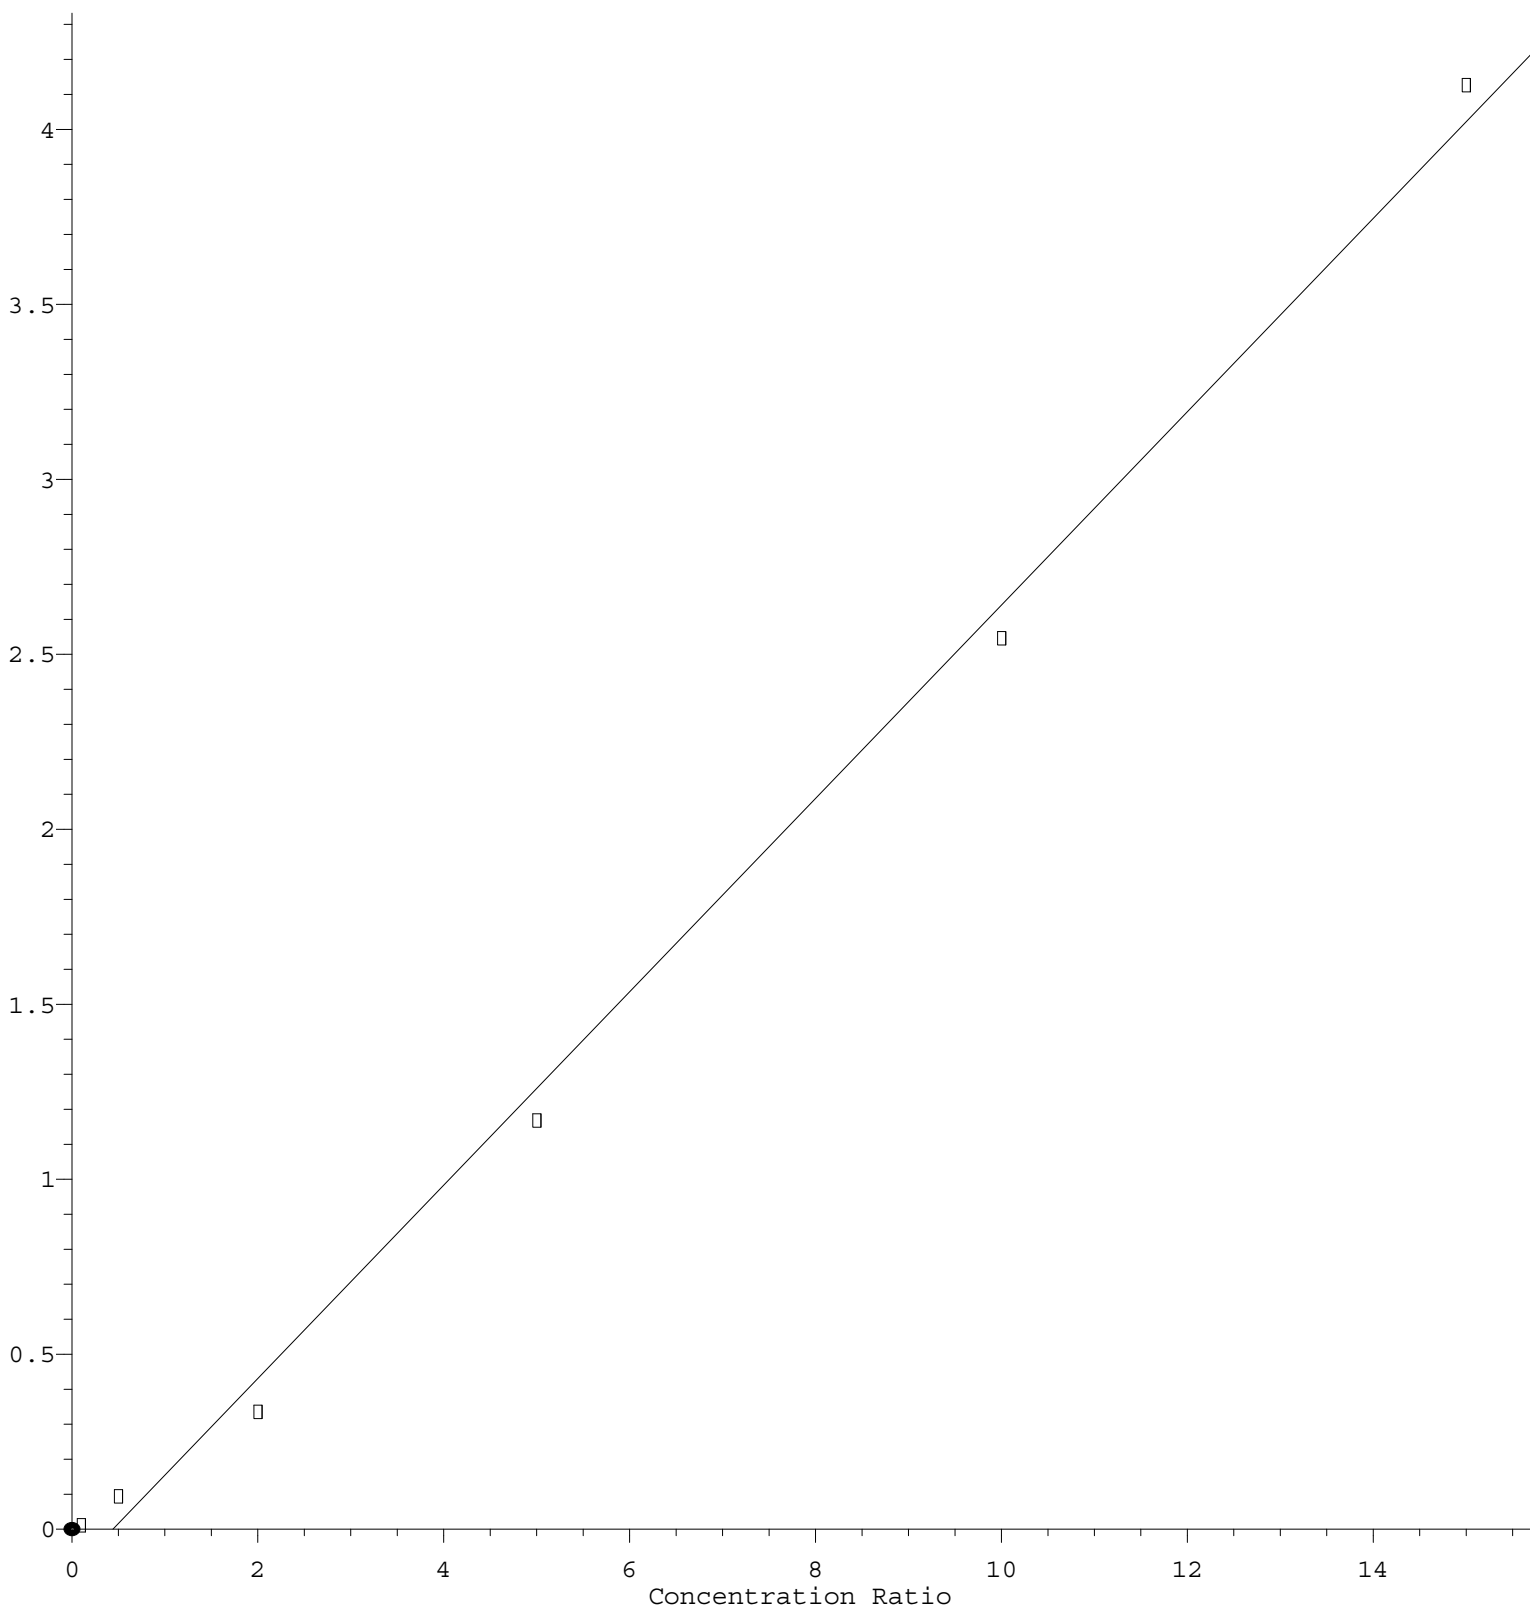

$\text{Response} = 2.762\text{e-}001 * \text{Amt} - 1.208\text{e-}001$
 Coef of Det (r^2) = 0.995980 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M
 Calibration Table Last Updated: Tue Sep 28 12:32:13 2021

Dibromochloromethane

Response Ratio

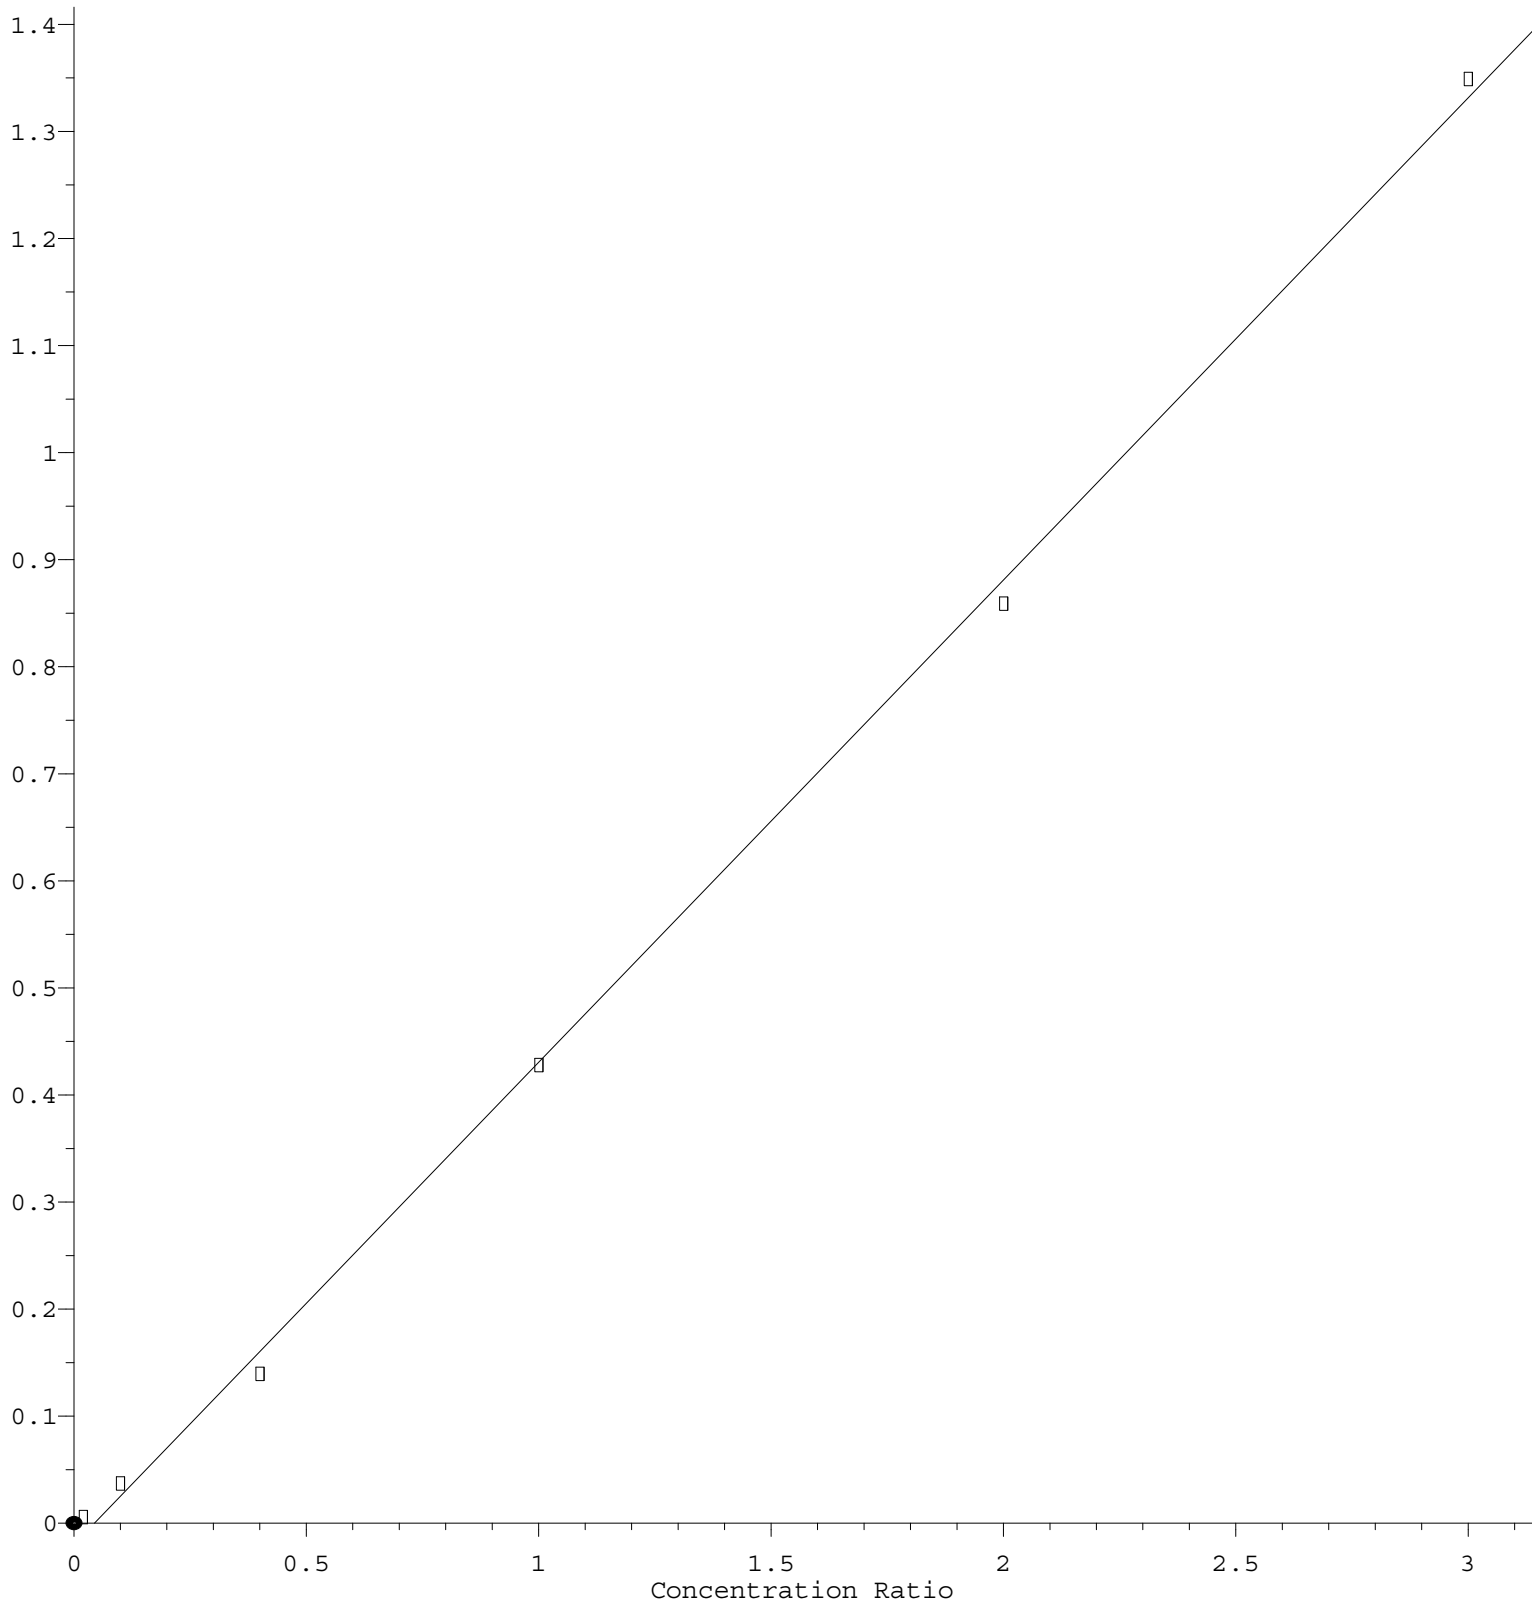

$$\text{Response} = 4.502\text{e-}001 * \text{Amt} - 1.959\text{e-}002$$


Coef of Det (r^2) = 0.998852 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M

Calibration Table Last Updated: Tue Sep 28 12:32:13 2021

Bromoform

Response Ratio

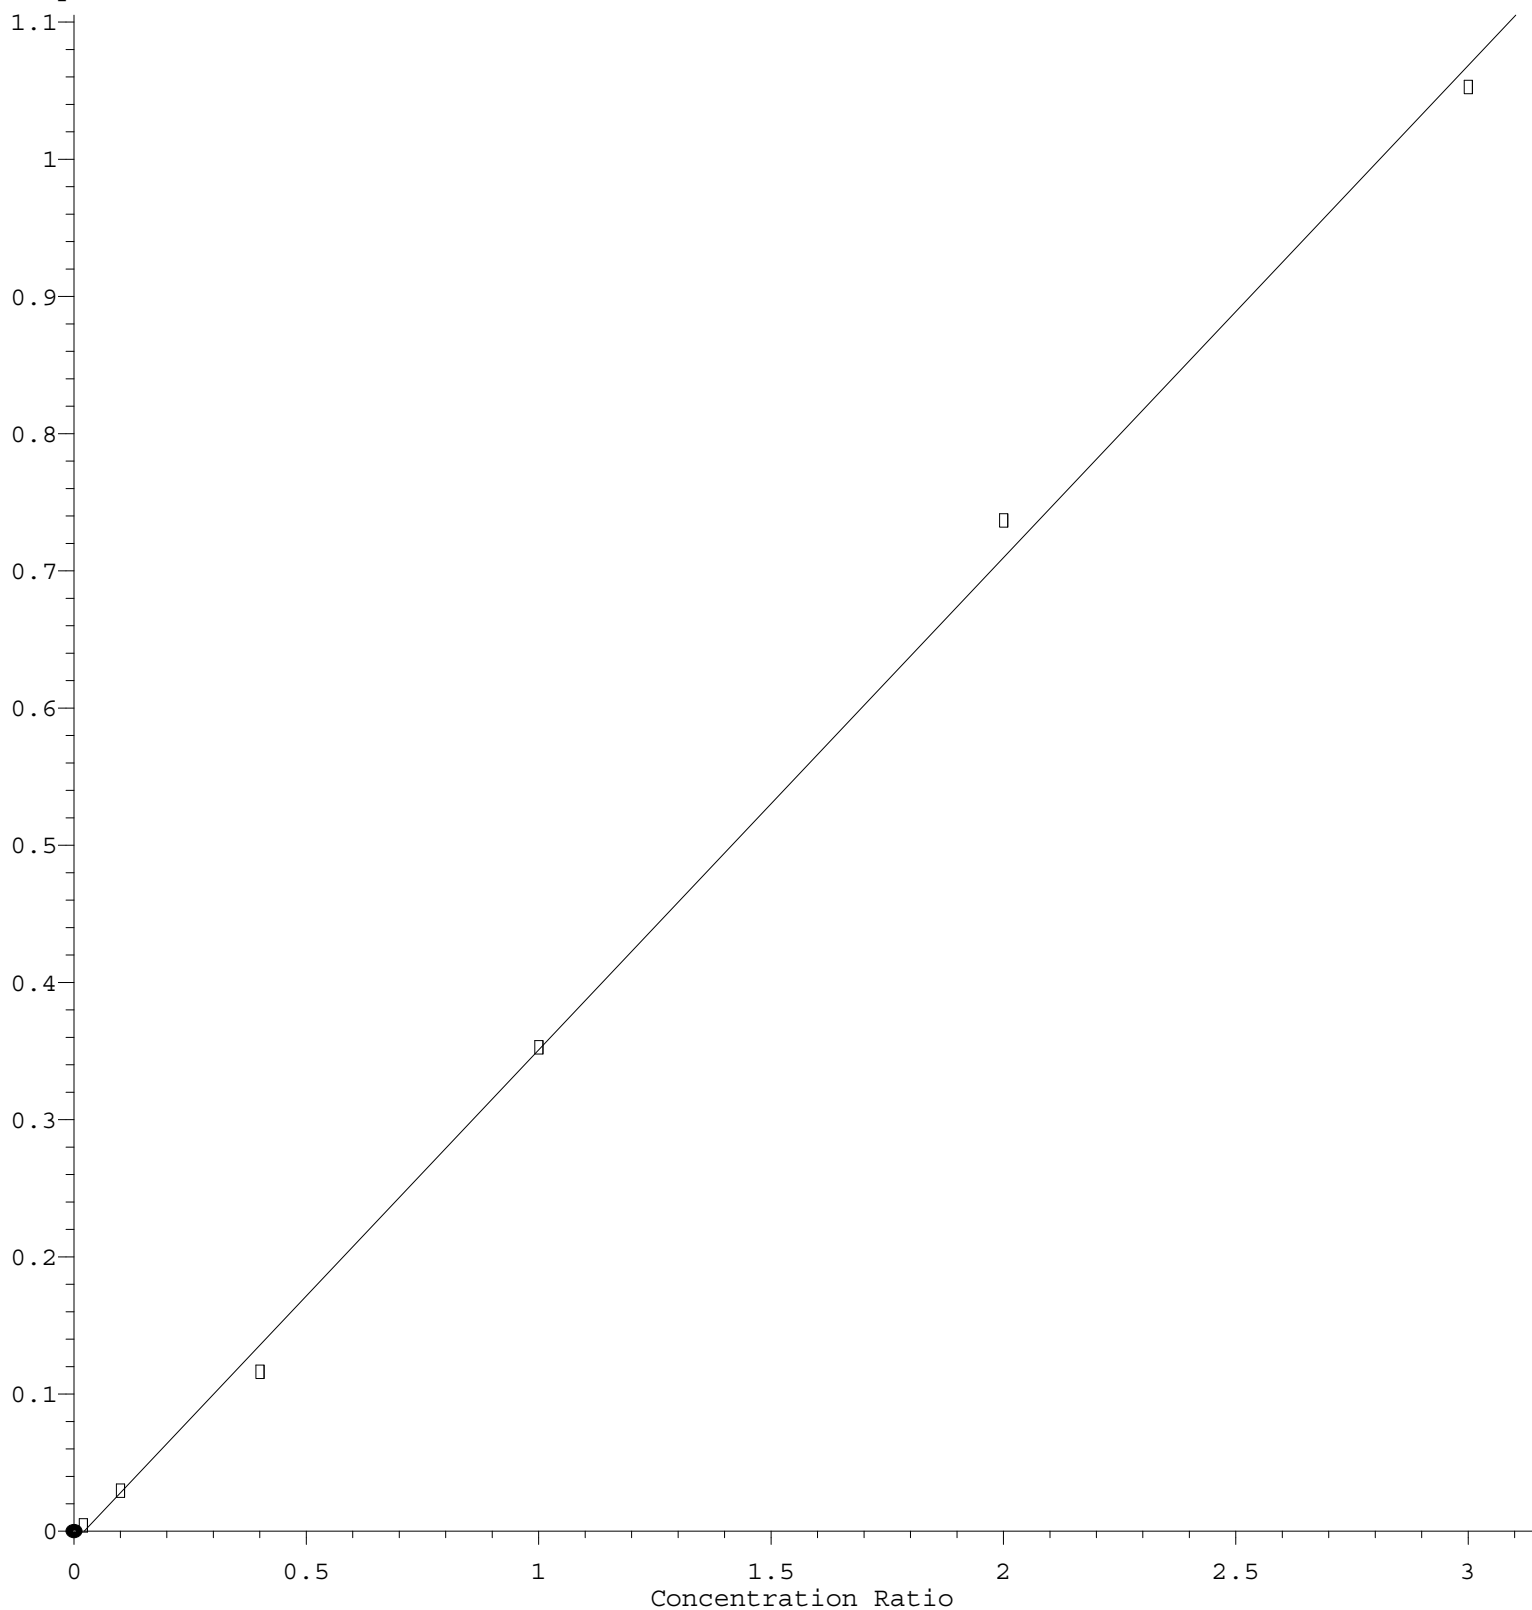

$$\text{Response} = 3.589\text{e-}001 * \text{Amt} - 8.031\text{e-}003$$

Coef of Det (r^2) = 0.998474 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U092821W.M

Calibration Table Last Updated: Tue Sep 28 12:32:13 2021