

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
 Data File : VU044959.D
 Acq On : 28 Sep 2021 23:00
 Operator : SY/MD
 Sample : VU0928WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0928WBL02

Quant Time: Sep 29 05:48:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 28 12:32:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.379	168	192705	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	342182	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	327980	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	162181	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.707	65	157663	49.150	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.300%
35) Dibromofluoromethane	5.295	113	109149	50.565	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.120%
50) Toluene-d8	7.903	98	438913	51.461	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	102.920%
62) 4-Bromofluorobenzene	10.636	95	162132	46.044	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
Data File : VU044959.D
Acq On : 28 Sep 2021 23:00
Operator : SY/MD
Sample : VU0928WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0928WBL02

Quant Time: Sep 29 05:48:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 28 12:32:13 2021
Response via : Initial Calibration




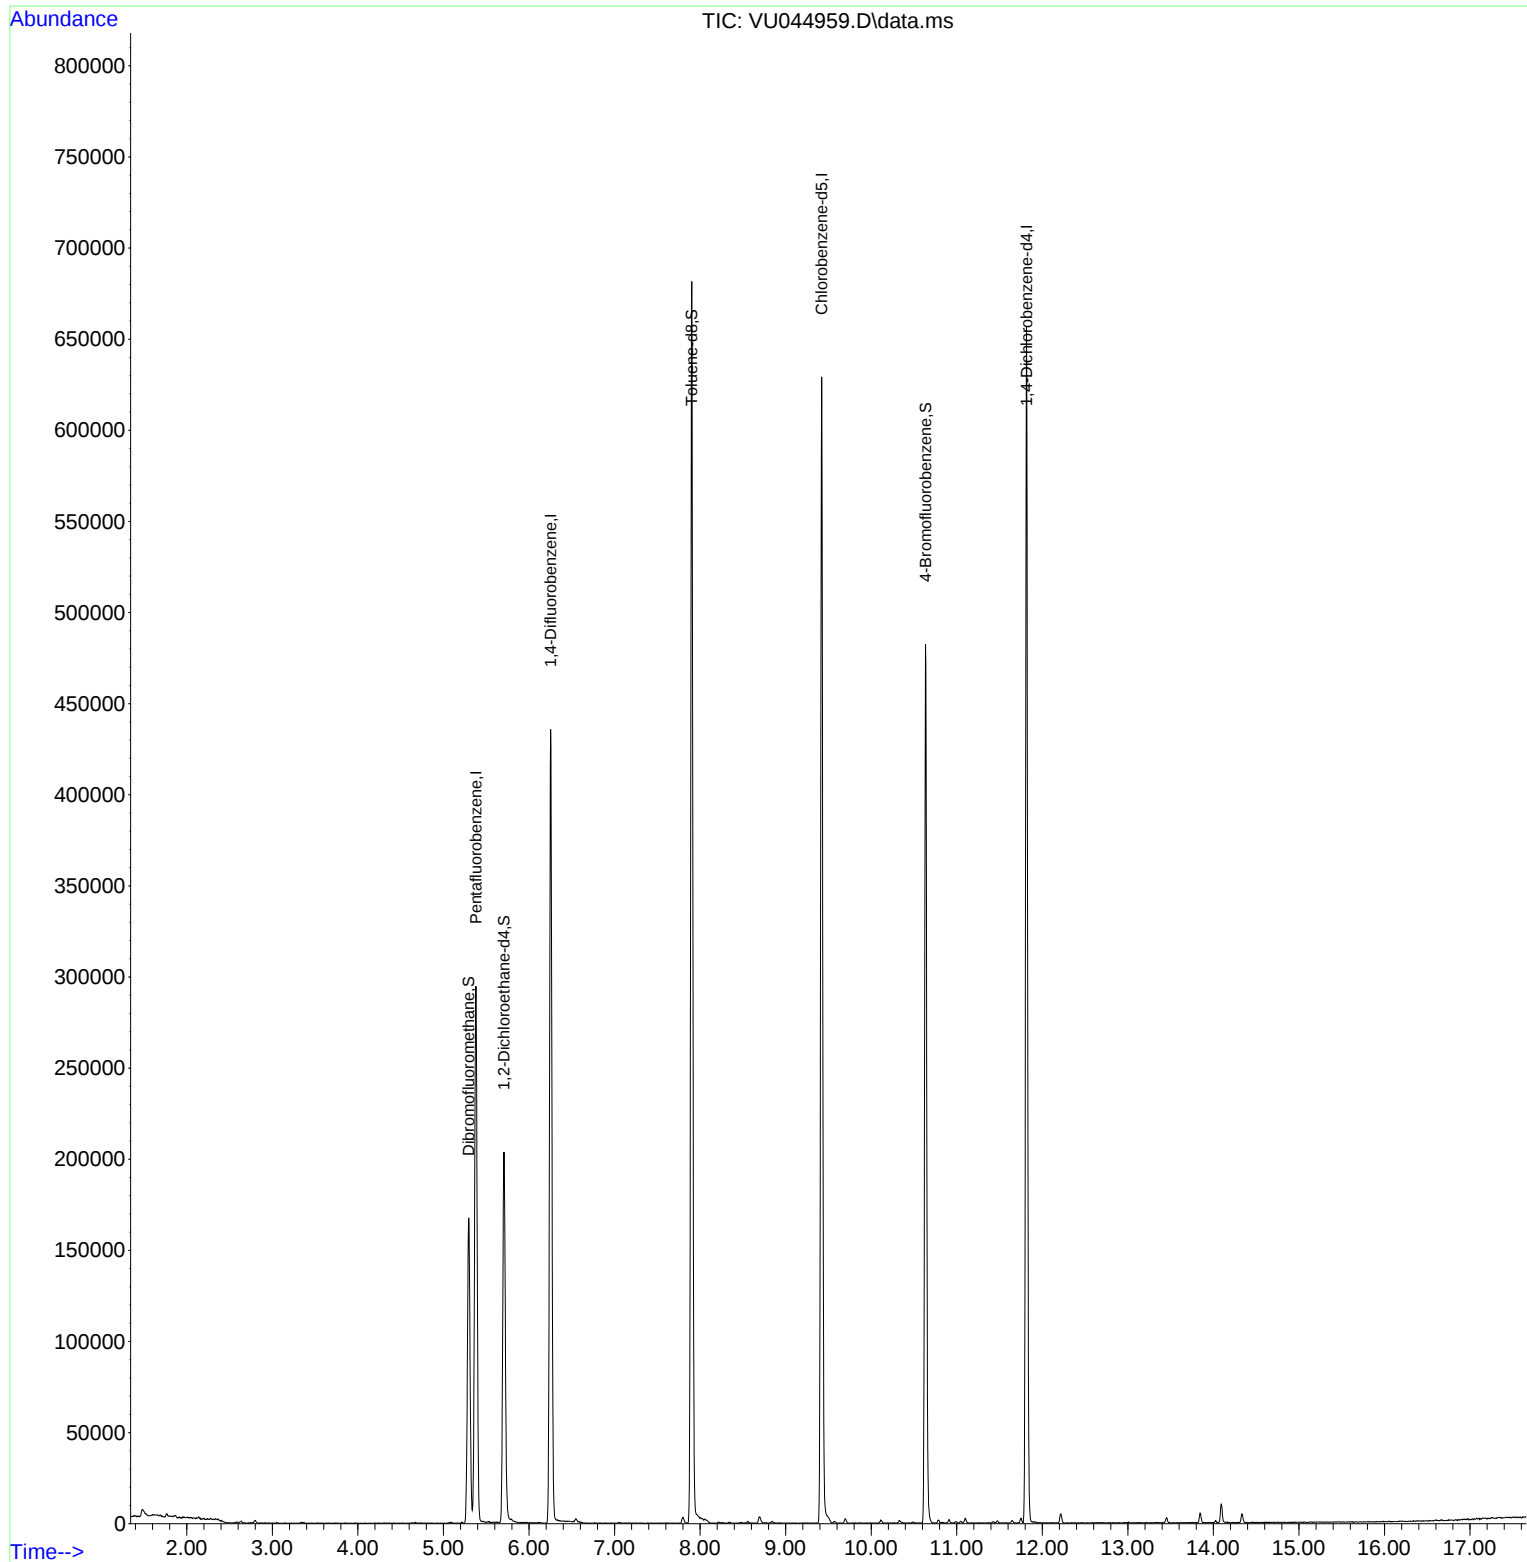


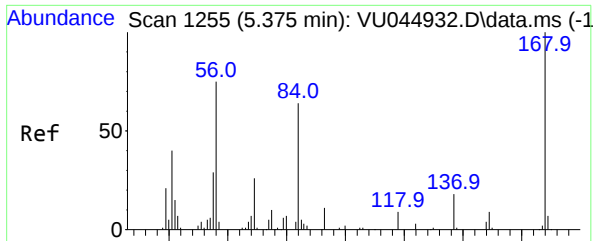

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 11
Delta R.T. 0.004 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00




Instrument :
MSVOA_U
ClientSampleId :
VU0928WBL02


Tgt Ion:168 Resp: 192705
Ion Ratio Lower Upper
168 100
99 65.0 51.4 77.0

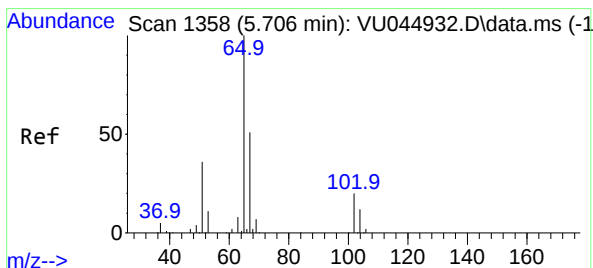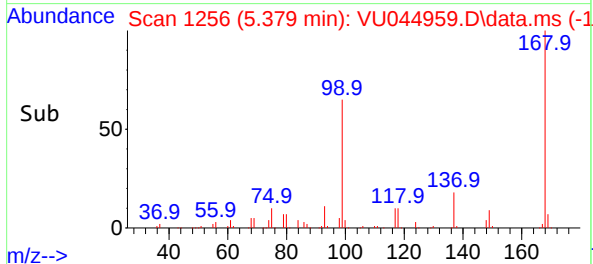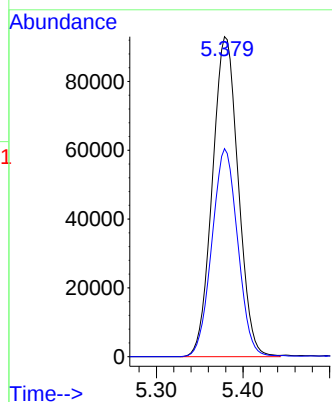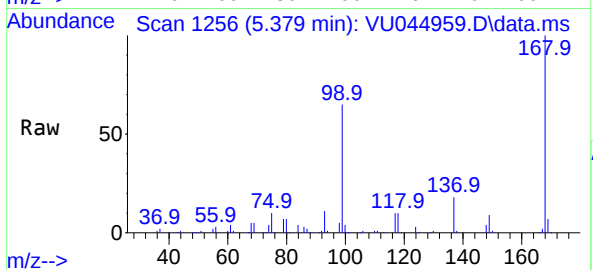

#33
1,2-Dichloroethane-d4
Concen: 49.150 ug/l
RT: 5.707 min Scan# 1358
Delta R.T. 0.000 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00

Tgt Ion: 65 Resp: 157663
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.8


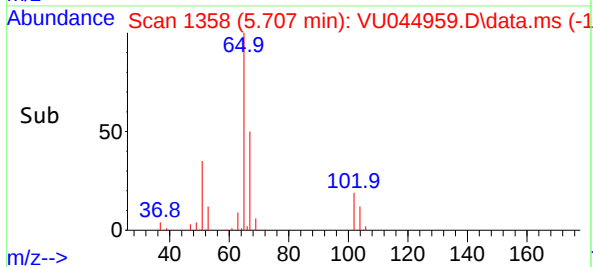
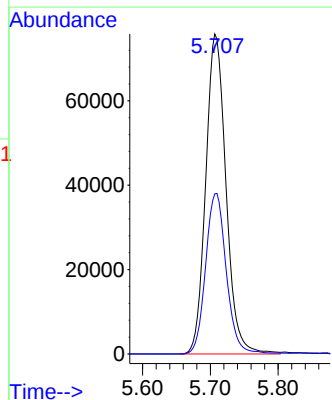
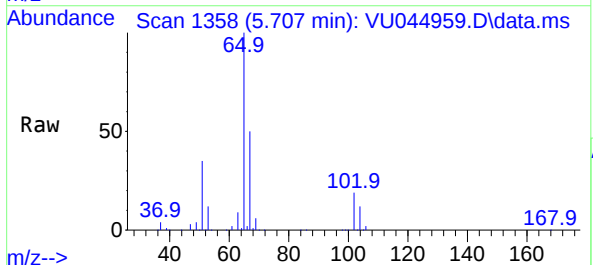


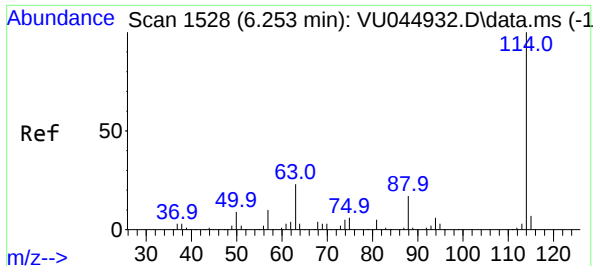

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.253 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00




Instrument :
MSVOA_U
ClientSampleId :
VU0928WBL02


Tgt Ion:114 Resp: 342182
Ion Ratio Lower Upper
114 100
63 22.7 0.0 47.8
88 16.3 0.0 32.8

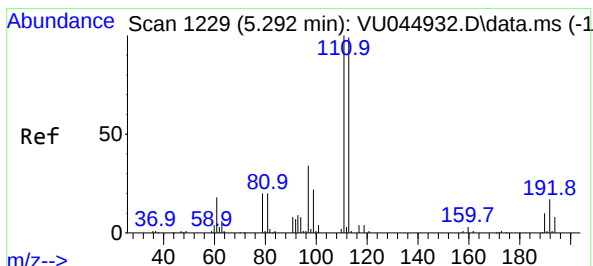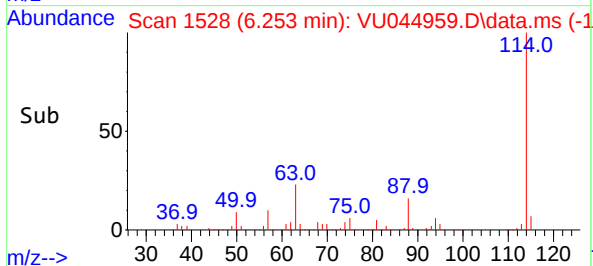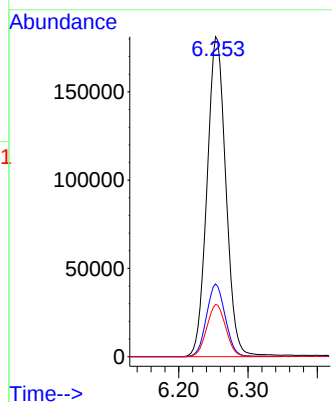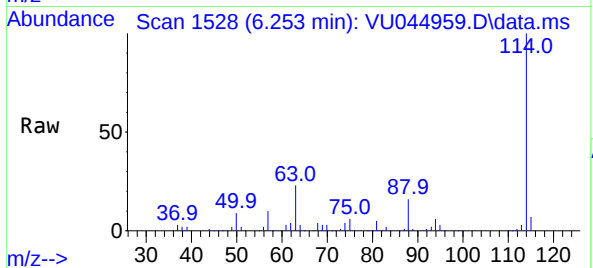

#35
Dibromofluoromethane
Concen: 50.565 ug/l
RT: 5.295 min Scan# 1230
Delta R.T. 0.003 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00

Tgt Ion:113 Resp: 109149
Ion Ratio Lower Upper
113 100
111 103.0 84.1 126.1
192 18.1 14.8 22.2


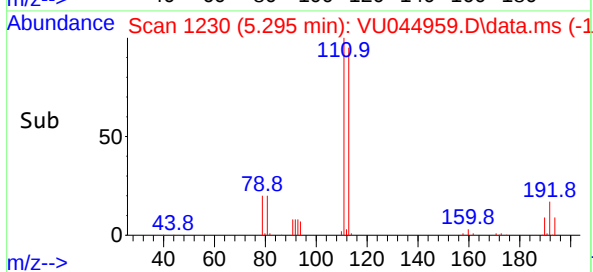
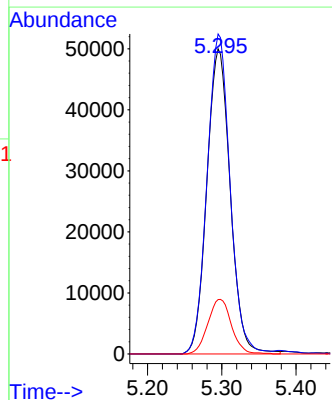
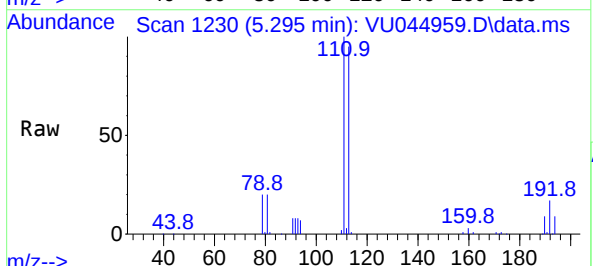


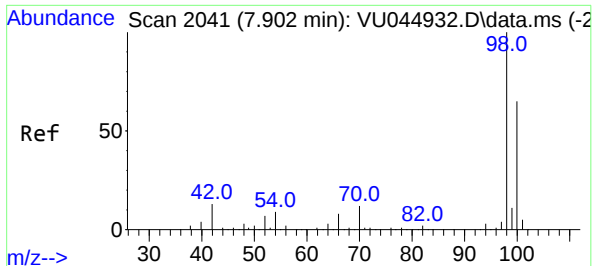

#50
Toluene-d8
Concen: 51.461 ug/l
RT: 7.903 min Scan# 2041
Delta R.T. 0.001 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00




Instrument :
MSVOA_U
ClientSampleId :
VU0928WBL02


Tgt Ion: 98 Resp: 438913
Ion Ratio Lower Upper
98 100
100 64.9 52.5 78.7

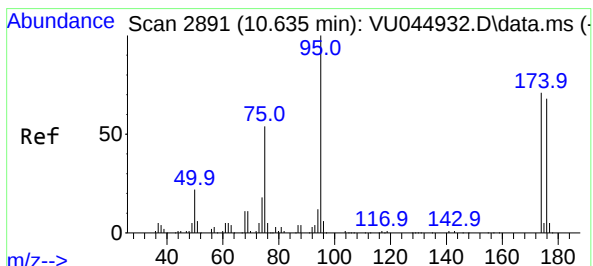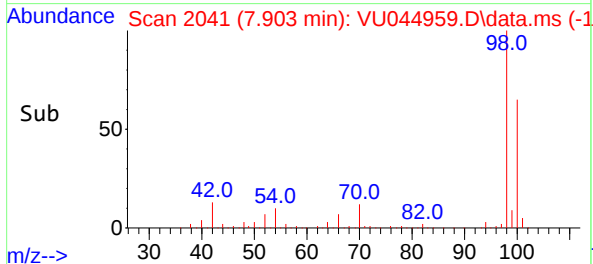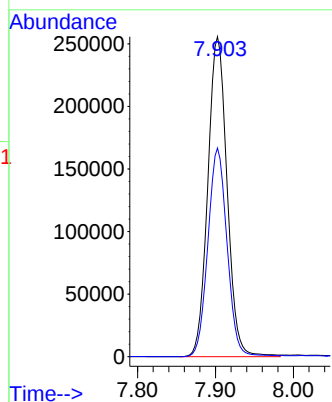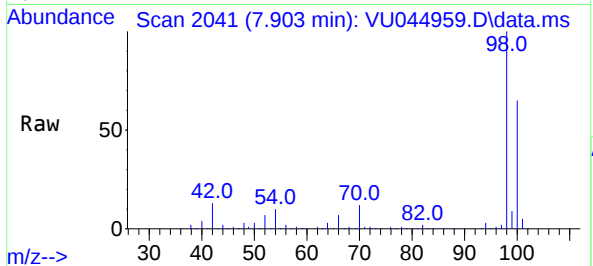

#62
4-Bromofluorobenzene
Concen: 46.044 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.001 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00

Tgt Ion: 95 Resp: 162132
Ion Ratio Lower Upper
95 100
174 72.9 0.0 146.6
176 70.0 0.0 141.2


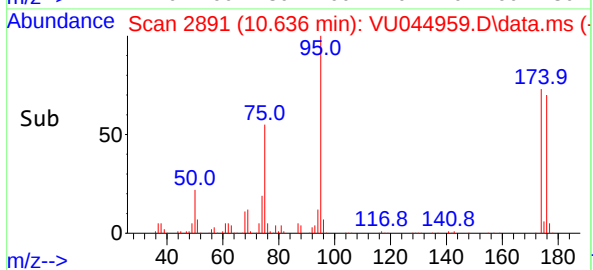
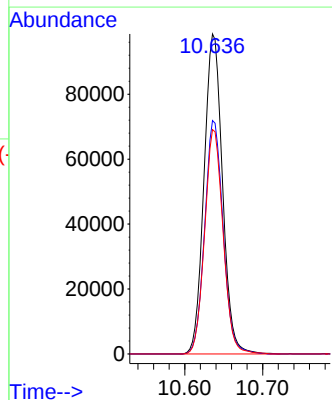
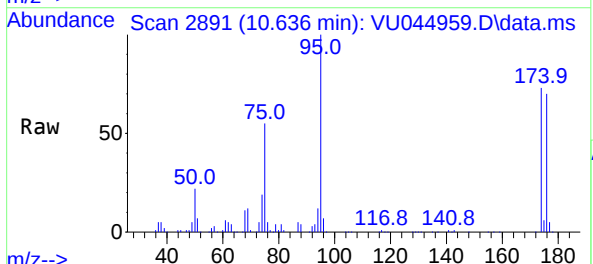


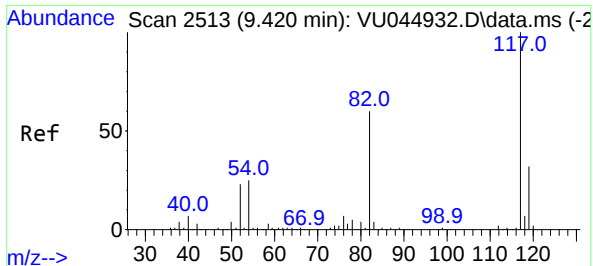

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00

Instrument :
MSVOA_U
ClientSampleId :
VU0928WBL02

Tgt Ion:117 Resp: 327980
Ion Ratio Lower Upper
117 100
82 60.5 47.8 71.8
119 31.6 25.8 38.6

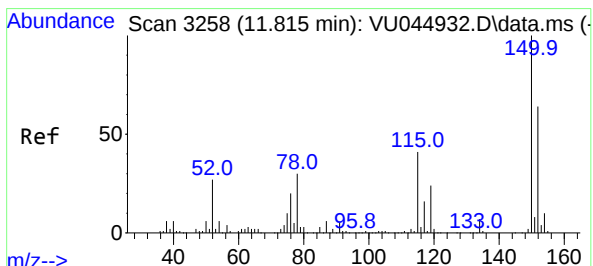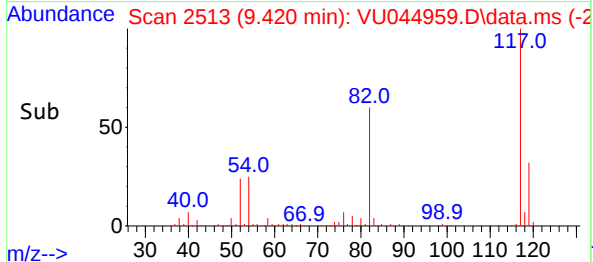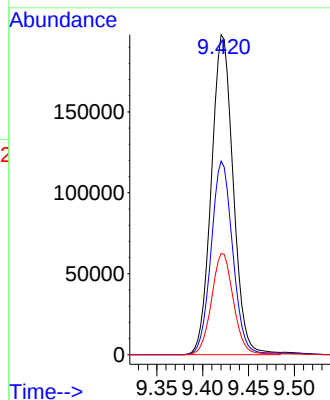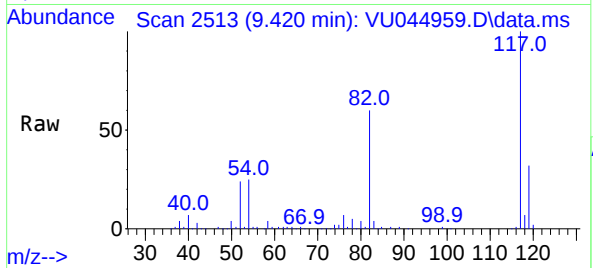

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.816 min Scan# 3258
Delta R.T. 0.001 min
Lab File: VU044959.D
Acq: 28 Sep 2021 23:00

Tgt Ion:152 Resp: 162181
Ion Ratio Lower Upper
152 100
115 60.8 43.5 130.7
150 155.8 0.0 350.0

