

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092821\  
 Data File : VU044973.D  
 Acq On : 29 Sep 2021 04:29  
 Operator : SY/MD  
 Sample : M3952-01  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 48 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 TRIP-BLANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U092821W.M

Title : SW846 8260

Signal : TIC: VU044973.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.478       | 36            | 43          | 54           | rBV      | 29654          | 31579         | 2.74%           | 0.507%        |
| 2         | 5.295       | 1214          | 1230        | 1243         | rBV2     | 167021         | 354855        | 30.75%          | 5.694%        |
| 3         | 5.378       | 1243          | 1256        | 1278         | rVB      | 282654         | 588503        | 50.99%          | 9.443%        |
| 4         | 5.706       | 1343          | 1358        | 1384         | rBV      | 199037         | 421238        | 36.50%          | 6.759%        |
| 5         | 6.253       | 1513          | 1528        | 1551         | rBV      | 421493         | 811518        | 70.31%          | 13.022%       |
| 6         | 7.902       | 2026          | 2041        | 2063         | rBV      | 672729         | 1154120       | 100.00%         | 18.519%       |
| 7         | 9.420       | 2499          | 2513        | 2554         | rBV      | 618712         | 1038851       | 90.01%          | 16.670%       |
| 8         | 10.635      | 2878          | 2891        | 2916         | rBV      | 476198         | 782510        | 67.80%          | 12.556%       |
| 9         | 11.816      | 3243          | 3258        | 3280         | rBV      | 652707         | 1048792       | 90.87%          | 16.829%       |




Sum of corrected areas: 6231966

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092821\  
Data File : VU044973.D  
Acq On : 29 Sep 2021 04:29  
Operator : SY/MD  
Sample : M3952-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 48 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U092821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

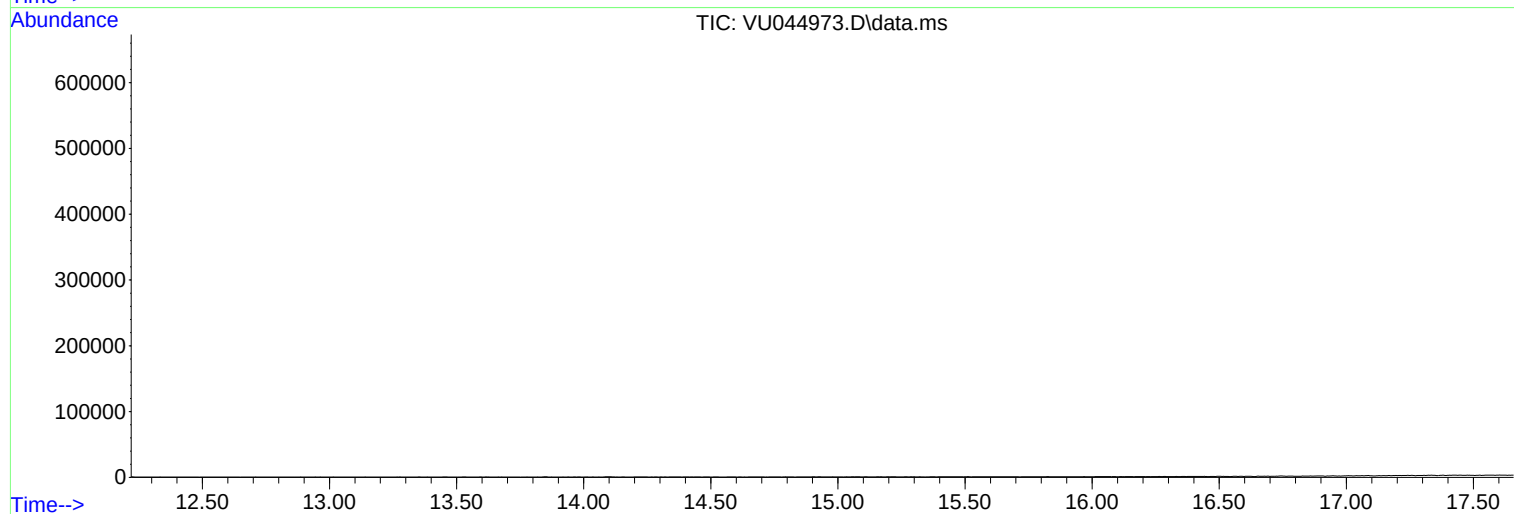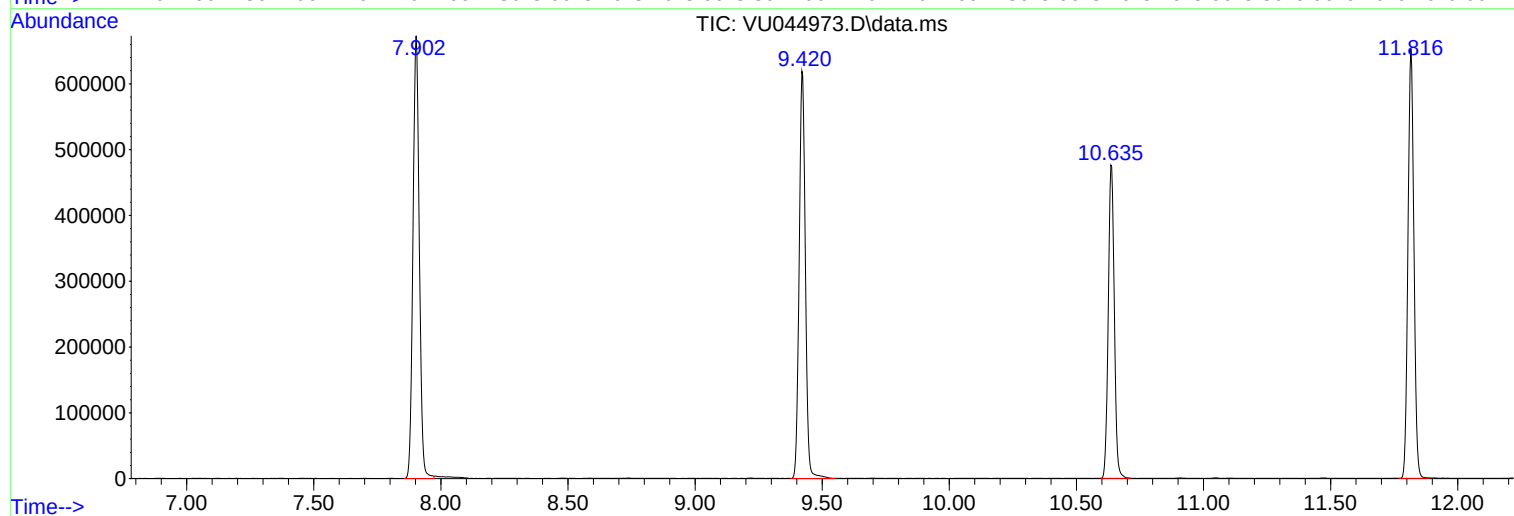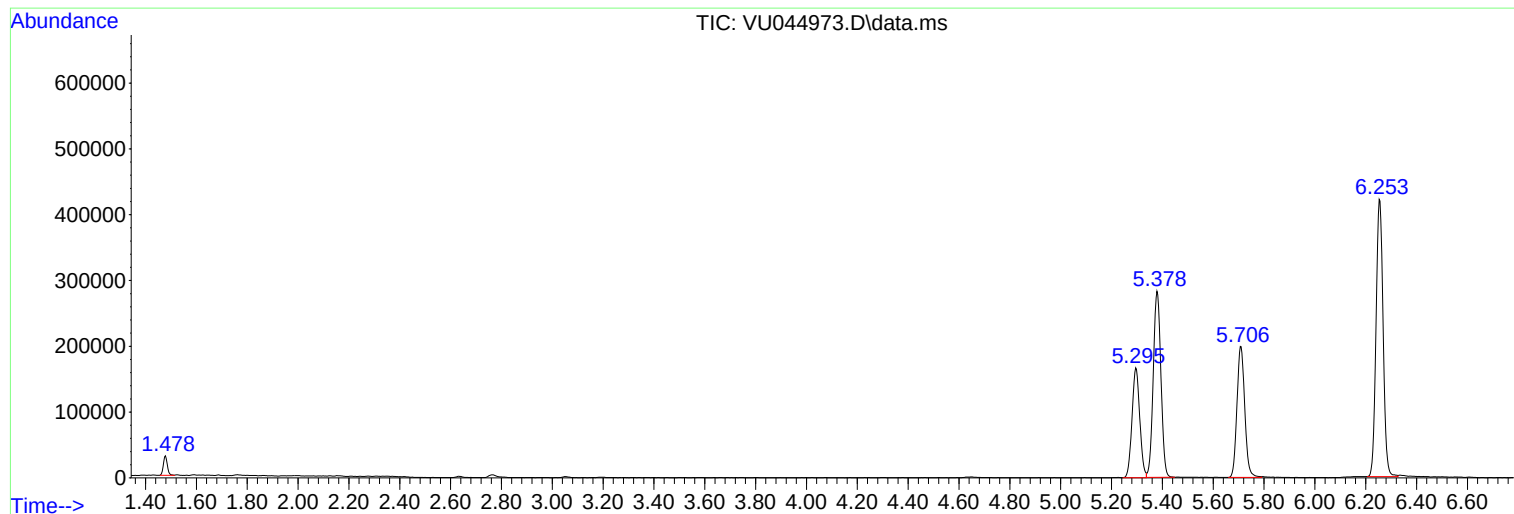

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092821\  
Data File : VU044973.D  
Acq On : 29 Sep 2021 04:29  
Operator : SY/MD  
Sample : M3952-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 48 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U092821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092821\  
Data File : VU044973.D  
Acq On : 29 Sep 2021 04:29  
Operator : SY/MD  
Sample : M3952-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 48 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U092821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |