


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092821\
 Data File : VU044928.D
 Acq On : 28 Sep 2021 09:41
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
 Title : SW846 8260
 Last Update : Tue Sep 28 12:32:13 2021

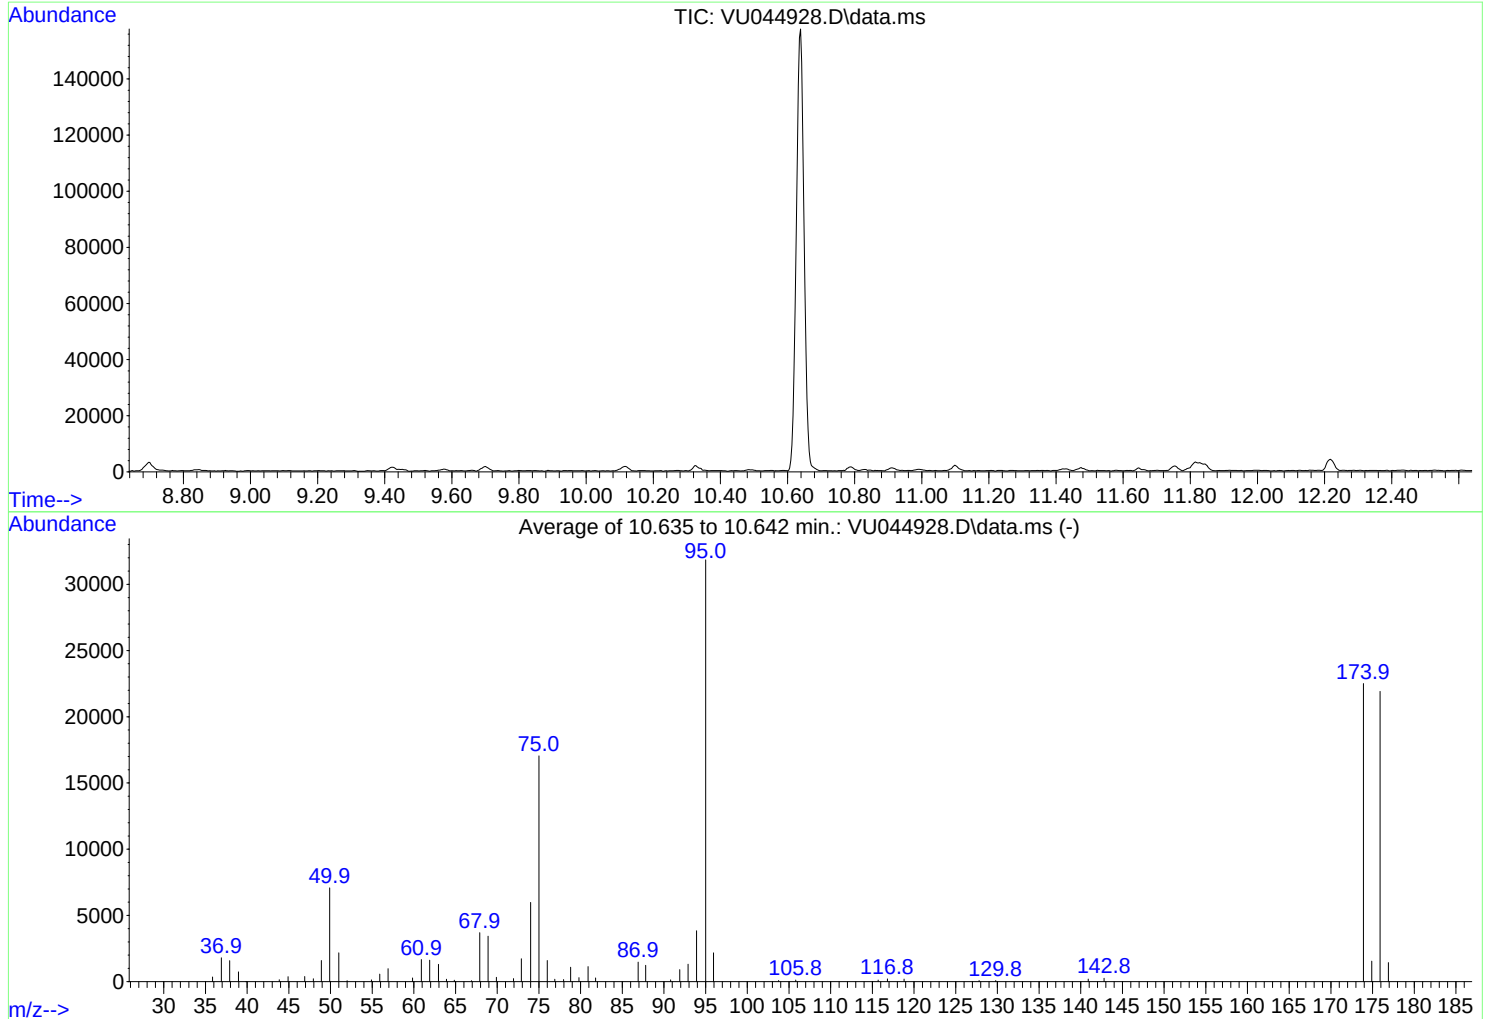

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	7075	PASS
75	95	30	60	53.5	17047	PASS
95	95	100	100	100.0	31848	PASS
96	95	5	9	6.8	2177	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.7	22509	PASS
175	174	5	9	6.9	1548	PASS
176	174	95	101	97.4	21915	PASS
177	176	5	9	6.6	1436	PASS