

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092823\
 Data File : VU055580.D
 Acq On : 28 Sep 2023 16:00
 Operator : MD/SY
 Sample : 04530-09DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYHY5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	106	rBV2	152584	181432	19.76%	2.560%
2	1.914	185	194	207	rBV	109383	138845	15.13%	1.959%
3	2.567	385	397	415	rBV	168000	282856	30.81%	3.991%
4	3.042	531	545	562	rBV2	20298	39826	4.34%	0.562%
5	3.184	575	589	607	rVB	15025	34408	3.75%	0.485%
6	4.663	1026	1049	1079	rBV3	304463	917982	100.00%	12.951%
7	5.062	1156	1173	1197	rVB2	160230	362590	39.50%	5.116%
8	5.724	1359	1379	1412	rBV2	315370	816099	88.90%	11.514%
9	6.248	1528	1542	1570	rBV	198073	394346	42.96%	5.564%
10	6.544	1620	1634	1650	rBV4	29442	62699	6.83%	0.885%
11	6.689	1665	1679	1706	rBV	190939	386224	42.07%	5.449%
12	7.566	1939	1952	1975	rBV	87319	166376	18.12%	2.347%
13	7.897	2042	2055	2077	rBV	362509	649464	70.75%	9.163%
14	8.180	2132	2143	2163	rBV	52910	98799	10.76%	1.394%
15	8.553	2249	2259	2273	rVB3	32659	55547	6.05%	0.784%
16	8.637	2273	2285	2318	rBV2	255221	663248	72.25%	9.357%
17	9.415	2515	2527	2558	rBV	301457	521264	56.78%	7.354%
18	10.753	2932	2943	2963	rVB2	134636	227322	24.76%	3.207%
19	11.811	3260	3272	3288	rBV	322396	528280	57.55%	7.453%
20	12.190	3376	3390	3413	rBV	327969	560365	61.04%	7.906%




Sum of corrected areas: 7087972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092823\
Data File : VU055580.D
Acq On : 28 Sep 2023 16:00
Operator : MD/SY
Sample : 04530-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

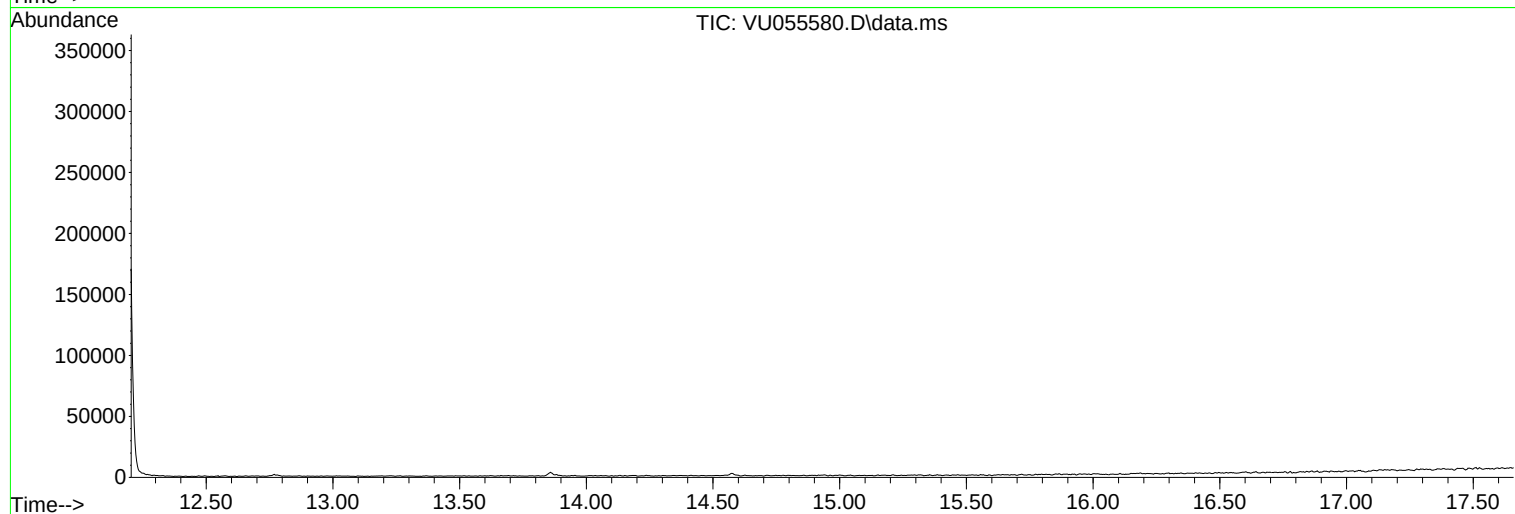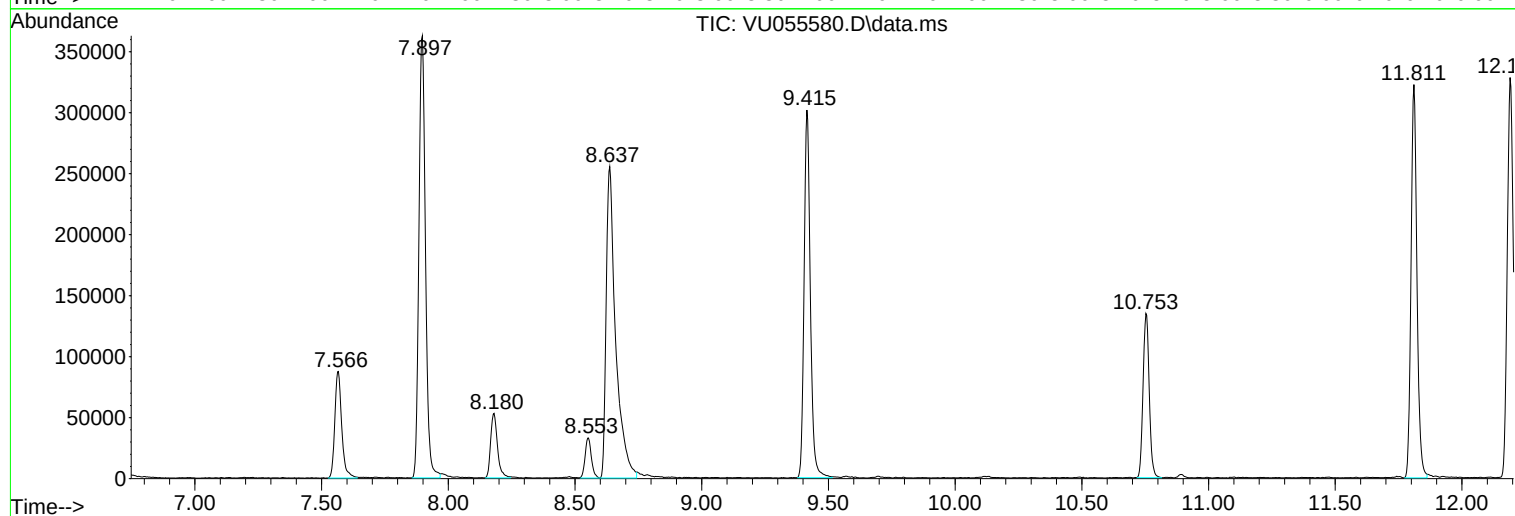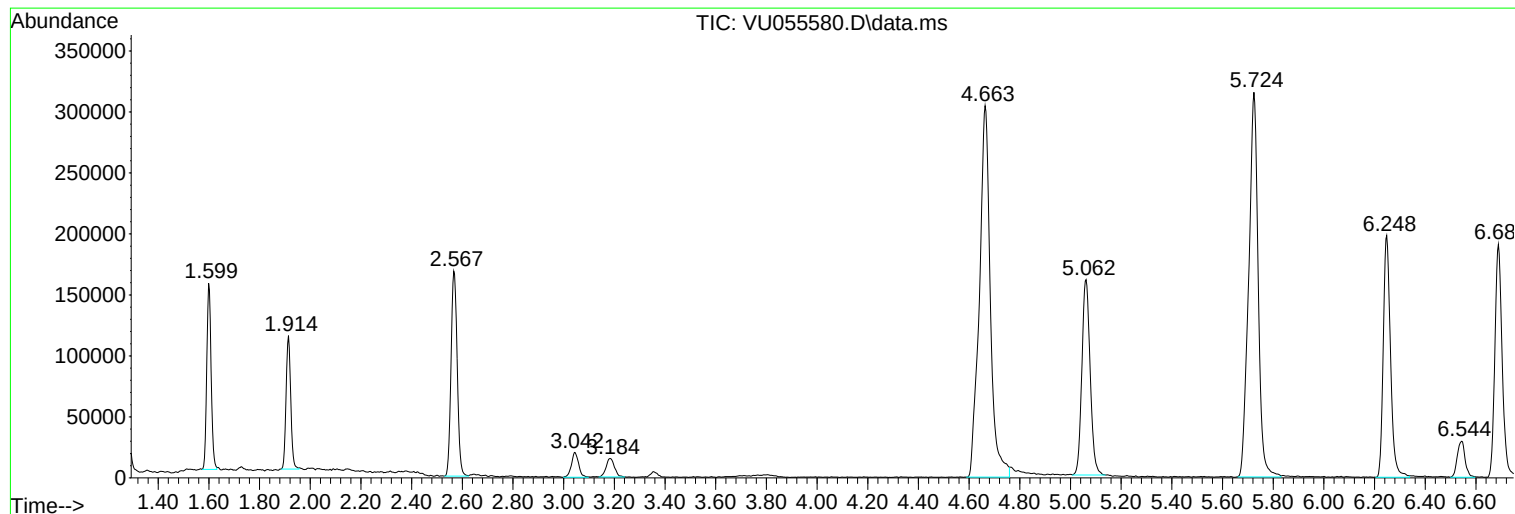

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092823\
Data File : VU055580.D
Acq On : 28 Sep 2023 16:00
Operator : MD/SY
Sample : 04530-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092823\
Data File : VU055580.D
Acq On : 28 Sep 2023 16:00
Operator : MD/SY
Sample : 04530-09DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYHY5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc