


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092823\
Data File : VU055570.D
Acq On : 28 Sep 2023 09:42
Operator : MD/SY
Sample : BFB054
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB054

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 27 23:33:30 2023

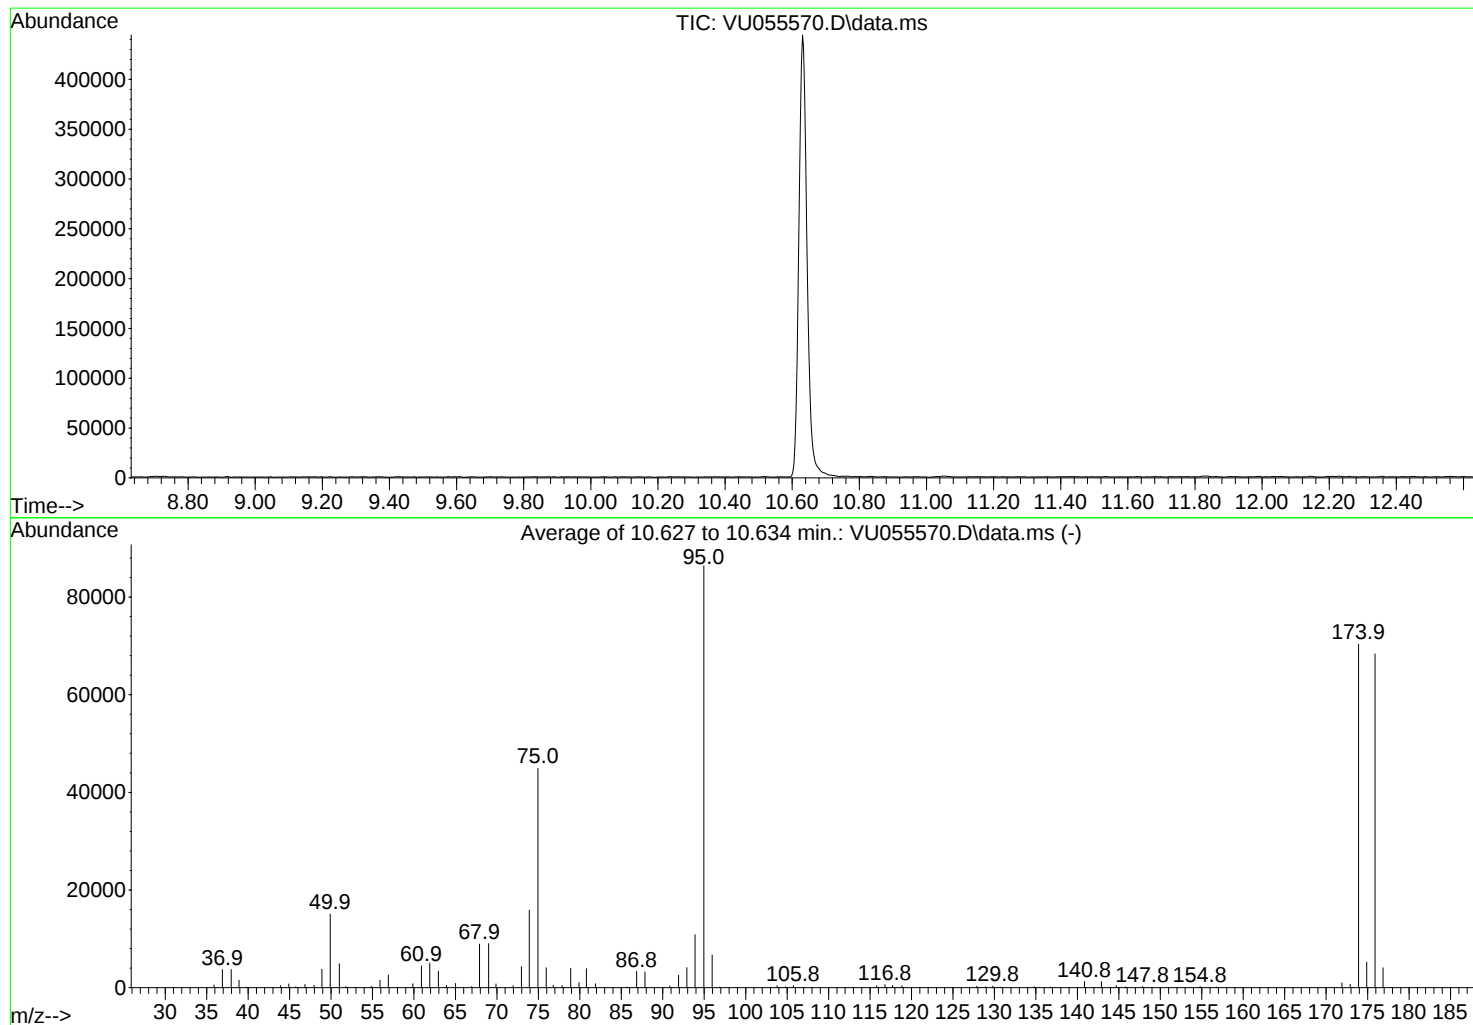

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	15095	PASS
75	95	30	80	52.0	44912	PASS
95	95	100	100	100.0	86403	PASS
96	95	5	9	7.8	6697	PASS
173	174	0.00	2	1.0	680	PASS
174	95	50	120	81.4	70357	PASS
175	174	5	9	7.4	5210	PASS
176	174	95	101	97.2	68381	PASS
177	176	5	9	5.9	4067	PASS

m/z	Abundance
39.80	347.0
43.90	617.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	641.0
36.90	3629.0
37.90	3733.0
38.90	1574.0
39.70	482.0
41.00	102.0
43.90	957.0
44.90	764.0
45.70	135.0
46.90	735.0
48.00	498.0
48.90	3553.0
49.90	14910.0
51.00	4770.0
51.80	174.0
53.00	107.0
54.80	311.0
55.90	1407.0
56.90	2436.0
59.90	762.0
60.90	3915.0
61.90	5190.0
63.00	3340.0
63.90	480.0
65.00	832.0
66.90	269.0
67.90	8746.0
69.00	8726.0
69.90	736.0
72.00	444.0
72.90	4232.0
73.90	15498.0
74.90	44568.0
75.90	4112.0
76.80	648.0
77.90	433.0
78.90	3836.0
79.90	1085.0
80.80	3861.0
81.90	730.0
82.80	127.0
85.70	151.0
86.80	3230.0
87.80	3160.0
90.90	362.0
91.90	2327.0
92.90	3982.0
93.90	10389.0
94.90	84376.0
96.00	6506.0
96.80	110.0
103.80	444.0
104.80	176.0
105.70	414.0
106.80	100.0
112.80	130.0
115.80	347.0
116.80	595.0
117.60	411.0
118.80	399.0
127.80	224.0
128.90	133.0
129.80	334.0
130.70	116.0
134.80	183.0
136.70	111.0
140.90	1148.0
142.90	1214.0
144.70	405.0
145.90	164.0
147.80	302.0
154.80	244.0
156.70	101.0
158.80	116.0
171.90	869.0
172.90	734.0
173.90	66176.0
174.90	5216.0
175.90	63504.0
176.90	4184.0
177.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	561.0
36.90	3719.0
38.00	3861.0
38.90	1561.0
39.70	448.0
43.90	1019.0
44.90	796.0
45.80	177.0
46.90	640.0
47.90	507.0
48.90	3947.0
49.90	15602.0
51.00	5063.0
51.80	241.0
52.90	104.0
54.80	265.0
55.90	1593.0
56.90	2642.0
59.80	807.0
60.90	4703.0
61.90	5244.0
62.90	3525.0
63.90	468.0
65.00	911.0
65.90	104.0
66.90	251.0
67.90	9236.0
69.00	9223.0
69.90	739.0
72.00	403.0
73.00	4396.0
73.90	16448.0
74.90	46168.0
75.90	4262.0
76.80	511.0
77.80	431.0
78.90	4169.0
79.90	1082.0
80.80	4033.0
81.90	812.0
85.70	151.0
86.80	3395.0
87.80	3326.0
90.90	309.0
91.90	2572.0
92.90	4268.0
93.90	11297.0
94.90	89136.0
96.00	6933.0
96.80	106.0
103.80	384.0
104.80	177.0
105.70	385.0
115.80	406.0
116.80	635.0
117.70	419.0
118.80	400.0
127.80	253.0
128.90	211.0
129.80	349.0
130.70	113.0
134.80	200.0
136.80	138.0
140.80	1293.0
142.90	1234.0
144.70	471.0
145.80	185.0
147.90	215.0
154.80	219.0
156.80	137.0
170.90	111.0
171.90	998.0
172.90	713.0
173.90	72640.0
174.90	5367.0
175.90	70536.0
176.80	4157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	476.0
36.90	3762.0
37.90	3504.0
38.90	1409.0
39.80	433.0
43.90	1079.0
44.90	754.0
45.80	169.0
46.80	628.0
47.90	426.0
48.90	3840.0
49.90	14773.0
51.00	4792.0
51.80	256.0
52.80	115.0
54.90	217.0
55.90	1494.0
56.90	2678.0
59.80	799.0
60.90	4805.0
61.90	4638.0
62.90	3235.0
63.90	453.0
65.00	784.0
66.00	156.0
67.00	191.0
67.90	8757.0
69.00	9143.0
69.90	751.0
71.90	353.0
73.00	4231.0
73.90	15734.0
75.00	44000.0
76.00	3843.0
76.90	348.0
77.80	452.0
78.90	3932.0
79.90	1013.0
80.80	3794.0
81.90	807.0
85.70	147.0
86.90	3400.0
87.90	3163.0
90.80	295.0
91.90	2663.0
92.90	4068.0
93.90	10911.0
95.00	85696.0
95.90	6651.0
96.90	125.0
103.80	314.0
104.80	133.0
105.80	362.0
115.80	430.0
116.80	635.0
117.80	436.0
118.90	423.0
127.90	313.0
128.90	243.0
129.80	344.0
130.80	117.0
134.80	188.0
136.80	147.0
140.80	1254.0
141.80	119.0
142.90	1218.0
144.70	454.0
145.70	181.0
147.90	172.0
154.80	193.0
156.70	174.0
171.00	163.0
171.90	1102.0
172.90	592.0
173.90	72256.0
174.90	5046.0
175.90	71104.0
176.80	3860.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054